

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011022\
 Data File : VN070545.D
 Acq On : 10 Jan 2022 16:03
 Operator : JC/MD
 Sample : N1037-03 10X
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 NWB-1542

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
 Title : SW846 8260

Signal : TIC: VN070545.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.236	82	92	110	rBV2	43867	90301	1.68%	0.152%
2	3.706	617	640	676	rVB2	410793	1237187	23.03%	2.076%
3	4.140	784	802	830	rBV	20384	60709	1.13%	0.102%
4	4.285	835	856	897	rVB	113269	341314	6.35%	0.573%
5	7.337	1975	1994	2011	rBV3	22618	65003	1.21%	0.109%
6	8.018	2224	2248	2259	rBV	650404	1560809	29.05%	2.619%
7	8.083	2260	2272	2297	rVB	1165688	2653166	49.38%	4.452%
8	8.434	2382	2403	2434	rBV	849857	2011172	37.43%	3.375%
9	8.965	2579	2601	2635	rBV	1803007	3751591	69.82%	6.295%
10	10.440	3130	3151	3163	rBV	2901927	5372996	100.00%	9.016%
11	10.502	3163	3174	3193	rVB	1155756	2170198	40.39%	3.642%
12	11.119	3381	3404	3406	rBV2	42884	77941	1.45%	0.131%
13	11.744	3614	3637	3659	rBV	2499812	4581278	85.26%	7.688%
14	11.843	3660	3674	3694	rVB	511366	890138	16.57%	1.494%
15	11.948	3695	3713	3738	rBV	2022803	3914586	72.86%	6.569%
16	12.277	3812	3836	3858	rBV	1529853	2694147	50.14%	4.521%
17	12.578	3936	3948	3960	rBV	96272	163708	3.05%	0.275%
18	12.728	3990	4004	4028	rVB	2241869	3919336	72.95%	6.577%
19	12.918	4059	4075	4085	rBV	232989	399208	7.43%	0.670%
20	12.980	4085	4098	4106	rBV	1049671	1771162	32.96%	2.972%
21	13.055	4118	4126	4141	rVB	663351	1147775	21.36%	1.926%
22	13.219	4169	4187	4202	rBV	620659	1121822	20.88%	1.882%
23	13.283	4204	4211	4225	rVV5	71932	130452	2.43%	0.219%
24	13.366	4227	4242	4270	rVV	2002939	3270929	60.88%	5.489%
25	13.498	4286	4291	4301	rVB	73546	93843	1.75%	0.157%
26	13.559	4303	4314	4324	rBV2	154172	246610	4.59%	0.414%
27	13.608	4324	4332	4342	rBV5	68444	114195	2.13%	0.192%
28	13.672	4343	4356	4389	rVV2	1991003	4855845	90.37%	8.148%
29	13.836	4408	4417	4419	rBV2	105908	113150	2.11%	0.190%
30	13.871	4420	4430	4438	rBV3	592020	981003	18.26%	1.646%
31	13.991	4465	4475	4488	rBV4	333121	550362	10.24%	0.924%
32	14.066	4494	4503	4514	rVB2	177455	265587	4.94%	0.446%
33	14.128	4517	4526	4531	rBV	227679	336878	6.27%	0.565%
34	14.214	4548	4558	4569	rVB	347337	525876	9.79%	0.882%
35	14.326	4588	4600	4611	rVB3	374083	622941	11.59%	1.045%
36	14.458	4639	4649	4659	rBV3	155110	278126	5.18%	0.467%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011022\
Data File : VN070545.D
Acq On : 10 Jan 2022 16:03
Operator : JC/MD
Sample : N1037-03 10X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NWB-1542

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Title : SW846 8260

37	14.576	4686	4693	4702	rVB	319435	441588	8.22%	0.741%
38	14.619	4703	4709	4717	rVV4	128355	161107	3.00%	0.270%
39	14.659	4720	4724	4740	rVB7	94896	151783	2.82%	0.255%
40	14.807	4770	4779	4786	rBV2	302013	486354	9.05%	0.816%
41	14.844	4788	4793	4806	rVB3	348574	513768	9.56%	0.862%
42	14.927	4808	4824	4838	rBV3	761681	1818727	33.85%	3.052%
43	15.083	4870	4882	4898	rVB	567027	996528	18.55%	1.672%
44	15.193	4915	4923	4932	rBV6	119032	178148	3.32%	0.299%
45	15.466	5015	5025	5034	rBV5	100504	187704	3.49%	0.315%
46	15.560	5051	5060	5070	rBV2	128447	208993	3.89%	0.351%
47	15.622	5074	5083	5084	rBV9	61522	78523	1.46%	0.132%
48	15.700	5106	5112	5133	rVB2	226149	395045	7.35%	0.663%
49	15.802	5141	5150	5167	rVB3	154209	313938	5.84%	0.527%
50	16.016	5222	5230	5249	rVB2	352263	668143	12.44%	1.121%
51	16.341	5341	5351	5366	rVB3	203704	390858	7.27%	0.656%
52	16.547	5419	5428	5443	rVB5	109359	219908	4.09%	0.369%


Sum of corrected areas: 59592459

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011022\
Data File : VN070545.D
Acq On : 10 Jan 2022 16:03
Operator : JC/MD
Sample : N1037-03 10X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NWB-1542

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

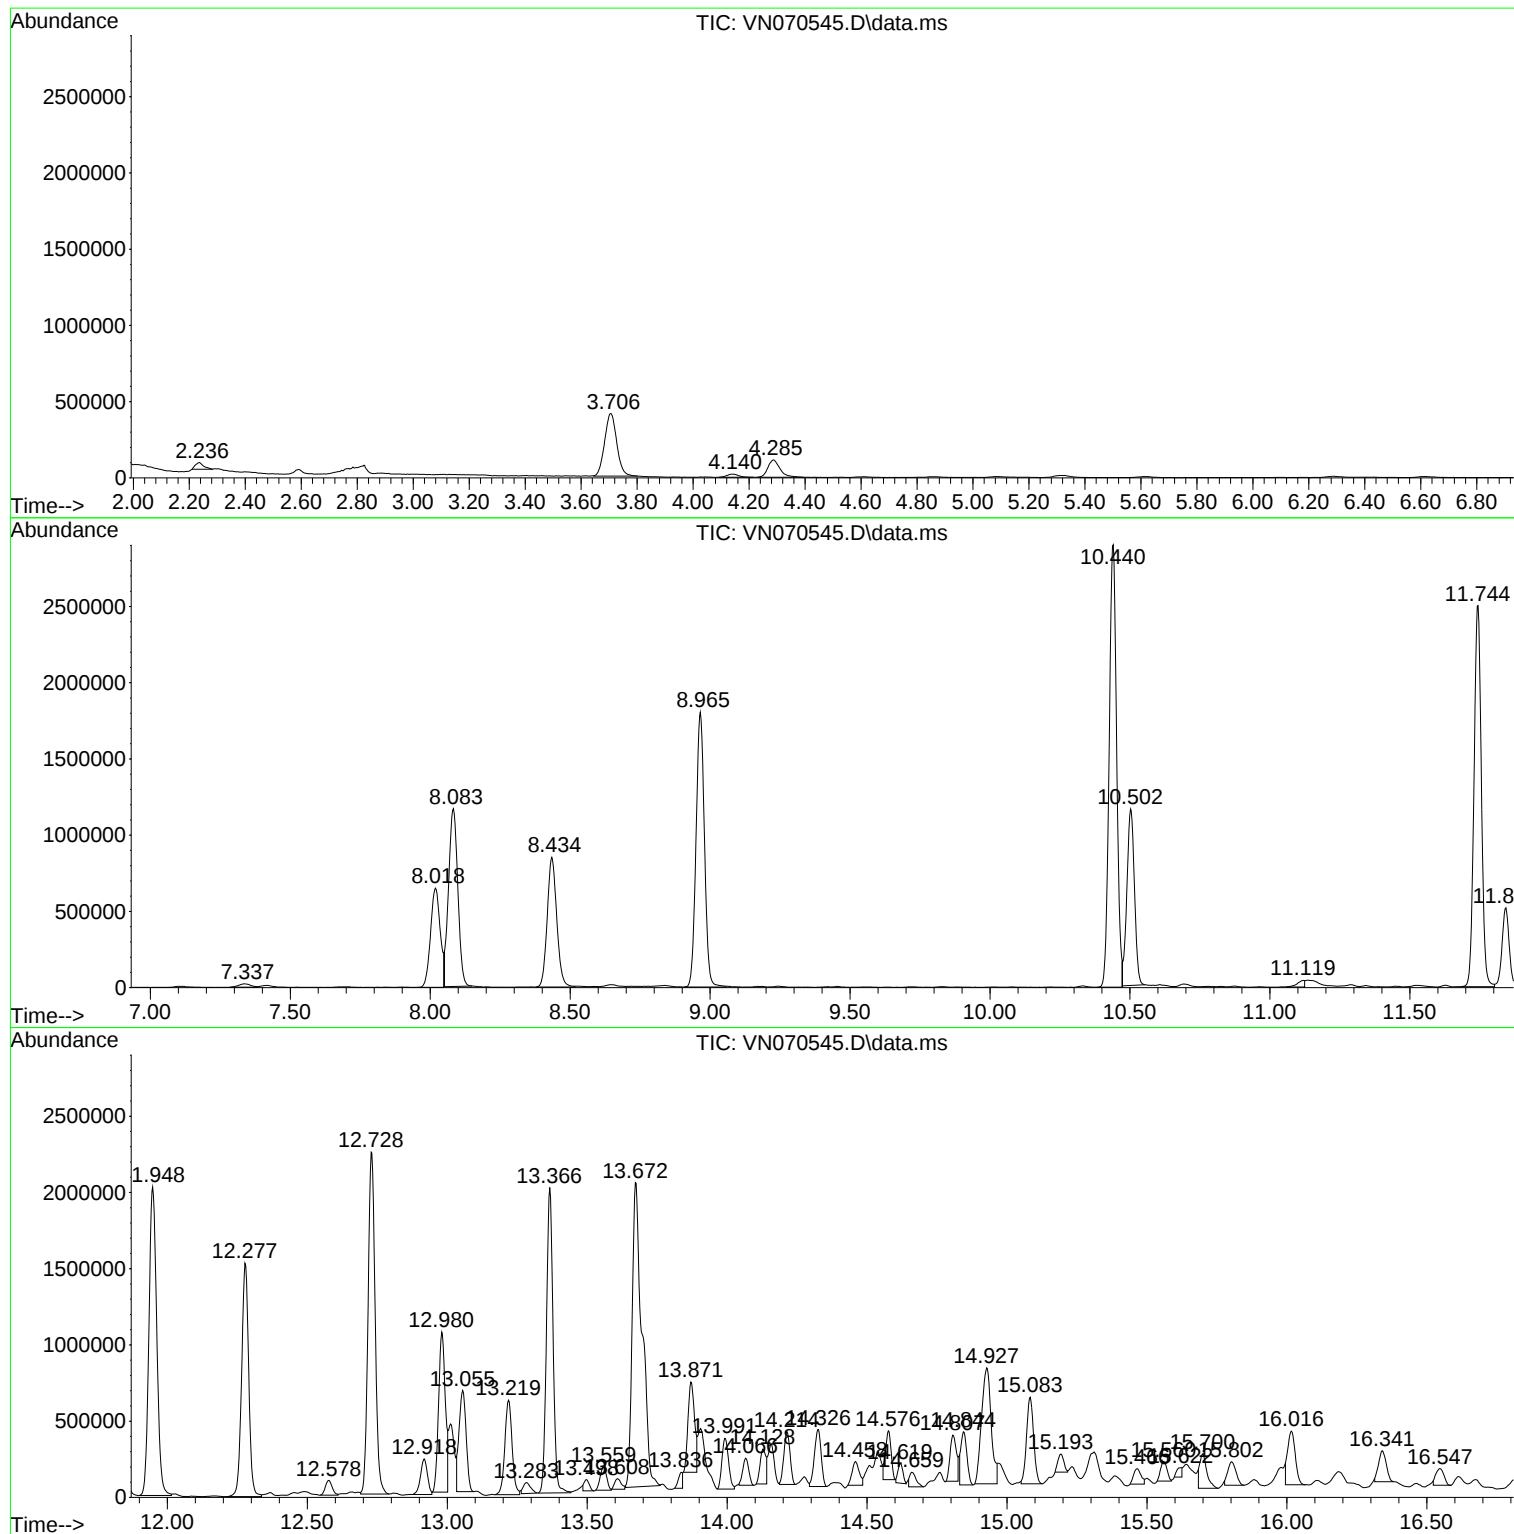

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011022\
Data File : VN070545.D
Acq On : 10 Jan 2022 16:03
Operator : JC/MD
Sample : N1037-03 10X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NWB-1542

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011022\
Data File : VN070545.D
Acq On : 10 Jan 2022 16:03
Operator : JC/MD
Sample : N1037-03 10X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NWB-1542

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc