
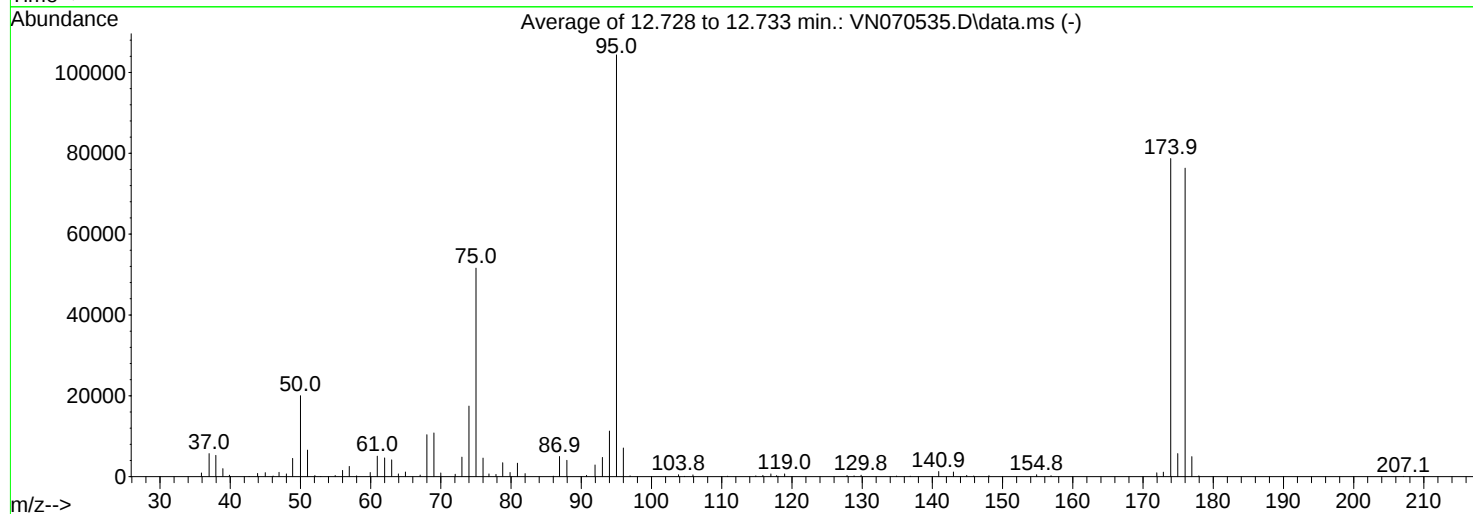


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011022\
Data File : VN070535.D
Acq On : 10 Jan 2022 9:38
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Title : SW846 8260
Last Update : Mon Dec 27 18:47:12 2021

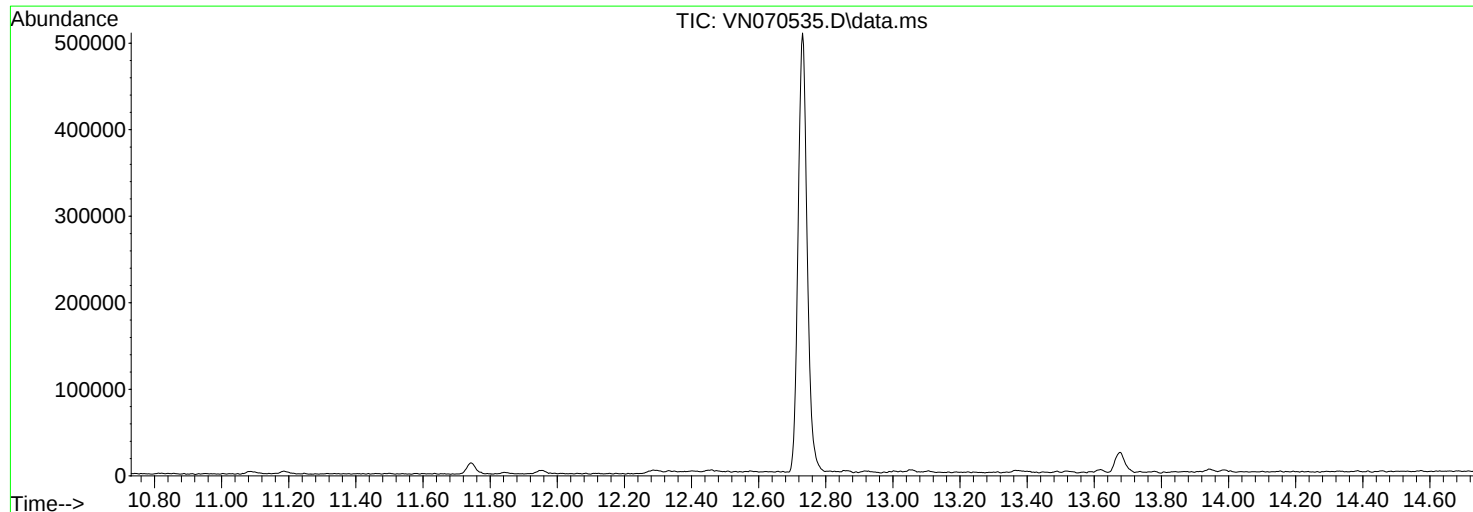

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3987

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	20035	PASS
75	95	30	60	49.4	51576	PASS
95	95	100	100	100.0	104352	PASS
96	95	5	9	6.8	7089	PASS
173	174	0.00	2	1.4	1122	PASS
174	95	50	100	75.4	78685	PASS
175	174	5	9	7.3	5706	PASS
176	174	95	101	97.0	76336	PASS
177	176	5	9	6.5	4937	PASS