
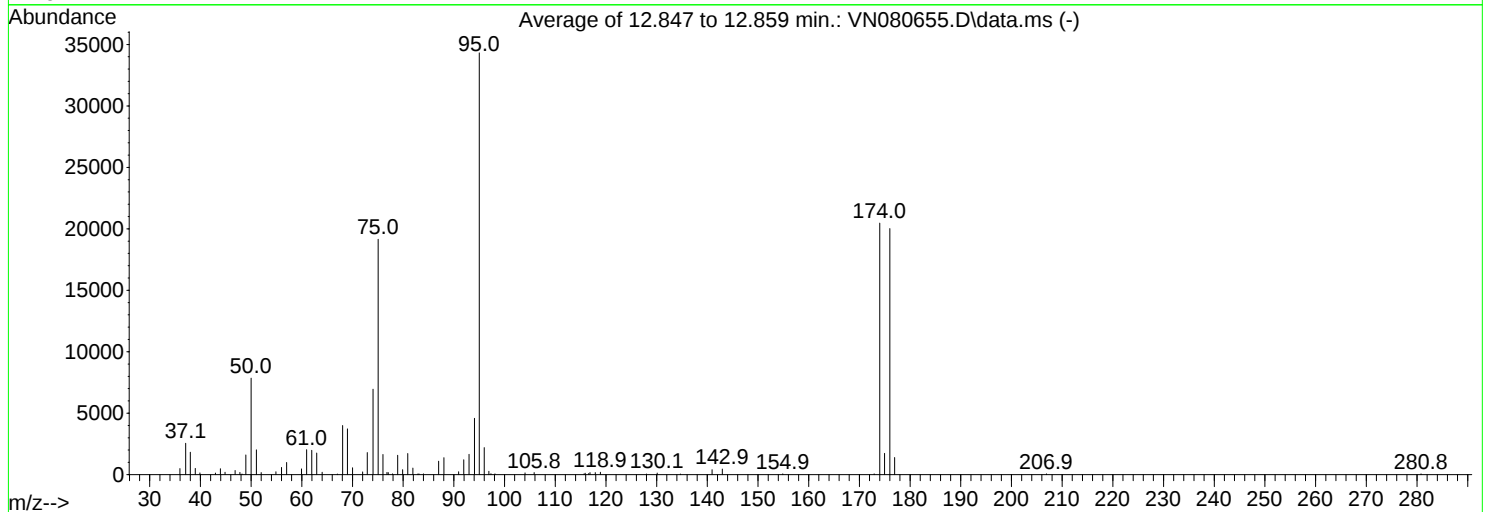


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011024\
Data File : VN080655.D
Acq On : 10 Jan 2024 09:04
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M
Title : SW846 8260
Last Update : Thu Jan 11 06:34:36 2024

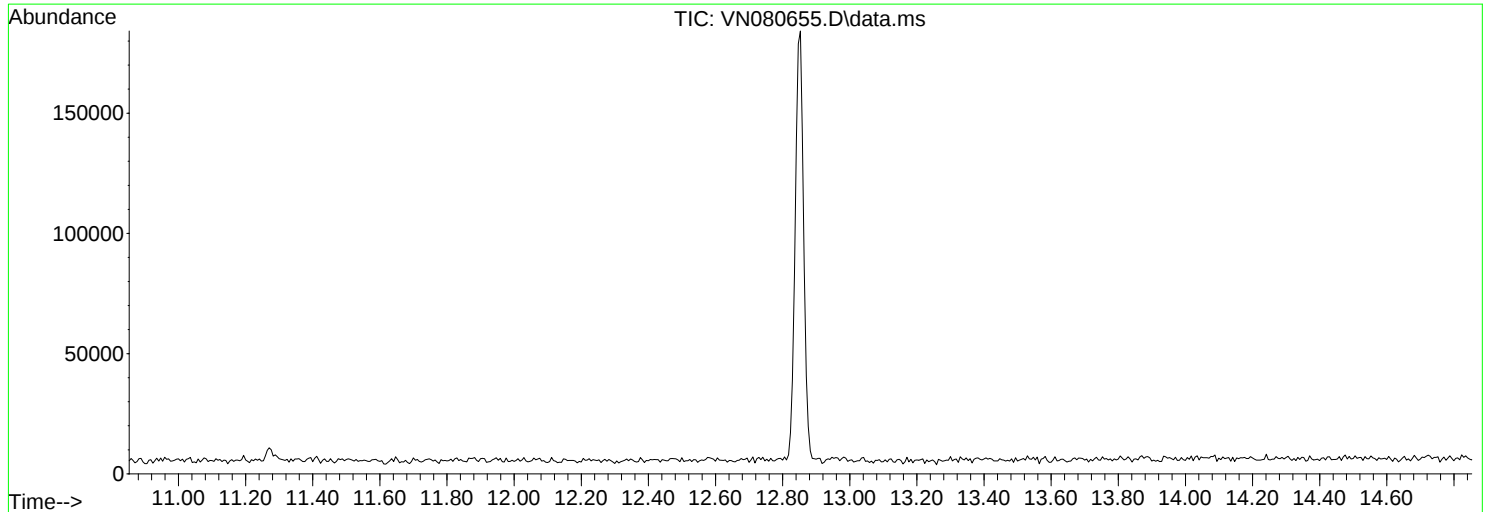

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	7847	PASS
75	95	30	60	55.8	19147	PASS
95	95	100	100	100.0	34320	PASS
96	95	5	9	6.4	2196	PASS
173	174	0.00	2	0.3	66	PASS
174	95	50	100	59.6	20461	PASS
175	174	5	9	8.5	1737	PASS
176	174	95	101	97.9	20029	PASS
177	176	5	9	7.0	1394	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	494	48.95	1604	64.00	190	77.05	164
37.10	2553	50.00	7847	67.00	51	77.90	61
38.00	1819	51.05	2025	68.05	3995	78.90	157
39.00	511	52.00	165	69.00	3722	79.90	40
39.90	138	54.90	235	70.00	566	80.90	1718
42.95	131	56.00	581	72.00	217	81.90	530
43.95	487	57.00	989	72.90	1794	82.90	52
44.85	195	59.95	471	74.05	6951	83.10	61
46.85	337	60.95	2030	75.05	19147	84.00	61
47.80	180	61.95	1984	76.00	1639	87.00	1099
48.20	53	62.95	1756	76.80	180	88.05	1382

Average of 12.847 to 12.859 min.: VN080655.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.95	240	115.70	64	154.90	68		
91.95	1213	115.90	112	172.90	66		
93.00	1656	116.60	94	174.00	20461		
94.05	4582	116.85	166	174.95	1737		
95.00	34320	117.90	169	176.00	20029		
96.00	2196	118.90	201	176.95	1394		
96.90	268	128.00	53	206.90	62		
97.30	83	130.10	136	280.80	61		
98.10	72	134.70	56				
104.05	148	140.95	398				
105.85	171	142.95	460				

Instrument :

MSVOA_N

ClientSampleId :

BFB