
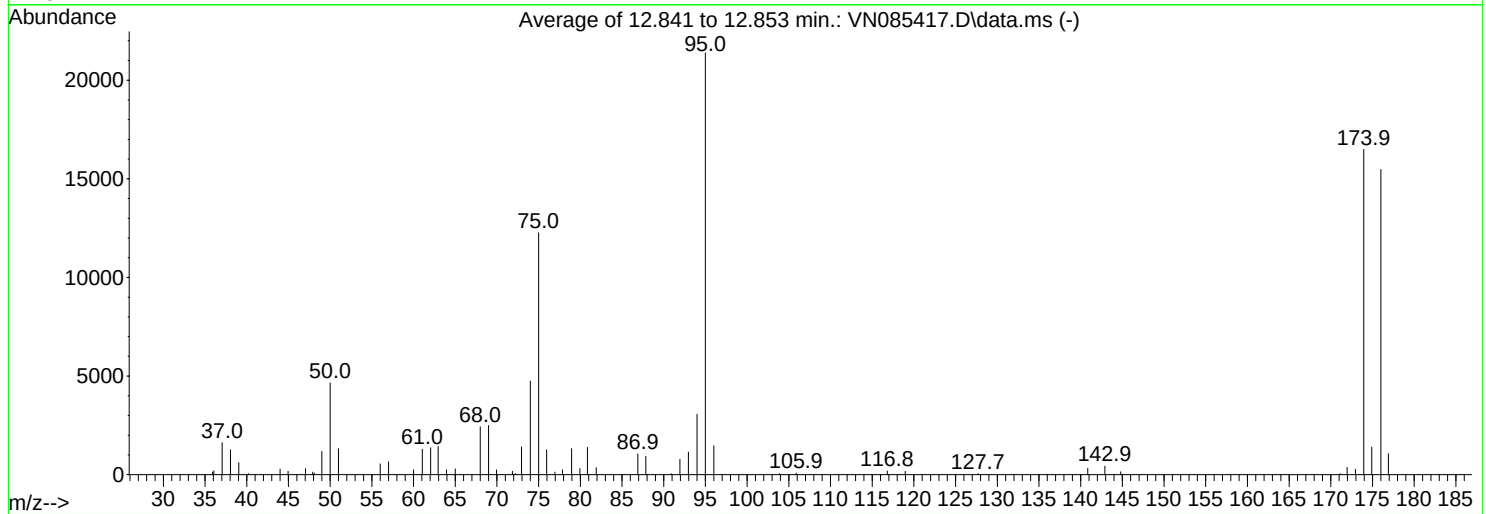


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011025\
Data File : VN085417.D
Acq On : 10 Jan 2025 09:42
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N122024W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Sat Dec 21 02:03:07 2024

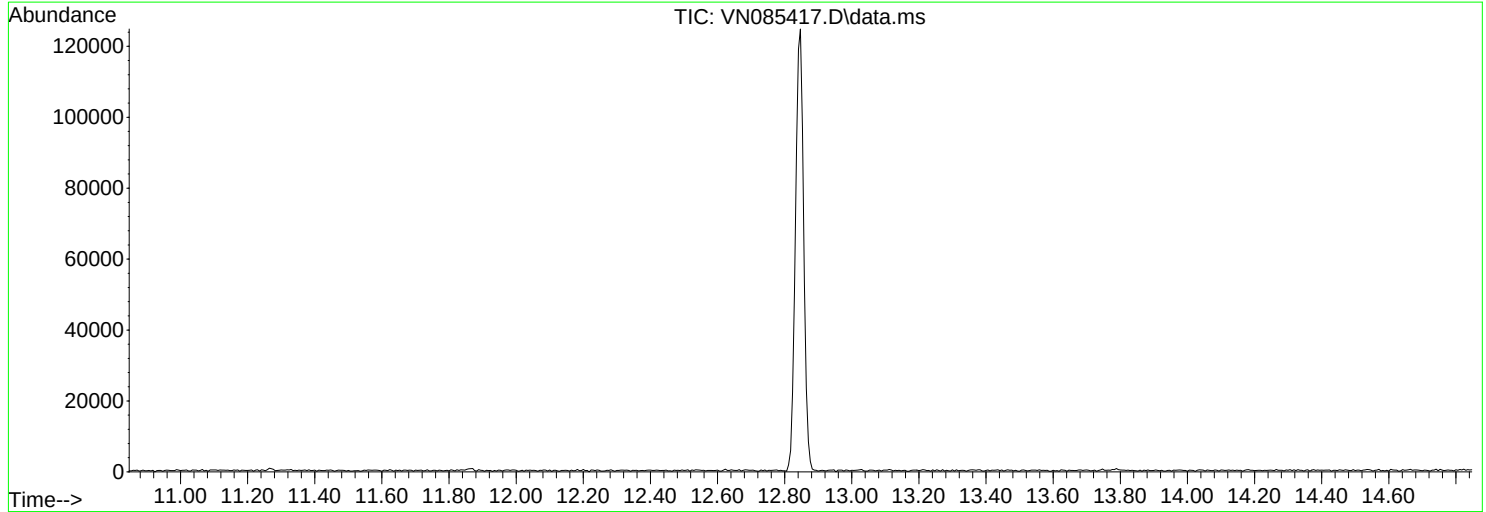

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.7	4650	PASS
75	95	30	60	57.3	12258	PASS
95	95	100	100	100.0	21387	PASS
96	95	5	9	6.9	1470	PASS
173	174	0.00	2	1.7	275	PASS
174	95	50	100	77.1	16492	PASS
175	174	5	9	8.4	1392	PASS
176	174	95	101	93.8	15468	FAIL*
177	176	5	9	6.8	1059	PASS