


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN011119\
Data File : VN053352.D
Acq On : 11 Jan 2019 8:29
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N010519W.M
Title : SW846 8260
Last Update : Mon Jan 07 09:34:27 2019

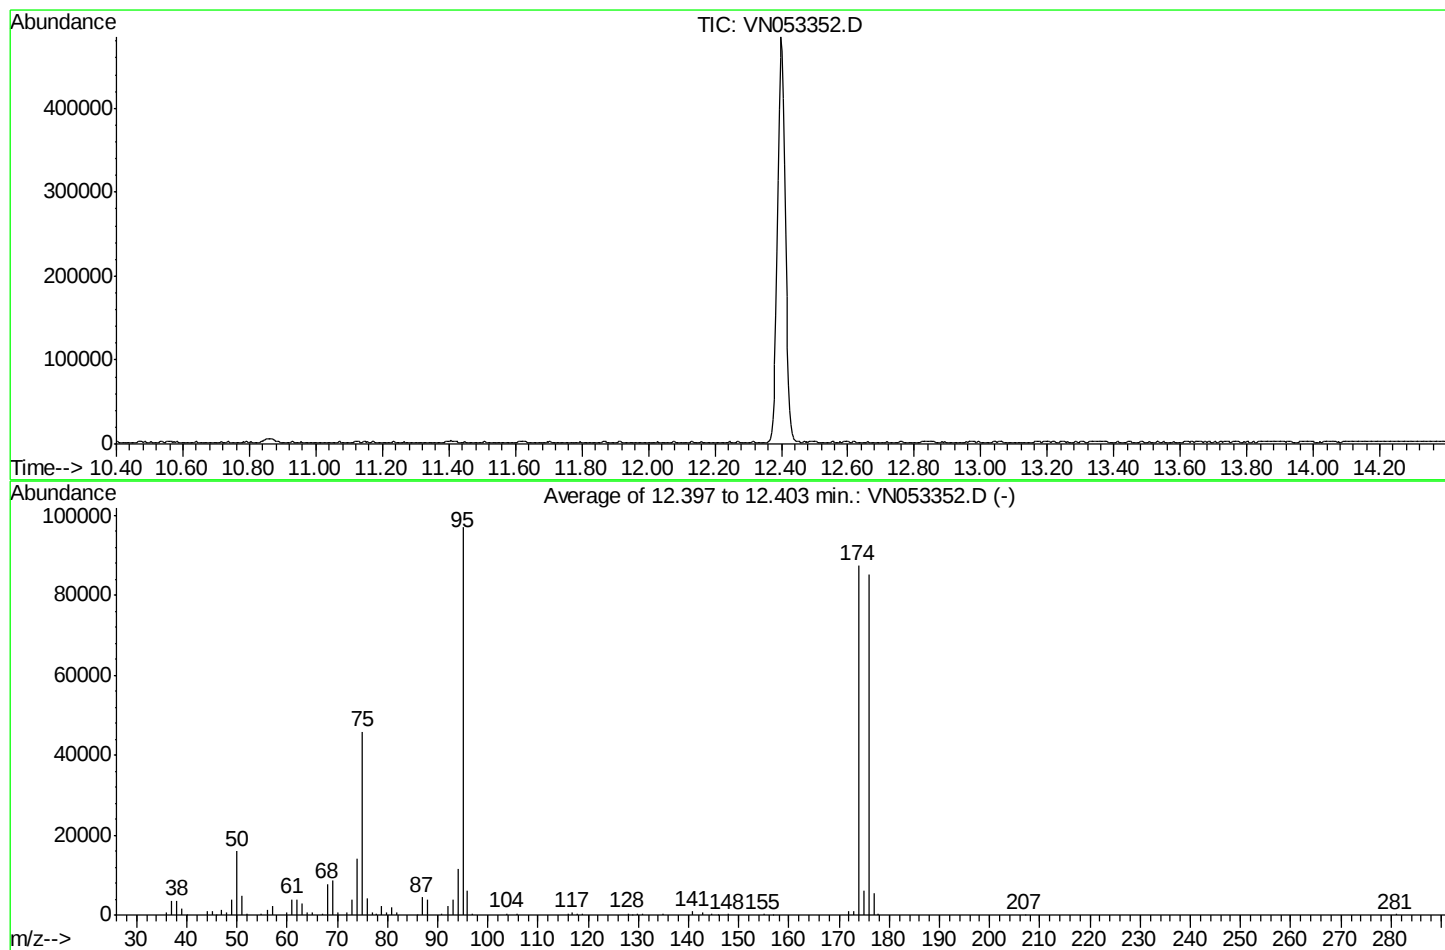

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	15912	PASS
75	95	30	60	47.3	45882	PASS
95	95	100	100	100.0	97058	PASS
96	95	5	9	6.3	6137	PASS
173	174	0.00	2	1.0	862	PASS
174	95	50	100	90.1	87437	PASS
175	174	5	9	6.8	5985	PASS
176	174	95	101	97.4	85173	PASS
177	176	5	9	6.4	5416	PASS