

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011121\
 Data File : VN065468.D
 Acq On : 11 Jan 2021 15:15
 Operator : JC/MD
 Sample : M1040-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jan 12 00:08:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 22 15:42:18 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.630	168	220634	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.553	114	362329	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.380	117	390695	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.318	152	172270	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.991	65	120779	48.49	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	96.98%		
35) Dibromofluoromethane	7.553	113	110376	50.49	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	100.98%		
50) Toluene-d8	10.061	98	448836	54.78	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	109.56%		
62) 4-Bromofluorobenzene	12.376	95	181196	55.32	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	110.64%		
Target Compounds						Qvalue
11) Tert butyl alcohol	4.778	59	1852	4.54	ug/l #	73
13) Acrolein	3.528	56	60	2.63	ug/l #	1
16) Acetone	3.791	43	31351	20.10	ug/l	92
18) Methyl Acetate	4.293	43	778	0.35	ug/l #	50
19) Methyl tert-butyl Ether	5.013	73	14031	2.04	ug/l	92
20) Methylene Chloride	4.508	84	22741	9.36	ug/l	98
22) Diisopropyl ether	5.920	45	17088	2.40	ug/l	98
23) Vinyl Acetate	5.920	43	9323	1.56	ug/l #	71
25) 2-Butanone	6.811	43	8510	6.09	ug/l	91
29) Tetrahydrofuran	7.190	42	760	0.84	ug/l #	32
31) Cyclohexane	7.621	56	6606	1.80	ug/l #	46
36) 1,1-Dichloropropene	7.627	75	13352	4.05	ug/l #	50
37) Ethyl Acetate	6.811	43	8510	2.61	ug/l #	66
38) Carbon Tetrachloride	7.630	117	18264	5.28	ug/l #	15
39) Methylcyclohexane	9.045	83	849	0.21	ug/l #	85
40) Benzene	8.003	78	308977	31.53	ug/l	97
41) Methacrylonitrile	7.184	41	1024	0.60	ug/l #	25
42) 1,2-Dichloroethane	8.003	62	2511	0.69	ug/l #	73
48) Methyl methacrylate	9.013	41	8248	3.02	ug/l #	39
51) 4-Methyl-2-Pentanone	9.958	43	1671	0.53	ug/l #	77
52) Toluene	10.126	92	568816	92.08	ug/l	98
53) t-1,3-Dichloropropene	10.126	75	6022	1.46	ug/l #	1
59) 2-Hexanone	10.823	43	26091	11.22	ug/l #	29
67) Ethyl Benzene	11.482	91	12852	0.90	ug/l	99
68) m/p-Xylenes	11.592	106	12487	2.31	ug/l	98
69) o-Xylene	11.920	106	45560	8.69	ug/l	100
70) Styrene	11.920	104	2239	0.26	ug/l #	1
74) N-amyl acetate	11.794	43	18626	3.57	ug/l #	15
76) 1,2,3-Trichloropropane	12.376	75	87123	24.79	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.707	105	16864	1.51	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.376	75	87123	62.51	ug/l #	15
84) 1,2,4-Trimethylbenzene	13.013	105	3124	0.29	ug/l	95
85) sec-Butylbenzene	13.013	105	3124	0.25	ug/l #	56
95) Naphthalene	15.109	128	394	3.41	ug/l #	69

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011121\
Data File : VN065468.D
Acq On : 11 Jan 2021 15:15
Operator : JC/MD
Sample : M1040-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jan 12 00:08:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
Quant Title : SW846 8260
QLast Update : Tue Dec 22 15:42:18 2020
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011121\
Data File : VN065468.D
Acq On : 11 Jan 2021 15:15
Operator : JC/MD
Sample : M1040-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampled :

Quant Time: Jan 12 00:08:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
Quant Title : SW846 8260
QLast Update : Tue Dec 22 15:42:18 2020
Response via : Initial Calibration




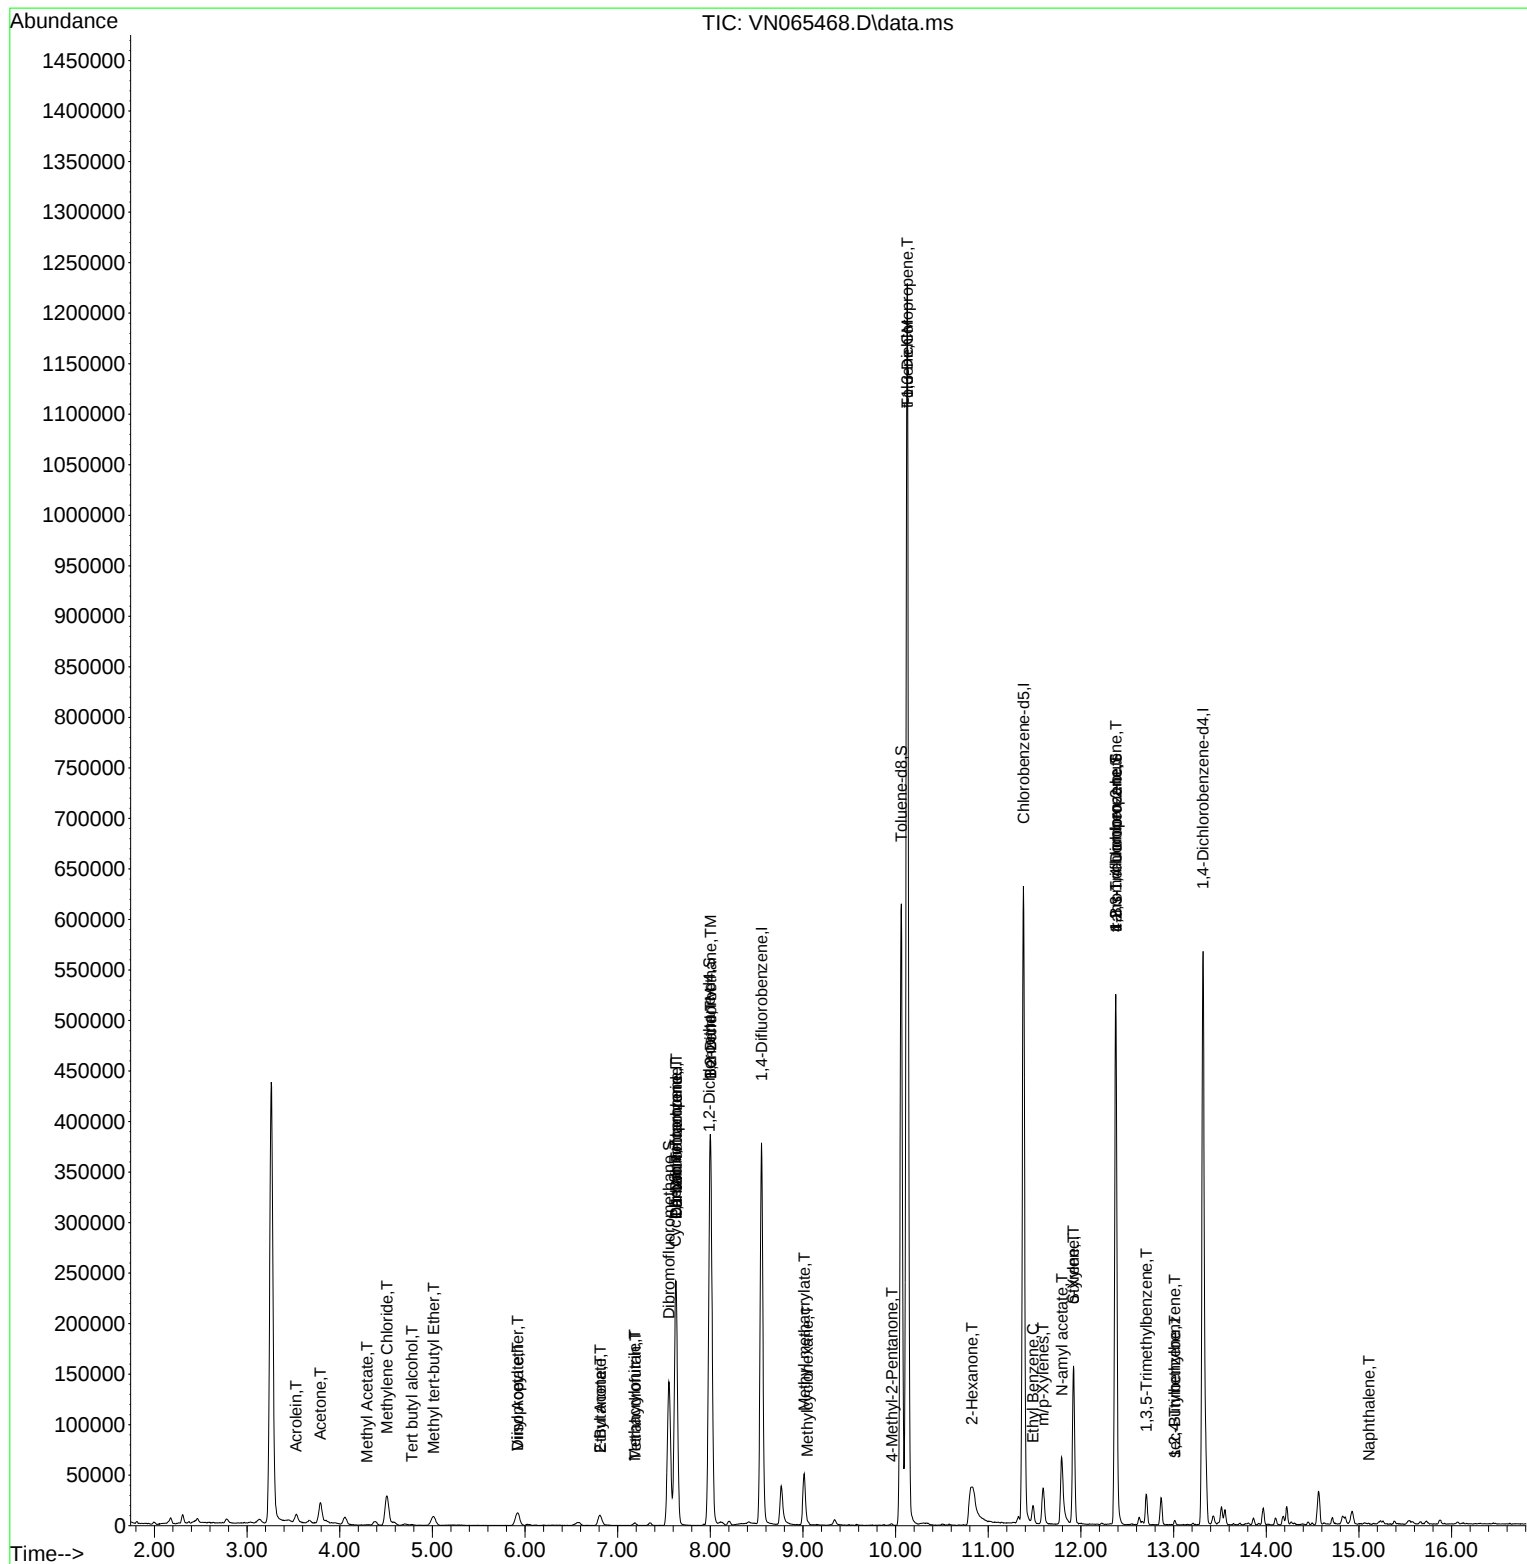




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.630 min Scan# 1832
Delta R.T. 0.003 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 220634
Ion Ratio Lower Upper
168 100
99 46.9 43.0 64.4

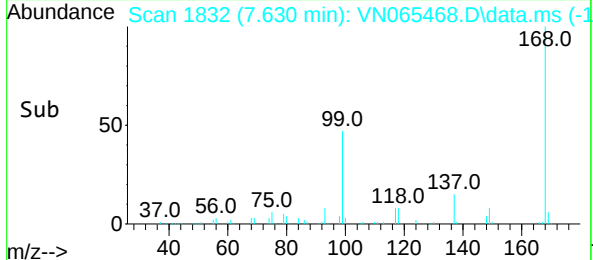

#11
Tert butyl alcohol
Concen: 4.54 ug/l
RT: 4.778 min Scan# 945
Delta R.T. 0.006 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15

Tgt Ion: 59 Resp: 1852
Ion Ratio Lower Upper
59 100
57 0.0 7.9 11.9#


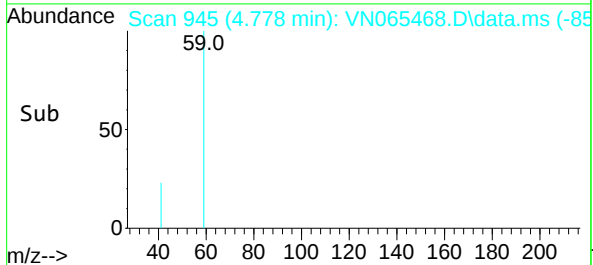

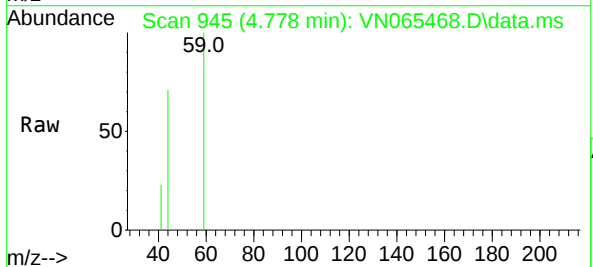




#13
Acrolein
Concen: 2.63 ug/l
RT: 3.528 min Scan# 556
Delta R.T. -0.045 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 60
Ion Ratio Lower Upper
56 100
55 12270.0 56.5 84.7#

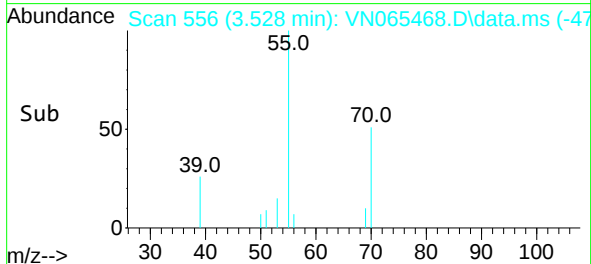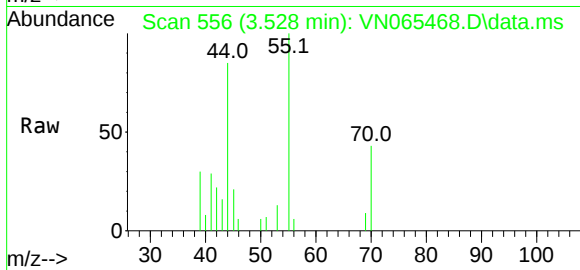

#16
Acetone
Concen: 20.10 ug/l
RT: 3.791 min Scan# 638
Delta R.T. 0.006 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15


Tgt Ion: 43 Resp: 31351
Ion Ratio Lower Upper
43 100
58 36.5 25.7 38.5

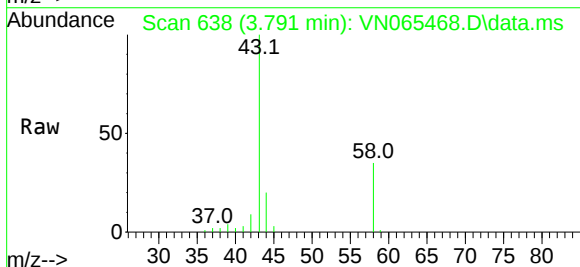



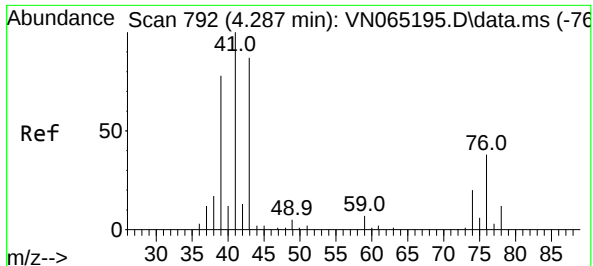


#18
Methyl Acetate
Concen: 0.35 ug/l
RT: 4.293 min Scan# 794
Delta R.T. 0.006 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion: 43 Resp: 778
Ion Ratio Lower Upper
43 100
74 0.0 20.2 30.2#

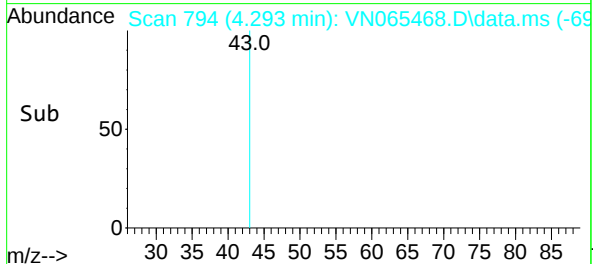

#19
Methyl tert-butyl Ether
Concen: 2.04 ug/l
RT: 5.013 min Scan# 1018
Delta R.T. 0.009 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15


Tgt Ion: 73 Resp: 14031
Ion Ratio Lower Upper
73 100
57 25.4 17.4 26.0

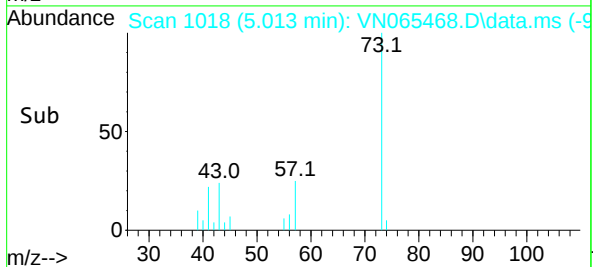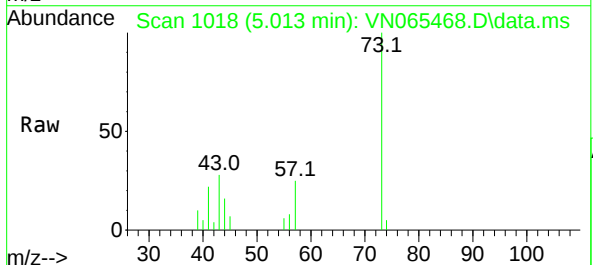



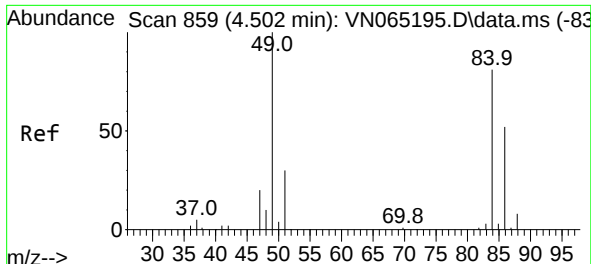


#20
Methylene Chloride
Concen: 9.36 ug/l
RT: 4.508 min Scan# 861
Delta R.T. 0.006 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion:	84	Resp:	22741
Ion	Ratio	Lower	Upper
84	100		
49	118.0	93.4	140.0
51	35.4	28.2	42.4
86	62.2	51.7	77.5

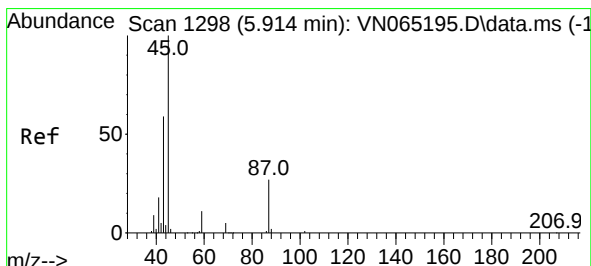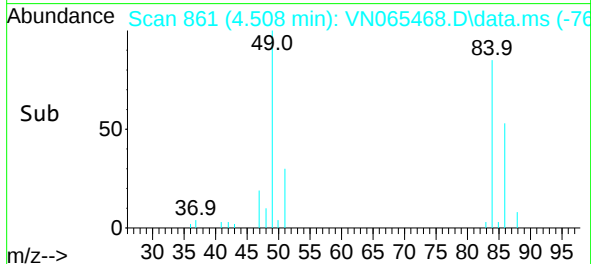


#22
Diisopropyl ether
Concen: 2.40 ug/l
RT: 5.920 min Scan# 1300
Delta R.T. 0.006 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15

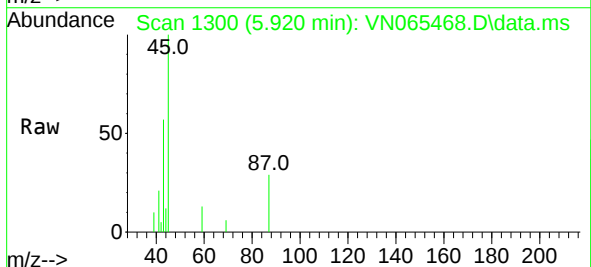

Tgt Ion:	45	Resp:	17088
Ion	Ratio	Lower	Upper
45	100		
43	56.6	46.2	69.2
87	28.8	24.1	36.1
59	13.4	9.0	13.4



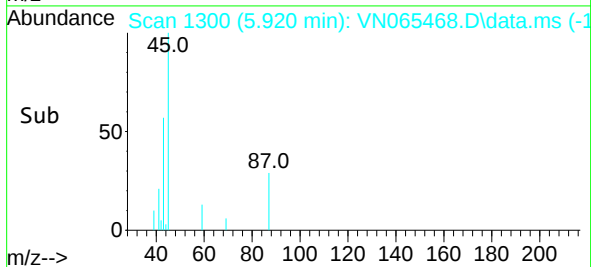
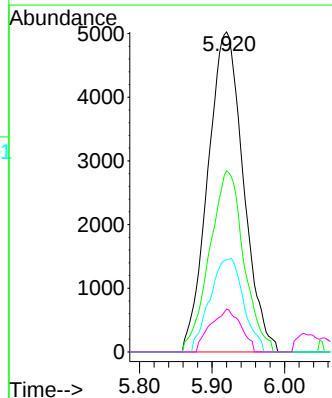




#23
 Vinyl Acetate
 Concen: 1.56 ug/l
 RT: 5.920 min Scan# 1300
 Delta R.T. 0.068 min
 Lab File: VN065468.D
 Acq: 11 Jan 2021 15:15




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion: 43 Resp: 9323
 Ion Ratio Lower Upper
 43 100
 86 0.0 8.9 13.3#

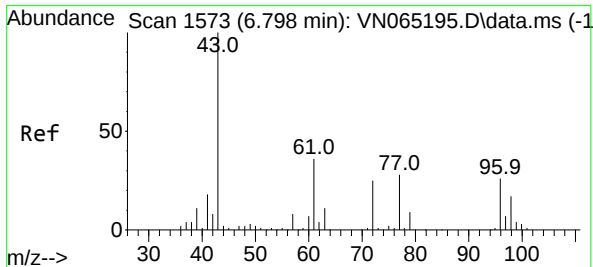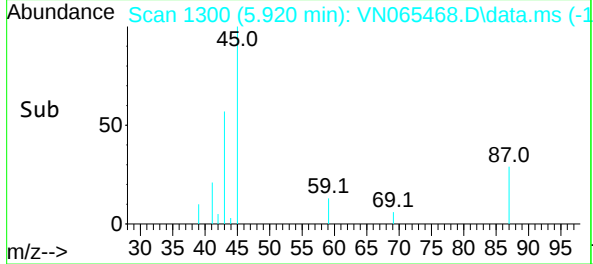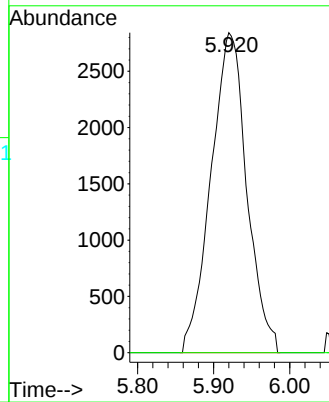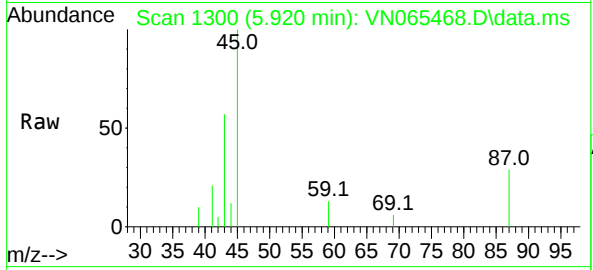

#25
 2-Butanone
 Concen: 6.09 ug/l
 RT: 6.811 min Scan# 1577
 Delta R.T. 0.013 min
 Lab File: VN065468.D
 Acq: 11 Jan 2021 15:15

Tgt Ion: 43 Resp: 8510
 Ion Ratio Lower Upper
 43 100
 72 30.8 21.0 31.6

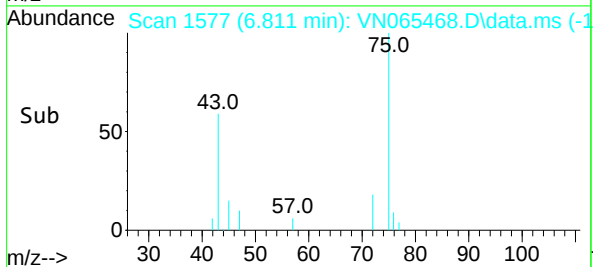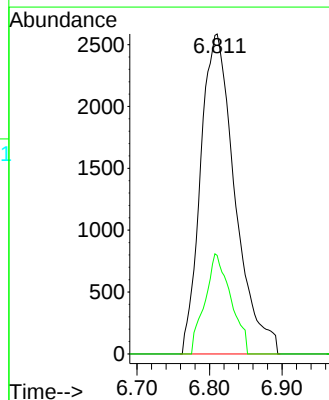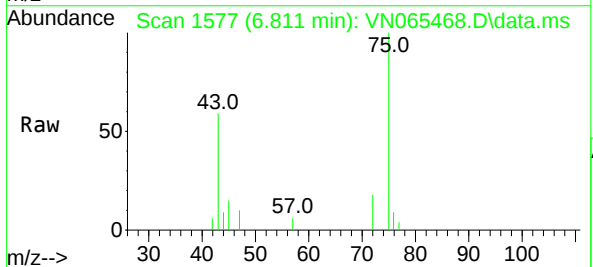

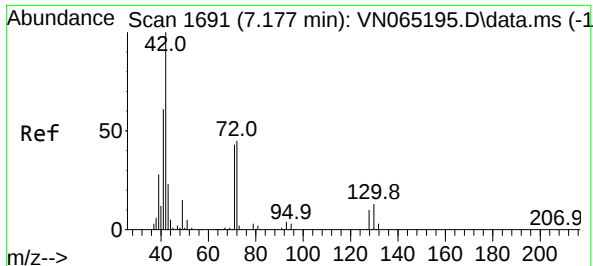

#29

Tetrahydrofuran

Concen: 0.84 ug/l

RT: 7.190 min Scan# 1695





Delta R.T. 0.013 min

Lab File: VN065468.D

Acq: 11 Jan 2021 15:15

Instrument :
MSVOA_N
ClientSampled :

Tgt Ion: 42	Resp:	760
Ion Ratio	Lower	Upper
42	100	
72	0.0	36.6 54.8#
71	0.0	33.6 50.4#

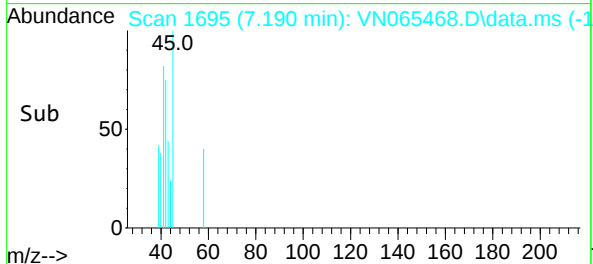

#31

Cyclohexane

Concen: 1.80 ug/l




RT: 7.621 min Scan# 1829


Delta R.T. 0.010 min

Lab File: VN065468.D

Acq: 11 Jan 2021 15:15

Tgt Ion: 56	Resp:	6606
Ion Ratio	Lower	Upper
56	100	
69	105.1	27.5 41.3#
84	119.1	73.9 110.9#


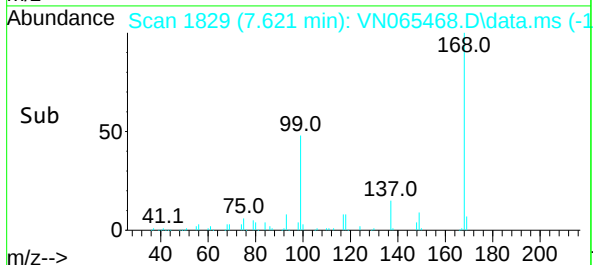

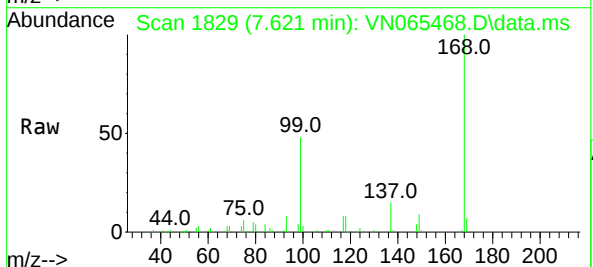


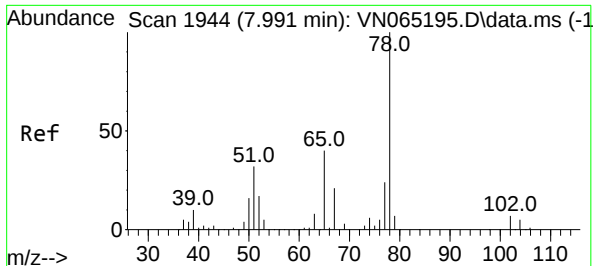

#33
1,2-Dichloroethane-d4
Concen: 48.49 ug/l
RT: 7.991 min Scan# 1944
Delta R.T. -0.000 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 65 Resp: 120779
Ion Ratio Lower Upper
65 100
67 52.8 0.0 108.2

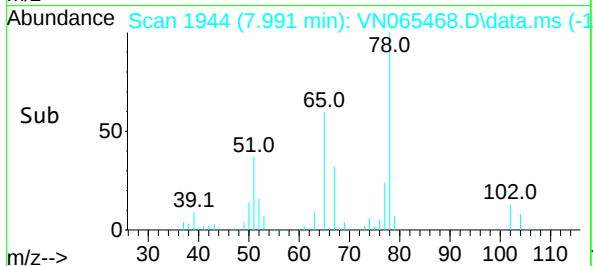

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.553 min Scan# 2119
Delta R.T. 0.003 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15


Tgt Ion: 114 Resp: 362329
Ion Ratio Lower Upper
114 100
63 18.8 0.0 38.6
88 15.4 0.0 32.6

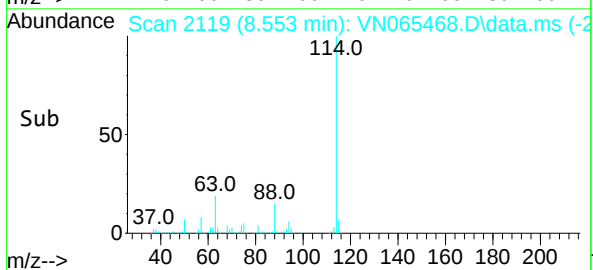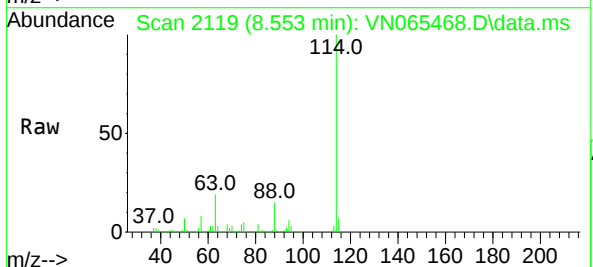



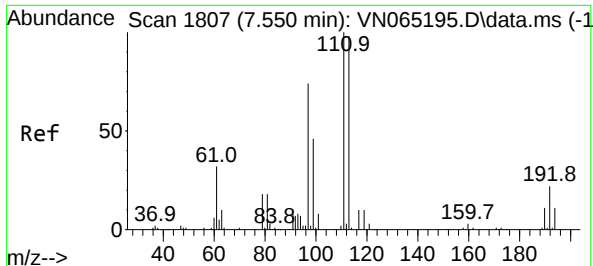


#35
Dibromofluoromethane
Concen: 50.49 ug/l
RT: 7.553 min Scan# 1808
Delta R.T. 0.003 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15


Instrument :
MSVOA_N
ClientSampled :

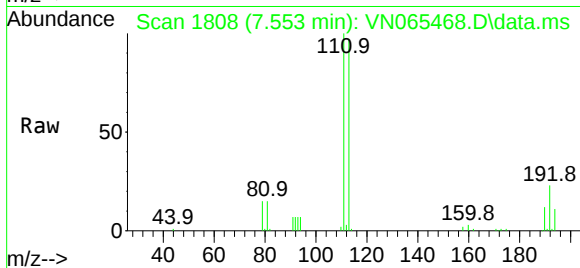



Tgt Ion:113 Resp: 110376
Ion Ratio Lower Upper
113 100
111 102.4 81.6 122.4
192 23.7 16.2 24.2

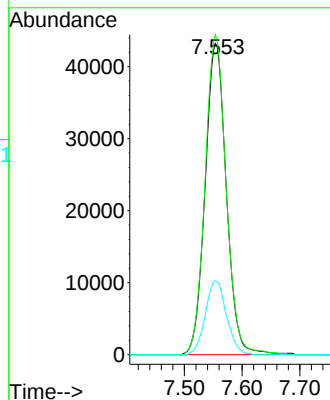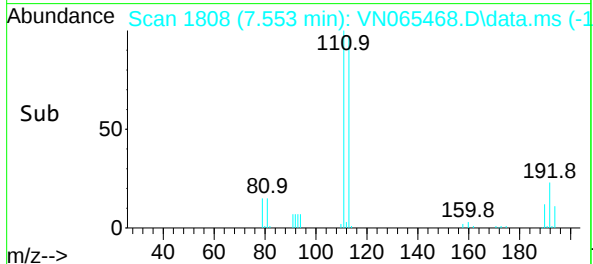


#36
1,1-Dichloropropene
Concen: 4.05 ug/l
RT: 7.627 min Scan# 1831
Delta R.T. -0.126 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15

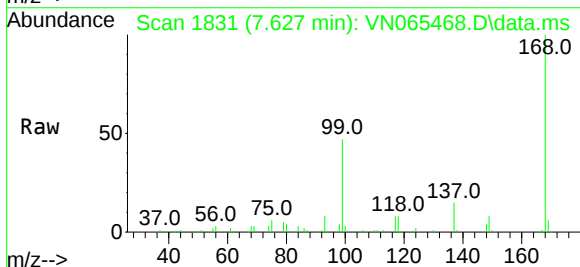

Tgt Ion: 75 Resp: 13352
Ion Ratio Lower Upper
75 100
110 9.3 17.8 53.3#
77 0.0 25.0 37.4#

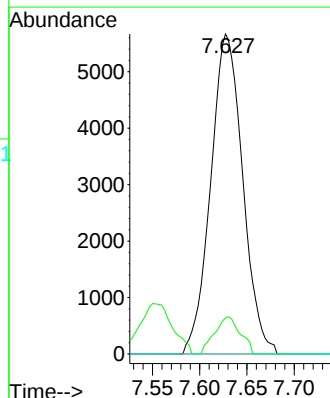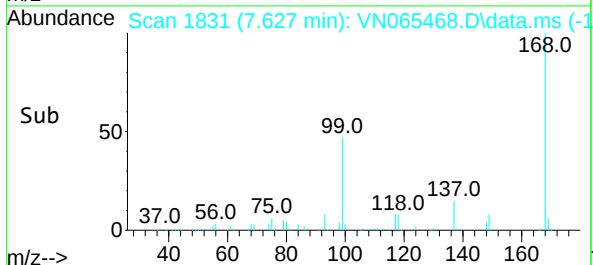

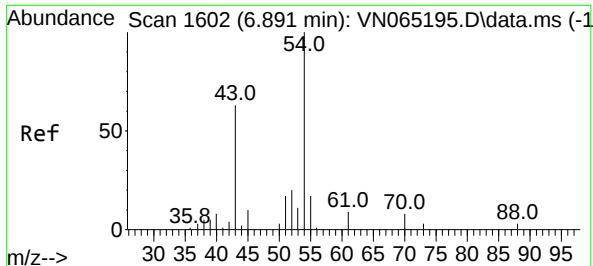

#37

Ethyl Acetate

Concen: 2.61 ug/l

RT: 6.811 min Scan# 1577





Delta R.T. -0.080 min

Lab File: VN065468.D

Acq: 11 Jan 2021 15:15

Tgt Ion:	43	Resp:	8510
Ion	Ratio	Lower	Upper
43	100		
61	0.0	12.8	19.2#
70	0.0	8.8	13.2#

Instrument :
MSVOA_N
ClientSampleId :

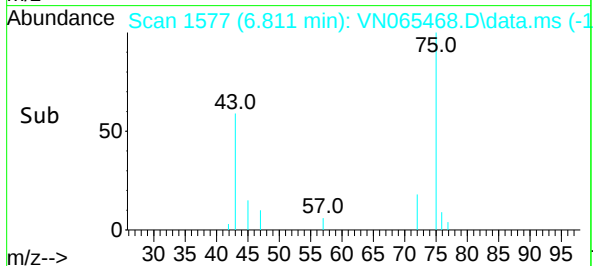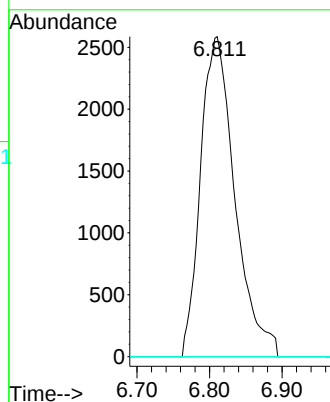

#38

Carbon Tetrachloride

Concen: 5.28 ug/l




RT: 7.630 min Scan# 1832


Delta R.T. -0.103 min

Lab File: VN065468.D

Acq: 11 Jan 2021 15:15

Tgt Ion:	117	Resp:	18264
Ion	Ratio	Lower	Upper
117	100		
119	4.3	76.7	115.1#
121	0.0	25.4	38.2#



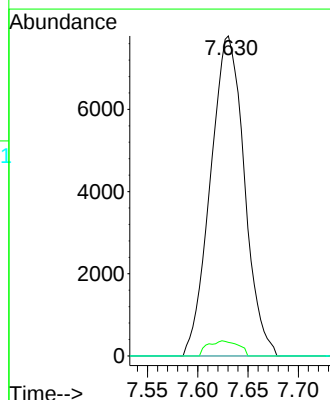
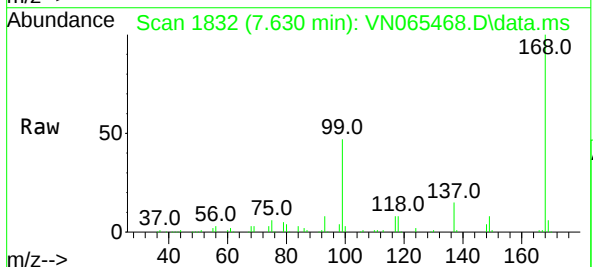




#39
Methylcyclohexane
Concen: 0.21 ug/l
RT: 9.045 min Scan# 2272
Delta R.T. 0.000 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 83 Resp: 849
Ion Ratio Lower Upper
83 100
55 63.3 60.2 90.2
98 58.7 37.4 56.2#

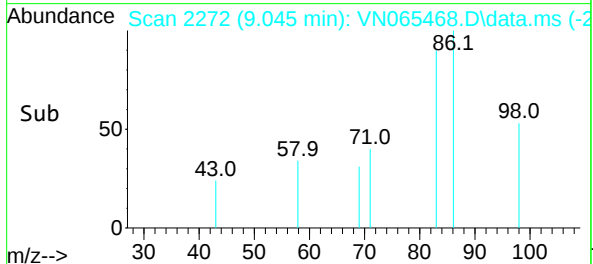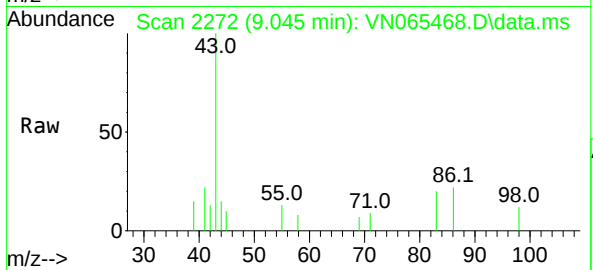

#40
Benzene
Concen: 31.53 ug/l
RT: 8.003 min Scan# 1948
Delta R.T. -0.001 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15


Tgt Ion: 78 Resp: 308977
Ion Ratio Lower Upper
78 100
77 23.7 17.9 26.9

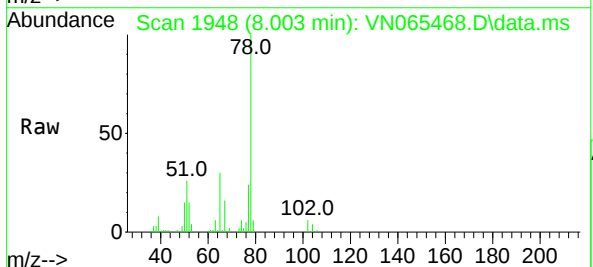



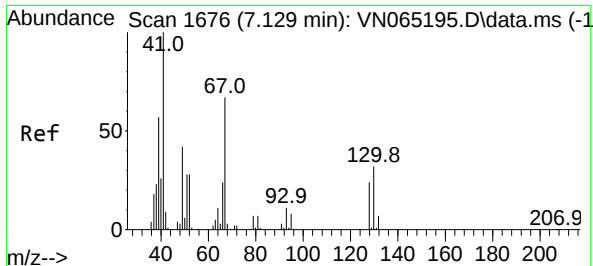


#41
Methacrylonitrile
Concen: 0.60 ug/l
RT: 7.184 min Scan# 1693
Delta R.T. 0.055 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15


Instrument :
MSVOA_N
ClientSampled :

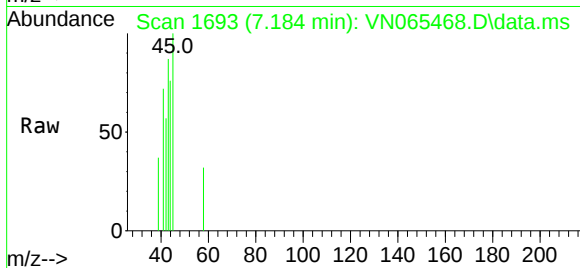



Tgt Ion: 41	Resp: 1024
Ion Ratio	Lower Upper
41	100
39	30.6 51.0 76.6#
67	0.0 79.8 119.8#
52	0.0 31.5 47.3#

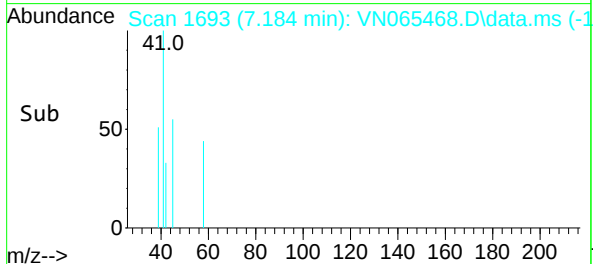


#42
1,2-Dichloroethane
Concen: 0.69 ug/l
RT: 8.003 min Scan# 1948
Delta R.T. -0.084 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15

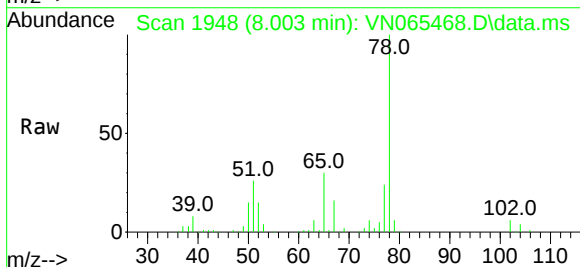

Tgt Ion: 62	Resp: 2511
Ion Ratio	Lower Upper
62	100
98	0.0 0.0 19.6



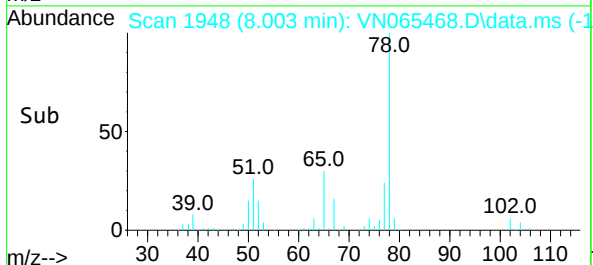



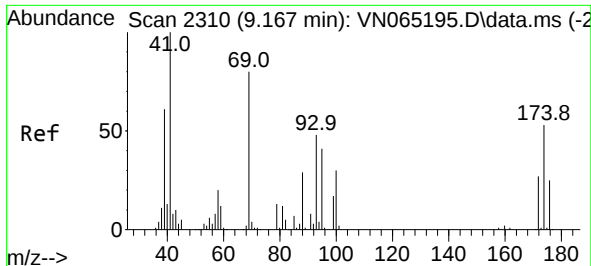

#48
Methyl methacrylate
Concen: 3.02 ug/l
RT: 9.013 min Scan# 2262
Delta R.T. -0.154 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 41 Resp: 8248
Ion Ratio Lower Upper
41 100
69 2.2 71.8 107.8#
39 60.8 44.1 66.1

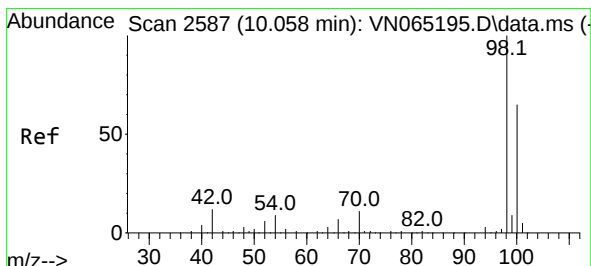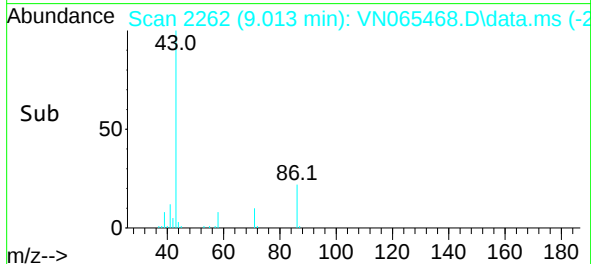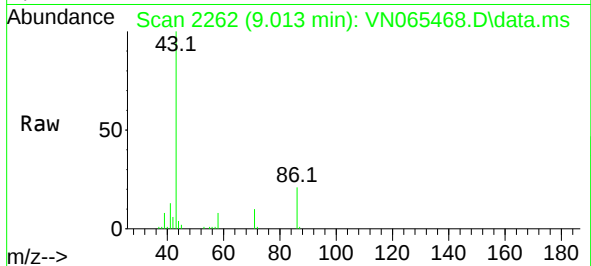

#50
Toluene-d8
Concen: 54.78 ug/l
RT: 10.061 min Scan# 2588
Delta R.T. 0.003 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15

Tgt Ion: 98 Resp: 448836
Ion Ratio Lower Upper
98 100
100 64.5 51.7 77.5




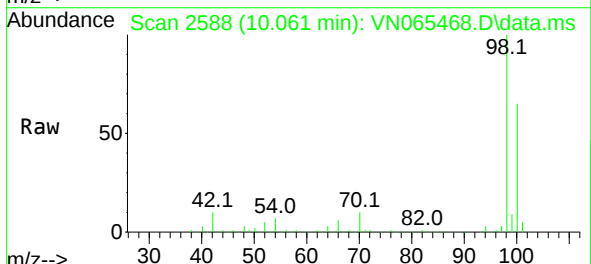


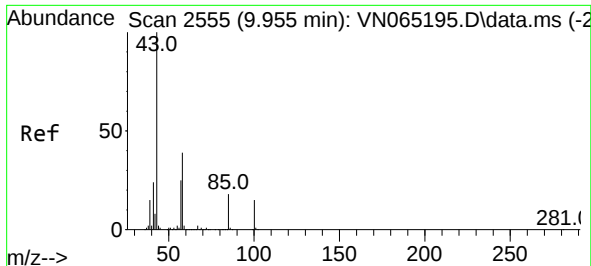

#51
4-Methyl-2-Pentanone
Concen: 0.53 ug/l
RT: 9.958 min Scan# 2556
Delta R.T. 0.003 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 1671
Ion Ratio Lower Upper
43 100
58 26.3 32.4 48.6#

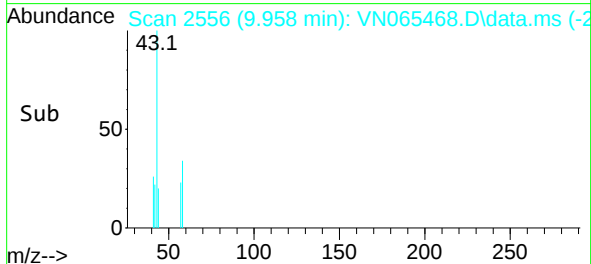

#52
Toluene
Concen: 92.08 ug/l
RT: 10.126 min Scan# 2608
Delta R.T. -0.000 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15


Tgt Ion: 92 Resp: 568816
Ion Ratio Lower Upper
92 100
91 171.7 139.1 208.7

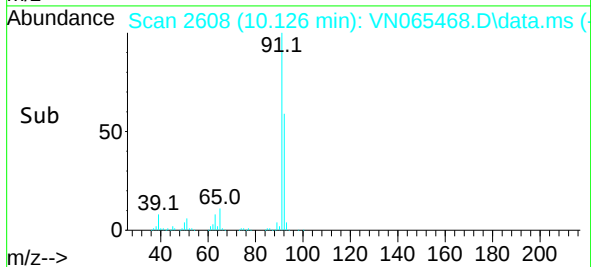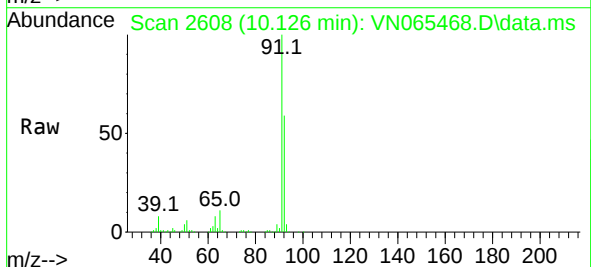



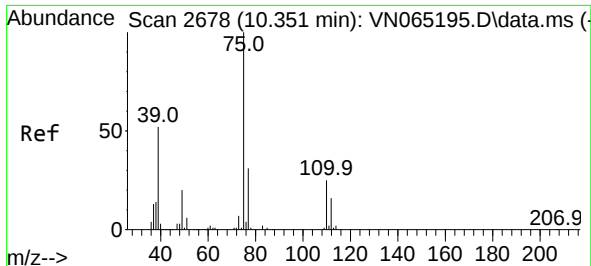


#53
t-1,3-Dichloropropene
Concen: 1.46 ug/l
RT: 10.126 min Scan# 2608
Delta R.T. -0.225 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15

Instrument :
MSVOA_N
ClientSampled :



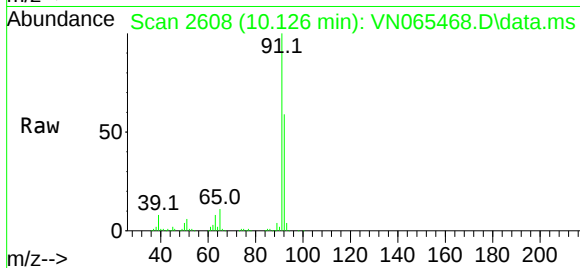



Tgt Ion: 75 Resp: 6022
Ion Ratio Lower Upper
75 100
77 181.3 25.8 38.6#

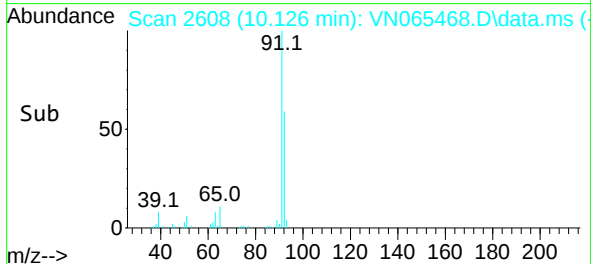

#59
2-Hexanone
Concen: 11.22 ug/l
RT: 10.823 min Scan# 2825
Delta R.T. 0.099 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15

Tgt Ion: 43 Resp: 26091
Ion Ratio Lower Upper
43 100
58 4.9 28.3 84.9#


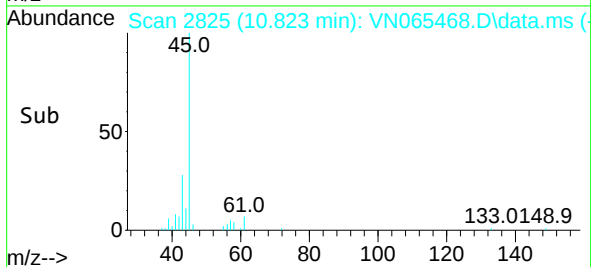

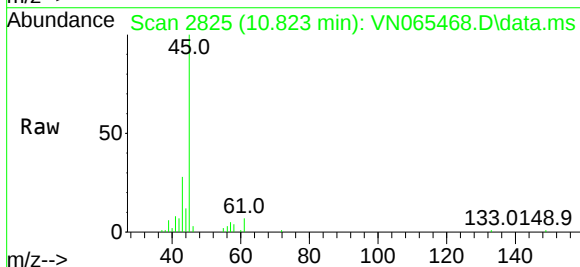


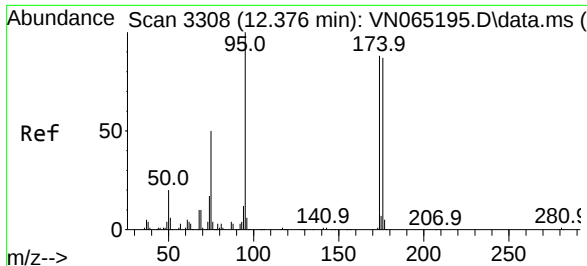

#62
4-Bromofluorobenzene
Concen: 55.32 ug/l
RT: 12.376 min Scan# 3308
Delta R.T. 0.000 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 181196
Ion Ratio Lower Upper
95 100
174 95.5 0.0 160.4
176 93.5 0.0 158.4

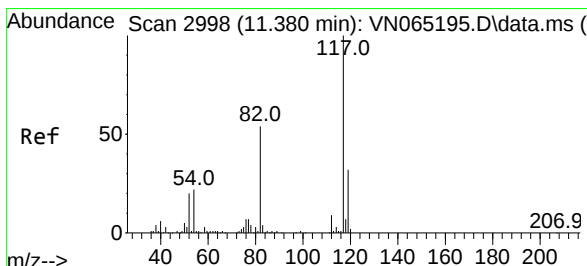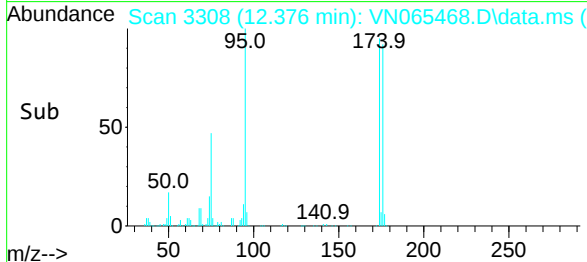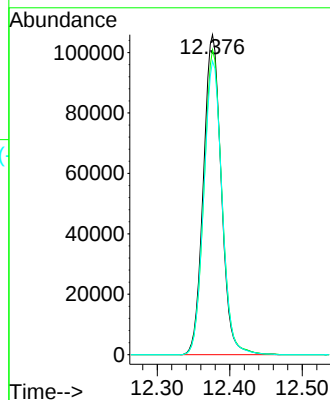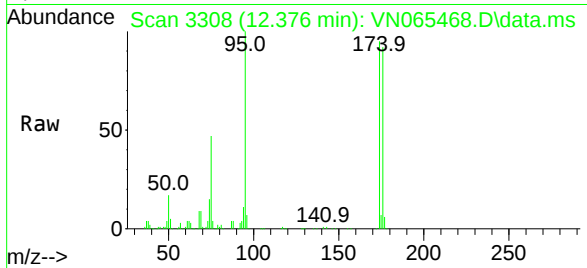

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.380 min Scan# 2998
Delta R.T. -0.001 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15

Tgt Ion: 117 Resp: 390695
Ion Ratio Lower Upper
117 100
82 52.3 44.2 66.2
119 32.4 25.8 38.6


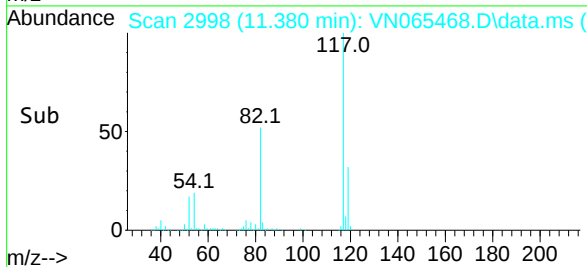
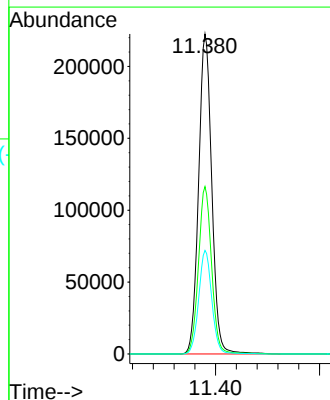
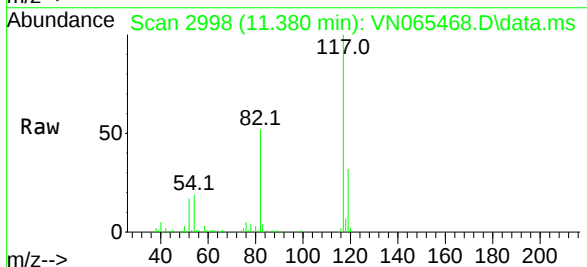




#67
Ethyl Benzene
Concen: 0.90 ug/l
RT: 11.482 min Scan# 3030
Delta R.T. 0.000 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 12852
Ion Ratio Lower Upper
91 100
106 31.1 25.2 37.8

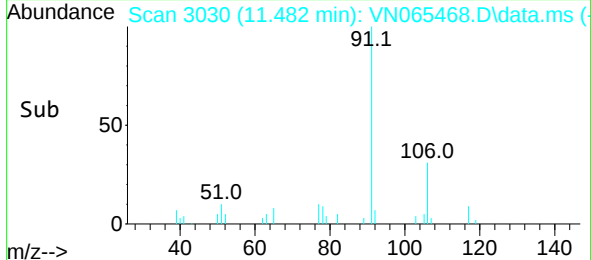

#68
m/p-Xylenes
Concen: 2.31 ug/l
RT: 11.592 min Scan# 3064
Delta R.T. -0.000 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15

Tgt Ion:106 Resp: 12487
Ion Ratio Lower Upper
106 100
91 198.0 161.0 241.4


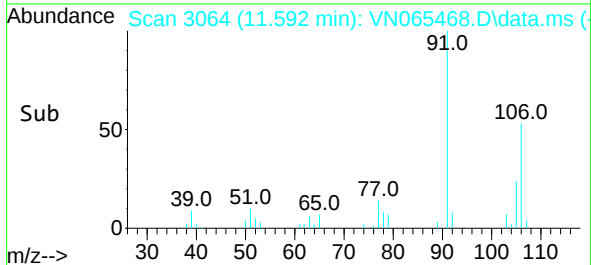

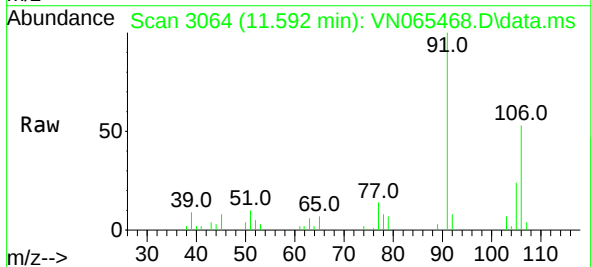


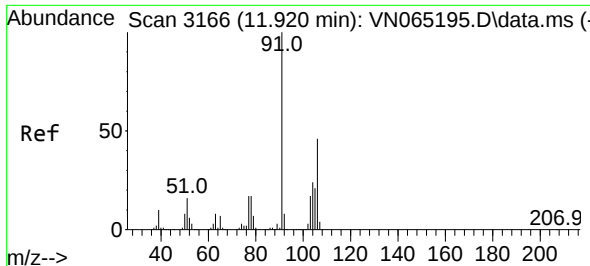

#69
o-Xylene
Concen: 8.69 ug/l
RT: 11.920 min Scan# 3166
Delta R.T. -0.000 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:106 Resp: 45560
Ion Ratio Lower Upper
106 100
91 211.4 105.5 316.5

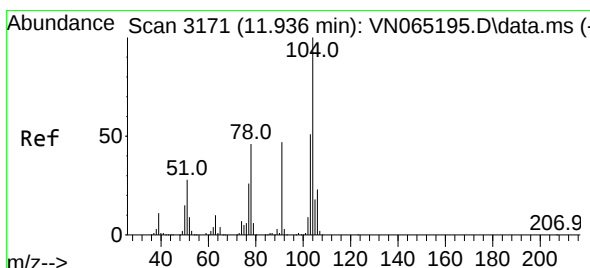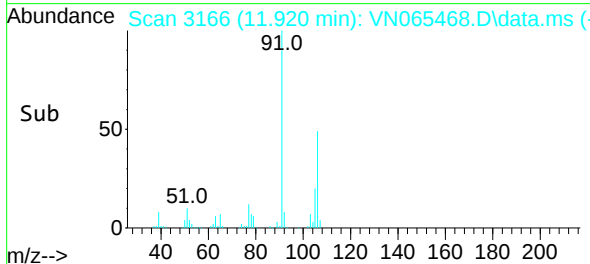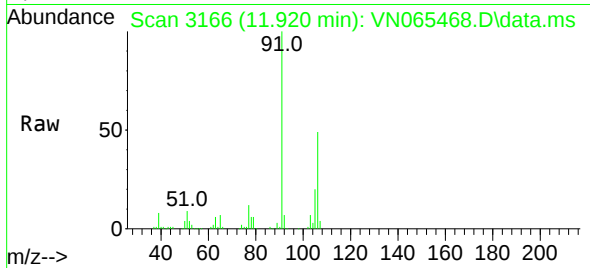

#70
Styrene
Concen: 0.26 ug/l
RT: 11.920 min Scan# 3166
Delta R.T. -0.016 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15

Tgt Ion:104 Resp: 2239
Ion Ratio Lower Upper
104 100
78 282.9 39.0 58.6#
103 281.5 44.3 66.5#


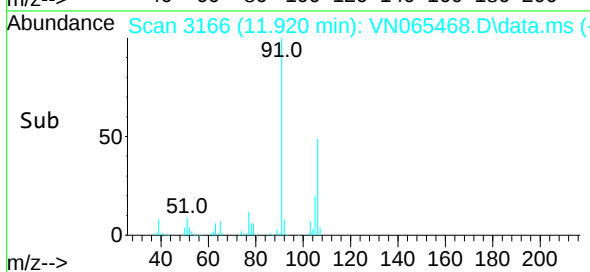

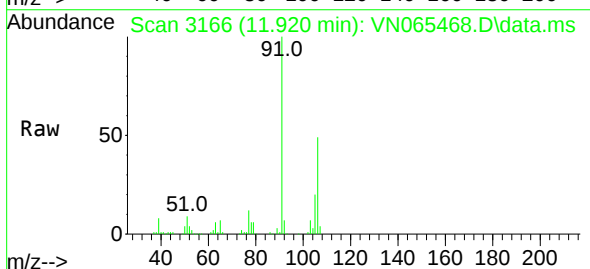


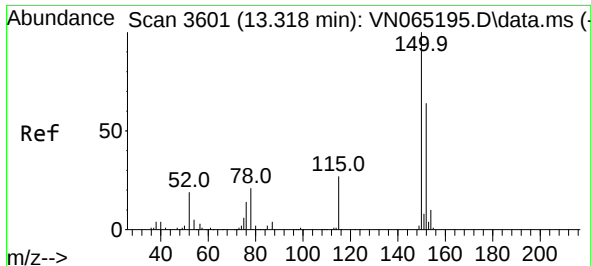

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.318 min Scan# 3601
Delta R.T. 0.000 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:152 Resp: 172270
Ion Ratio Lower Upper
152 100
115 55.2 29.7 89.1
150 156.3 0.0 350.6

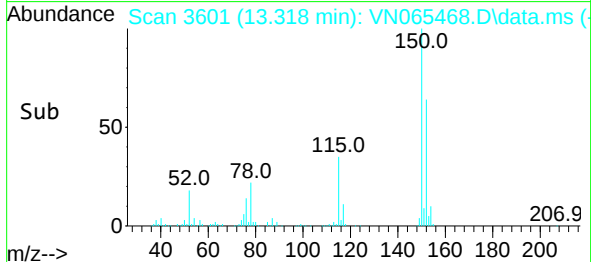

#74
N-ethyl acetate
Concen: 3.57 ug/l
RT: 11.794 min Scan# 3127
Delta R.T. -0.248 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15

Tgt Ion: 43 Resp: 18626
Ion Ratio Lower Upper
43 100
70 5.7 34.5 51.7#
55 108.5 20.4 30.6#
61 0.0 20.0 30.0#


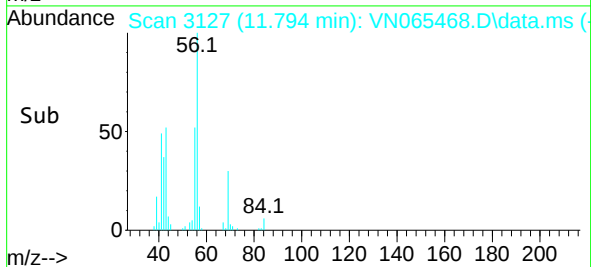

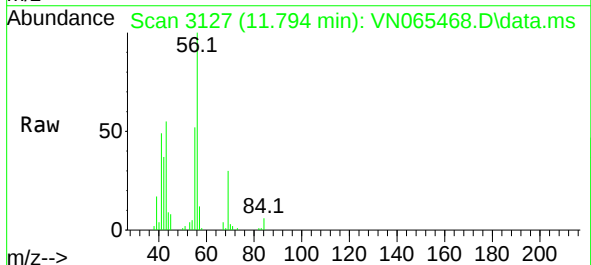


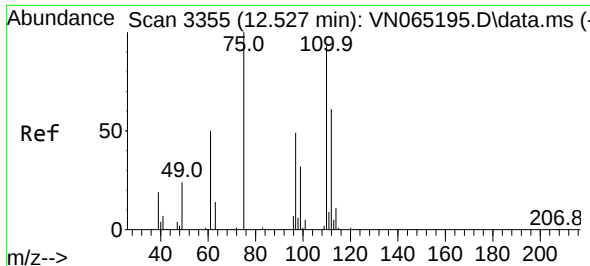

#76
1,2,3-Trichloropropane
Concen: 24.79 ug/l
RT: 12.376 min Scan# 3308
Delta R.T. -0.151 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 87123
Ion Ratio Lower Upper
75 100
77 1.0 0.0 0.0#

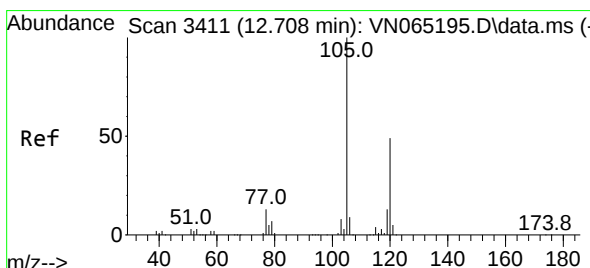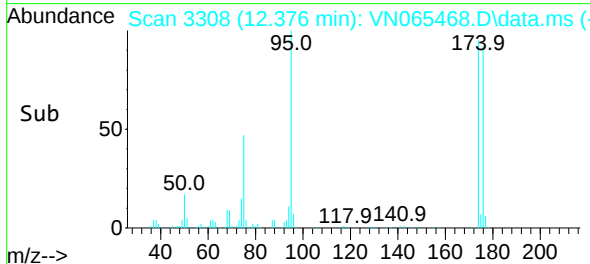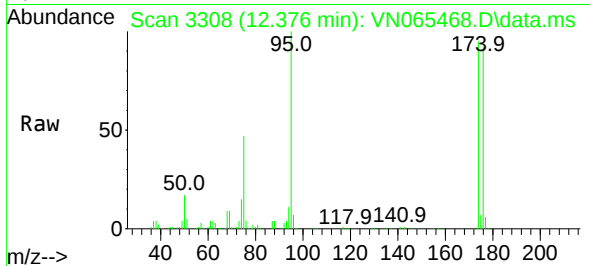

#80
1,3,5-Trimethylbenzene
Concen: 1.51 ug/l
RT: 12.707 min Scan# 3411
Delta R.T. -0.001 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15


Tgt Ion: 105 Resp: 16864
Ion Ratio Lower Upper
105 100
120 50.8 24.6 73.6

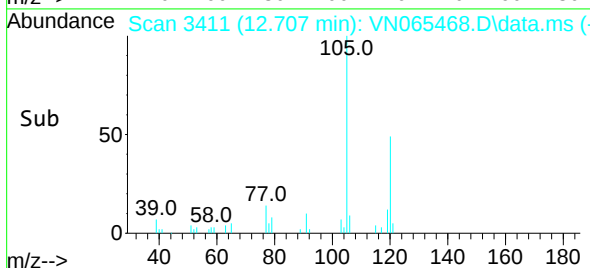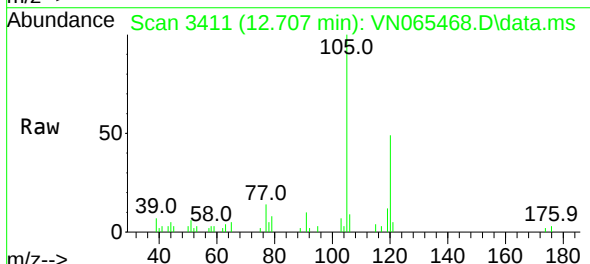



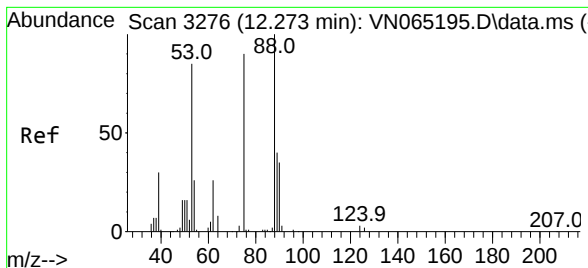


#81
trans-1,4-Dichloro-2-butene
Concen: 62.51 ug/l
RT: 12.376 min Scan# 3308
Delta R.T. 0.103 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15

Instrument :
MSVOA_N
ClientSampleId :



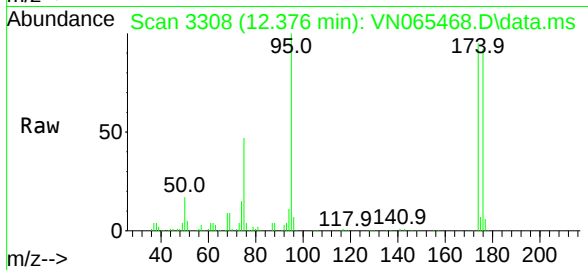



Tgt Ion: 75 Resp: 87123
Ion Ratio Lower Upper
75 100
53 0.0 67.0 100.4#
89 0.0 39.6 59.4#

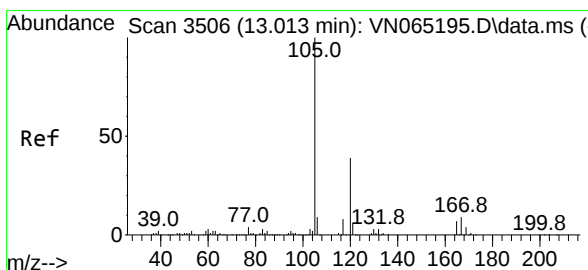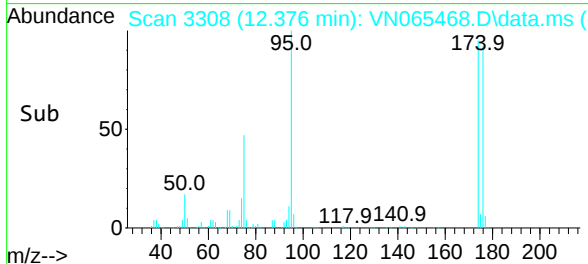

#84
1,2,4-Trimethylbenzene
Concen: 0.29 ug/l
RT: 13.013 min Scan# 3506
Delta R.T. -0.000 min
Lab File: VN065468.D
Acq: 11 Jan 2021 15:15

Tgt Ion: 105 Resp: 3124
Ion Ratio Lower Upper
105 100
120 42.7 23.1 69.2


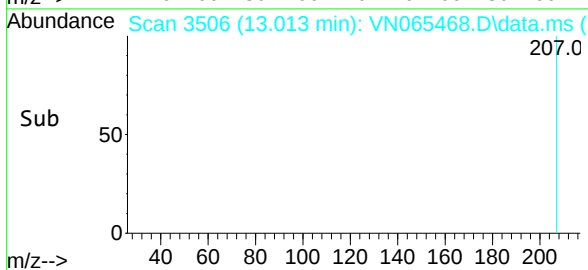

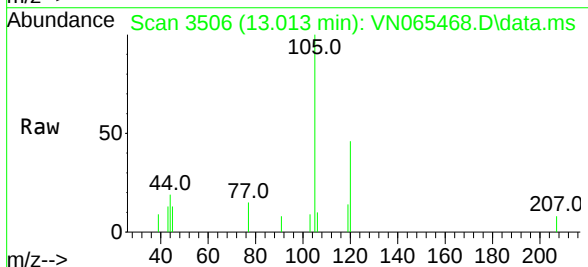


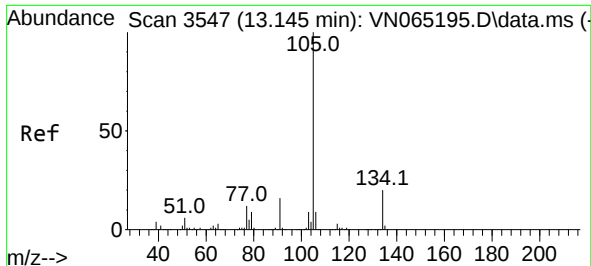

#85
 sec-Butylbenzene
 Concen: 0.25 ug/l
 RT: 13.013 min Scan# 3506
 Delta R.T. -0.132 min
 Lab File: VN065468.D
 Acq: 11 Jan 2021 15:15

Instrument :
 MSVOA_N
 ClientSampled :

Tgt Ion:105 Resp: 3124
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.1 30.1#

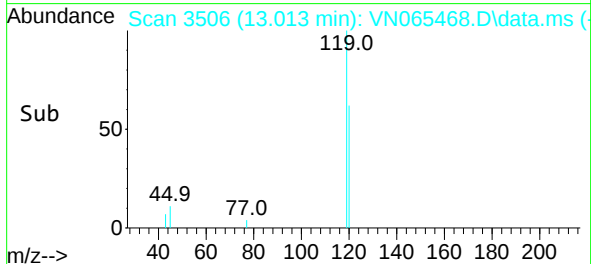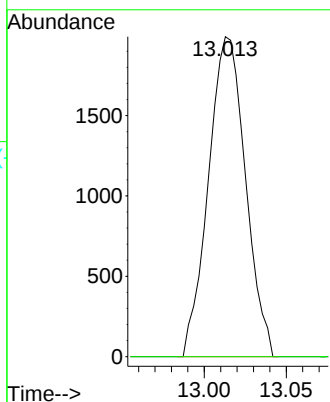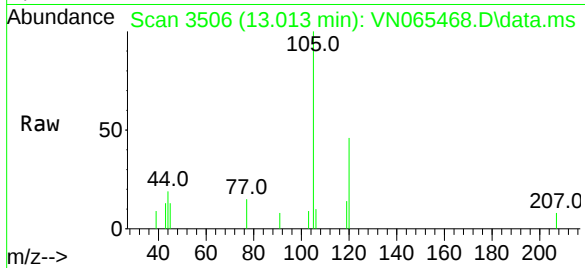

#95
 Naphthalene
 Concen: 3.41 ug/l
 RT: 15.109 min Scan# 4158
 Delta R.T. 0.013 min
 Lab File: VN065468.D
 Acq: 11 Jan 2021 15:15

Tgt Ion:128 Resp: 394
 Ion Ratio Lower Upper
 128 100
 127 0.0 10.3 15.5#
 129 0.0 8.7 13.1#

