
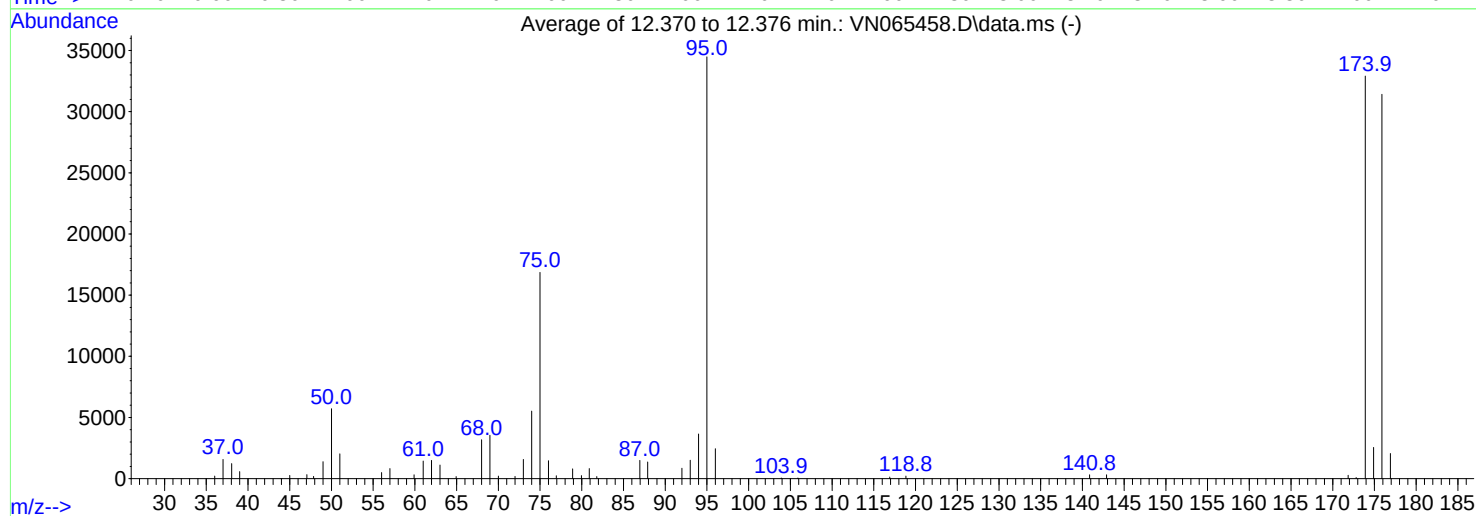


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011121\
 Data File : VN065458.D
 Acq On : 11 Jan 2021 10:04
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
 Title : SW846 8260
 Last Update : Tue Dec 22 15:42:18 2020

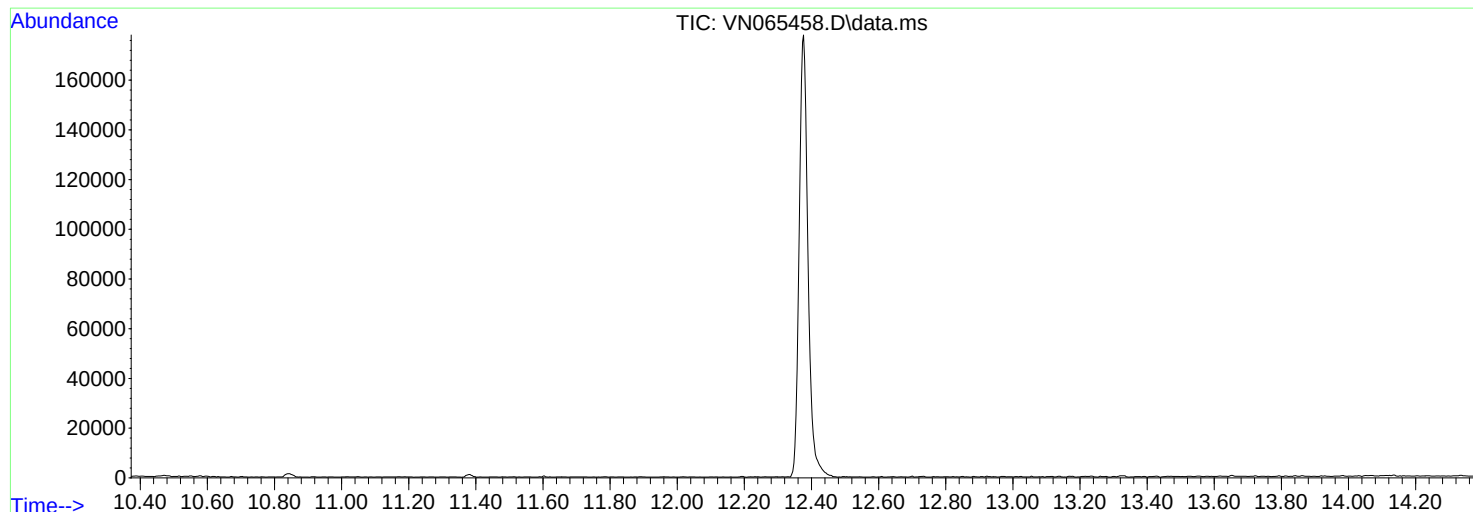

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	5711	PASS
75	95	30	60	48.9	16860	PASS
95	95	100	100	100.0	34480	PASS
96	95	5	9	7.1	2447	PASS
173	174	0.00	2	0.3	89	PASS
174	95	50	100	95.4	32909	PASS
175	174	5	9	7.8	2554	PASS
176	174	95	101	95.5	31419	PASS
177	176	5	9	6.5	2057	PASS