

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011122\
 Data File : VN070571.D
 Acq On : 11 Jan 2022 16:08
 Operator : JC/MD
 Sample : N1066-01ME
 Misc : 10.76g/5mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jan 12 06:01:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 27 18:47:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.077	168	877803	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.960	114	1463299	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	1392751	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.672	152	643484	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.431	65	665388	52.720	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 105.440%			
35) Dibromofluoromethane	8.016	113	458085	51.739	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 103.480%			
50) Toluene-d8	10.438	98	2032765	56.203	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 112.400%			
62) 4-Bromofluorobenzene	12.728	95	865091	66.223	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 132.440%			
Target Compounds						Qvalue
11) Tert butyl alcohol	5.304	59	23486	11.176	ug/l #	72
13) Acrolein	4.030	56	1359	0.797	ug/l #	26
16) Acetone	4.293	43	12070	1.473	ug/l	98
18) Methyl Acetate	4.843	43	16817	0.710	ug/l #	71
25) 2-Butanone	7.340	43	13752	1.333	ug/l	95
31) Cyclohexane	8.077	56	22068	1.108	ug/l #	1
36) 1,1-Dichloropropene	8.077	75	71367	4.873	ug/l #	47
37) Ethyl Acetate	7.340	43	13752	0.724	ug/l #	71
38) Carbon Tetrachloride	8.077	117	85691	6.127	ug/l #	16
39) Methylcyclohexane	9.453	83	45054	2.541	ug/l #	87
48) Methyl methacrylate	9.502	41	4228	0.296	ug/l #	27
55) 1,1,2-Trichloroethane	10.872	97	50064	4.655	ug/l #	21
56) Ethyl methacrylate	10.733	69	11945	0.672	ug/l #	87
58) 2-Chloroethyl Vinyl ether	10.038	63	5934	19.724	ug/l	95
59) 2-Hexanone	11.049	43	111329	8.117	ug/l #	30
73) Isopropylbenzene	12.575	105	292049	4.887	ug/l	98
74) N-amyl acetate	12.363	43	210902	8.394	ug/l #	44
75) 1,1,2,2-Tetrachloroethane	12.806	83	22869	1.493	ug/l #	90
76) 1,2,3-Trichloropropane	12.728	75	443526	24.743	ug/l #	1
78) n-propylbenzene	12.916	91	634705	9.586	ug/l	95
79) 2-Chlorotoluene	12.916	91	634705	14.941	ug/l #	38
81) trans-1,4-Dichloro-2-b...	12.728	75	443526	84.211	ug/l #	6
82) 4-Chlorotoluene	12.916	91	634942	15.956	ug/l #	38
83) tert-Butylbenzene	13.321	119	71120	1.687	ug/l	92
84) 1,2,4-Trimethylbenzene	13.498	105	874634	18.968	ug/l #	31
85) sec-Butylbenzene	13.498	105	874634	15.278	ug/l	88
86) p-Isopropyltoluene	13.769	119	196511	4.370	ug/l	94
89) n-Butylbenzene	13.940	91	368925	9.836	ug/l	96
90) Hexachloroethane	14.214	117	155828	19.947	ug/l #	6
92) 1,2-Dibromo-3-Chloropr...	14.621	75	4877	1.409	ug/l #	1
93) 1,2,4-Trichlorobenzene	15.262	180	2644	0.249	ug/l #	1
95) Naphthalene	15.461	128	26247	2.660	ug/l #	1
96) 1,2,3-Trichlorobenzene	15.689	180	141	0.840	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_N
ClientSampleId :

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011122\
Data File : VN070571.D
Acq On : 11 Jan 2022 16:08
Operator : JC/MD
Sample : N1066-01ME
Misc : 10.76g/5mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jan 12 06:01:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260
QLast Update : Mon Dec 27 18:47:12 2021
Response via : Initial Calibration




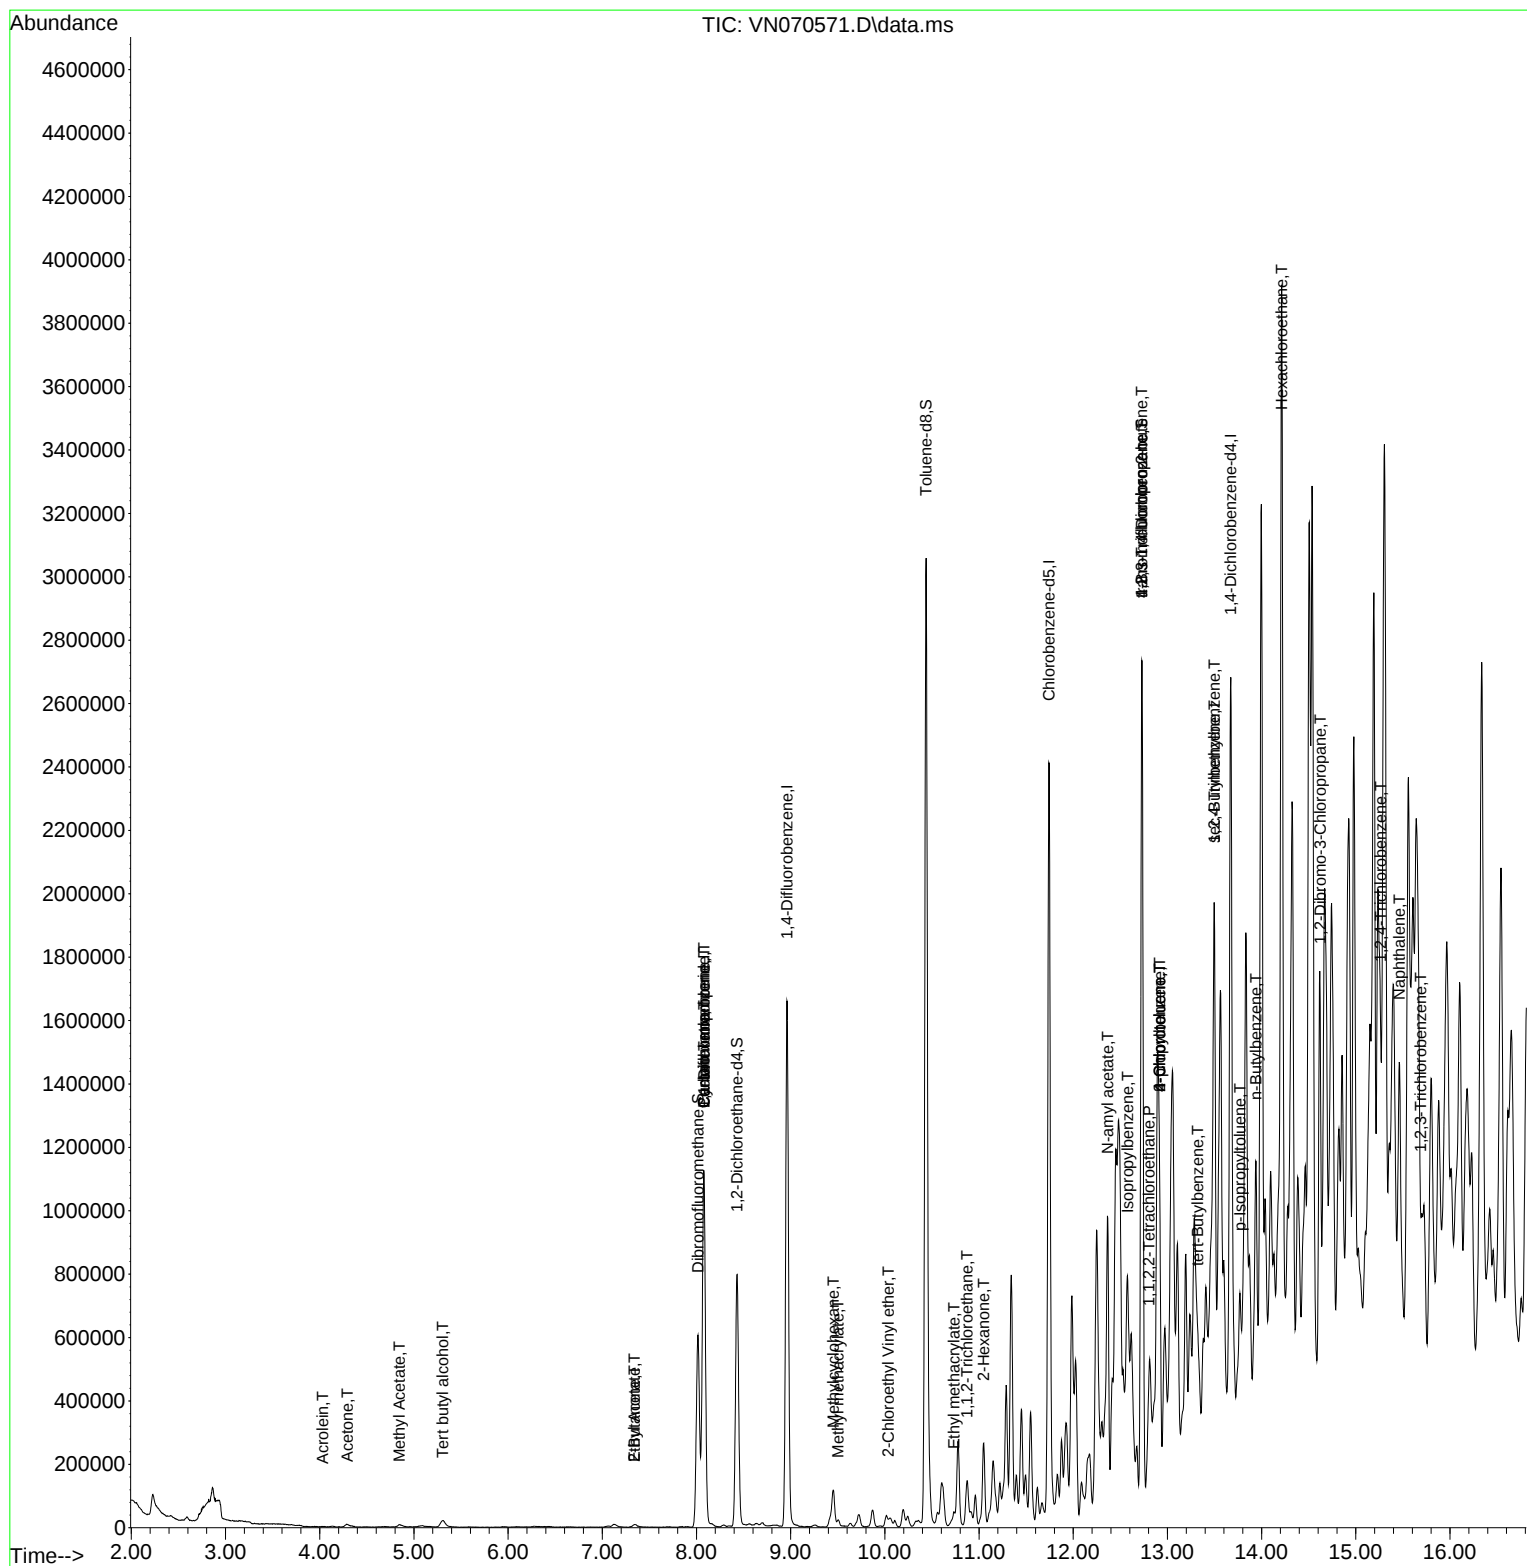


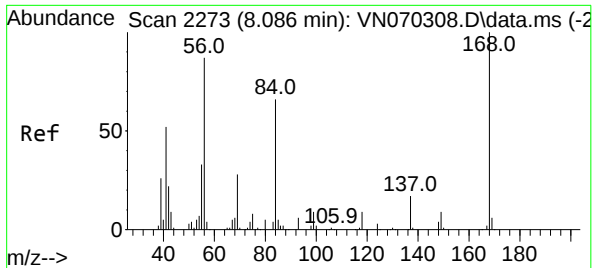

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.077 min Scan# 21
Delta R.T. -0.009 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 877803
Ion Ratio Lower Upper
168 100
99 57.6 41.3 61.9

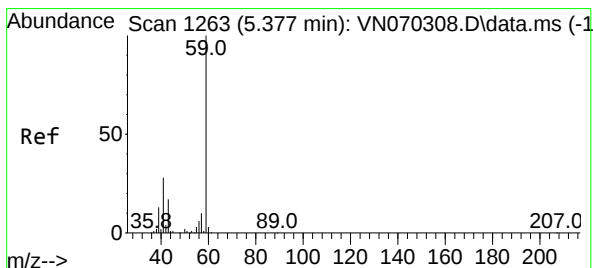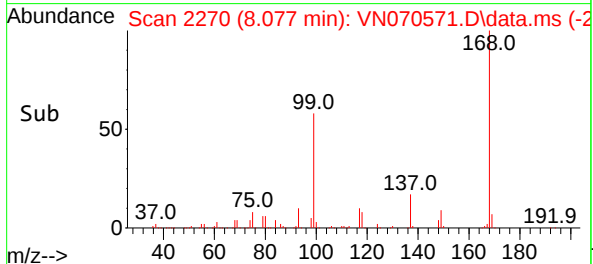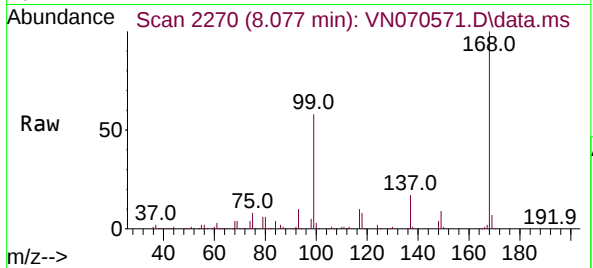

#11
Tert butyl alcohol
Concen: 11.176 ug/l
RT: 5.304 min Scan# 1236
Delta R.T. -0.073 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08

Tgt Ion: 59 Resp: 23486
Ion Ratio Lower Upper
59 100
57 0.4 8.7 13.1#


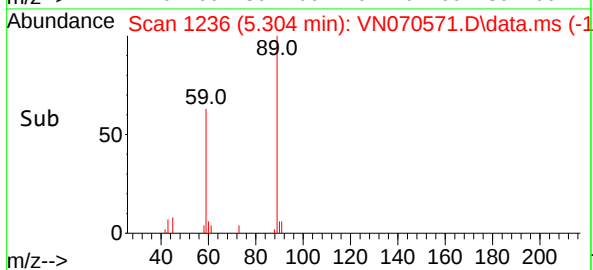

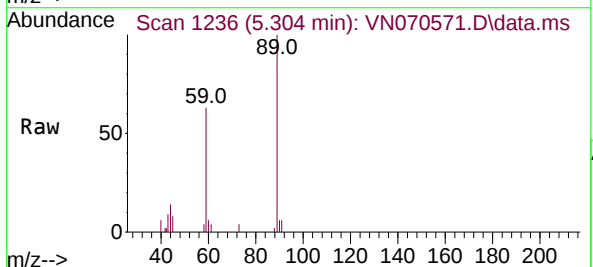




#13
Acrolein
Concen: 0.797 ug/l
RT: 4.030 min Scan# 761
Delta R.T. -0.011 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 56 Resp: 1359
Ion Ratio Lower Upper
56 100
55 9.6 56.6 85.0#

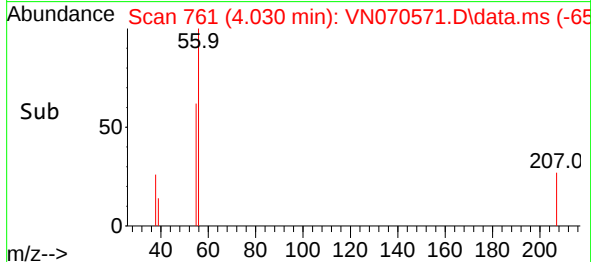

#16
Acetone
Concen: 1.473 ug/l
RT: 4.293 min Scan# 859
Delta R.T. 0.008 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08


Tgt Ion: 43 Resp: 12070
Ion Ratio Lower Upper
43 100
58 28.0 23.1 34.7

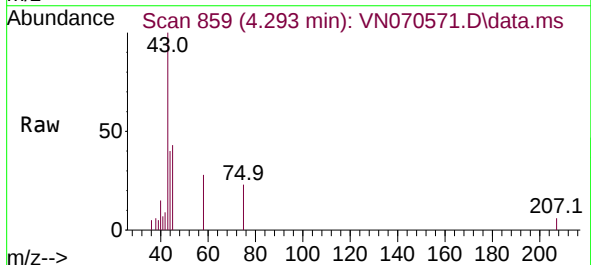






#18
Methyl Acetate
Concen: 0.710 ug/l
RT: 4.843 min Scan# 1064
Delta R.T. -0.011 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 16817
Ion Ratio Lower Upper
43 100
74 9.7 19.4 29.2#

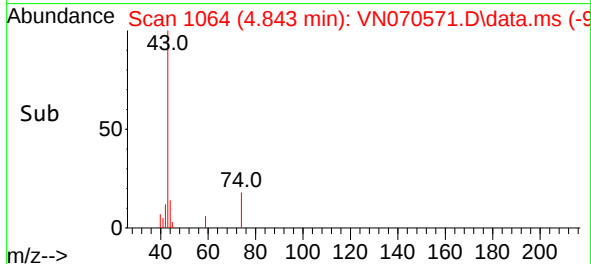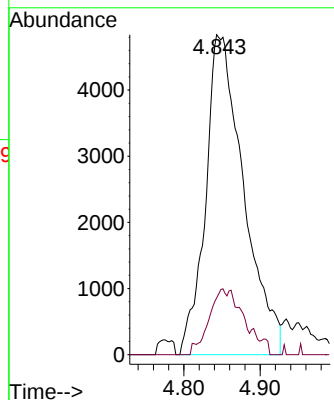

#25
2-Butanone
Concen: 1.333 ug/l
RT: 7.340 min Scan# 1995
Delta R.T. 0.005 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08


Tgt Ion: 43 Resp: 13752
Ion Ratio Lower Upper
43 100
72 24.4 21.7 32.5

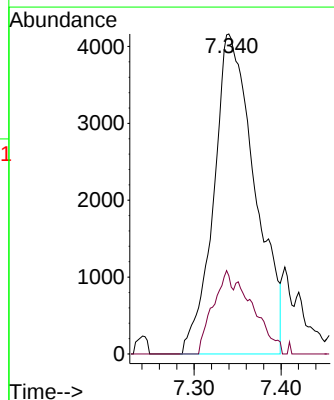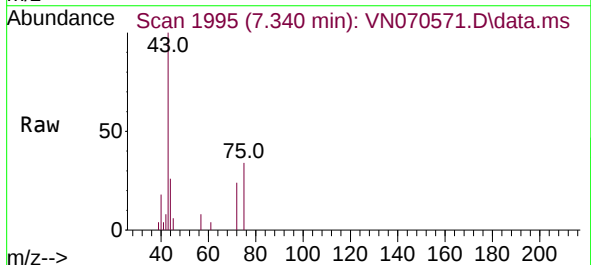






#31
Cyclohexane
Concen: 1.108 ug/l
RT: 8.077 min Scan# 21
Delta R.T. -0.017 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 22068
Ion Ratio Lower Upper
56 100
69 154.2 27.1 40.7#
84 146.4 73.4 110.0#



#33
1,2-Dichloroethane-d4
Concen: 52.720 ug/l
RT: 8.431 min Scan# 2402
Delta R.T. -0.005 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08


Tgt Ion: 65 Resp: 665388
Ion Ratio Lower Upper
65 100
67 53.4 0.0 103.0

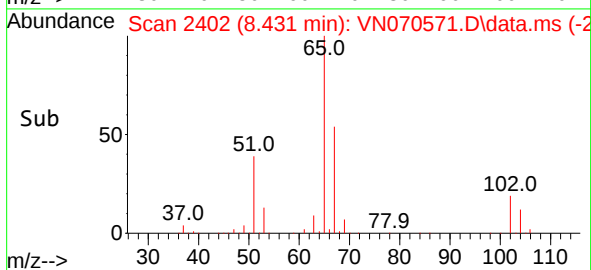






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.960 min Scan# 21
Delta R.T. -0.008 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:114 Resp: 1463299
Ion Ratio Lower Upper
114 100
63 23.3 0.0 37.8
88 16.4 0.0 27.4

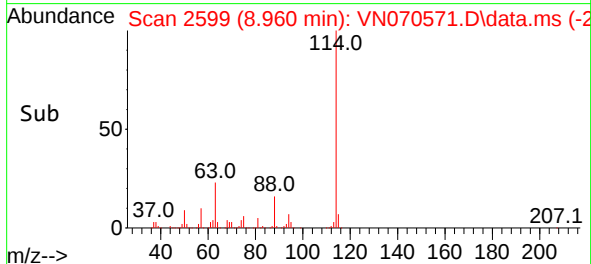

#35
Dibromofluoromethane
Concen: 51.739 ug/l
RT: 8.016 min Scan# 2247
Delta R.T. -0.005 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08


Tgt Ion:113 Resp: 458085
Ion Ratio Lower Upper
113 100
111 102.4 82.2 123.2
192 19.7 16.9 25.3

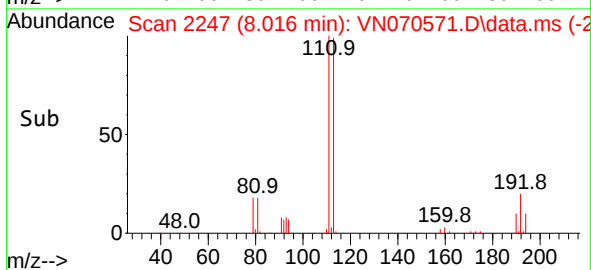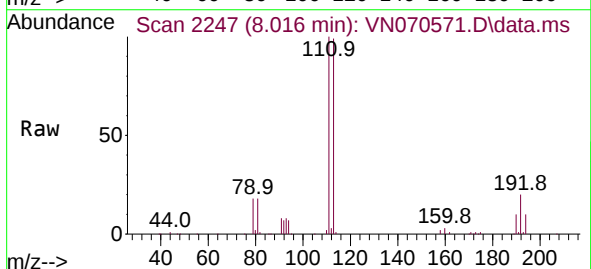






#36
 1,1-Dichloropropene
 Concen: 4.873 ug/l
 RT: 8.077 min Scan# 21
 Delta R.T. -0.143 min
 Lab File: VN070571.D
 Acq: 11 Jan 2022 16:08


Instrument :
 MSVOA_N
 ClientSampleId :





Tgt Ion: 75 Resp: 71367
 Ion Ratio Lower Upper
 75 100
 110 7.2 18.4 55.2#
 77 0.0 24.4 36.6#

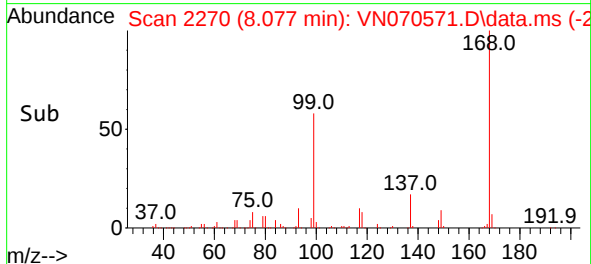


#37
 Ethyl Acetate
 Concen: 0.724 ug/l
 RT: 7.340 min Scan# 1995
 Delta R.T. -0.072 min
 Lab File: VN070571.D
 Acq: 11 Jan 2022 16:08




Tgt Ion: 43 Resp: 13752
 Ion Ratio Lower Upper
 43 100
 61 1.6 11.5 17.3#
 70 0.0 7.9 11.9#

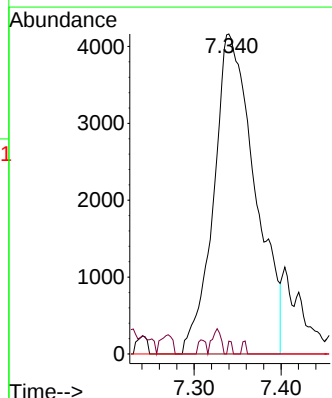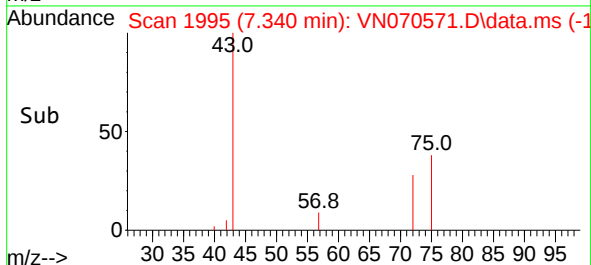






#38
Carbon Tetrachloride
Concen: 6.127 ug/l
RT: 8.077 min Scan# 21
Delta R.T. -0.129 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:117 Resp: 85691
Ion Ratio Lower Upper
117 100
119 4.3 76.1 114.1#
121 0.0 24.2 36.2#

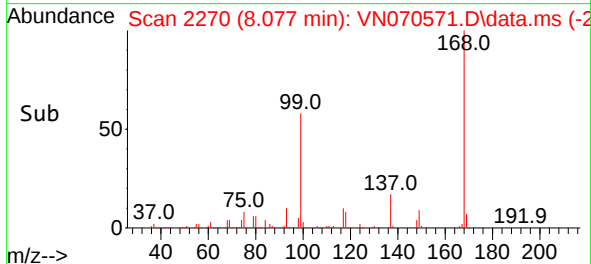

#39
Methylcyclohexane
Concen: 2.541 ug/l
RT: 9.453 min Scan# 2783
Delta R.T. -0.006 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08

Tgt Ion: 83 Resp: 45054
Ion Ratio Lower Upper
83 100
55 90.0 58.1 87.1#
98 49.6 38.4 57.6









#48
Methyl methacrylate
Concen: 0.296 ug/l
RT: 9.502 min Scan# 21
Delta R.T. -0.056 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 41 Resp: 4228
Ion Ratio Lower Upper
41 100
69 0.0 72.4 108.6#
39 35.9 58.4 87.6#

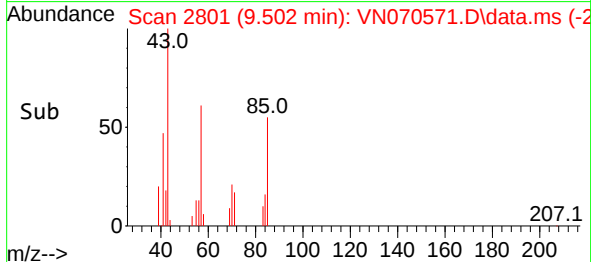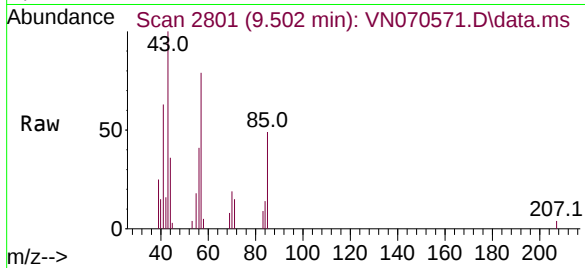

#50
Toluene-d8
Concen: 56.203 ug/l
RT: 10.438 min Scan# 3150
Delta R.T. -0.002 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08

Tgt Ion: 98 Resp: 2032765
Ion Ratio Lower Upper
98 100
100 64.1 50.4 75.6




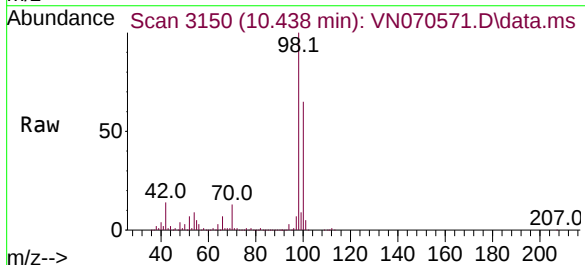




#55
1,1,2-Trichloroethane
Concen: 4.655 ug/l
RT: 10.872 min Scan# 31
Delta R.T. -0.024 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 97 Resp: 50064
Ion Ratio Lower Upper
97 100
83 8.9 67.8 101.6#
85 5.7 45.4 68.2#
99 0.0 49.4 74.0#

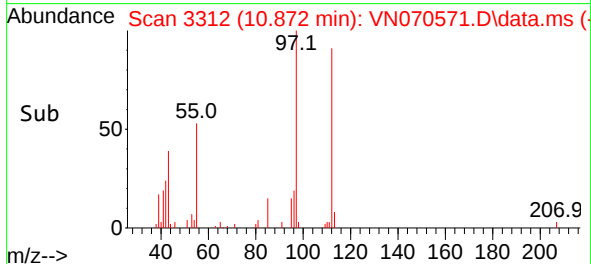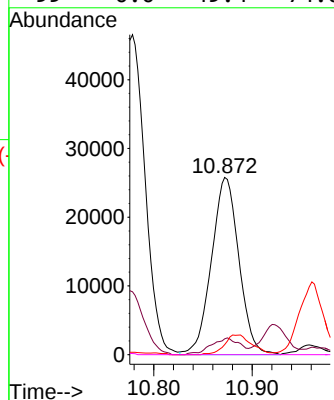

#56
Ethyl methacrylate
Concen: 0.672 ug/l
RT: 10.733 min Scan# 3260
Delta R.T. -0.027 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08

Tgt Ion: 69 Resp: 11945
Ion Ratio Lower Upper
69 100
41 62.7 51.4 77.0
39 25.0 34.6 52.0#


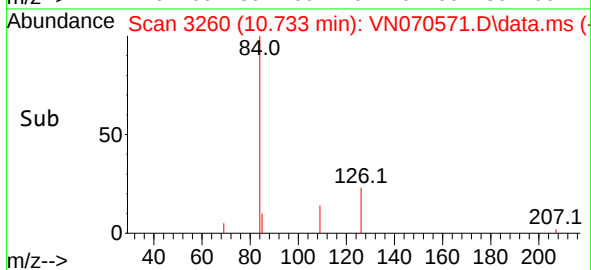
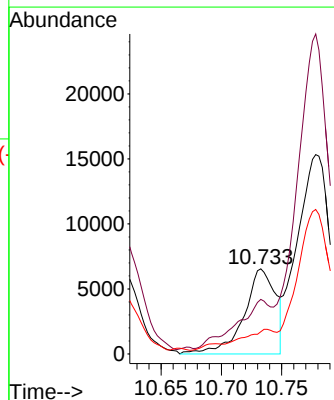





#58
2-Chloroethyl Vinyl ether
Concen: 19.724 ug/l
RT: 10.038 min Scan# 3002
Delta R.T. -0.003 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 63 Resp: 5934
Ion Ratio Lower Upper
63 100
106 27.4 23.9 35.9

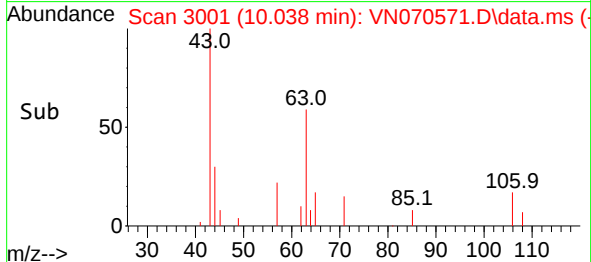

#59
2-Hexanone
Concen: 8.117 ug/l
RT: 11.049 min Scan# 3378
Delta R.T. -0.035 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08

Tgt Ion: 43 Resp: 111329
Ion Ratio Lower Upper
43 100
58 3.5 26.9 80.7#




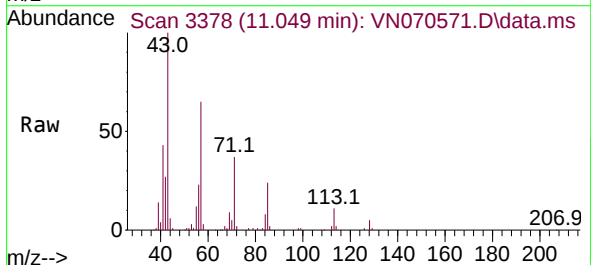




#62
4-Bromofluorobenzene
Concen: 66.223 ug/l
RT: 12.728 min Scan# 4005
Delta R.T. -0.003 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 865091
Ion Ratio Lower Upper
95 100
174 74.8 0.0 187.2
176 72.1 0.0 181.4

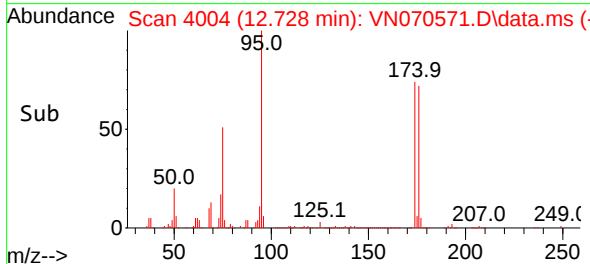

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. -0.000 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08


Tgt Ion: 117 Resp: 1392751
Ion Ratio Lower Upper
117 100
82 57.6 42.4 63.6
119 31.7 25.4 38.2

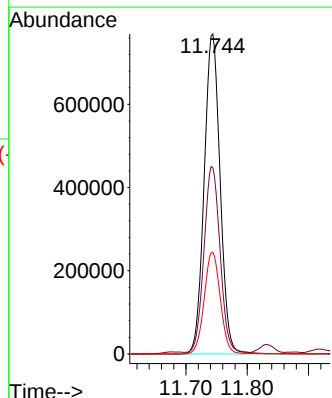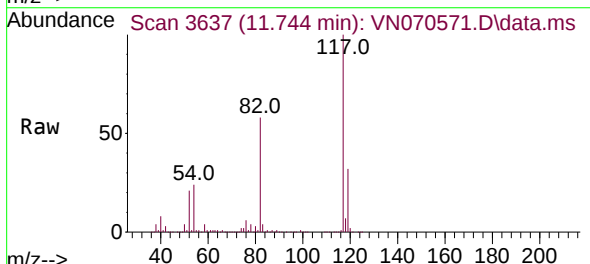






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.672 min Scan# 41
Delta R.T. 0.000 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:152 Resp: 643484
Ion Ratio Lower Upper
152 100
115 59.4 27.5 82.5
150 156.4 0.0 344.4

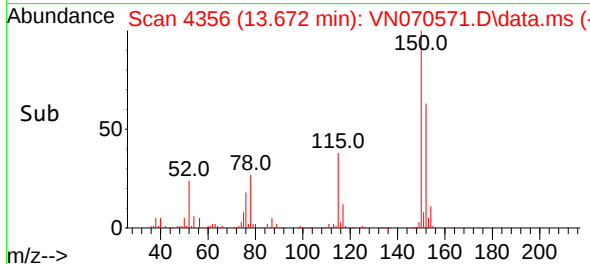


#73
Isopropylbenzene
Concen: 4.887 ug/l
RT: 12.575 min Scan# 3947
Delta R.T. -0.003 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08

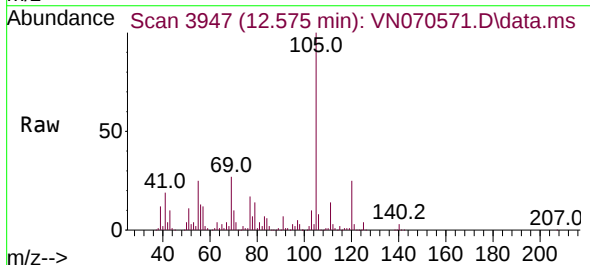


Tgt Ion:105 Resp: 292049
Ion Ratio Lower Upper
105 100
120 25.6 13.4 40.1

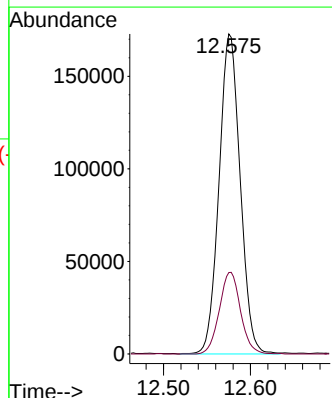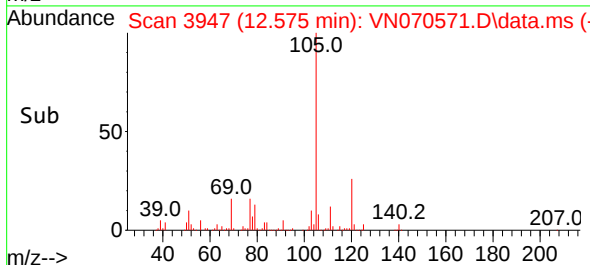






#74
N-amy1 acetate
Concen: 8.394 ug/l
RT: 12.363 min Scan# 3868
Delta R.T. -0.022 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:	43	Resp:	210902
Ion Ratio	Lower	Upper	
43	100		
70	0.0	33.4	50.0#
55	0.0	19.3	28.9#
61	0.3	18.5	27.7#

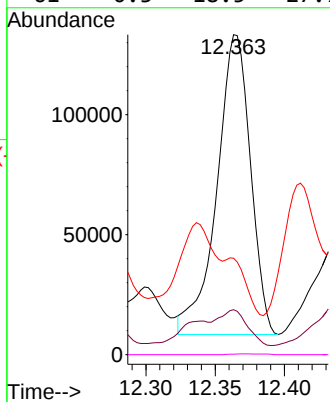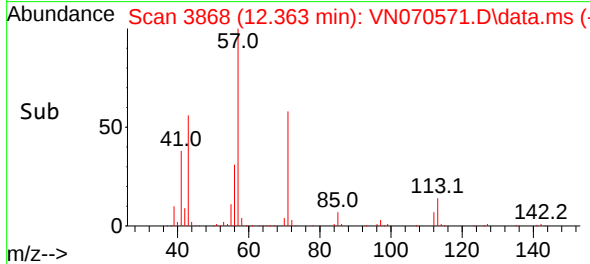

#75
1,1,2,2-Tetrachloroethane
Concen: 1.493 ug/l
RT: 12.806 min Scan# 4033
Delta R.T. -0.019 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08

Tgt Ion:	83	Resp:	22869
Ion Ratio	Lower	Upper	
83	100		
131	0.0	5.5	16.5#
85	59.2	32.4	97.2


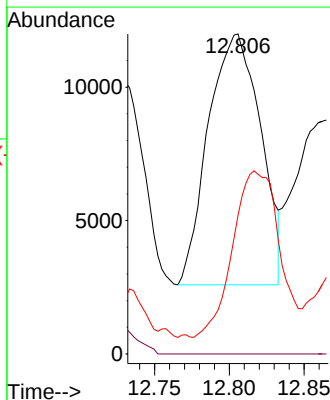
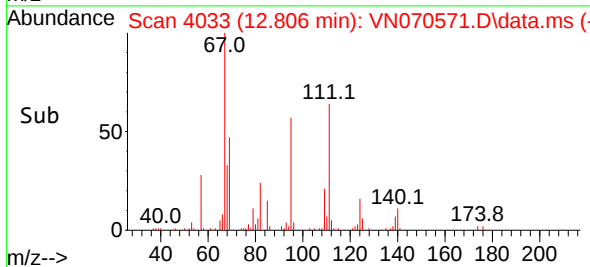
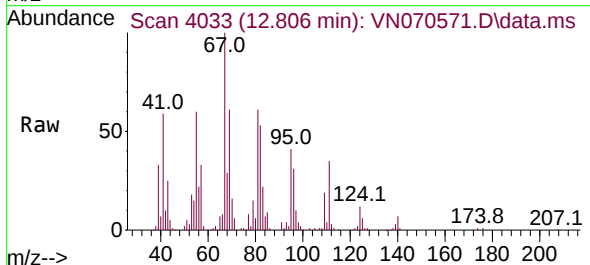




#76
1,2,3-Trichloropropane
Concen: 24.743 ug/l
RT: 12.728 min Scan# 4060
Delta R.T. -0.150 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 443526
Ion Ratio Lower Upper
75 100
77 1.7 82.6 247.8#

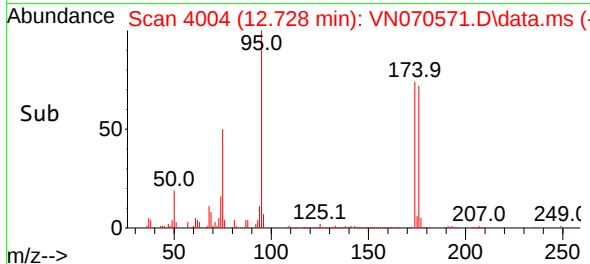

#78
n-propylbenzene
Concen: 9.586 ug/l
RT: 12.916 min Scan# 4074
Delta R.T. -0.003 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08

Tgt Ion: 91 Resp: 634705
Ion Ratio Lower Upper
91 100
120 21.7 11.9 35.9


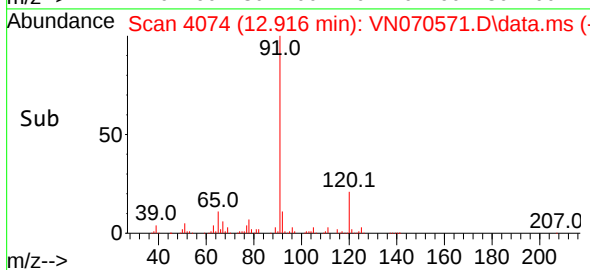

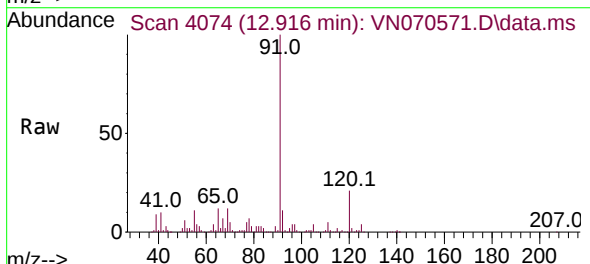




#79
2-Chlorotoluene
Concen: 14.941 ug/l
RT: 12.916 min Scan# 4004
Delta R.T. -0.091 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 634705
Ion Ratio Lower Upper
91 100
126 0.0 18.3 54.8#

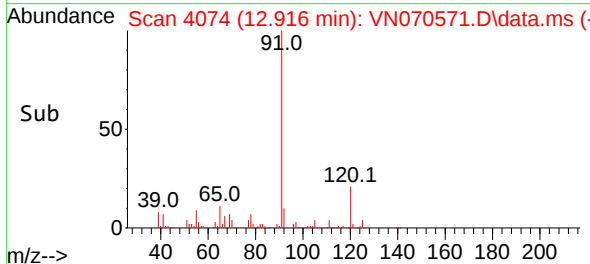

#81
trans-1,4-Dichloro-2-butene
Concen: 84.211 ug/l
RT: 12.728 min Scan# 4004
Delta R.T. 0.104 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08

Tgt Ion: 75 Resp: 443526
Ion Ratio Lower Upper
75 100
53 1.8 90.5 135.7#
89 0.0 38.2 57.4#


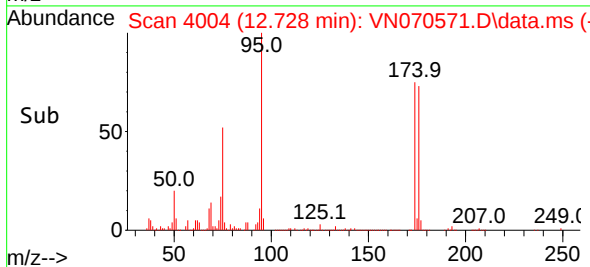

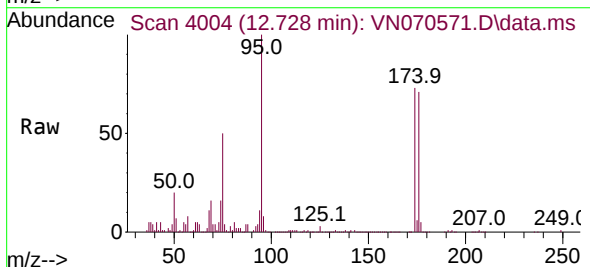




#82
4-Chlorotoluene
Concen: 15.956 ug/l
RT: 12.916 min Scan# 4074
Delta R.T. -0.188 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 634942
Ion Ratio Lower Upper
91 100
126 0.0 18.2 54.6#

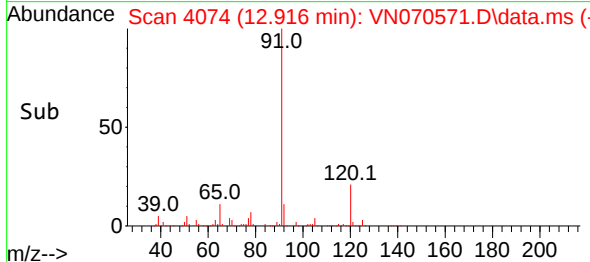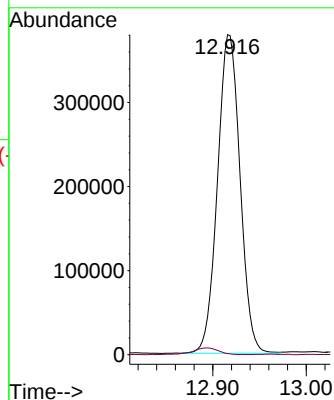

#83
tert-Butylbenzene
Concen: 1.687 ug/l
RT: 13.321 min Scan# 4225
Delta R.T. -0.000 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08

Tgt Ion: 119 Resp: 71120
Ion Ratio Lower Upper
119 100
91 71.2 31.5 94.5
134 24.3 12.4 37.4

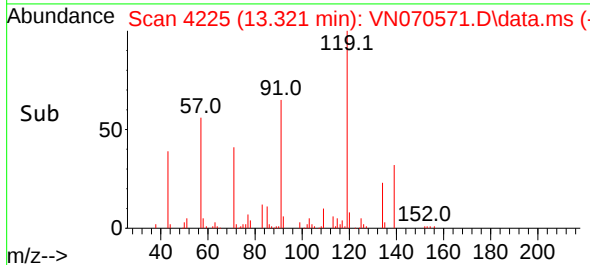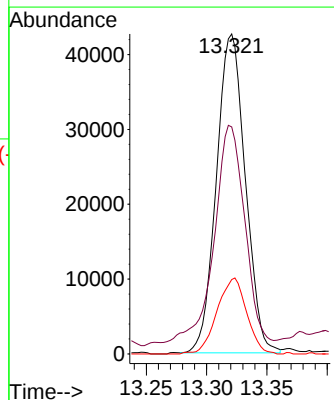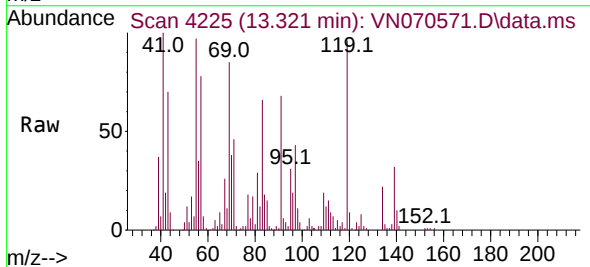



#84

1,2,4-Trimethylbenzene

Concen: 18.968 ug/l

RT: 13.498 min Scan# 4291

Delta R.T. 0.132 min

Lab File: VN070571.D

Acq: 11 Jan 2022 16:08

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:105 Resp: 874634

Ion Ratio Lower Upper

105 100

120 0.2 22.8 68.4#

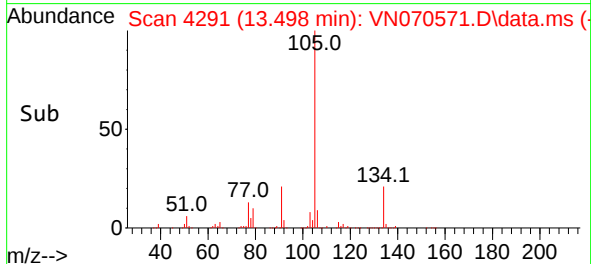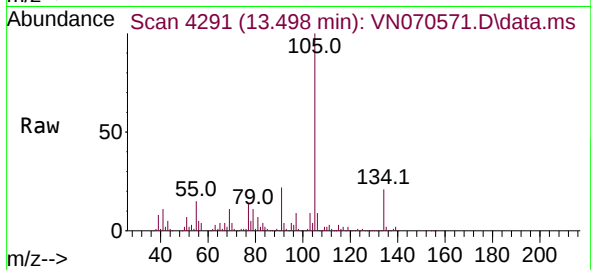

#85

sec-Butylbenzene

Concen: 15.278 ug/l

RT: 13.498 min Scan# 4291

Delta R.T. -0.003 min

Lab File: VN070571.D




Acq: 11 Jan 2022 16:08


Tgt Ion:105 Resp: 874634

Ion Ratio Lower Upper

105 100

134 26.3 10.4 31.1

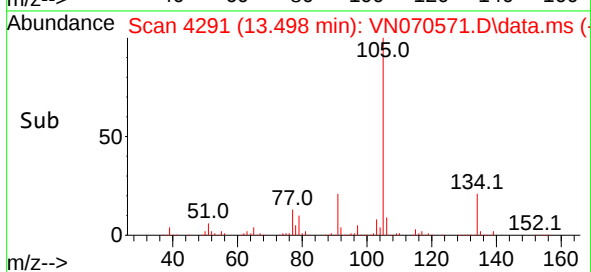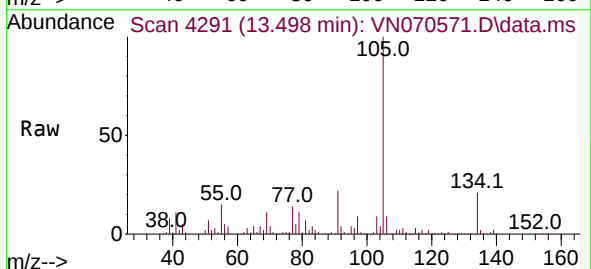



#86

p-Isopropyltoluene

Concen: 4.370 ug/l

RT: 13.769 min Scan# 41

Delta R.T. 0.156 min

Lab File: VN070571.D

Acq: 11 Jan 2022 16:08

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:119 Resp: 196511

Ion Ratio Lower Upper

119 100

134 27.5 13.6 40.7

91 28.2 11.4 34.1

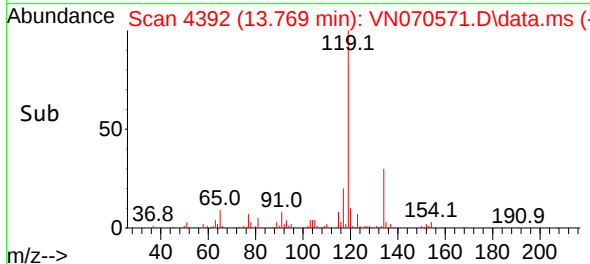

#89

n-Butylbenzene

Concen: 9.836 ug/l

RT: 13.940 min Scan# 4456

Delta R.T. 0.000 min

Lab File: VN070571.D

Acq: 11 Jan 2022 16:08




Tgt Ion: 91 Resp: 368925


Ion Ratio Lower Upper

91 100

92 52.5 25.4 76.0

134 30.7 13.6 40.8


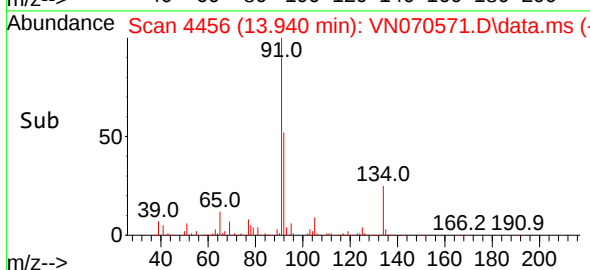






#90
Hexachloroethane
Concen: 19.947 ug/l
RT: 14.214 min Scan# 41
Delta R.T. 0.005 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 155828
Ion Ratio Lower Upper
117 100
201 0.0 43.9 131.6#

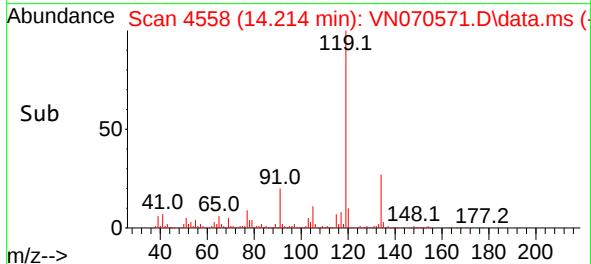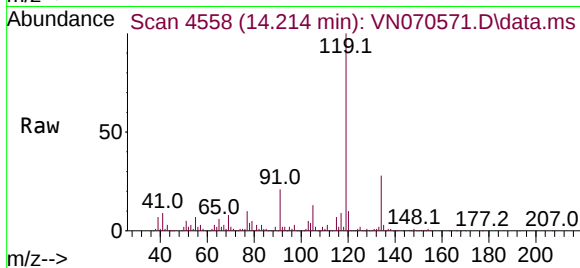

#92
1,2-Dibromo-3-Chloropropane
Concen: 1.409 ug/l
RT: 14.621 min Scan# 4710
Delta R.T. 0.021 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08

Tgt Ion: 75 Resp: 4877
Ion Ratio Lower Upper
75 100
155 0.0 46.9 140.7#
157 1.7 60.6 181.7#




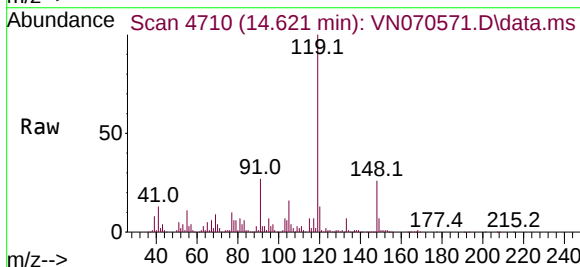




#93
1,2,4-Trichlorobenzene
Concen: 0.249 ug/l
RT: 15.262 min Scan# 4949
Delta R.T. -0.001 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:180 Resp: 2644
Ion Ratio Lower Upper
180 100
182 96.4 48.3 144.9
145 16837.3 14.5 43.5#

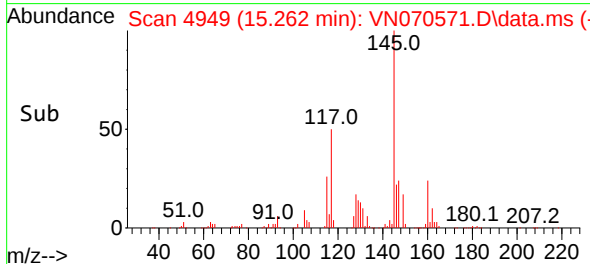

#95
Naphthalene
Concen: 2.660 ug/l
RT: 15.461 min Scan# 5023
Delta R.T. -0.043 min
Lab File: VN070571.D
Acq: 11 Jan 2022 16:08


Tgt Ion:128 Resp: 26247
Ion Ratio Lower Upper
128 100
127 40.9 10.5 15.7#
129 111.5 8.7 13.1#

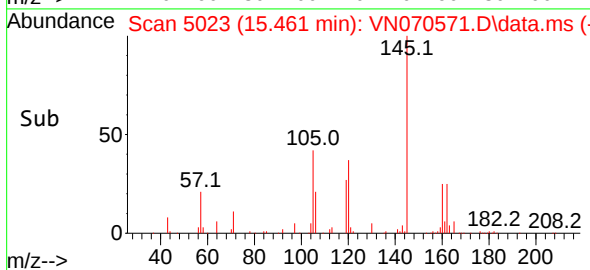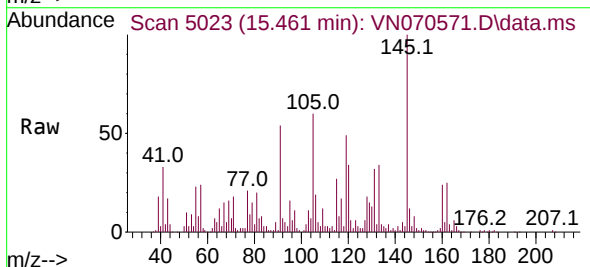



#96
 1,2,3-Trichlorobenzene
 Concen: 0.840 ug/l
 RT: 15.689 min Scan# 511
 Delta R.T. -0.011 min
 Lab File: VN070571.D
 Acq: 11 Jan 2022 16:08

Instrument :
 MSVOA_N
 ClientSampleId :

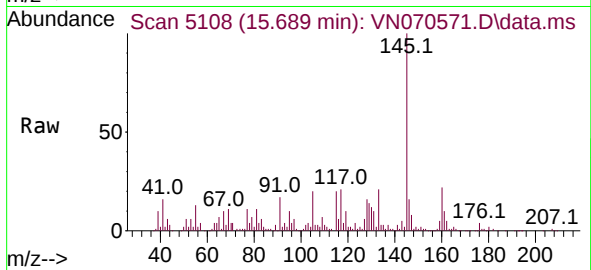

Tgt Ion:180 Resp: 141
 Ion Ratio Lower Upper
 180 100
 182 939.7 47.4 142.2#
 145 0.0 15.0 45.1#

