
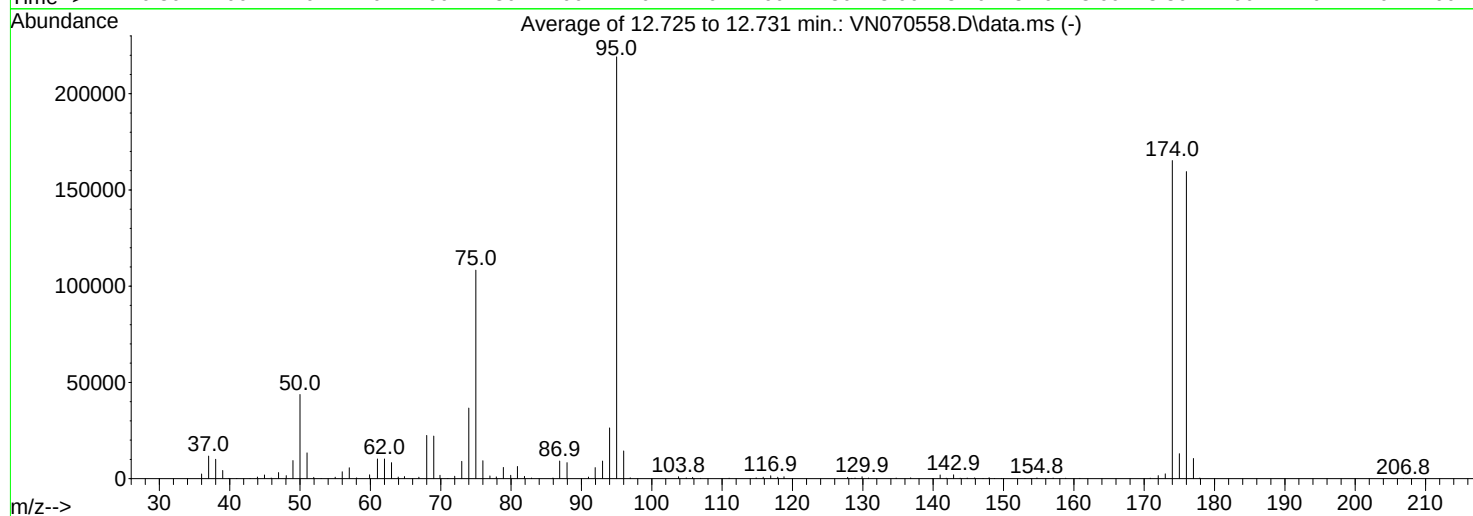


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011122\
Data File : VN070558.D
Acq On : 11 Jan 2022 9:40
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Title : SW846 8260
Last Update : Mon Dec 27 18:47:12 2021

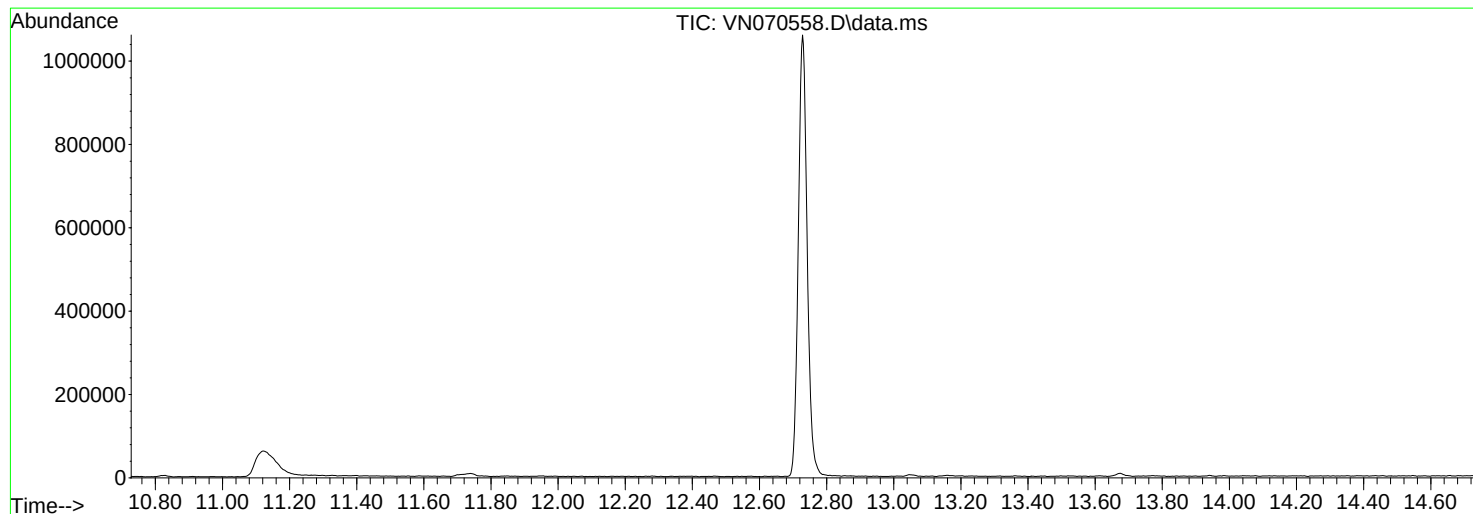

AutoFind: Scans 4003, 4004, 4005; Background Corrected with Scan 3985

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	43752	PASS
75	95	30	60	49.4	108352	PASS
95	95	100	100	100.0	219157	PASS
96	95	5	9	6.6	14409	PASS
173	174	0.00	2	1.5	2468	PASS
174	95	50	100	75.4	165248	PASS
175	174	5	9	7.8	12969	PASS
176	174	95	101	96.6	159552	PASS
177	176	5	9	6.6	10480	PASS