


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011124\
Data File : VN080665.D
Acq On : 11 Jan 2024 09:29
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N011124W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Jan 12 05:20:11 2024

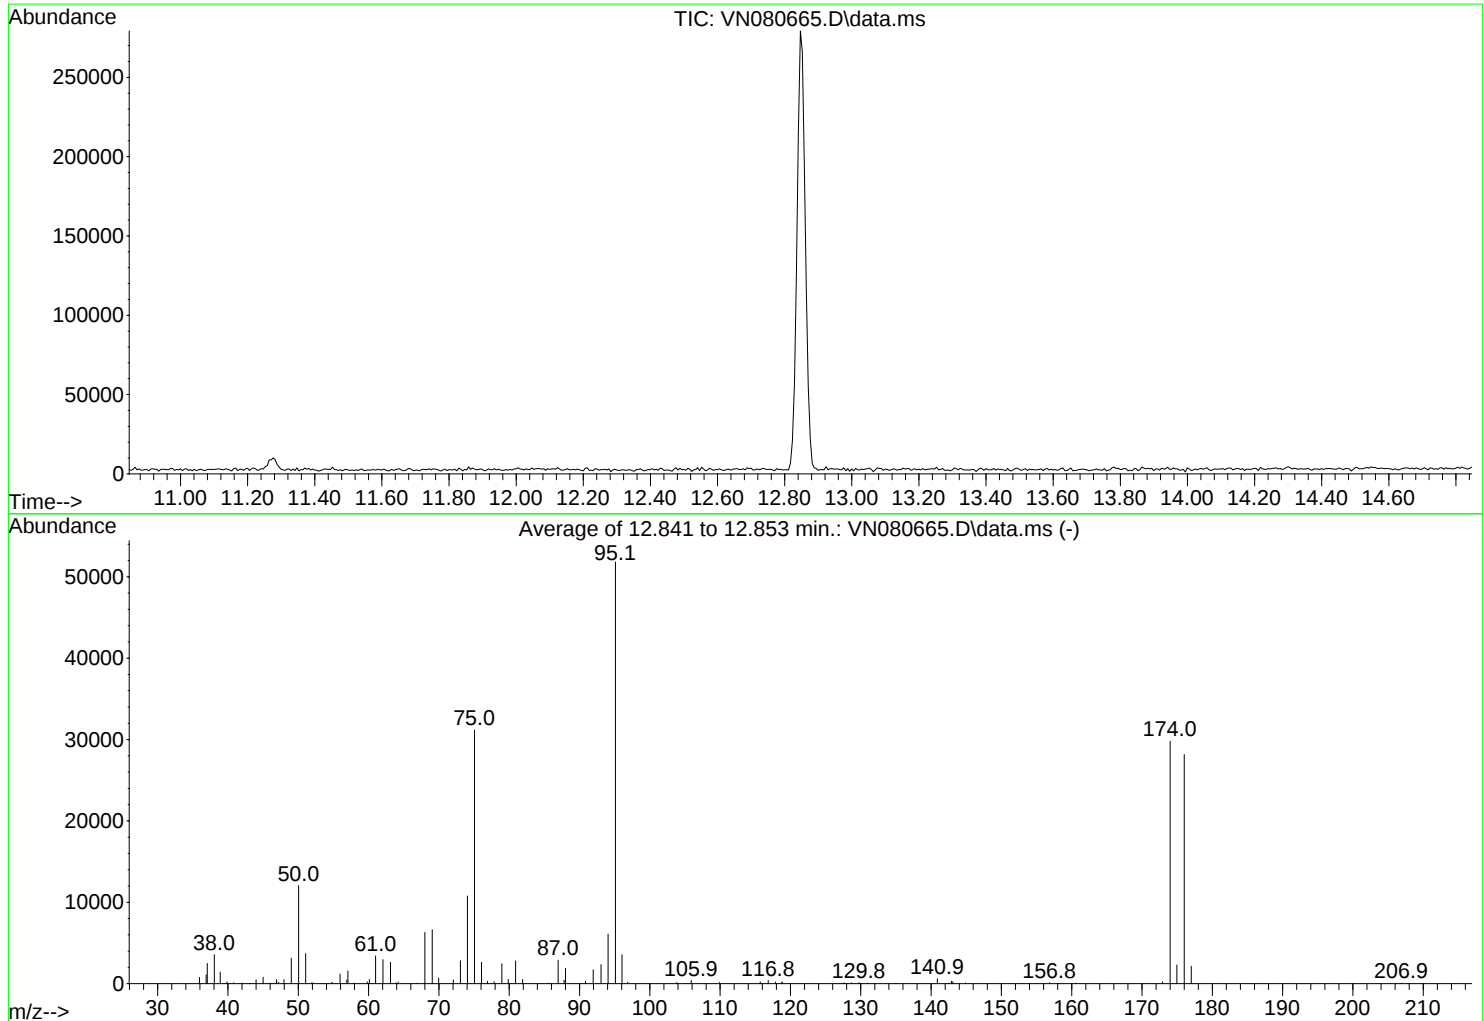

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.2	12052	PASS
75	95	30	60	60.1	31165	FAIL*
95	95	100	100	100.0	51845	PASS
96	95	5	9	6.9	3564	PASS
173	174	0.00	2	0.8	226	PASS
174	95	50	100	57.5	29805	PASS
175	174	5	9	7.7	2293	PASS
176	174	95	101	94.5	28168	FAIL*
177	176	5	9	7.6	2150	PASS