
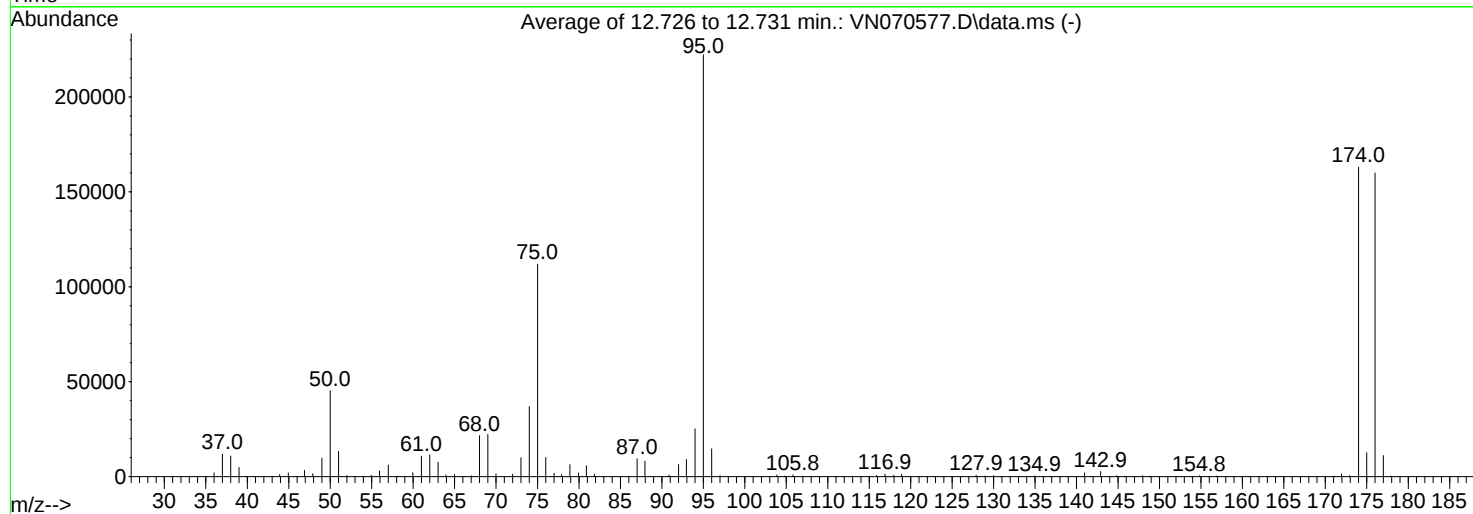


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011222\
 Data File : VN070577.D
 Acq On : 12 Jan 2022 9:46
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
 Title : SW846 8260
 Last Update : Mon Dec 27 18:47:12 2021

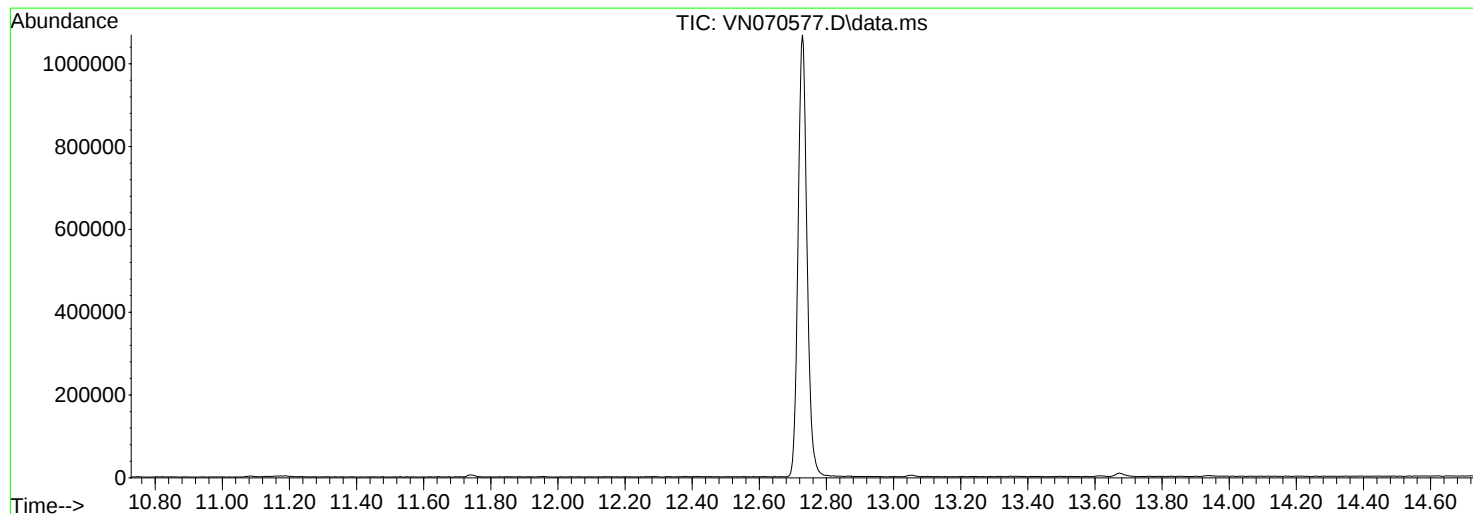

AutoFind: Scans 4003, 4004, 4005; Background Corrected with Scan 3985

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	45309	PASS
75	95	30	60	50.4	111904	PASS
95	95	100	100	100.0	222187	PASS
96	95	5	9	6.6	14674	PASS
173	174	0.00	2	0.4	592	PASS
174	95	50	100	73.4	163029	PASS
175	174	5	9	7.8	12665	PASS
176	174	95	101	98.1	159936	PASS
177	176	5	9	7.0	11133	PASS