
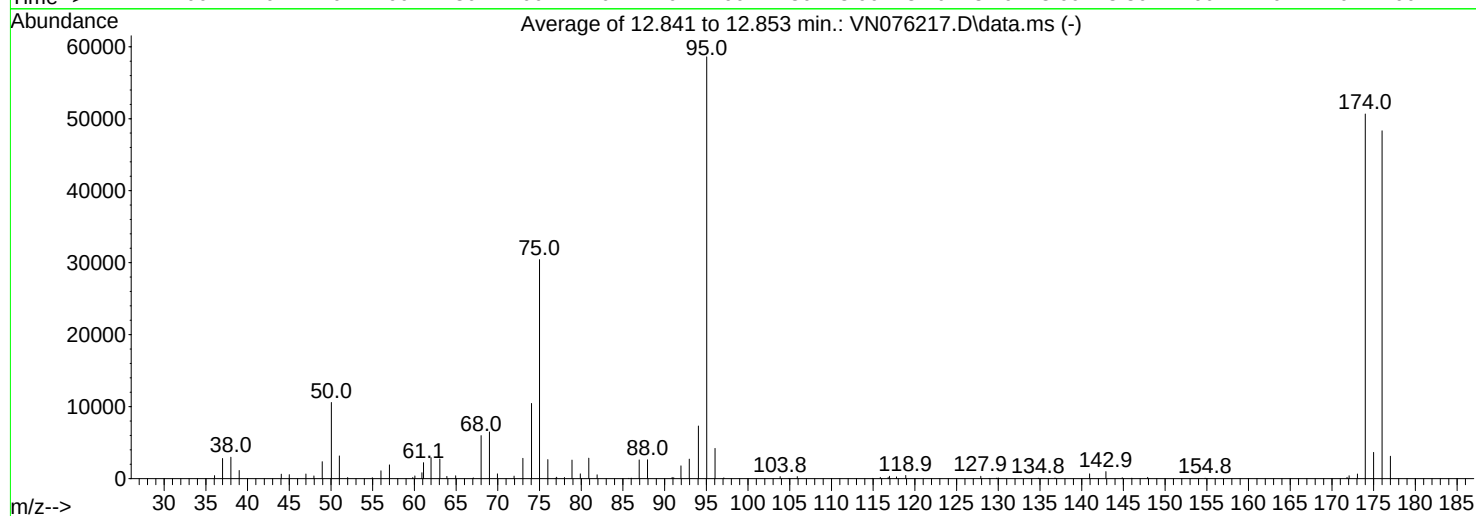


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011223\
 Data File : VN076217.D
 Acq On : 12 Jan 2023 08:26
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Title : SW846 8260
 Last Update : Wed Dec 14 13:03:41 2022

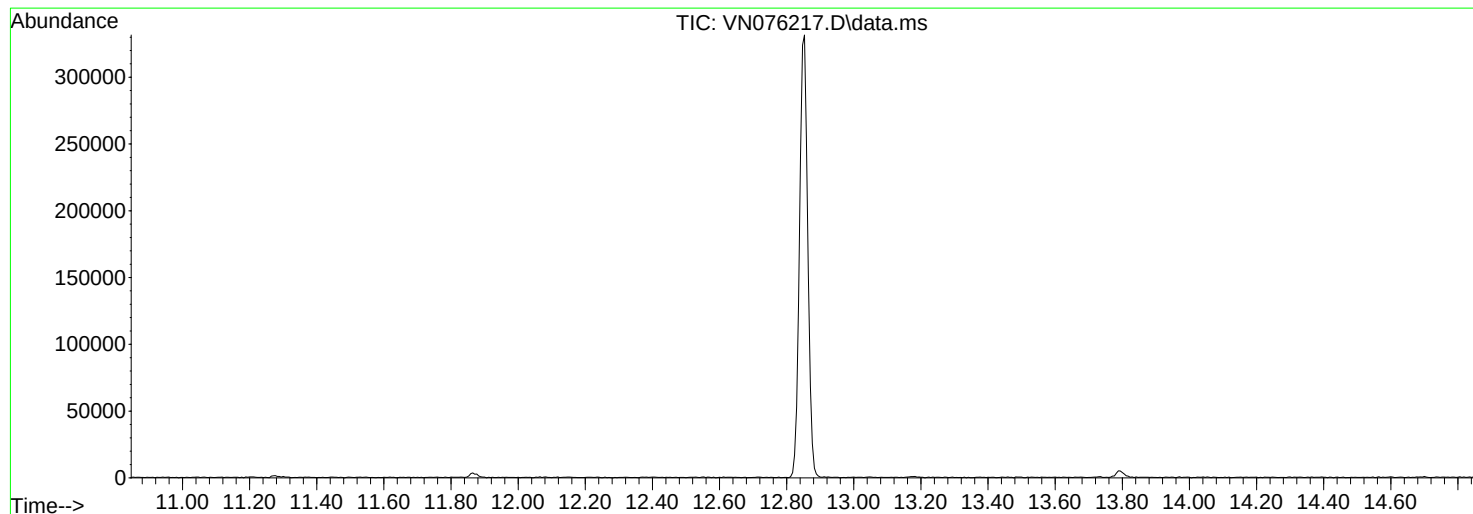

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	10575	PASS
75	95	30	60	51.9	30437	PASS
95	95	100	100	100.0	58595	PASS
96	95	5	9	7.2	4197	PASS
173	174	0.00	2	1.3	645	PASS
174	95	50	100	86.4	50648	PASS
175	174	5	9	7.2	3638	PASS
176	174	95	101	95.4	48331	PASS
177	176	5	9	6.5	3120	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	431	52.00	161	64.95	395	77.05	20
37.00	2803	54.95	140	67.05	109	78.00	15
38.00	2985	56.00	1089	68.00	5976	78.90	258
39.00	1134	57.00	1905	69.00	6502	79.90	67
44.05	633	59.80	154	69.95	668	80.90	2850
45.00	556	60.05	385	71.95	367	81.90	529
47.00	654	60.90	825	73.00	2824	85.70	54
47.95	379	61.10	2229	74.05	10441	86.00	59
48.95	2355	62.00	2922	75.00	30437	86.95	2613
50.05	10575	63.05	2727	76.00	2638	87.95	2616
51.00	3150	63.90	322	76.90	69	90.90	169

Average of 12.841 to 12.853 min.: VN076217.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.10	127	115.85	177	140.95	663	176.00	48331
91.95	1783	116.80	154	142.90	973	177.00	3120
92.95	2719	116.95	332	144.85	138		
94.05	7305	117.80	257	146.00	68		
95.05	58595	118.90	442	147.90	185		
96.05	4197	127.90	332	154.80	79		
97.10	109	128.90	55	171.80	168		
103.85	297	129.80	67	172.05	403		
104.90	50	130.00	122	173.05	645		
105.90	296	134.80	69	174.00	50648		
114.90	54	136.80	85	175.00	3638		

Instrument :

MSVOA_N

ClientSampleId :

BFB