

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011224\
 Data File : VN080701.D
 Acq On : 12 Jan 2024 19:41
 Operator : JC\MD
 Sample : P1111-07
 Misc : 2.45g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 DRYER-7

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M

Title : SW846 8260

Signal : TIC: VN080701.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.889	149	159	160	rBV8	24925	61622	5.01%	0.922%
2	6.294	728	738	748	rVB6	8428	25906	2.11%	0.387%
3	8.165	1044	1056	1060	rBV2	135792	326951	26.59%	4.890%
4	8.218	1060	1065	1076	rVB	244086	554572	45.10%	8.295%
5	8.577	1117	1126	1138	rBV2	149059	351248	28.56%	5.254%
6	9.100	1207	1215	1224	rBV	452795	925842	75.29%	13.848%
7	10.565	1455	1464	1474	rBV	590021	1120938	91.15%	16.766%
8	11.282	1579	1586	1591	rBV3	8260	15076	1.23%	0.225%
9	11.865	1677	1685	1694	rBV	677323	1229770	100.00%	18.394%
10	12.853	1846	1853	1861	rVB	438101	774082	62.95%	11.578%
11	13.794	2005	2013	2020	rBV	650310	1102664	89.66%	16.493%
12	13.870	2023	2026	2032	rVB4	10962	18513	1.51%	0.277%
13	14.958	2207	2211	2215	rBV4	11054	15392	1.25%	0.230%
14	15.041	2221	2225	2230	rBV6	7653	12500	1.02%	0.187%
15	15.435	2290	2292	2299	rVB6	7674	12678	1.03%	0.190%
16	15.582	2313	2317	2322	rBV6	7863	15201	1.24%	0.227%
17	15.835	2355	2360	2368	rVB3	23002	41522	3.38%	0.621%
18	16.170	2413	2417	2423	rVB7	9425	15388	1.25%	0.230%
19	16.476	2462	2469	2476	rBV	29678	65929	5.36%	0.986%




Sum of corrected areas: 6685794

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011224\
Data File : VN080701.D
Acq On : 12 Jan 2024 19:41
Operator : JC\MD
Sample : P1111-07
Misc : 2.45g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DRYER-7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

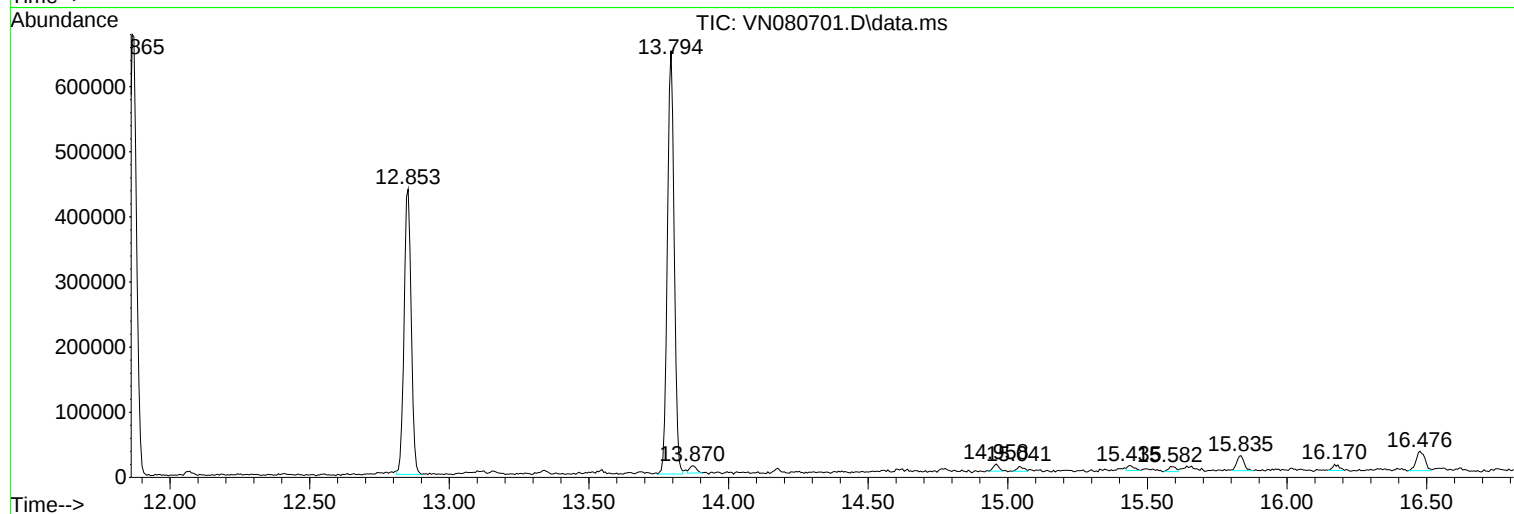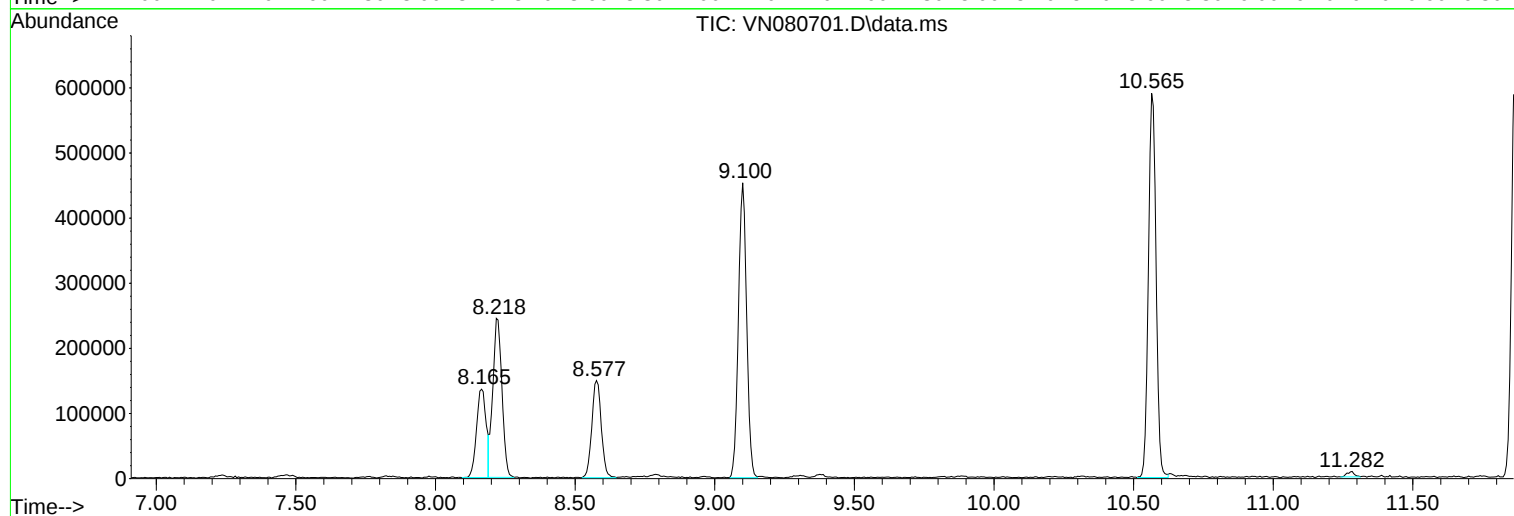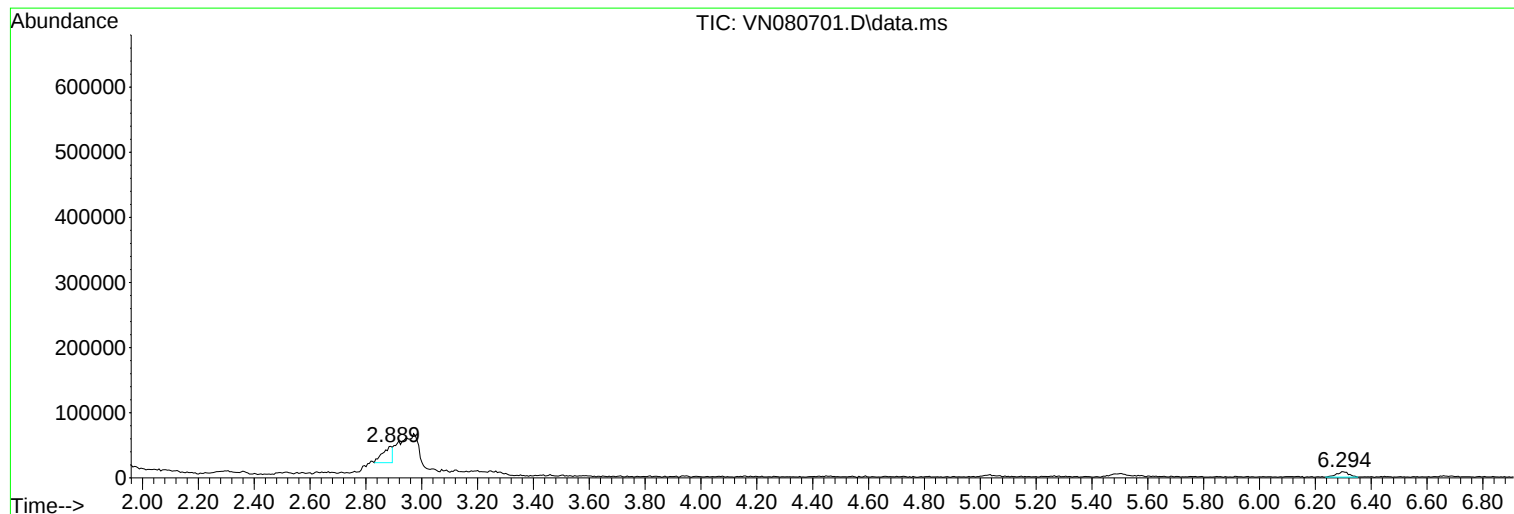

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011224\
Data File : VN080701.D
Acq On : 12 Jan 2024 19:41
Operator : JC\MD
Sample : P1111-07
Misc : 2.45g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DRYER-7










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown2.889 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.889	5.56 ug/l	61622	Pentafluorobenzene	8.218

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1,2-bis(2-chloroethoxy)-	186	C6H12Cl2O2	000112-26-5	27
2			n-Propyl chloroformate	122	C4H7ClO2	000109-61-5	22
3			Azetidine, 1-chloro-	91	C3H6ClN	032115-53-0	16
4			3,3,5-Trichloro-2,4-dithiahexane...	288	C4H7Cl3O4S2	068483-82-9	16
5			2-Pyrrol2-[2-(2-chloro-ethoxy)-e...	260	C12H17ClO4	1000317-43-5	12

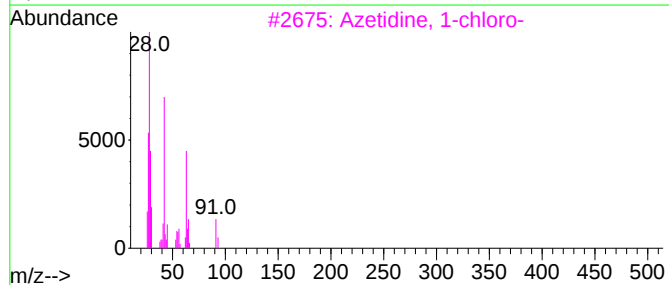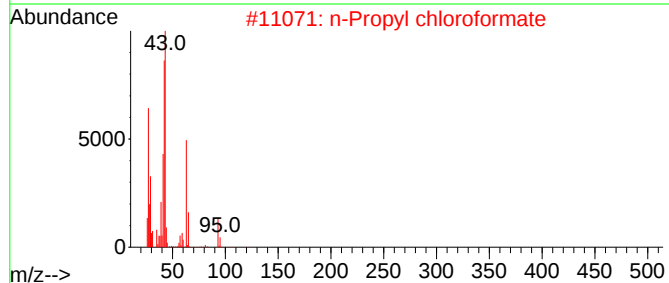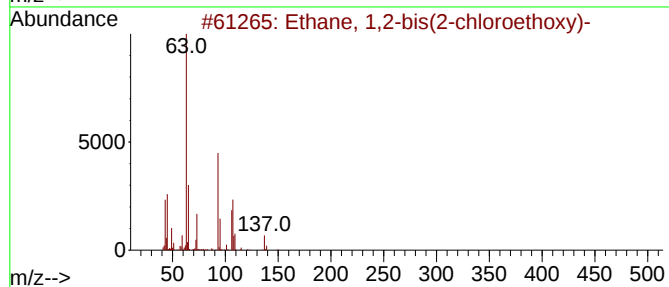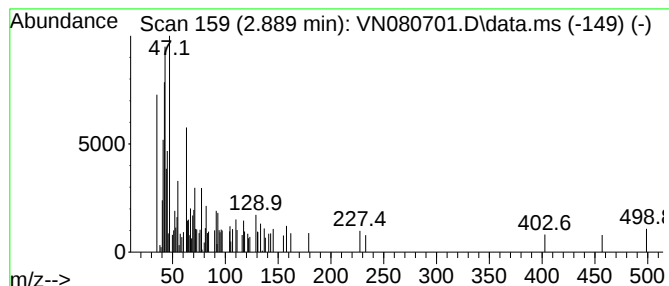

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011224\
Data File : VN080701.D
Acq On : 12 Jan 2024 19:41
Operator : JC\MD
Sample : P1111-07
Misc : 2.45g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DRYER-7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown2.889	2.889	5.6	ug/l	61622	1	8.218	554572	50.0