
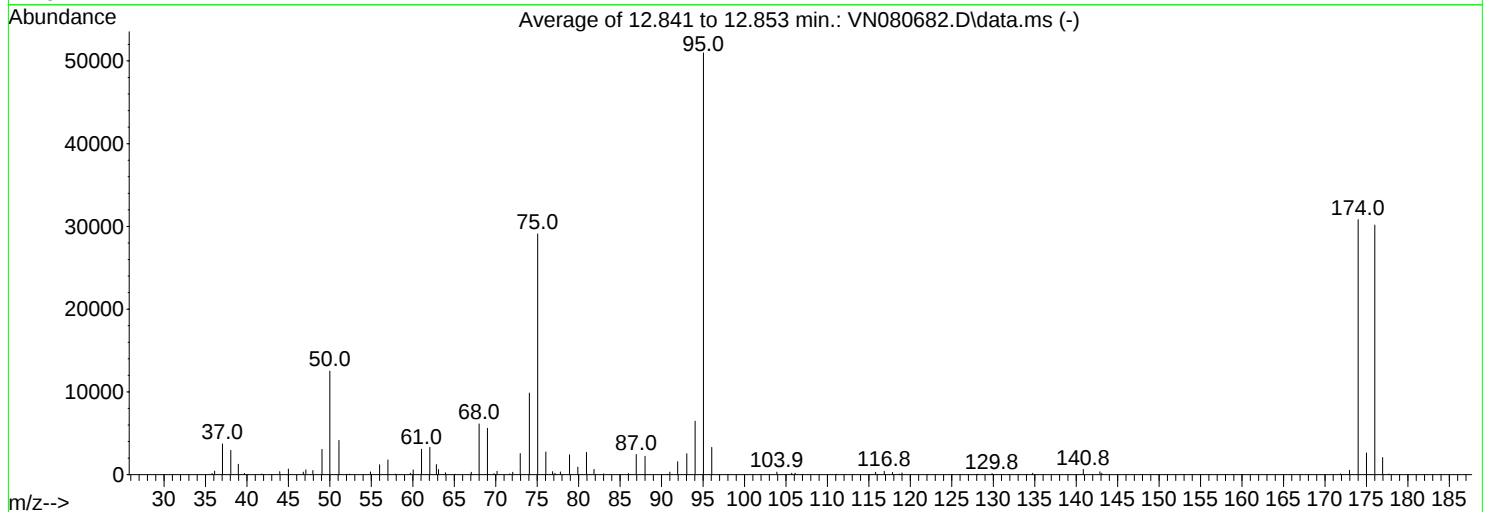


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011224\
Data File : VN080682.D
Acq On : 12 Jan 2024 10:29
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M
Title : SW846 8260
Last Update : Thu Jan 11 06:34:36 2024

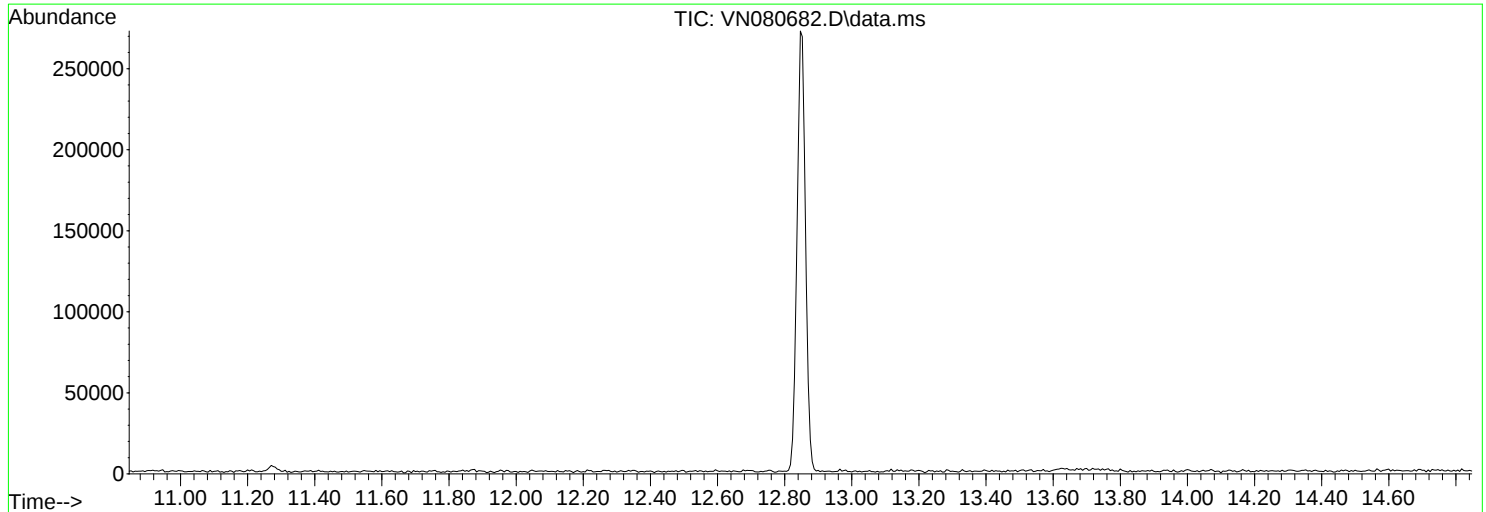

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.5	12511	PASS
75	95	30	60	57.1	29104	PASS
95	95	100	100	100.0	50979	PASS
96	95	5	9	6.5	3295	PASS
173	174	0.00	2	1.7	515	PASS
174	95	50	100	60.5	30821	PASS
175	174	5	9	8.5	2624	PASS
176	174	95	101	97.9	30171	PASS
177	176	5	9	6.9	2068	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	142	47.95	498	60.05	576	70.15	401
36.10	426	49.05	3049	61.05	3073	71.70	101
37.05	3710	50.00	12511	62.05	3309	72.05	281
38.05	2947	51.10	4146	62.85	1227	72.95	254
38.95	1255	52.00	51	63.10	619	74.05	9870
39.70	148	52.40	52	63.95	235	75.05	29104
41.80	74	54.90	329	65.10	56	76.05	2749
43.95	363	56.00	1204	67.05	282	76.85	377
45.00	685	57.00	1780	68.00	6131	77.15	166
46.80	311	57.90	73	69.00	5612	77.80	326
47.10	587	59.70	171	69.80	113	78.90	2392

Average of 12.841 to 12.853 min.: VN080682.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.90	906	94.05	6452	119.00	218	176.00	30171
80.95	2693	95.05	50979	128.10	60	176.95	2068
81.85	647	96.05	3295	129.85	130	177.70	71
83.00	106	103.90	302	134.75	172		
86.00	131	105.70	172	140.85	633		
86.95	2437	106.10	184	142.85	355		
88.00	2219	111.10	54	143.10	181		
90.70	55	115.80	284	171.90	97		
91.00	318	116.85	416	172.95	515		
91.95	1570	117.85	277	174.00	30821		
93.05	2539	118.70	82	175.00	2624		

Instrument :

MSVOA_N

ClientSampleId :

BFB