



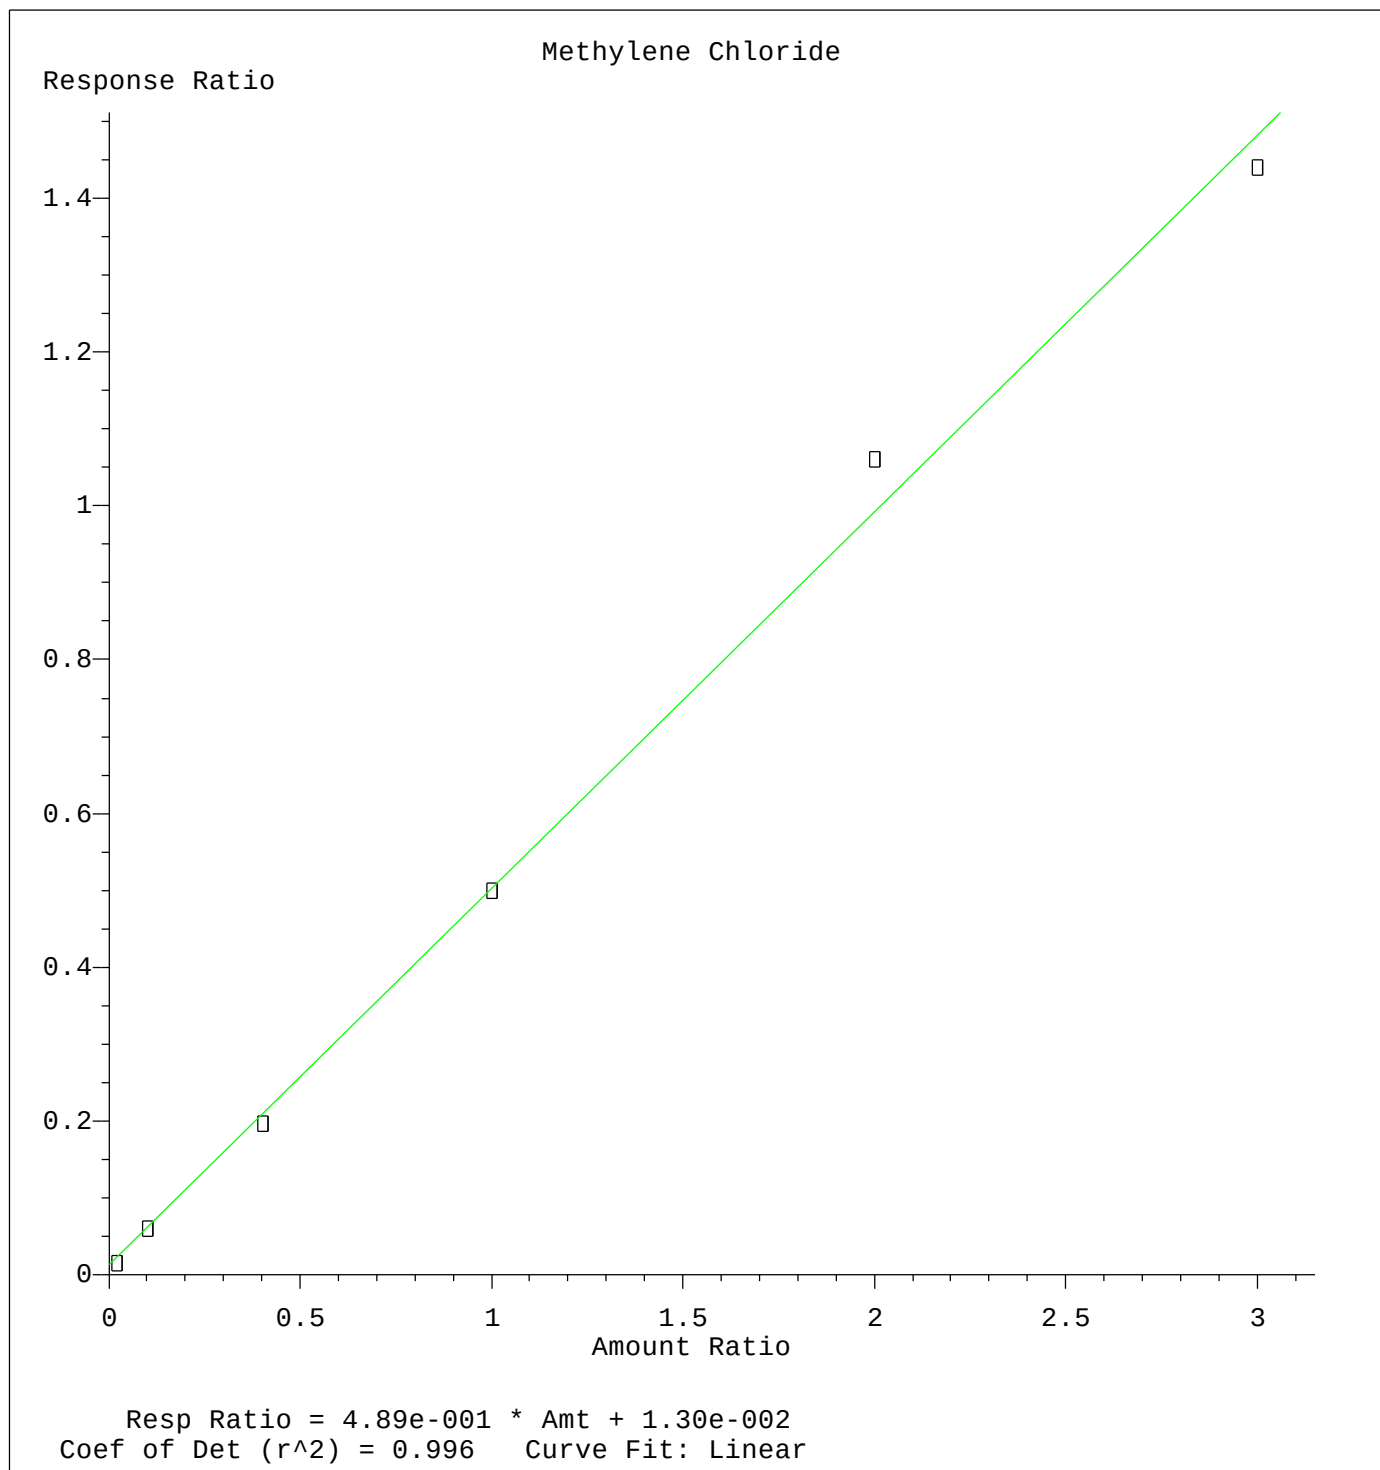

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011320W.M
Calibration Table Last Updated: Tue Jan 14 08:58:21 2020

1,2-Dibromo-3-Chloropropane

Response Ratio

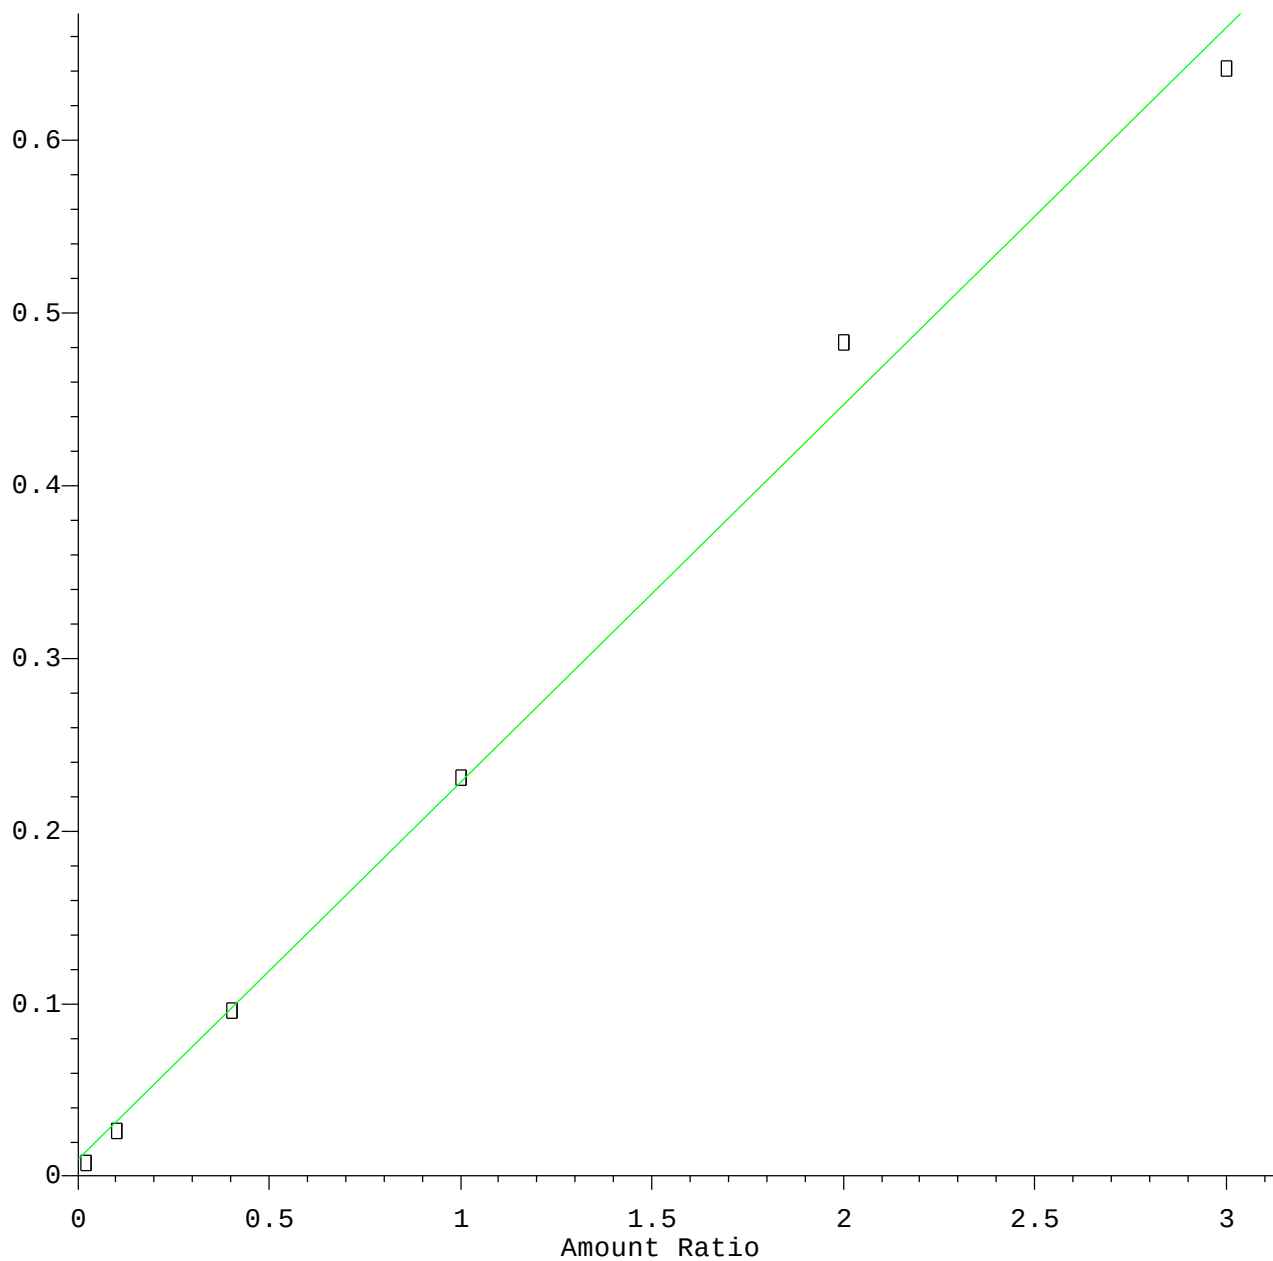


Resp Ratio = $2.19 \times 10^{-1} \times \text{Amt} + 9.53 \times 10^{-3}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011320W.M
Calibration Table Last Updated: Tue Jan 14 08:58:21 2020


Dichlorodifluoromethane

Response Ratio

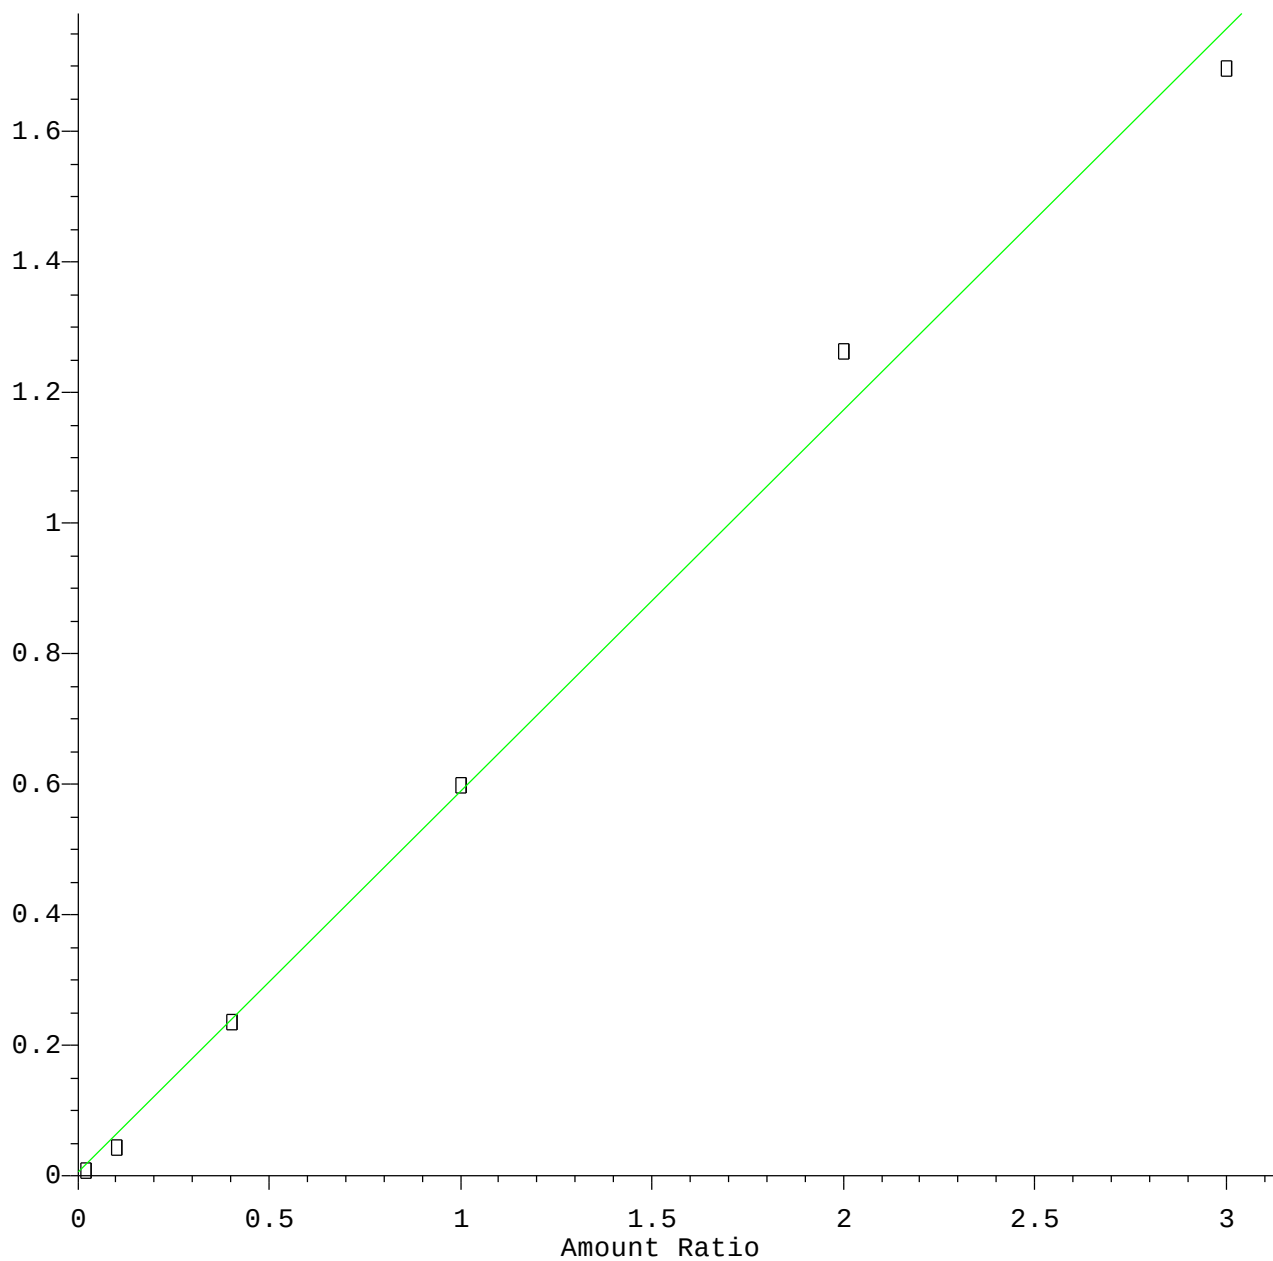

Resp Ratio = $5.83 \times 10^{-1} \times \text{Amt} + 6.17 \times 10^{-3}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011320W.M
Calibration Table Last Updated: Tue Jan 14 08:58:21 2020

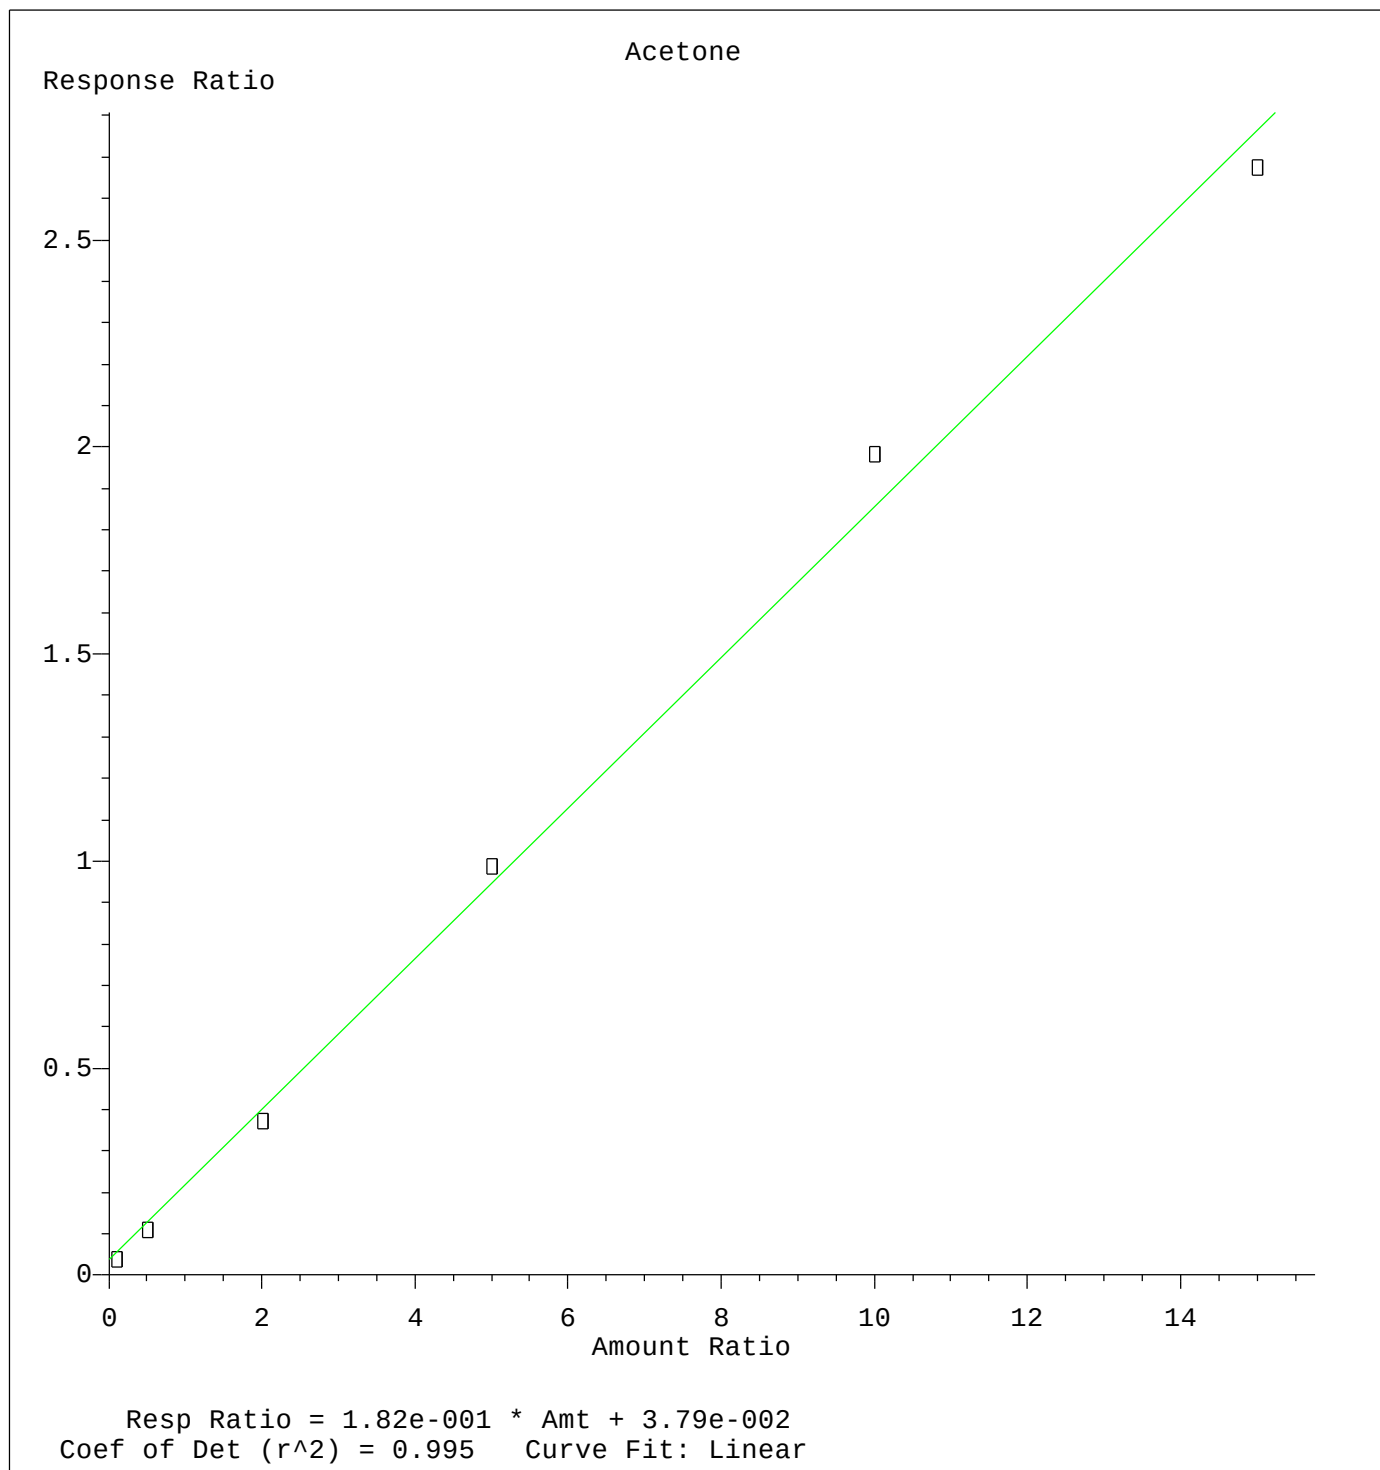

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011320W.M
Calibration Table Last Updated: Tue Jan 14 08:58:21 2020