

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011322\
 Data File : VN070609.D
 Acq On : 13 Jan 2022 14:08
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: Jan 14 04:53:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 27 18:47:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.086	168	765678	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	1300632	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	1169457	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	411696	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	629423	57.174	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 114.340%	
35) Dibromofluoromethane	8.021	113	443730	56.386	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 112.780%	
50) Toluene-d8	10.440	98	1776047	55.247	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 110.500%	
62) 4-Bromofluorobenzene	12.731	95	651966	56.151	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 112.300%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011322\
Data File : VN070609.D
Acq On : 13 Jan 2022 14:08
Operator : JC/MD
Sample : IBLK
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Time: Jan 14 04:53:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260
QLast Update : Mon Dec 27 18:47:12 2021
Response via : Initial Calibration




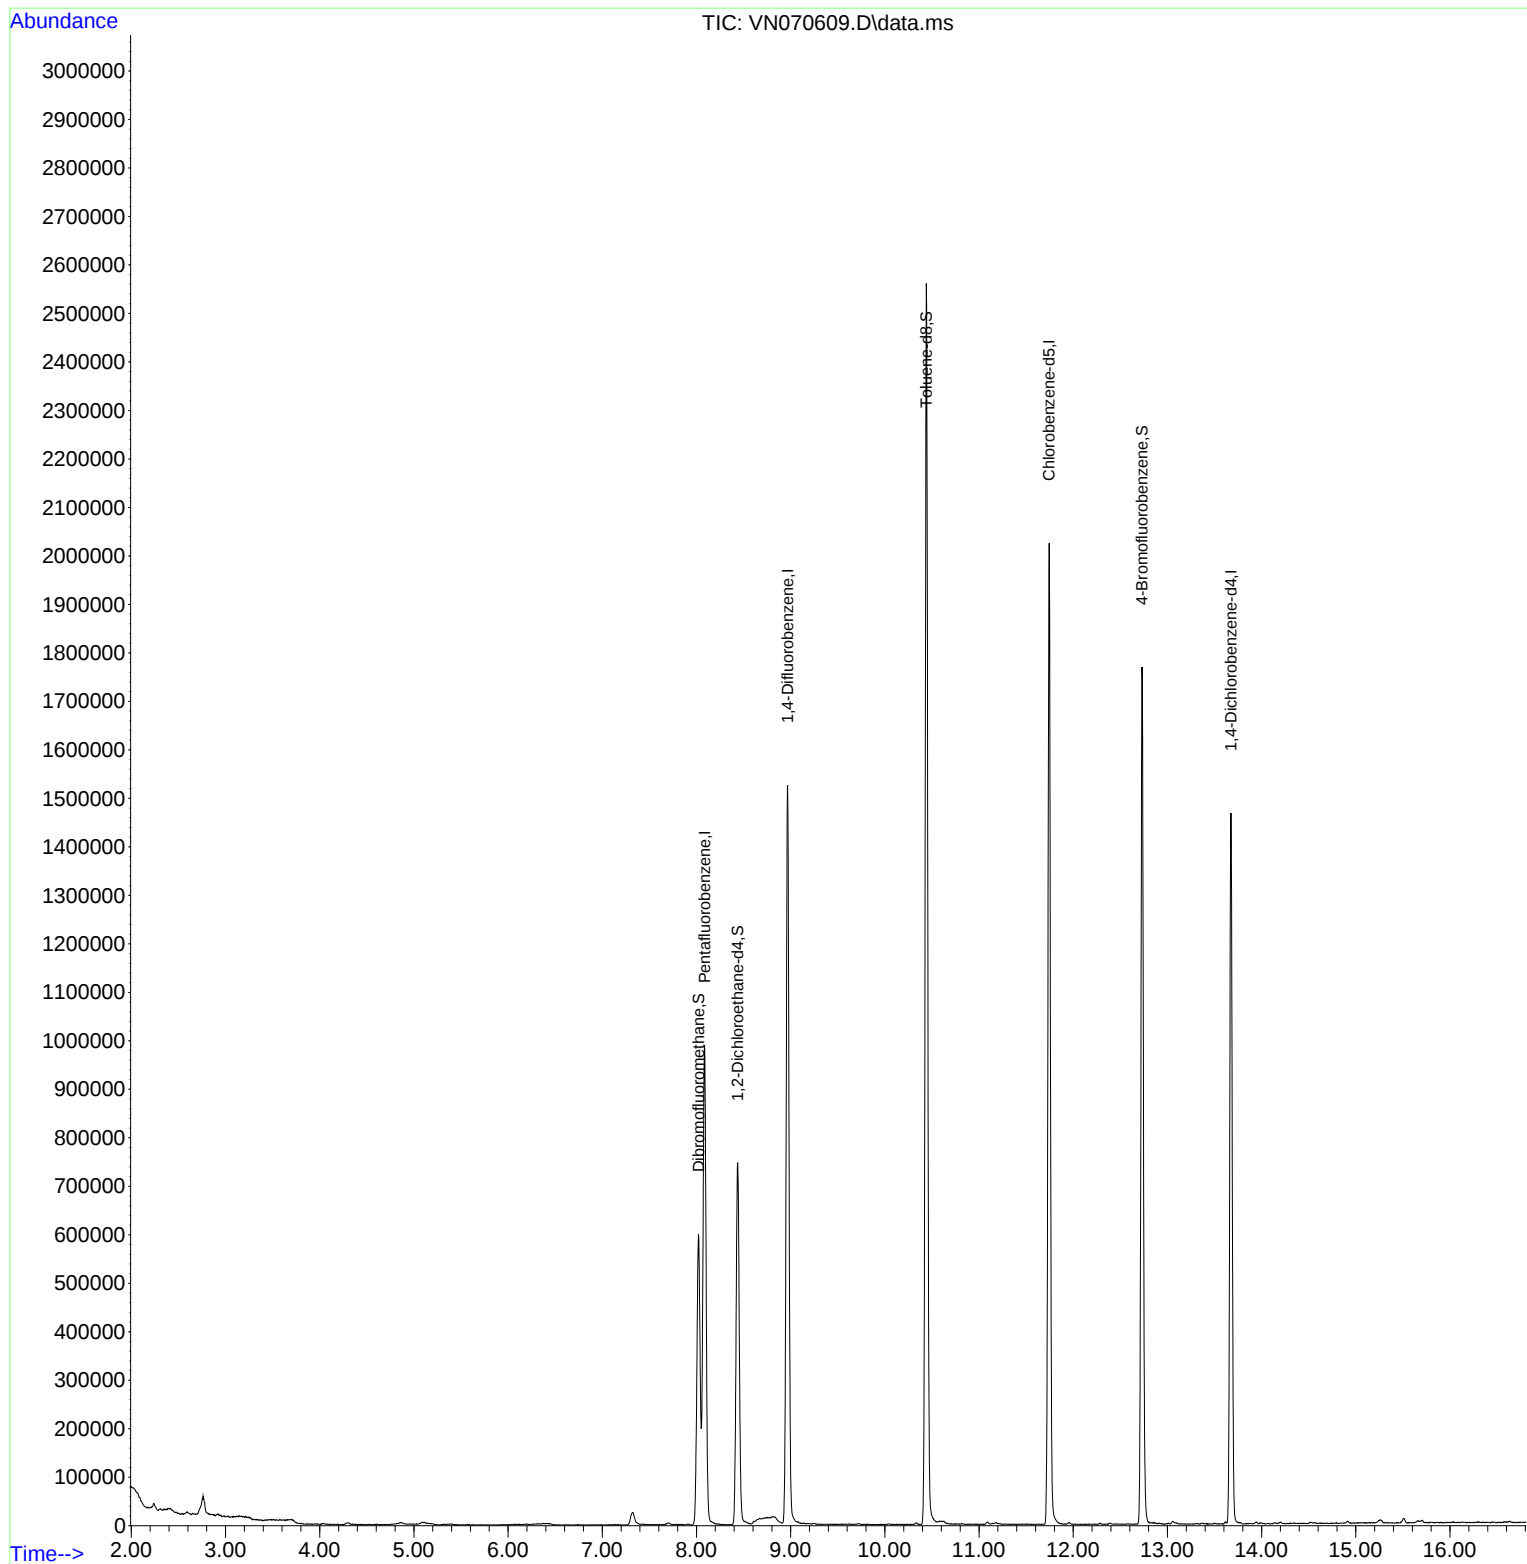


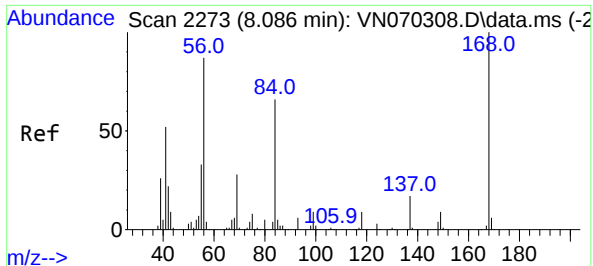

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN070609.D
Acq: 13 Jan 2022 14:08




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 765678
Ion Ratio Lower Upper
168 100
99 58.3 41.3 61.9

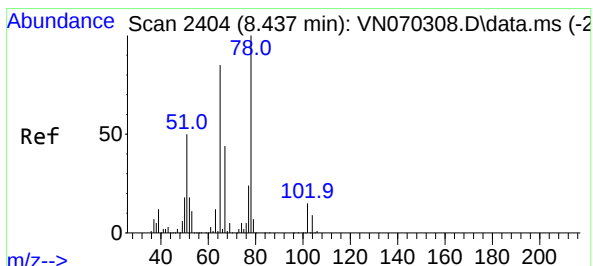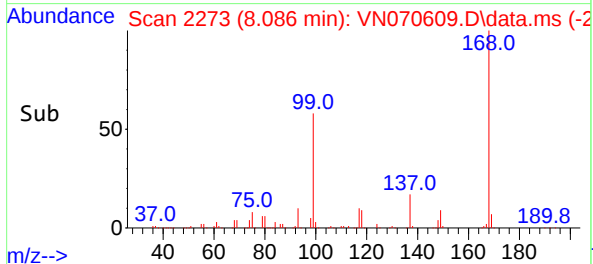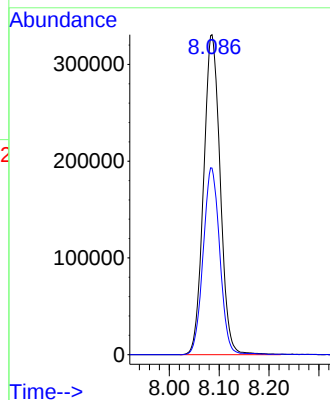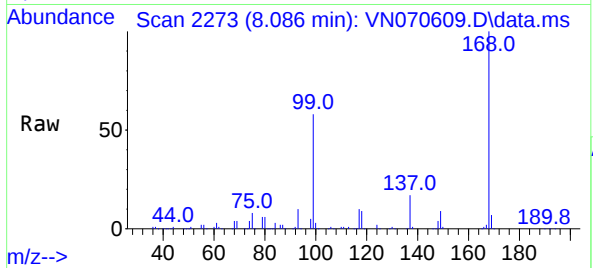

#33
1,2-Dichloroethane-d4
Concen: 57.174 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. -0.000 min
Lab File: VN070609.D
Acq: 13 Jan 2022 14:08

Tgt Ion: 65 Resp: 629423
Ion Ratio Lower Upper
65 100
67 53.7 0.0 103.0

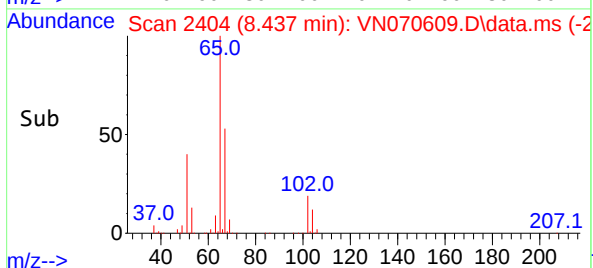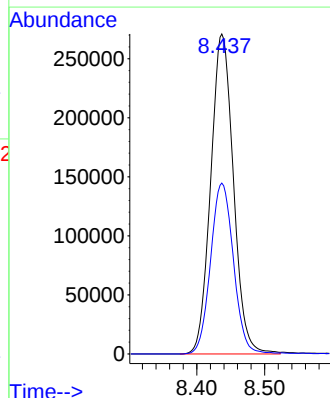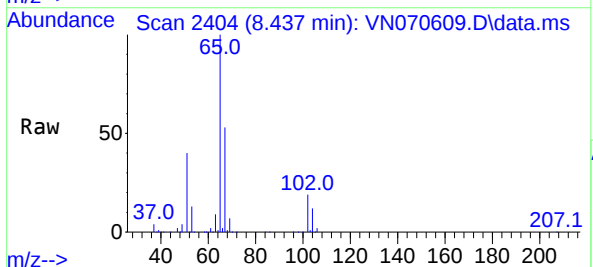

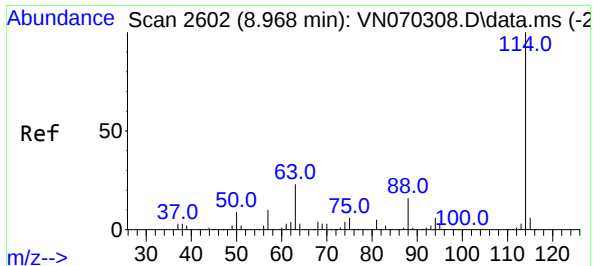

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.968 min Scan# 2602

Delta R.T. -0.000 min

Lab File: VN070609.D

Acq: 13 Jan 2022 14:08

Instrument :

MSVOA_N

ClientSampleId :

IBLK





Tgt Ion:114 Resp: 1300632

Ion Ratio Lower Upper

114 100

63 23.6 0.0 37.8

88 16.6 0.0 27.4

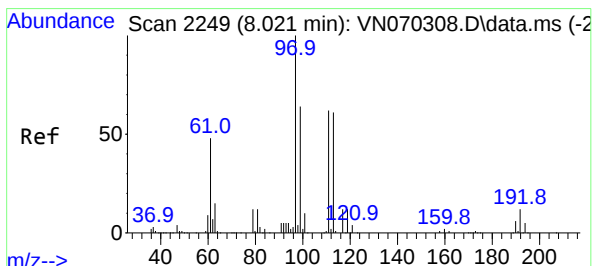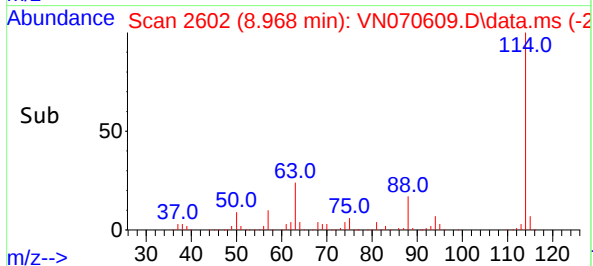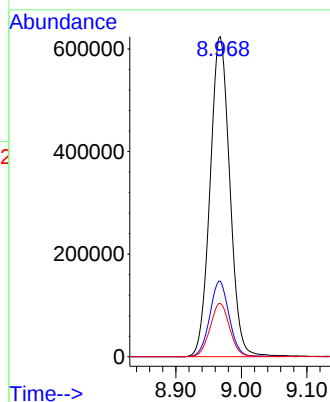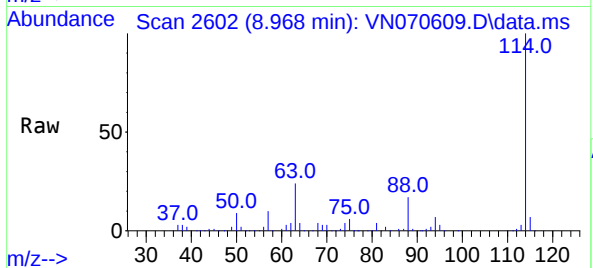

#35

Dibromofluoromethane

Concen: 56.386 ug/l

RT: 8.021 min Scan# 2249

Delta R.T. 0.000 min

Lab File: VN070609.D

Acq: 13 Jan 2022 14:08




Tgt Ion:113 Resp: 443730


Ion Ratio Lower Upper

113 100

111 103.4 82.2 123.2

192 20.0 16.9 25.3


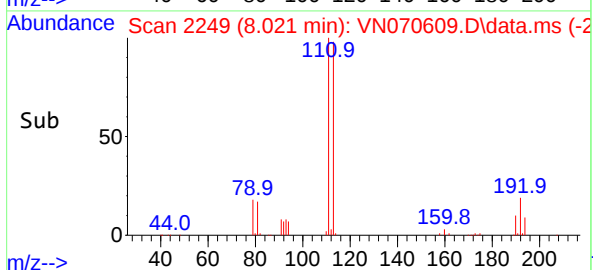
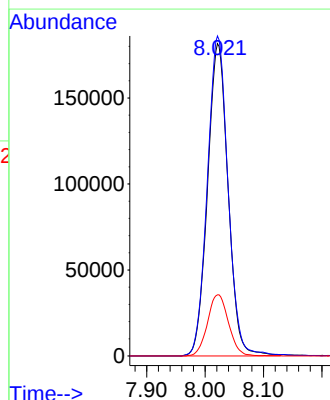
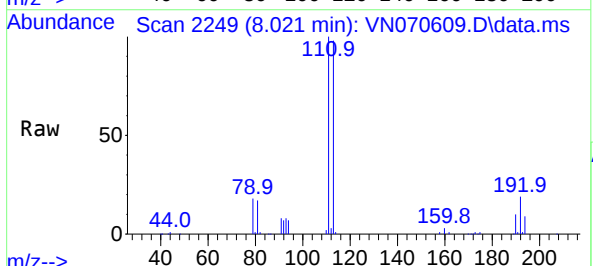


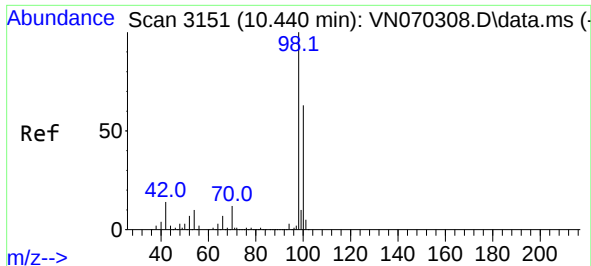

#50
Toluene-d8
Concen: 55.247 ug/l
RT: 10.440 min Scan# 3151
Delta R.T. 0.000 min
Lab File: VN070609.D
Acq: 13 Jan 2022 14:08




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 1776047
Ion Ratio Lower Upper
98 100
100 63.9 50.4 75.6

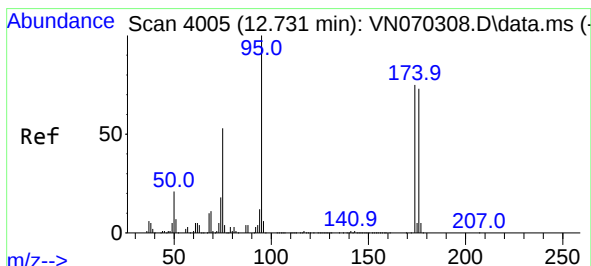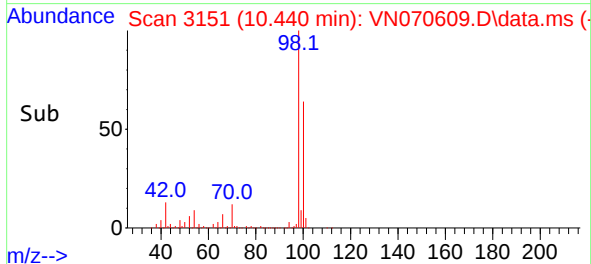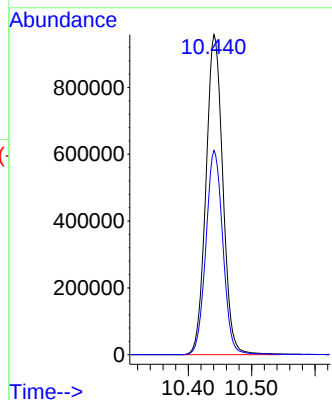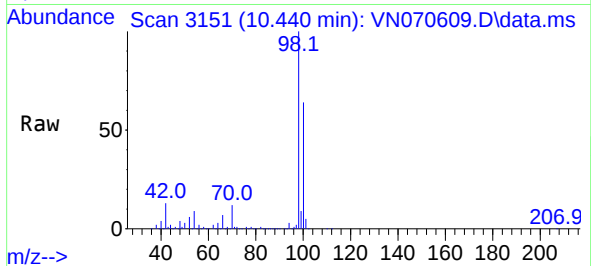

#62
4-Bromofluorobenzene
Concen: 56.151 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.000 min
Lab File: VN070609.D
Acq: 13 Jan 2022 14:08

Tgt Ion: 95 Resp: 651966
Ion Ratio Lower Upper
95 100
174 75.5 0.0 187.2
176 72.3 0.0 181.4


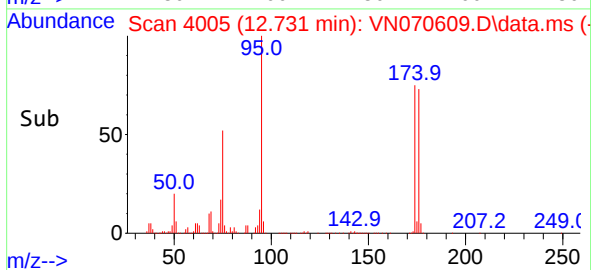
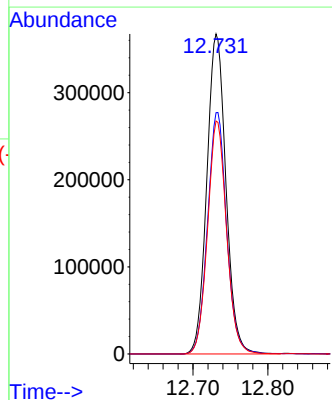
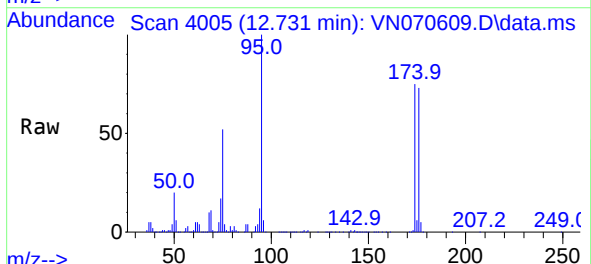


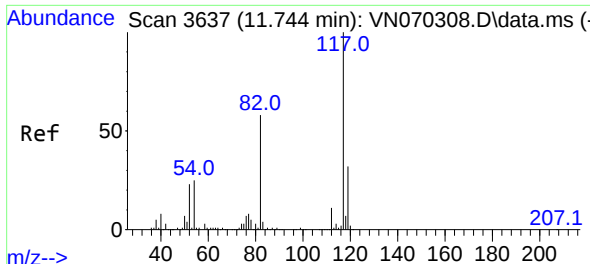

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 30
Delta R.T. -0.000 min
Lab File: VN070609.D
Acq: 13 Jan 2022 14:08

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Tgt Ion:117 Resp: 1169457
Ion Ratio Lower Upper
117 100
82 60.9 42.4 63.6
119 32.4 25.4 38.2

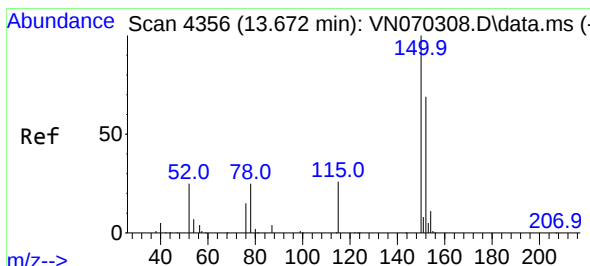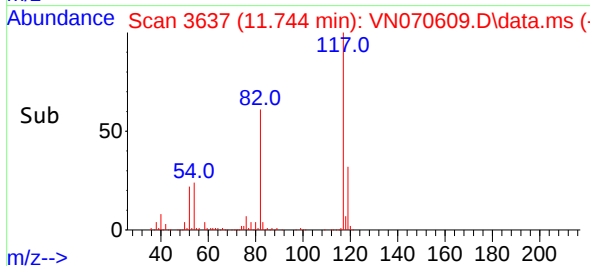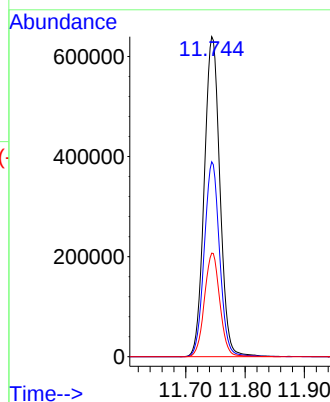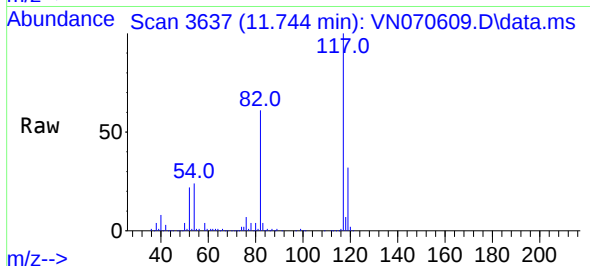

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. 0.003 min
Lab File: VN070609.D
Acq: 13 Jan 2022 14:08

Tgt Ion:152 Resp: 411696
Ion Ratio Lower Upper
152 100
115 60.5 27.5 82.5
150 157.1 0.0 344.4

