

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN011323\  
 Data File : VN076247.D  
 Acq On : 13 Jan 2023 14:39  
 Operator : JC\MD  
 Sample : 01135-02  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 13 Sample Multiplier: 1


Instrument :  
 MSVOA\_N  
 ClientSampleId :


Quant Time: Jan 16 01:08:54 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N121422W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Dec 14 13:03:41 2022  
 Response via : Initial Calibration

| Compound                      | R.T.           | QIon | Response            | Conc   | Units  | Dev(Min) |
|-------------------------------|----------------|------|---------------------|--------|--------|----------|
| -----                         |                |      |                     |        |        |          |
| Internal Standards            |                |      |                     |        |        |          |
| 1) Pentafluorobenzene         | 8.230          | 168  | 351317              | 50.000 | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 9.106          | 114  | 572909              | 50.000 | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 11.871         | 117  | 519263              | 50.000 | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 13.794         | 152  | 218729              | 50.000 | ug/l   | 0.00     |
|                               |                |      |                     |        |        |          |
| System Monitoring Compounds   |                |      |                     |        |        |          |
| 33) 1,2-Dichloroethane-d4     | 8.583          | 65   | 192191              | 50.285 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 74 - 125 |      | Recovery = 100.580% |        |        |          |
| 35) Dibromofluoromethane      | 8.177          | 113  | 169862              | 47.876 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 75 - 124 |      | Recovery = 95.760%  |        |        |          |
| 50) Toluene-d8                | 10.571         | 98   | 676307              | 50.983 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 86 - 113 |      | Recovery = 101.960% |        |        |          |
| 62) 4-Bromofluorobenzene      | 12.853         | 95   | 212661              | 48.402 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 83 - 123 |      | Recovery = 96.800%  |        |        |          |
|                               |                |      |                     |        |        |          |
| Target Compounds              |                |      |                     |        |        | Qvalue   |
| 11) Tert butyl alcohol        | 5.536          | 59   | 327                 | 0.605  | ug/l # | 72       |
| 16) Acetone                   | 4.448          | 43   | 42852               | 32.525 | ug/l   | 99       |
| 18) Methyl Acetate            | 5.053          | 43   | 3645                | 0.936  | ug/l # | 82       |
| 20) Methylene Chloride        | 5.295          | 84   | 12689               | 2.998  | ug/l # | 85       |
| 25) 2-Butanone                | 7.506          | 43   | 6375                | 3.456  | ug/l   | 94       |
| 29) Tetrahydrofuran           | 7.865          | 42   | 325                 | 0.281  | ug/l # | 45       |
| 31) Cyclohexane               | 8.230          | 56   | 7465                | 1.364  | ug/l # | 35       |
| 36) 1,1-Dichloropropene       | 8.230          | 75   | 26509               | 5.625  | ug/l # | 49       |
| 37) Ethyl Acetate             | 7.571          | 43   | 34875               | 9.212  | ug/l   | 97       |
| 38) Carbon Tetrachloride      | 8.236          | 117  | 34755               | 6.589  | ug/l # | 16       |
| 42) 1,2-Dichloroethane        | 8.694          | 62   | 1509                | 0.312  | ug/l # | 72       |
| 43) Isopropyl Acetate         | 8.694          | 43   | 291250              | 46.638 | ug/l # | 74       |
| 45) 1,2-Dichloropropane       | 9.741          | 63   | 2054                | 0.580  | ug/l # | 43       |
| 48) Methyl methacrylate       | 9.671          | 41   | 4943                | 1.757  | ug/l # | 34       |
| 49) 1,4-Dioxane               | 9.747          | 88   | 128                 | 1.851  | ug/l # | 1        |
| 51) 4-Methyl-2-Pentanone      | 10.447         | 43   | 15959               | 4.226  | ug/l # | 72       |
| 53) t-1,3-Dichloropropene     | 10.735         | 75   | 1437                | 0.285  | ug/l   | 97       |
| 54) cis-1,3-Dichloropropene   | 10.359         | 75   | 72637               | 13.131 | ug/l # | 64       |
| 56) Ethyl methacrylate        | 10.982         | 69   | 1982                | 0.401  | ug/l # | 1        |
| 57) 1,3-Dichloropropane       | 11.206         | 76   | 8604                | 1.411  | ug/l # | 42       |
| 59) 2-Hexanone                | 11.171         | 43   | 142743              | 51.827 | ug/l # | 20       |
| 71) Bromoform                 | 12.853         | 173  | 1561                | 0.543  | ug/l # | 1        |
| 74) N-amyl acetate            | 12.488         | 43   | 2192                | 0.473  | ug/l # | 37       |
| 76) 1,2,3-Trichloropropane    | 12.853         | 75   | 114282              | 25.920 | ug/l # | 1        |
| 81) trans-1,4-Dichloro-2-b... | 12.853         | 75   | 114282              | 93.299 | ug/l # | 12       |
| 95) Naphthalene               | 15.641         | 128  | 1146                | 2.270  | ug/l # | 76       |
| -----                         |                |      |                     |        |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Quant Time: Jan 16 01:08:54 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N121422W.M  
Quant Title : SW846 8260  
QLast Update : Wed Dec 14 13:03:41 2022  
Response via : Initial Calibration








#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 8.230 min Scan# 1050  
Delta R.T. -0.000 min  
Lab File: VN076247.D  
Acq: 13 Jan 2023 14:39

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion:168 Resp: 351317  
Ion Ratio Lower Upper  
168 100  
99 59.1 44.2 66.4

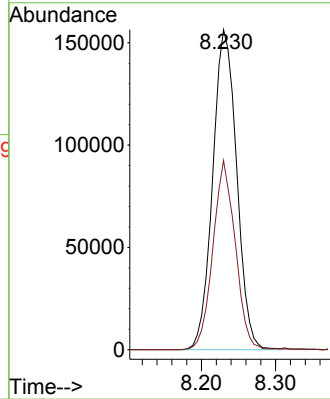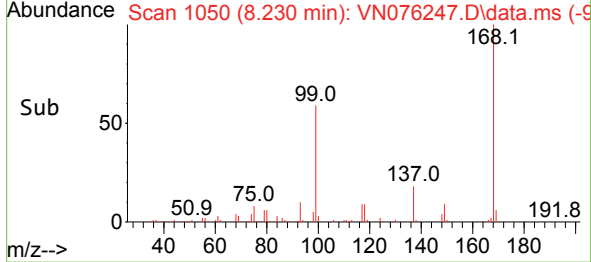

#11  
Tert butyl alcohol  
Concen: 0.605 ug/l  
RT: 5.536 min Scan# 592  
Delta R.T. 0.000 min  
Lab File: VN076247.D  
Acq: 13 Jan 2023 14:39

Tgt Ion: 59 Resp: 327  
Ion Ratio Lower Upper  
59 100  
57 0.0 8.2 12.4#


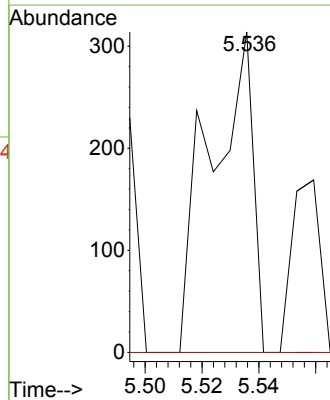
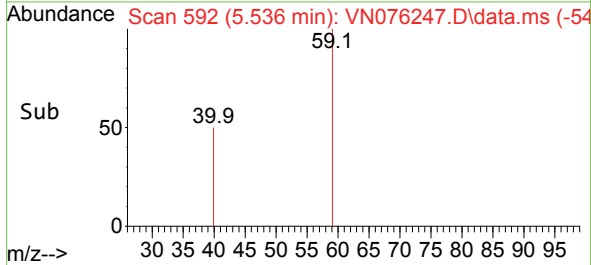



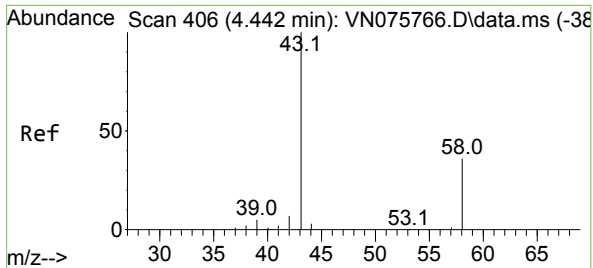

#16  
Acetone  
Concen: 32.525 ug/l  
RT: 4.448 min Scan# 406  
Delta R.T. 0.006 min  
Lab File: VN076247.D  
Acq: 13 Jan 2023 14:39




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 43 Resp: 42852  
Ion Ratio Lower Upper  
43 100  
58 36.2 28.6 43.0

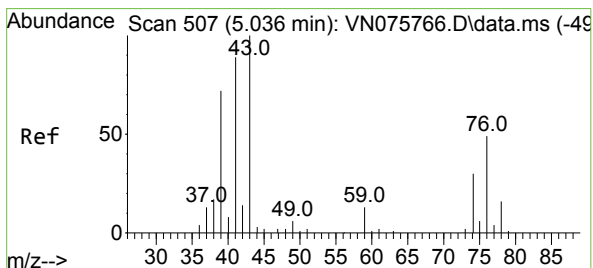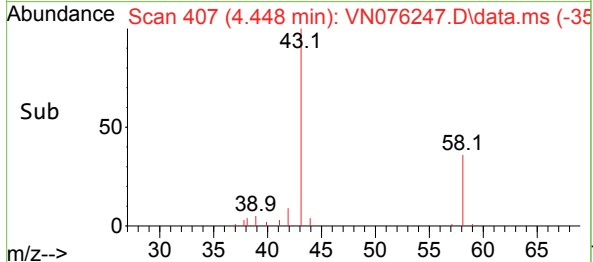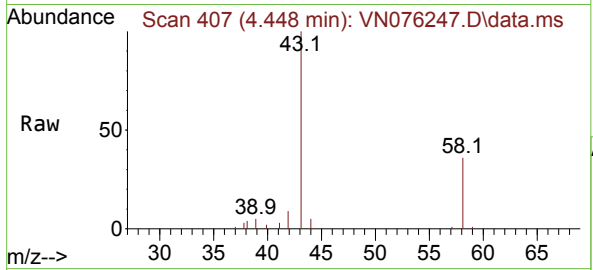

#18  
Methyl Acetate  
Concen: 0.936 ug/l  
RT: 5.053 min Scan# 510  
Delta R.T. 0.018 min  
Lab File: VN076247.D  
Acq: 13 Jan 2023 14:39


Tgt Ion: 43 Resp: 3645  
Ion Ratio Lower Upper  
43 100  
74 19.6 23.6 35.4#

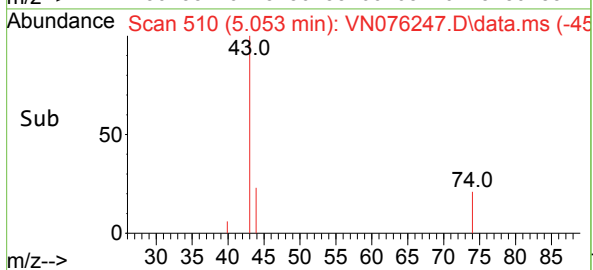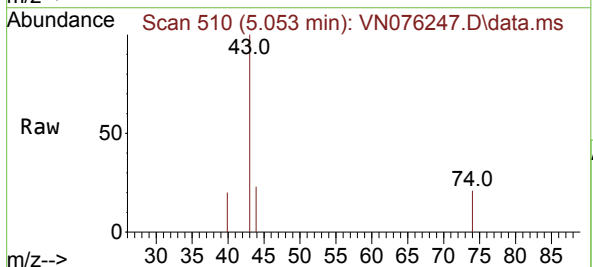






#20  
Methylene Chloride  
Concen: 2.998 ug/l  
RT: 5.295 min Scan# 51  
Delta R.T. 0.006 min  
Lab File: VN076247.D  
Acq: 13 Jan 2023 14:39

Instrument :  
MSVOA\_N  
ClientSampleId :







|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 84    | Resp: | 12689  |
| Ion      | Ratio | Lower | Upper  |
| 84       | 100   |       |        |
| 49       | 77.6  | 81.8  | 122.6# |
| 51       | 26.3  | 26.7  | 40.1#  |
| 86       | 63.4  | 51.5  | 77.3   |

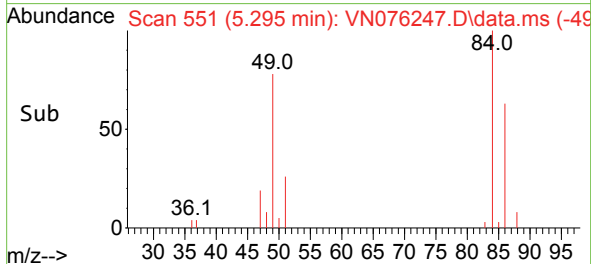

#25  
2-Butanone  
Concen: 3.456 ug/l  
RT: 7.506 min Scan# 927  
Delta R.T. 0.018 min  
Lab File: VN076247.D  
Acq: 13 Jan 2023 14:39

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 43    | Resp: | 6375  |
| Ion      | Ratio | Lower | Upper |
| 43       | 100   |       |       |
| 72       | 31.4  | 28.0  | 42.0  |

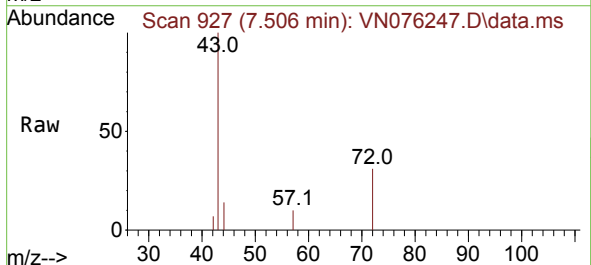



#29

Tetrahydrofuran

Concen: 0.281 ug/l

RT: 7.865 min Scan# 91

Delta R.T. 0.024 min


Lab File: VN076247.D

Acq: 13 Jan 2023 14:39




Instrument :

MSVOA\_N

ClientSampleId :



|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 42    | Resp: | 325   |
| Ion      | Ratio | Lower | Upper |
| 42       | 100   |       |       |
| 72       | 0.0   | 44.5  | 66.7# |
| 71       | 29.5  | 41.0  | 61.6# |

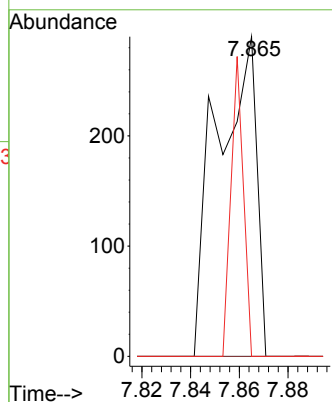

#31

Cyclohexane

Concen: 1.364 ug/l




RT: 8.230 min Scan# 1050


Delta R.T. -0.035 min

Lab File: VN076247.D

Acq: 13 Jan 2023 14:39

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 56    | Resp: | 7465   |
| Ion      | Ratio | Lower | Upper  |
| 56       | 100   |       |        |
| 69       | 138.6 | 24.7  | 37.1#  |
| 84       | 117.7 | 76.5  | 114.7# |





#33

1,2-Dichloroethane-d4

Concen: 50.285 ug/l

RT: 8.583 min Scan# 1110

Delta R.T. 0.000 min

Lab File: VN076247.D

Acq: 13 Jan 2023 14:39

Instrument :

MSVOA\_N





ClientSampleId :

Tgt Ion: 65 Resp: 192191

Ion Ratio Lower Upper

65 100

67 51.5 0.0 103.4

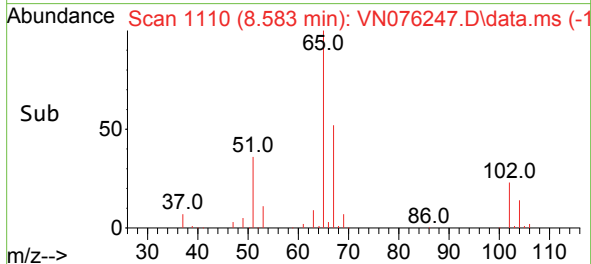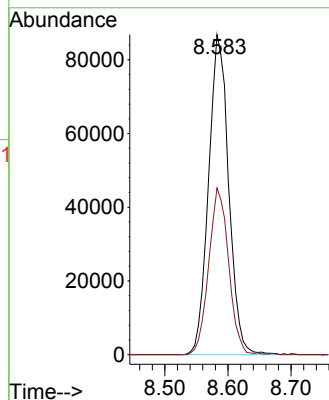

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN076247.D

Acq: 13 Jan 2023 14:39




Tgt Ion: 114 Resp: 572909


Ion Ratio Lower Upper

114 100

63 18.5 0.0 34.4


88 15.5 0.0 28.8

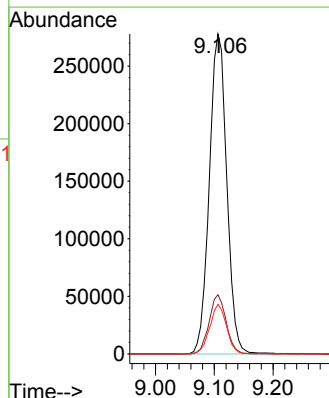






#35  
Dibromofluoromethane  
Concen: 47.876 ug/l  
RT: 8.177 min Scan# 1040  
Delta R.T. 0.006 min  
Lab File: VN076247.D  
Acq: 13 Jan 2023 14:39

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion:113 Resp: 169862  
Ion Ratio Lower Upper  
113 100  
111 104.2 83.4 125.2  
192 19.7 16.1 24.1

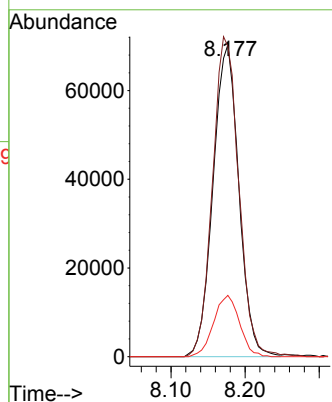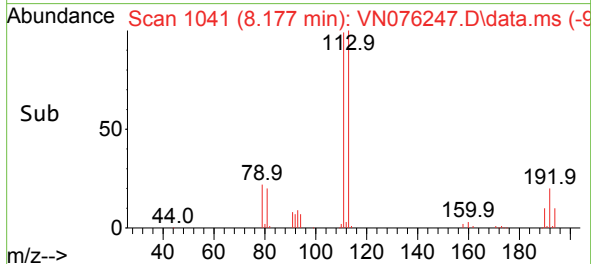

#36  
1,1-Dichloropropene  
Concen: 5.625 ug/l  
RT: 8.230 min Scan# 1050  
Delta R.T. -0.147 min  
Lab File: VN076247.D  
Acq: 13 Jan 2023 14:39


Tgt Ion: 75 Resp: 26509  
Ion Ratio Lower Upper  
75 100  
110 8.6 18.8 56.4#  
77 0.0 24.1 36.1#








#37  
Ethyl Acetate  
Concen: 9.212 ug/l  
RT: 7.571 min Scan# 91  
Delta R.T. 0.006 min  
Lab File: VN076247.D  
Acq: 13 Jan 2023 14:39

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion: 43 Resp: 34875  
Ion Ratio Lower Upper  
43 100  
61 14.5 13.0 19.4  
70 11.4 9.4 14.0

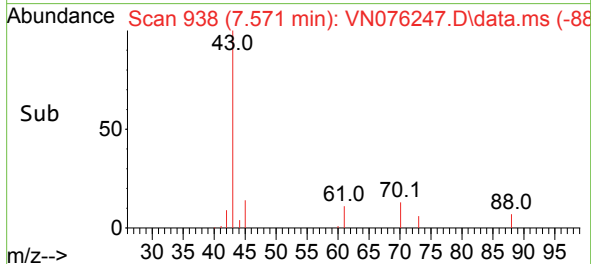

#38  
Carbon Tetrachloride  
Concen: 6.589 ug/l  
RT: 8.236 min Scan# 1051  
Delta R.T. -0.129 min  
Lab File: VN076247.D  
Acq: 13 Jan 2023 14:39

Tgt Ion: 117 Resp: 34755  
Ion Ratio Lower Upper  
117 100  
119 4.9 76.1 114.1#  
121 0.0 24.5 36.7#





#42

1,2-Dichloroethane

Concen: 0.312 ug/l

RT: 8.694 min Scan# 1129

Delta R.T. 0.018 min

Lab File: VN076247.D

Acq: 13 Jan 2023 14:39

Instrument :

MSVOA\_N





ClientSampleId :

Tgt Ion: 62 Resp: 1509

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.8

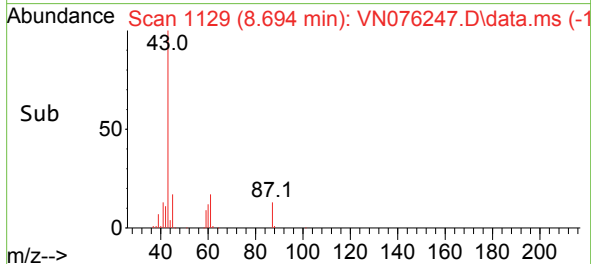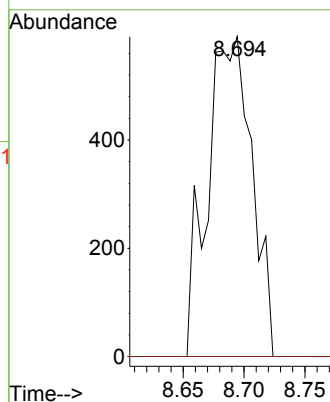

#43

Isopropyl Acetate

Concen: 46.638 ug/l

RT: 8.694 min Scan# 1129

Delta R.T. 0.000 min

Lab File: VN076247.D

Acq: 13 Jan 2023 14:39




Tgt Ion: 43 Resp: 291250


Ion Ratio Lower Upper

43 100

61 13.2 24.2 36.4#

87 9.8 13.3 19.9#

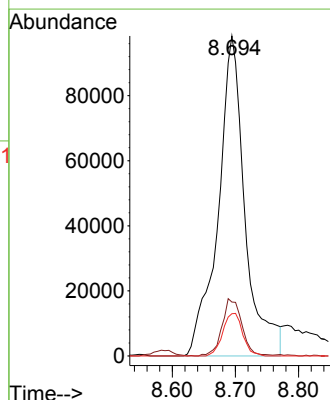



#45

1,2-Dichloropropane

Concen: 0.580 ug/l

RT: 9.741 min Scan# 11

Delta R.T. 0.118 min

Lab File: VN076247.D

Acq: 13 Jan 2023 14:39

Instrument :

MSVOA\_N





ClientSampleId :

Tgt Ion: 63 Resp: 2054

Ion Ratio Lower Upper

63 100

65 0.0 25.7 38.5#

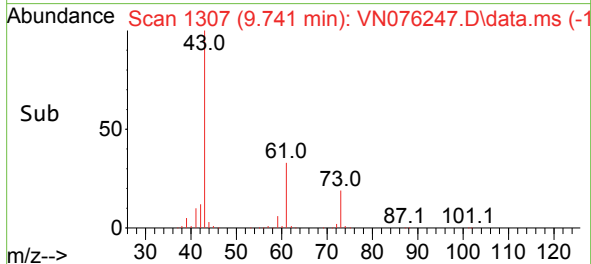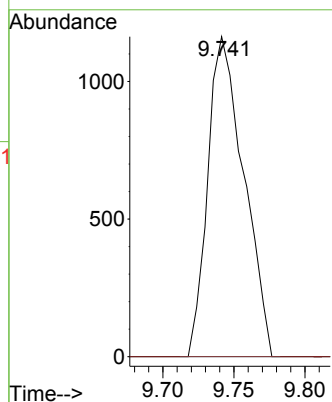

#48

Methyl methacrylate

Concen: 1.757 ug/l

RT: 9.671 min Scan# 1295

Delta R.T. -0.012 min

Lab File: VN076247.D

Acq: 13 Jan 2023 14:39




Tgt Ion: 41 Resp: 4943


Ion Ratio Lower Upper

41 100

69 0.0 81.9 122.9#

39 55.5 51.6 77.4





#49

1,4-Dioxane

Concen: 1.851 ug/l

RT: 9.747 min Scan# 1308

Delta R.T. 0.047 min

Lab File: VN076247.D

Acq: 13 Jan 2023 14:39

Instrument :

MSVOA\_N

ClientSampleId :





Tgt Ion: 88 Resp: 128

Ion Ratio Lower Upper

88 100

43 1139691.4 17.1 25.7#

58 5627.3 47.8 71.8#

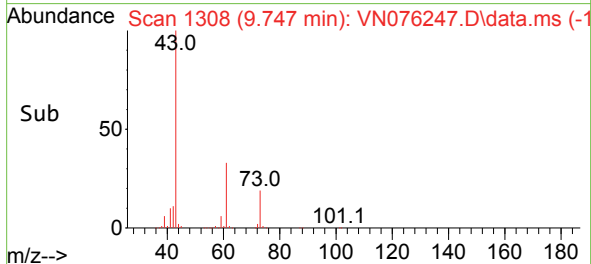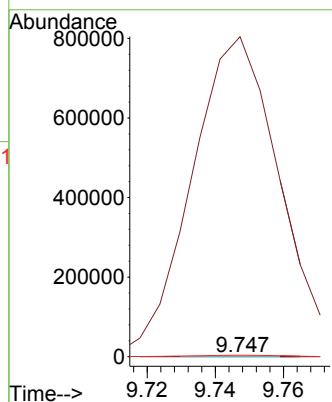

#50

Toluene-d8

Concen: 50.983 ug/l

RT: 10.571 min Scan# 1448

Delta R.T. 0.000 min

Lab File: VN076247.D




Acq: 13 Jan 2023 14:39


Tgt Ion: 98 Resp: 676307

Ion Ratio Lower Upper

98 100

100 65.7 52.1 78.1









#51  
4-Methyl-2-Pentanone  
Concen: 4.226 ug/l  
RT: 10.447 min Scan# 1427  
Delta R.T. 0.000 min  
Lab File: VN076247.D  
Acq: 13 Jan 2023 14:39




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 43 Resp: 15959  
Ion Ratio Lower Upper  
43 100  
58 26.0 35.5 53.3#

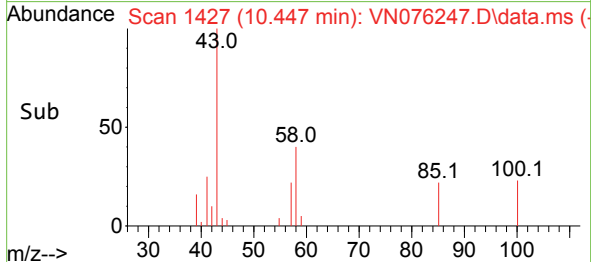

#53  
t-1,3-Dichloropropene  
Concen: 0.285 ug/l  
RT: 10.735 min Scan# 1476  
Delta R.T. -0.100 min  
Lab File: VN076247.D  
Acq: 13 Jan 2023 14:39

Tgt Ion: 75 Resp: 1437  
Ion Ratio Lower Upper  
75 100  
77 32.6 24.9 37.3


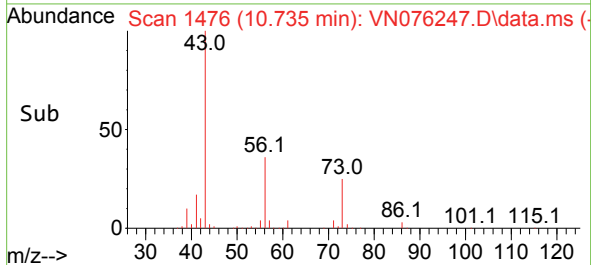




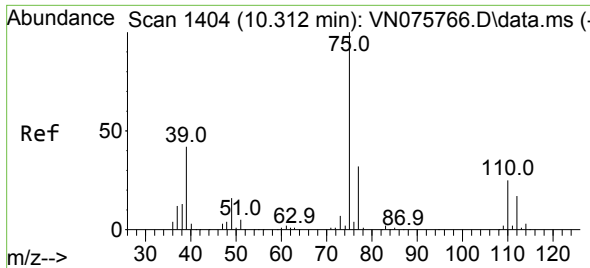

#54  
 cis-1,3-Dichloropropene  
 Concen: 13.131 ug/l  
 RT: 10.359 min Scan# 14  
 Delta R.T. 0.047 min  
 Lab File: VN076247.D  
 Acq: 13 Jan 2023 14:39




Instrument :  
 MSVOA\_N  
 ClientSampleId :


Tgt Ion: 75 Resp: 72637  
 Ion Ratio Lower Upper  
 75 100  
 77 0.4 25.8 38.8#  
 39 29.0 33.4 50.2#

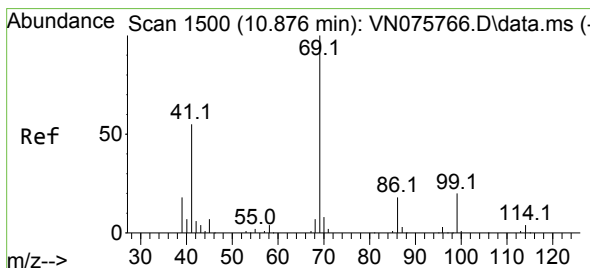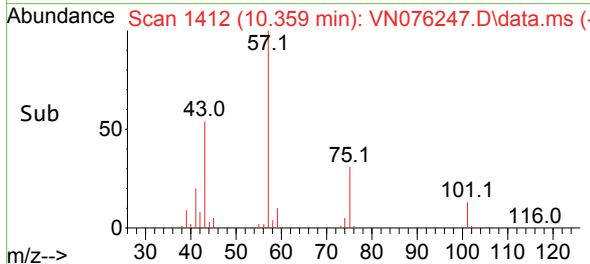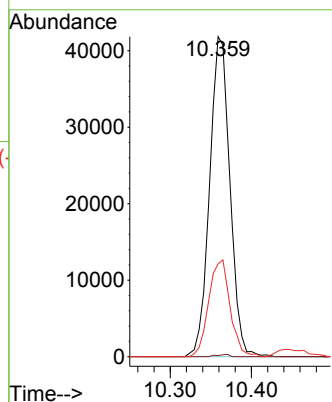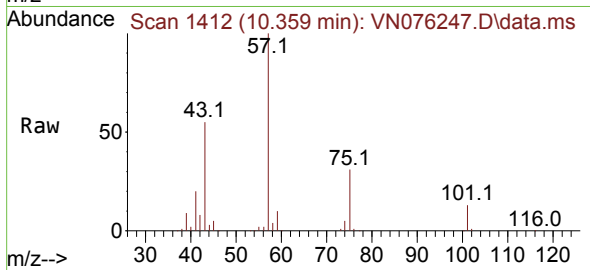

#56  
 Ethyl methacrylate  
 Concen: 0.401 ug/l  
 RT: 10.982 min Scan# 1518  
 Delta R.T. 0.106 min  
 Lab File: VN076247.D  
 Acq: 13 Jan 2023 14:39

Tgt Ion: 69 Resp: 1982  
 Ion Ratio Lower Upper  
 69 100  
 41 5111.1 44.2 66.4#  
 39 2303.3 26.4 39.6#

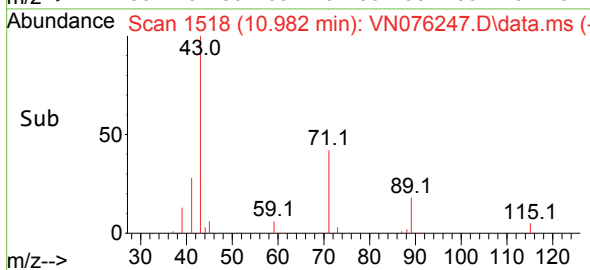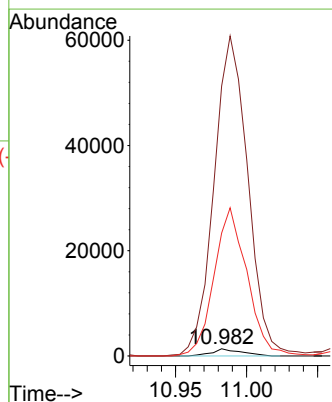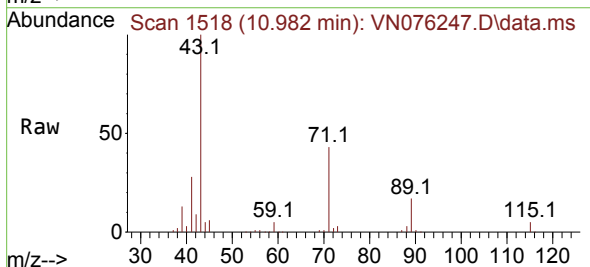

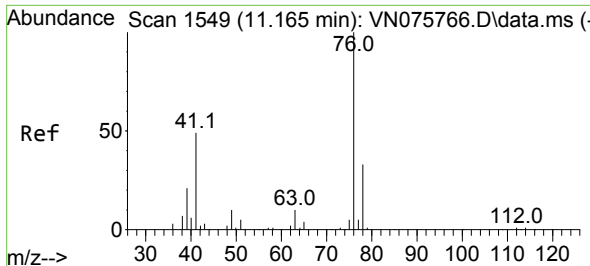

#57

1,3-Dichloropropane

Concen: 1.411 ug/l

RT: 11.206 min Scan# 11

Delta R.T. 0.041 min

Lab File: VN076247.D

Acq: 13 Jan 2023 14:39

Instrument :

MSVOA\_N





ClientSampleId :

Tgt Ion: 76 Resp: 8604

Ion Ratio Lower Upper

76 100

78 0.0 26.2 39.2#

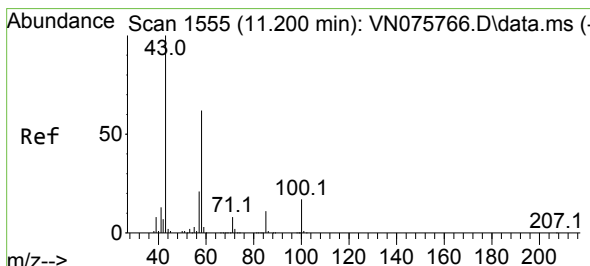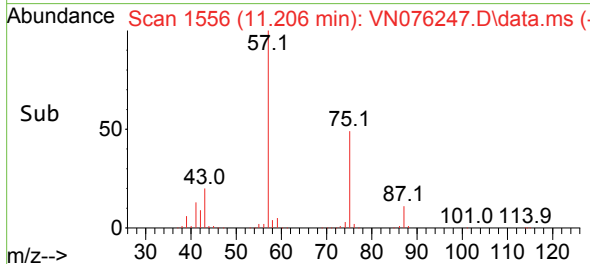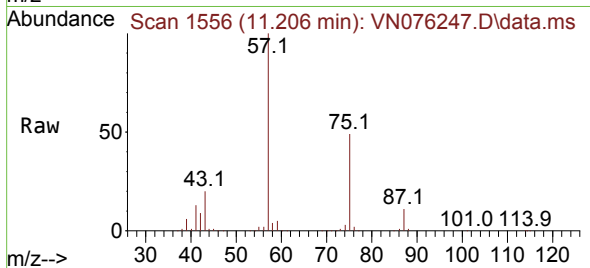

#59

2-Hexanone

Concen: 51.827 ug/l

RT: 11.171 min Scan# 1550

Delta R.T. -0.029 min

Lab File: VN076247.D




Acq: 13 Jan 2023 14:39


Tgt Ion: 43 Resp: 142743

Ion Ratio Lower Upper

43 100

58 0.0 30.6 92.0#

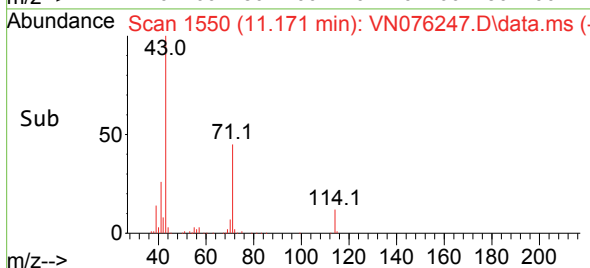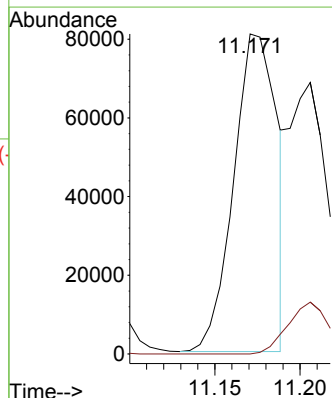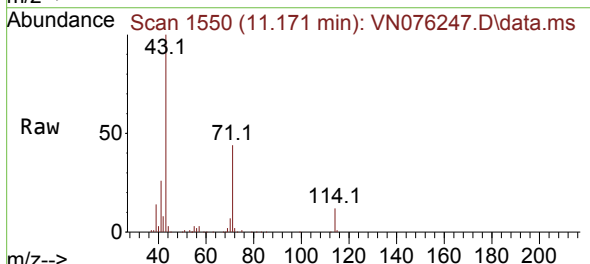



#62

4-Bromofluorobenzene

Concen: 48.402 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. 0.000 min

Lab File: VN076247.D

Acq: 13 Jan 2023 14:39

Instrument :

MSVOA\_N

ClientSampleId :





Tgt Ion: 95 Resp: 212661

Ion Ratio Lower Upper

95 100

174 86.5 0.0 171.6

176 83.9 0.0 169.2

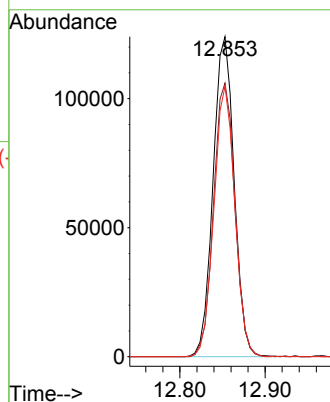

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.871 min Scan# 1669

Delta R.T. 0.006 min

Lab File: VN076247.D

Acq: 13 Jan 2023 14:39




Tgt Ion: 117 Resp: 519263


Ion Ratio Lower Upper

117 100

82 51.0 41.3 61.9

119 30.9 24.6 37.0

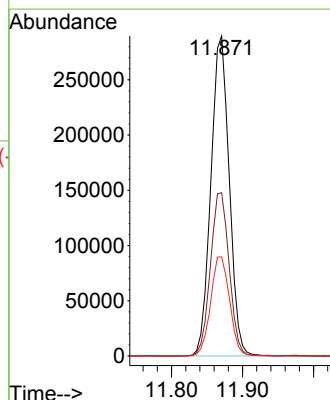



#71

Bromoform

Concen: 0.543 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. 0.271 min


Lab File: VN076247.D

Acq: 13 Jan 2023 14:39

Instrument :

MSVOA\_N

ClientSampleId :






Tgt Ion:173 Resp: 1561

Ion Ratio Lower Upper

173 100

175 702.3 24.3 72.8#

254 0.0 0.0 0.0

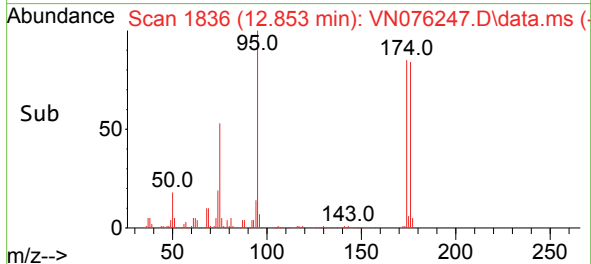

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 1996

Delta R.T. 0.000 min

Lab File: VN076247.D

Acq: 13 Jan 2023 14:39




Tgt Ion:152 Resp: 218729


Ion Ratio Lower Upper

152 100

115 57.5 29.1 87.4

150 155.8 0.0 347.0









#74  
N-amy1 acetate  
Concen: 0.473 ug/l  
RT: 12.488 min Scan# 1774  
Delta R.T. -0.006 min  
Lab File: VN076247.D  
Acq: 13 Jan 2023 14:39




Instrument :  
MSVOA\_N  
ClientSampleId :


|             |                |
|-------------|----------------|
| Tgt Ion: 43 | Resp: 2192     |
| Ion Ratio   | Lower Upper    |
| 43          | 100            |
| 70          | 0.0 41.4 62.0# |
| 55          | 0.0 21.3 31.9# |
| 61          | 0.0 21.2 31.8# |

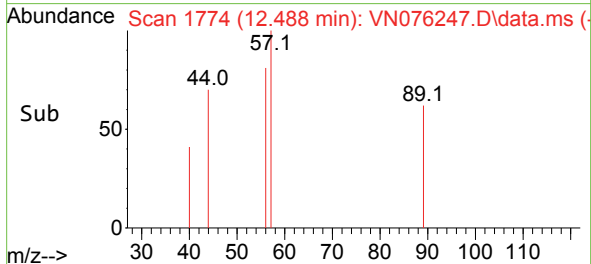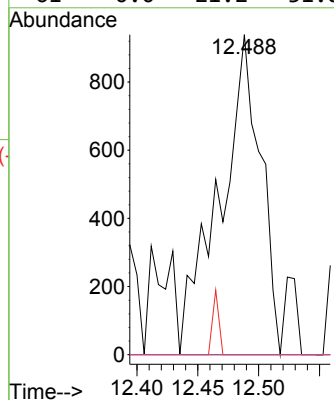

#76  
1,2,3-Trichloropropane  
Concen: 25.920 ug/l  
RT: 12.853 min Scan# 1836  
Delta R.T. -0.141 min  
Lab File: VN076247.D  
Acq: 13 Jan 2023 14:39


|             |                 |
|-------------|-----------------|
| Tgt Ion: 75 | Resp: 114282    |
| Ion Ratio   | Lower Upper     |
| 75          | 100             |
| 77          | 1.1 82.6 247.8# |

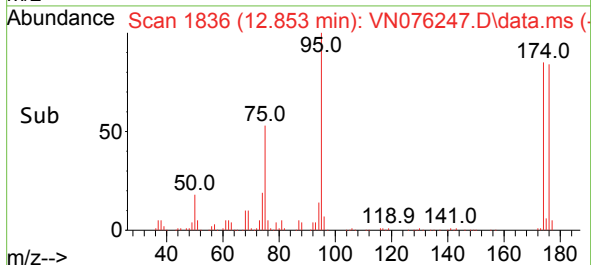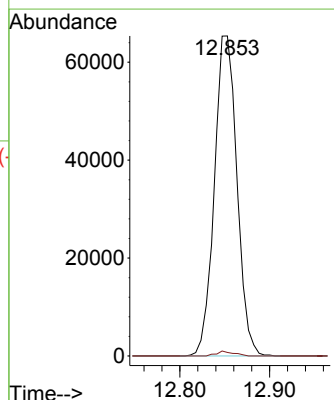






#81  
trans-1,4-Dichloro-2-butene  
Concen: 93.299 ug/l  
RT: 12.853 min Scan# 11  
Delta R.T. 0.112 min  
Lab File: VN076247.D  
Acq: 13 Jan 2023 14:39


Instrument :  
MSVOA\_N  
ClientSampleId :



Tgt Ion: 75 Resp: 114282  
Ion Ratio Lower Upper  
75 100  
53 0.0 73.8 110.6#  
89 0.0 39.5 59.3#

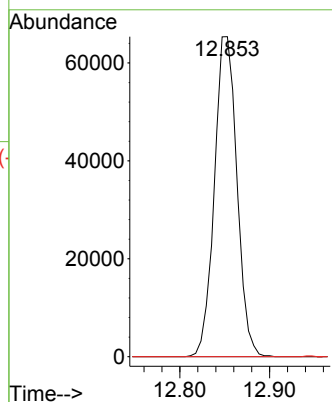

#95  
Naphthalene  
Concen: 2.270 ug/l  
RT: 15.641 min Scan# 2310  
Delta R.T. -0.000 min  
Lab File: VN076247.D  
Acq: 13 Jan 2023 14:39



Tgt Ion:128 Resp: 1146  
Ion Ratio Lower Upper  
128 100  
127 5.0 10.4 15.6#  
129 0.0 8.7 13.1#

