
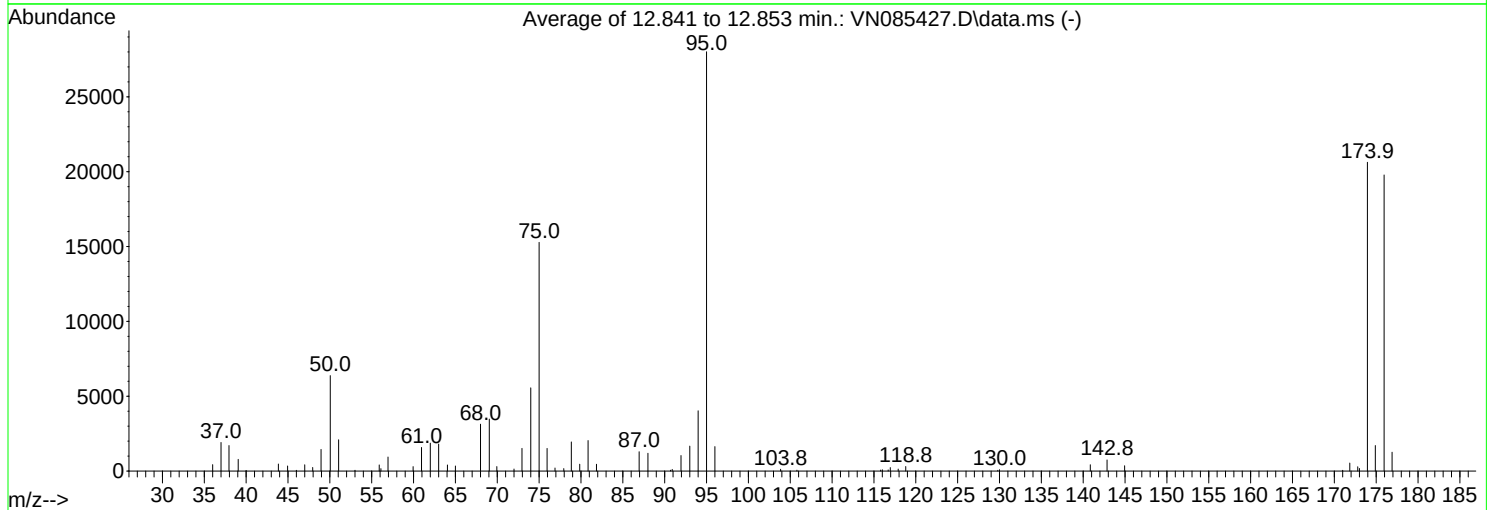


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011325\
Data File : VN085427.D
Acq On : 13 Jan 2025 13:04
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122724W.M
Title : SW846 8260
Last Update : Sat Dec 28 01:36:16 2024

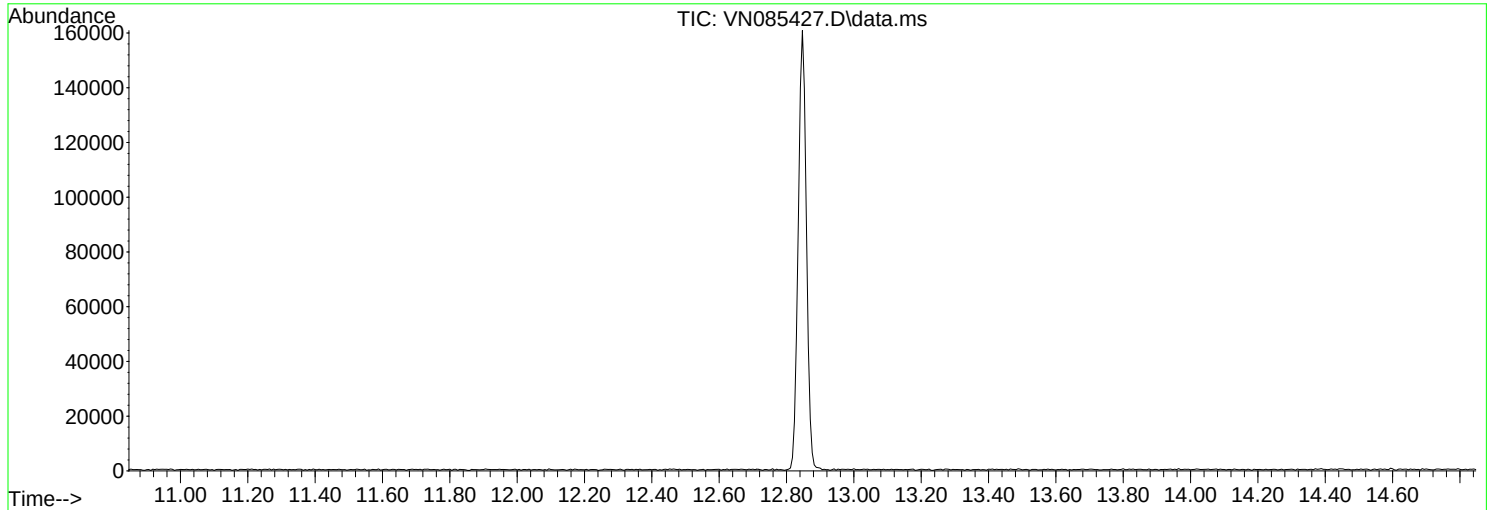

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	6378	PASS
75	95	30	60	54.5	15281	PASS
95	95	100	100	100.0	28013	PASS
96	95	5	9	5.8	1637	PASS
173	174	0.00	2	1.4	289	PASS
174	95	50	100	73.6	20629	PASS
175	174	5	9	8.3	1706	PASS
176	174	95	101	95.9	19781	PASS
177	176	5	9	6.4	1261	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	429	50.05	6378	65.00	341	78.85	1946
37.00	1912	51.05	2090	68.00	3134	79.85	460
37.95	1706	53.00	56	69.05	3472	80.85	2038
39.05	783	55.90	410	69.95	301	81.85	454
40.00	37	56.10	163	72.00	139	86.95	1292
43.85	473	56.95	940	72.95	1516	88.00	1189
44.95	340	59.95	299	74.00	5559	90.70	58
46.00	51	60.95	1577	75.00	15281	90.90	113
47.00	419	62.00	1866	75.95	1514	91.95	1038
47.95	242	63.00	1807	76.90	204	93.00	1666
48.95	1446	64.05	406	77.95	166	94.00	4029

Average of 12.841 to 12.853 min.: VN085427.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.00	28013	130.00	92	176.90	1261		
96.00	1637	140.85	422				
103.85	122	142.85	744				
105.80	60	144.95	357				
115.80	69	171.00	51				
116.00	89	171.85	535				
116.70	76	172.80	289				
116.95	234	173.00	174				
117.90	134	173.95	20629				
118.80	304	174.90	1706				
129.80	51	175.95	19781				

Instrument :

MSVOA_N

ClientSampleId :

BFB