


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN011419\
 Data File : VN053378.D
 Acq On : 14 Jan 2019 8:24
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N010519W.M
 Title : SW846 8260
 Last Update : Mon Jan 07 09:34:27 2019

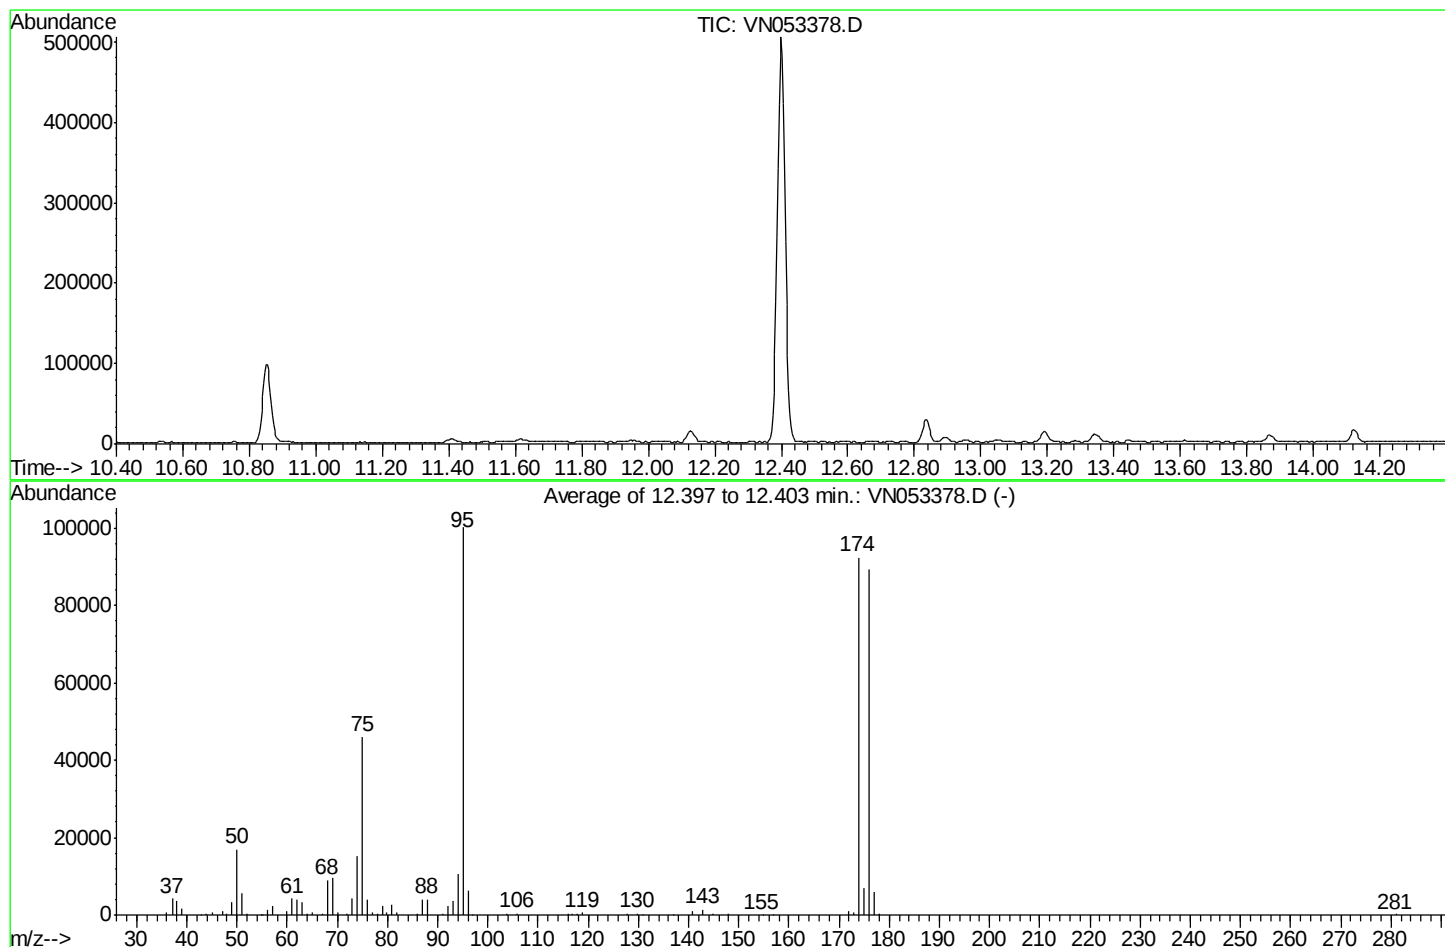

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	16963	PASS
75	95	30	60	45.9	46000	PASS
95	95	100	100	100.0	100192	PASS
96	95	5	9	6.2	6250	PASS
173	174	0.00	2	0.7	616	PASS
174	95	50	100	92.3	92445	PASS
175	174	5	9	7.7	7080	PASS
176	174	95	101	96.6	89282	PASS
177	176	5	9	6.6	5850	PASS