


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN011420\
 Data File : VN059694.D
 Acq On : 14 Jan 2020 8:44
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011320W.M
 Title : SW846 8260
 Last Update : Tue Jan 14 08:58:21 2020

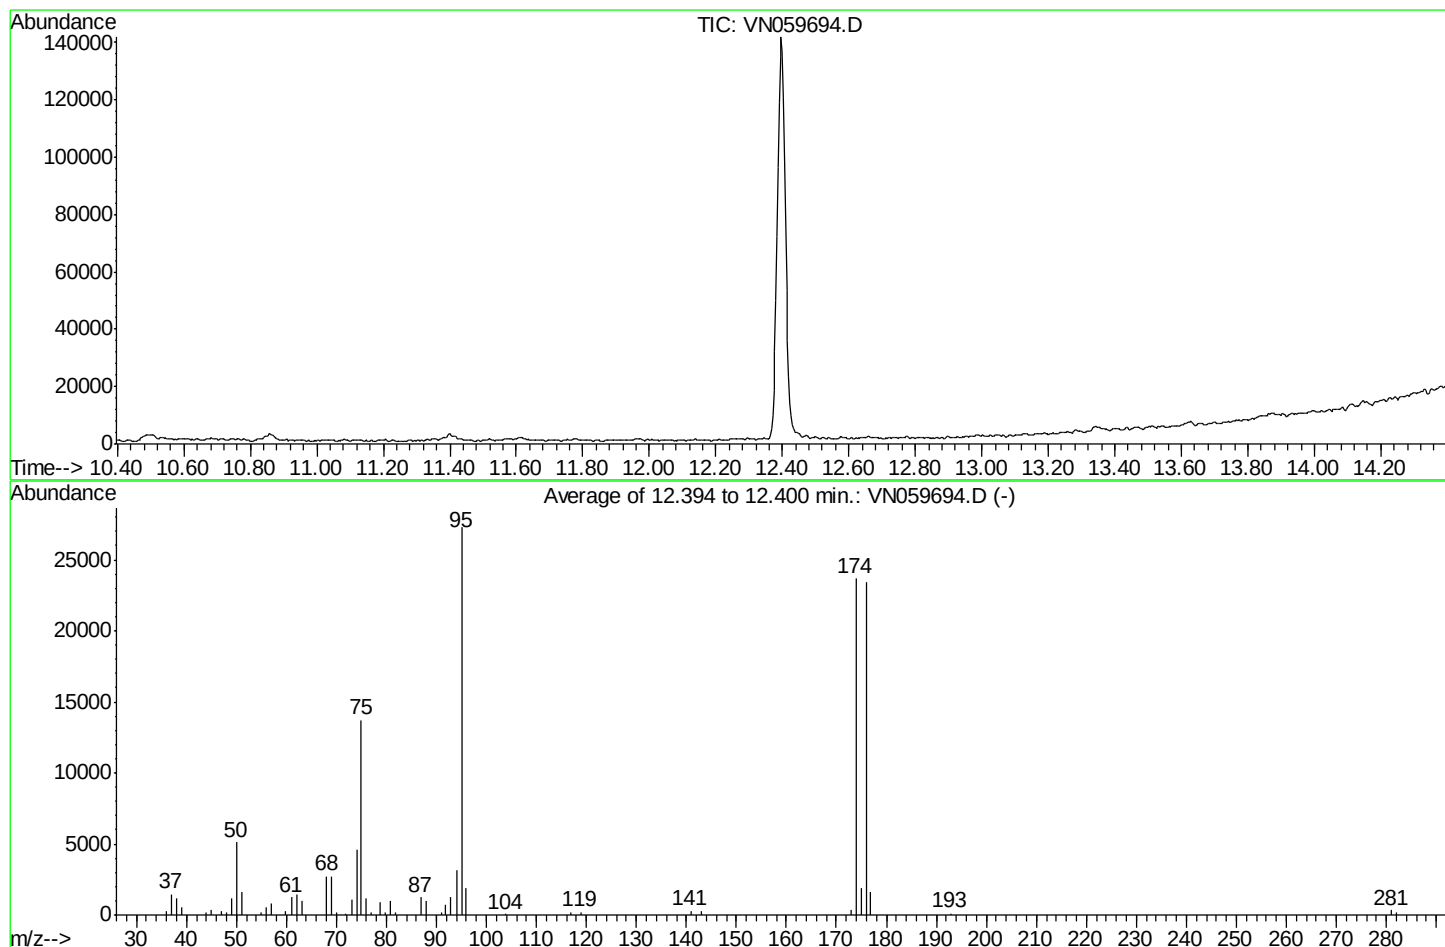

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	5118	PASS
75	95	30	60	50.3	13722	PASS
95	95	100	100	100.0	27290	PASS
96	95	5	9	7.0	1911	PASS
173	174	0.00	2	1.6	376	PASS
174	95	50	100	86.8	23696	PASS
175	174	5	9	7.9	1864	PASS
176	174	95	101	98.7	23392	PASS
177	176	5	9	7.0	1646	PASS