




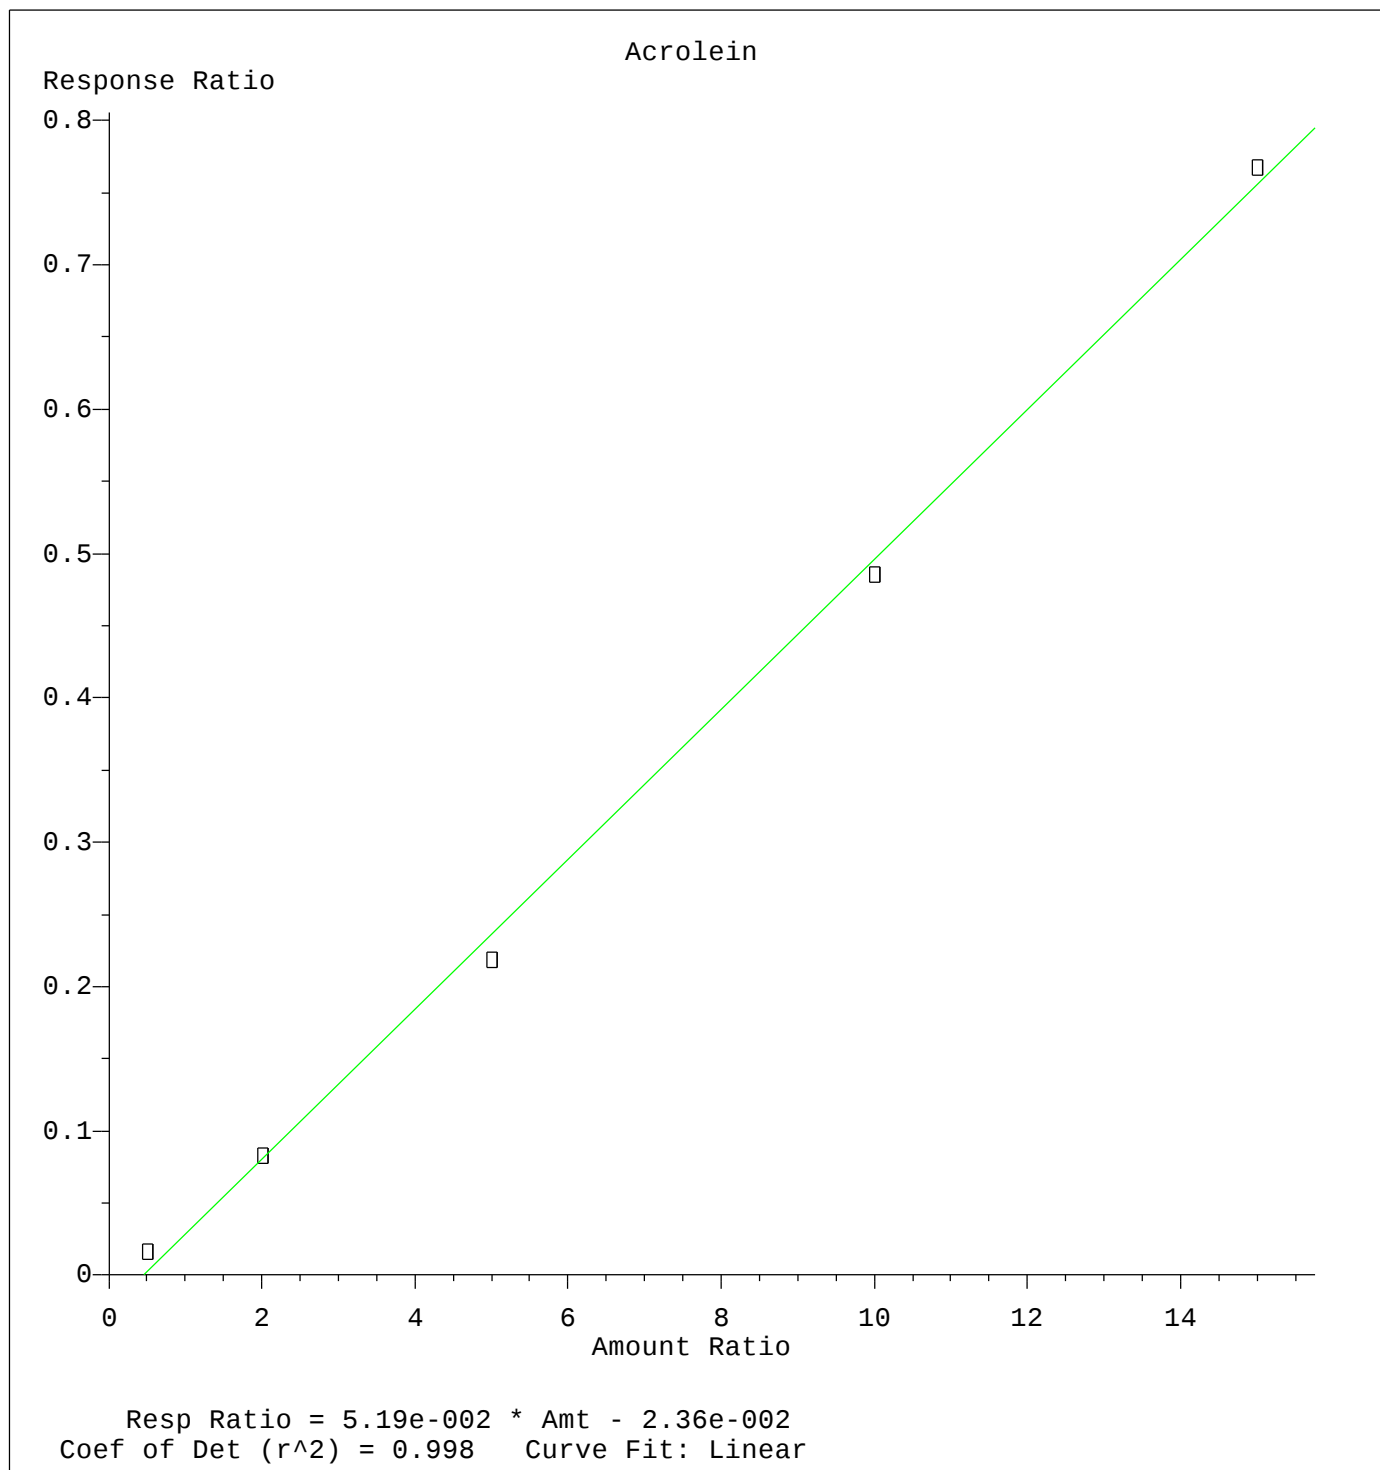


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011519W.M
Calibration Table Last Updated: Wed Jan 16 03:10:53 2019

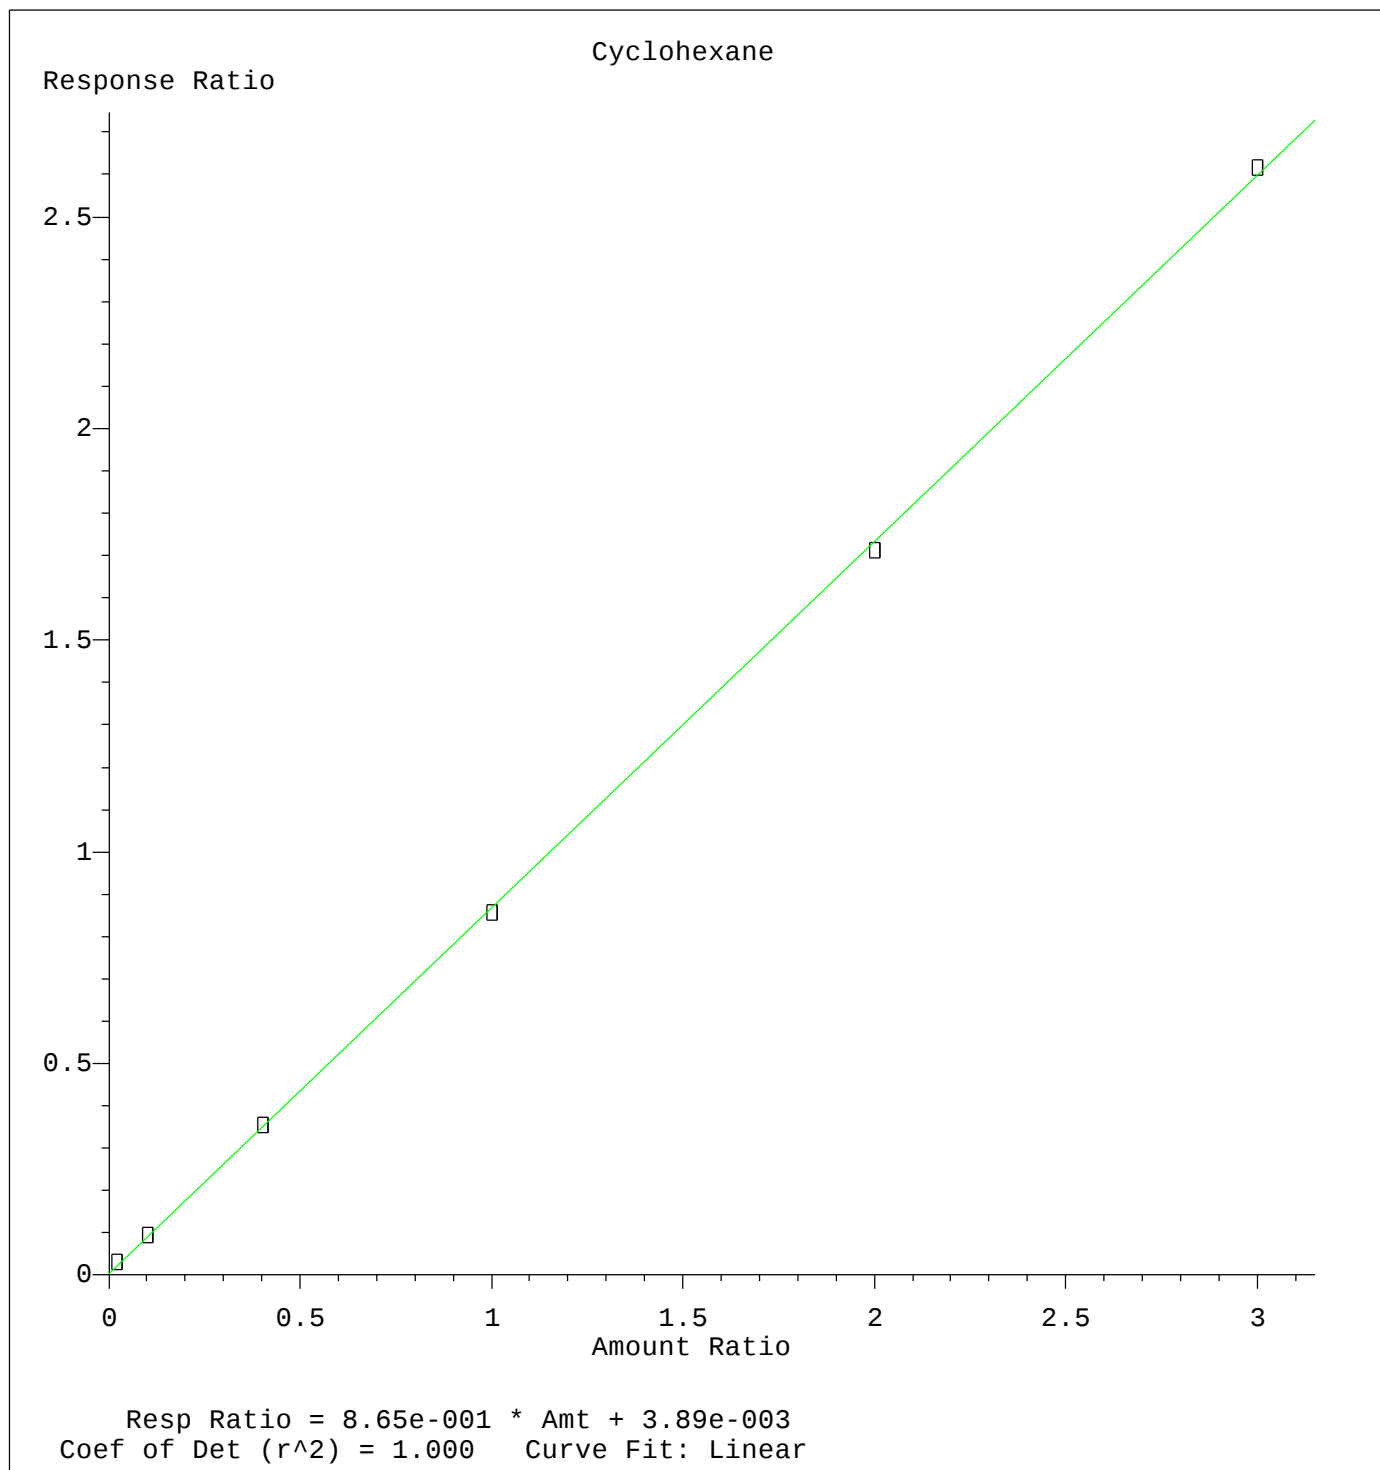

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011519W.M
Calibration Table Last Updated: Wed Jan 16 03:10:53 2019

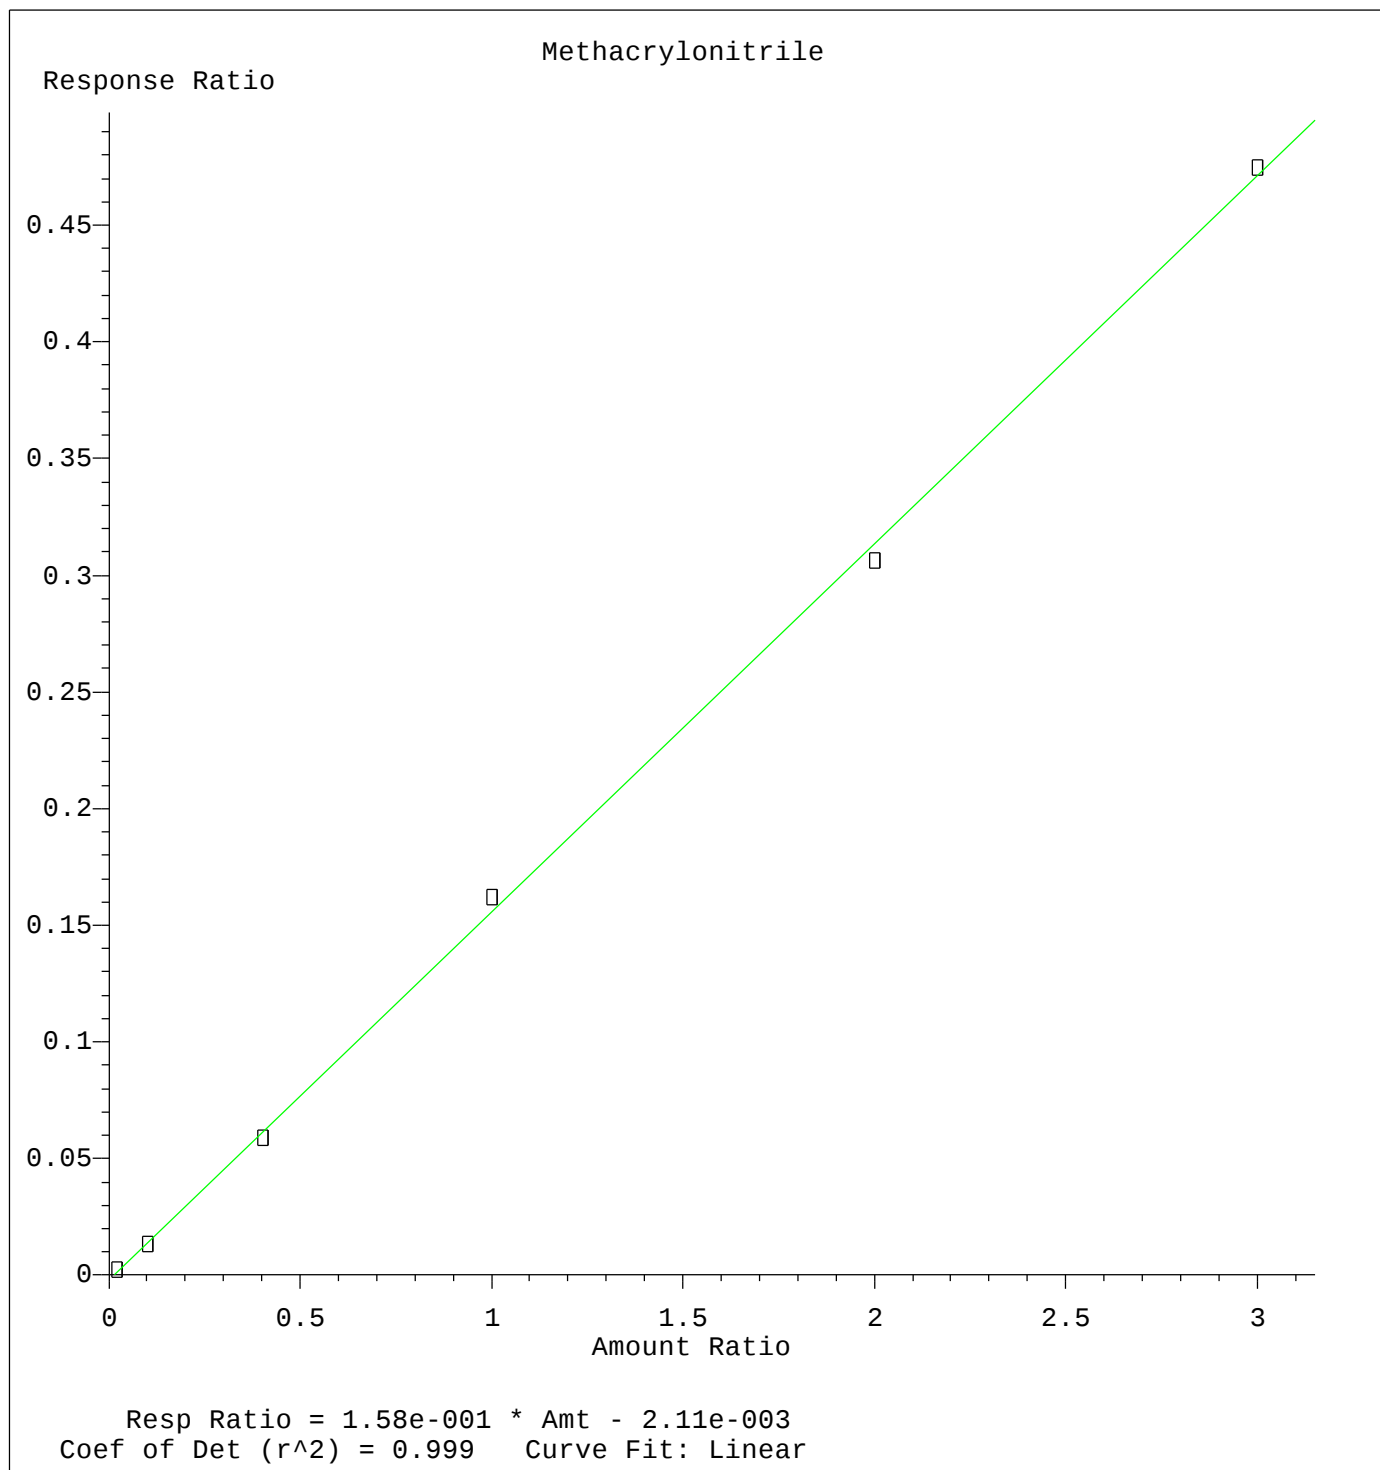


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011519W.M
Calibration Table Last Updated: Wed Jan 16 03:10:53 2019

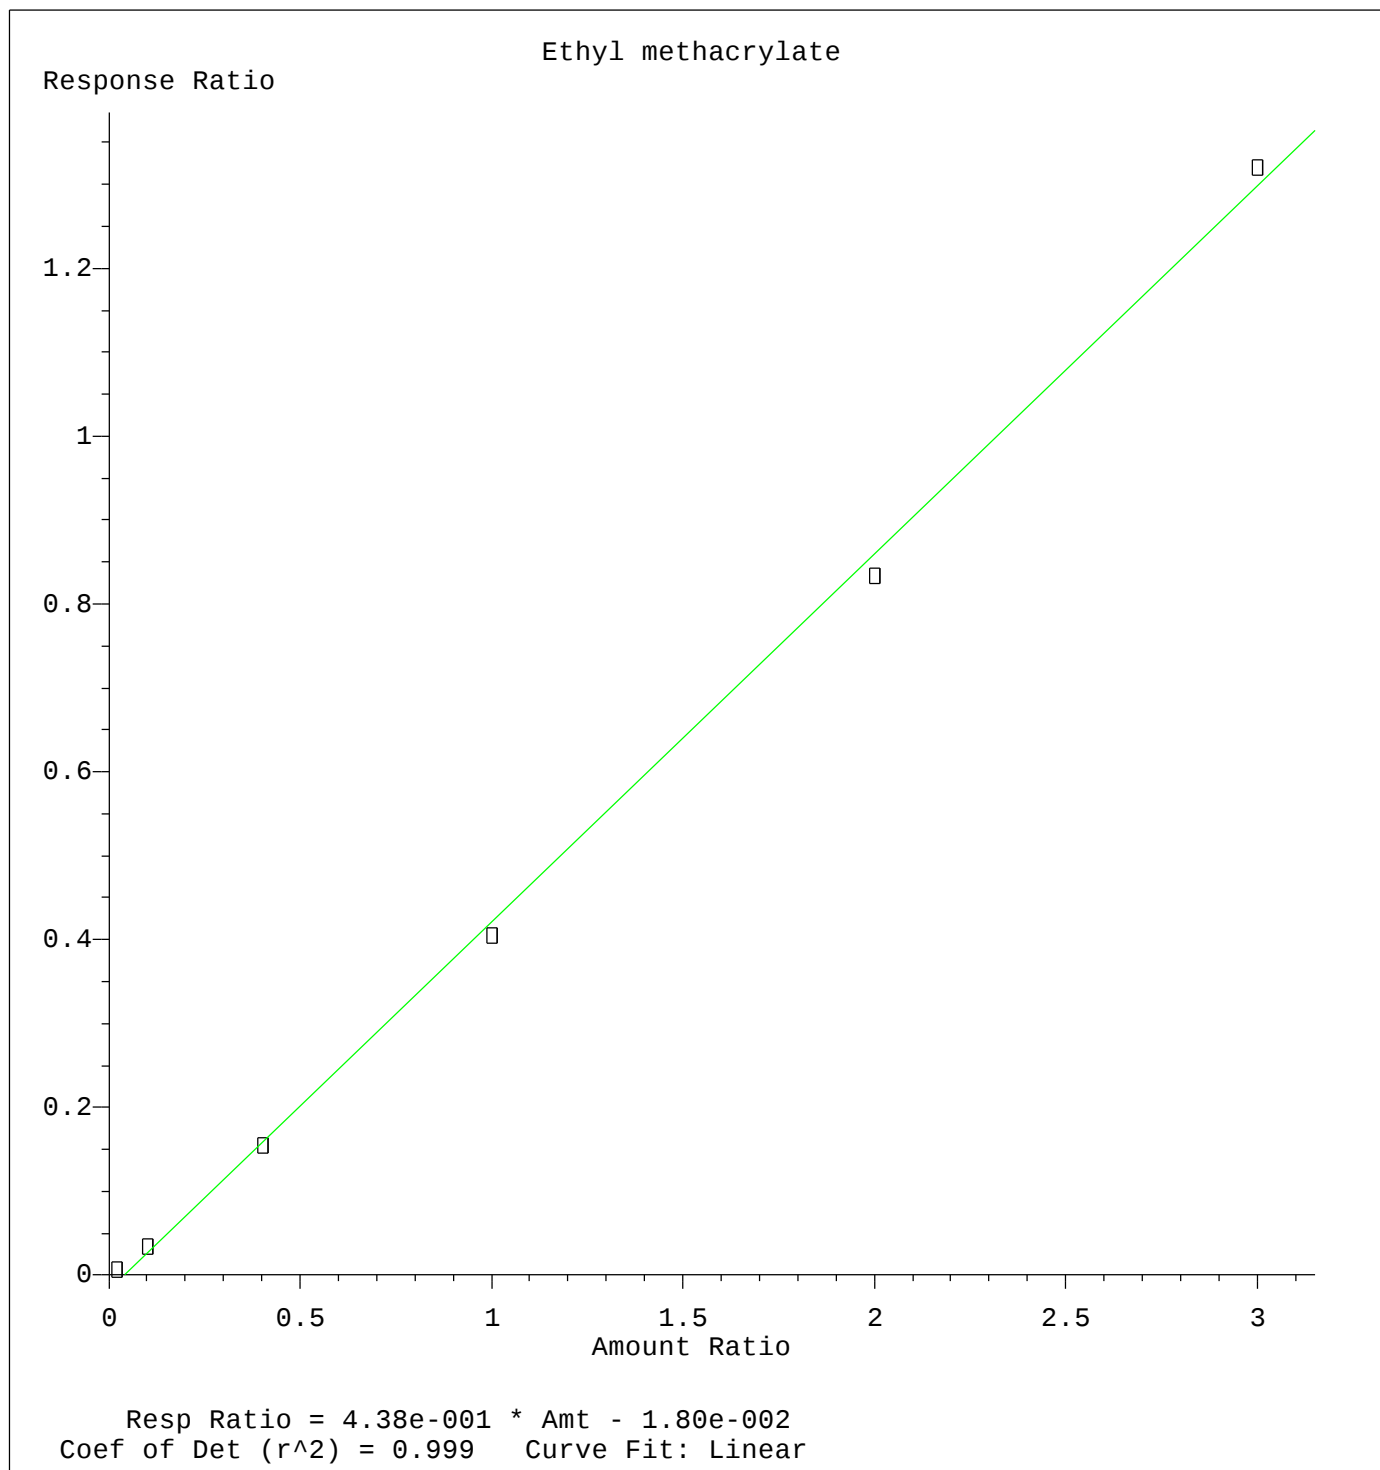

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011519W.M
Calibration Table Last Updated: Wed Jan 16 03:10:53 2019

trans-1,4-Dichloro-2-butene

Response Ratio

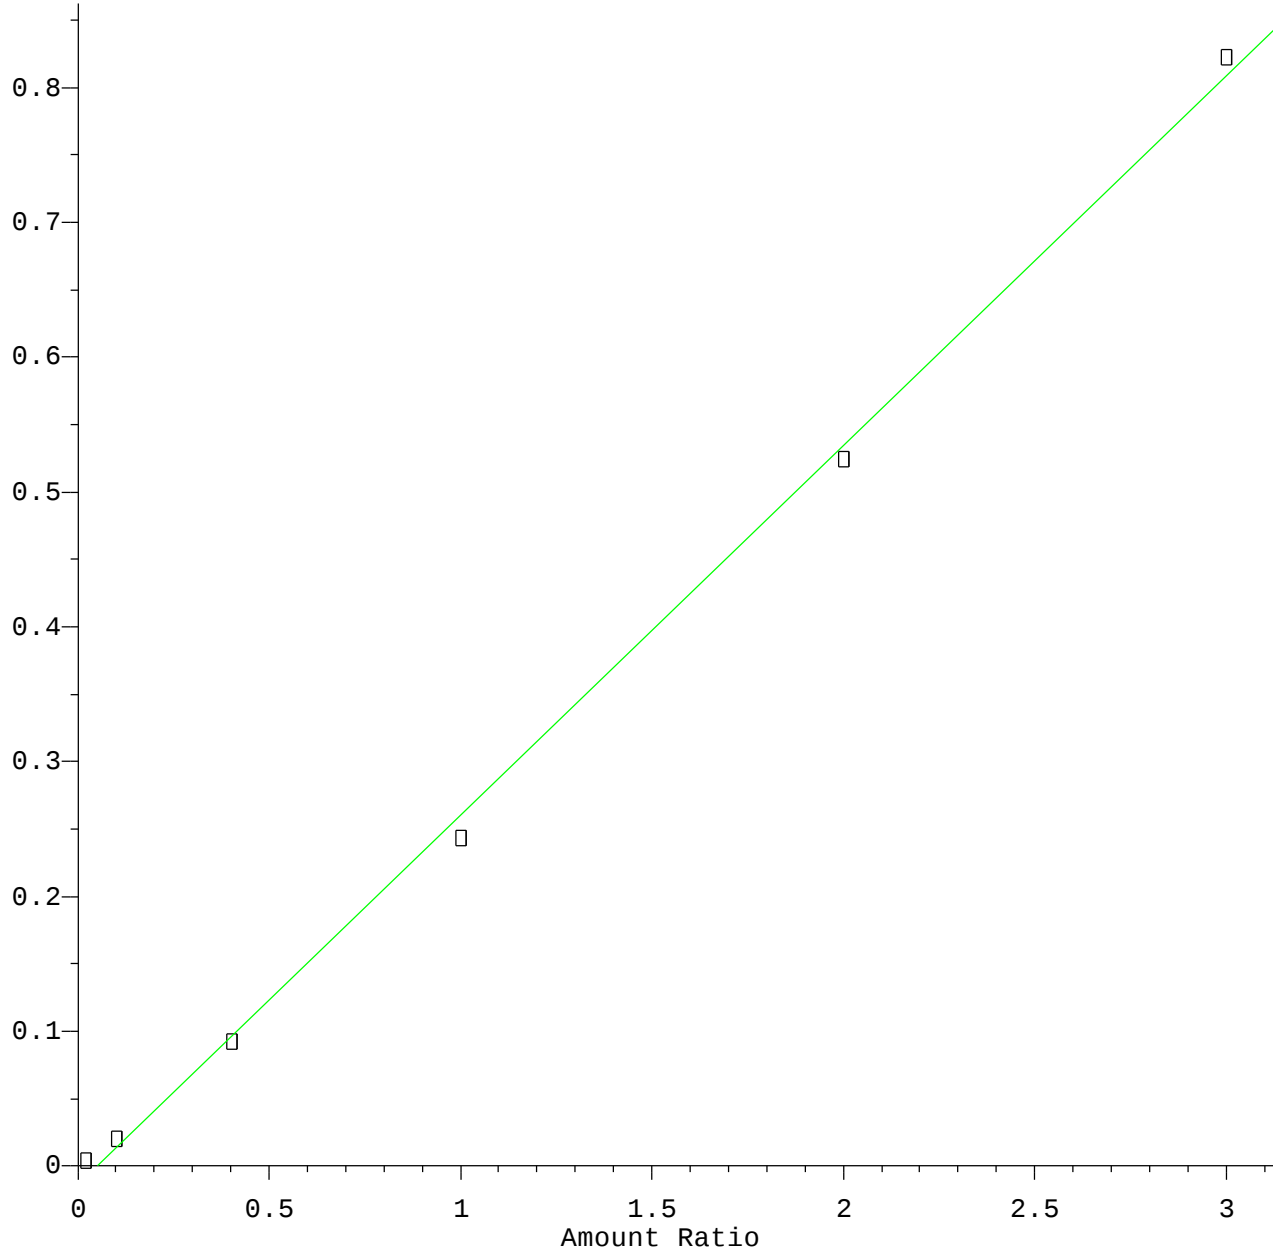


Resp Ratio = $2.74 \times 10^{-1} \times \text{Amt} - 1.39 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011519W.M
Calibration Table Last Updated: Wed Jan 16 03:10:53 2019

1,2,4-Trichlorobenzene

Response Ratio

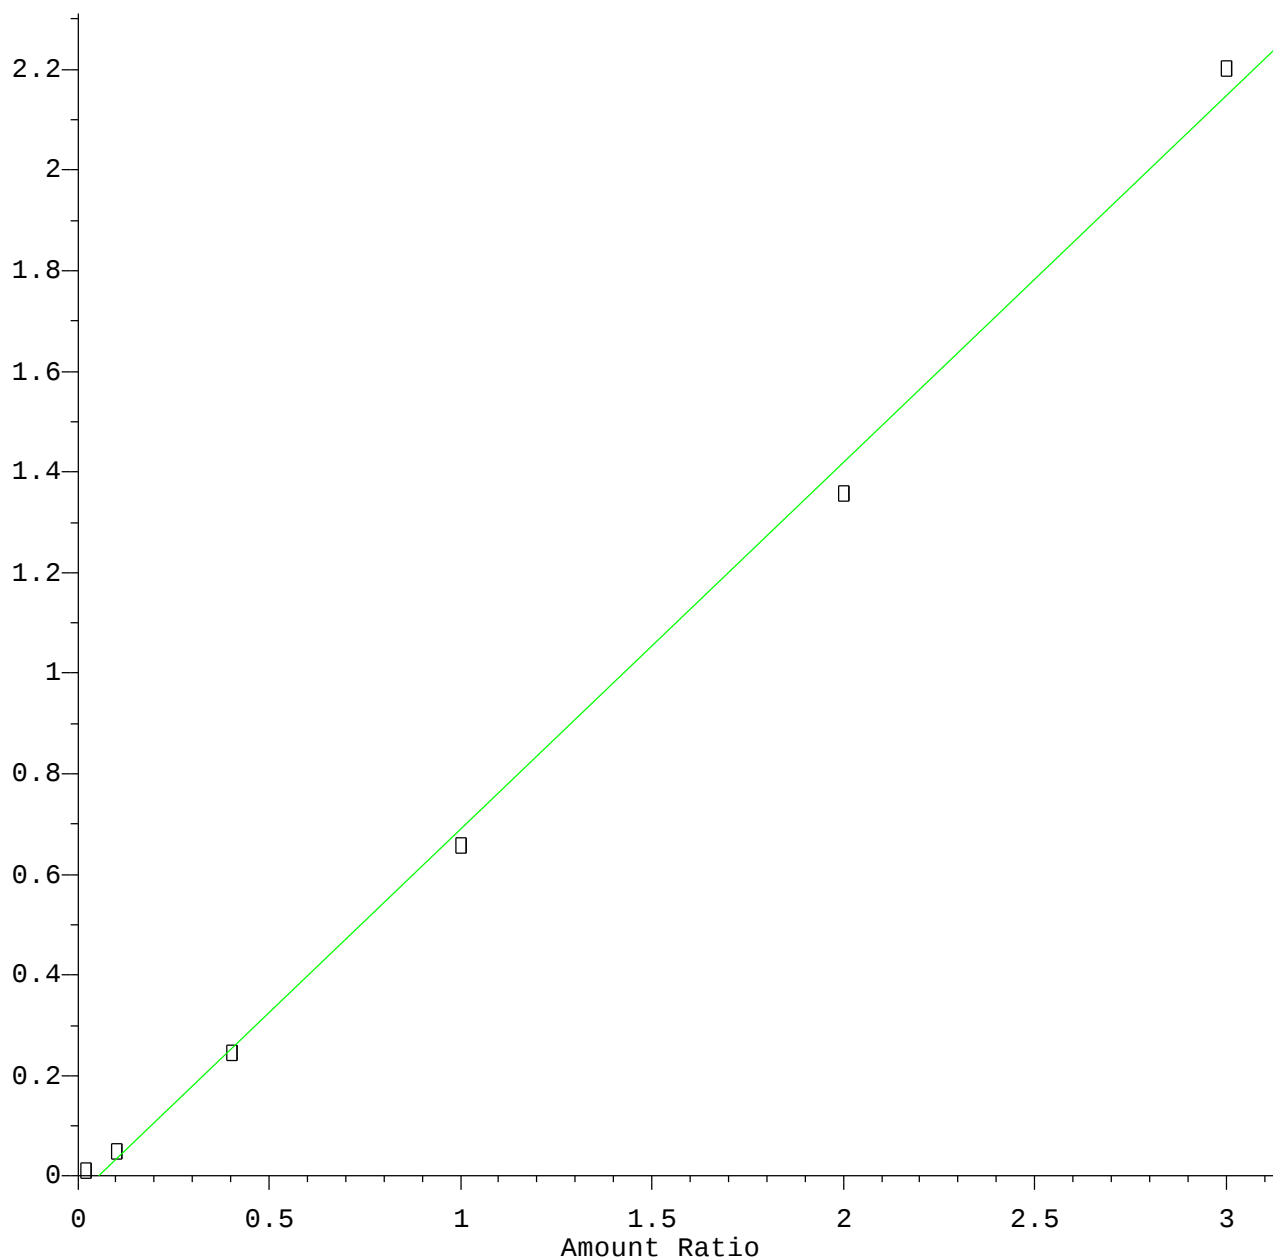


Resp Ratio = $7.29 \times 10^{-1} \times \text{Amt} - 4.03 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011519W.M
Calibration Table Last Updated: Wed Jan 16 03:10:53 2019

Naphthalene

Response Ratio

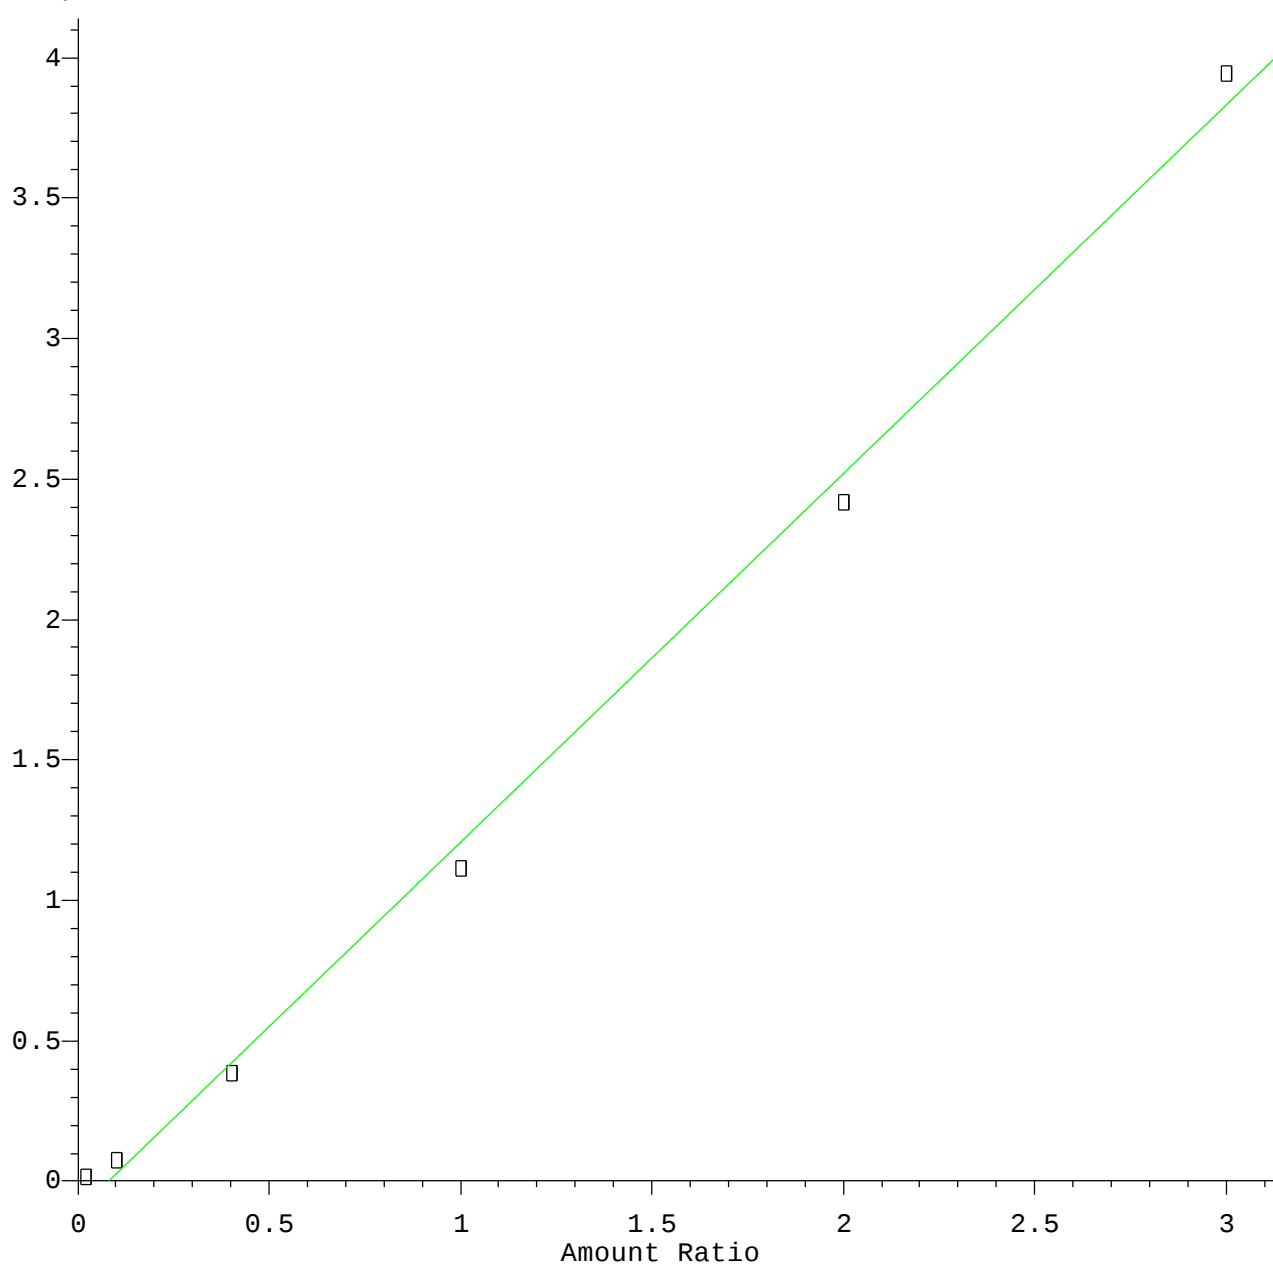


Resp Ratio = 1.31e+000 * Amt - 1.03e-001
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011519W.M
Calibration Table Last Updated: Wed Jan 16 03:10:53 2019

1,2,3-Trichlorobenzene

Response Ratio

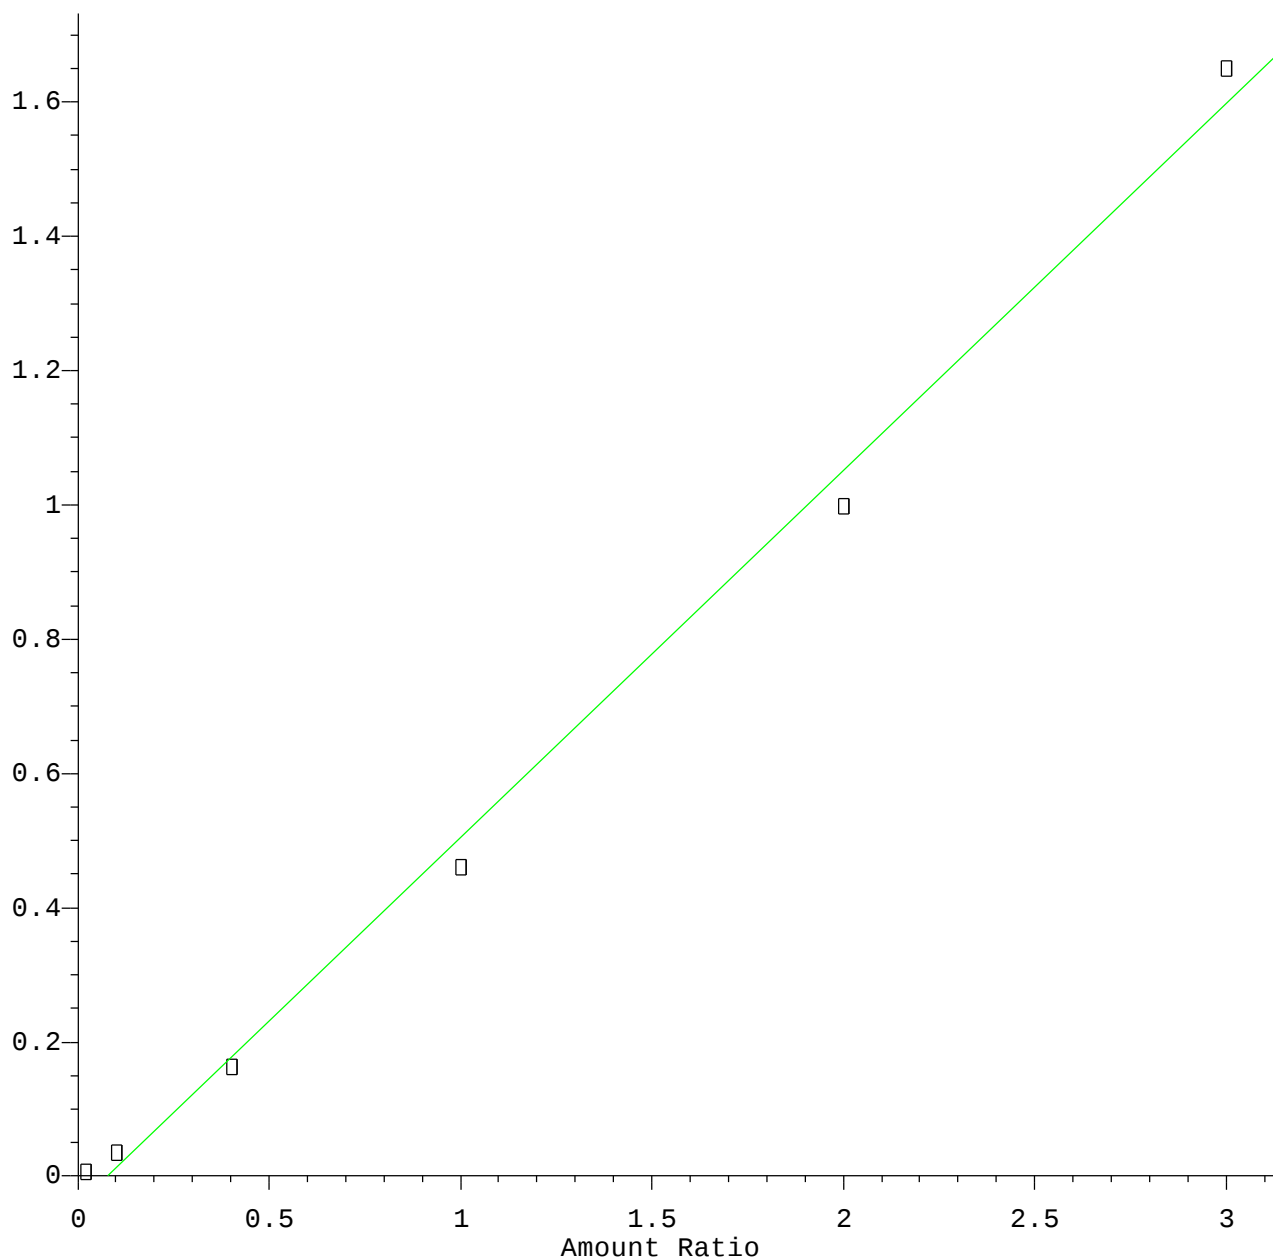

Resp Ratio = $5.47 \times 10^{-1} \times \text{Amt} - 4.27 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011519W.M
Calibration Table Last Updated: Wed Jan 16 03:10:53 2019