


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN011519\
 Data File : VN053395.D
 Acq On : 15 Jan 2019 8:44
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011519W.M
 Title : SW846 8260
 Last Update : Wed Jan 16 03:10:53 2019

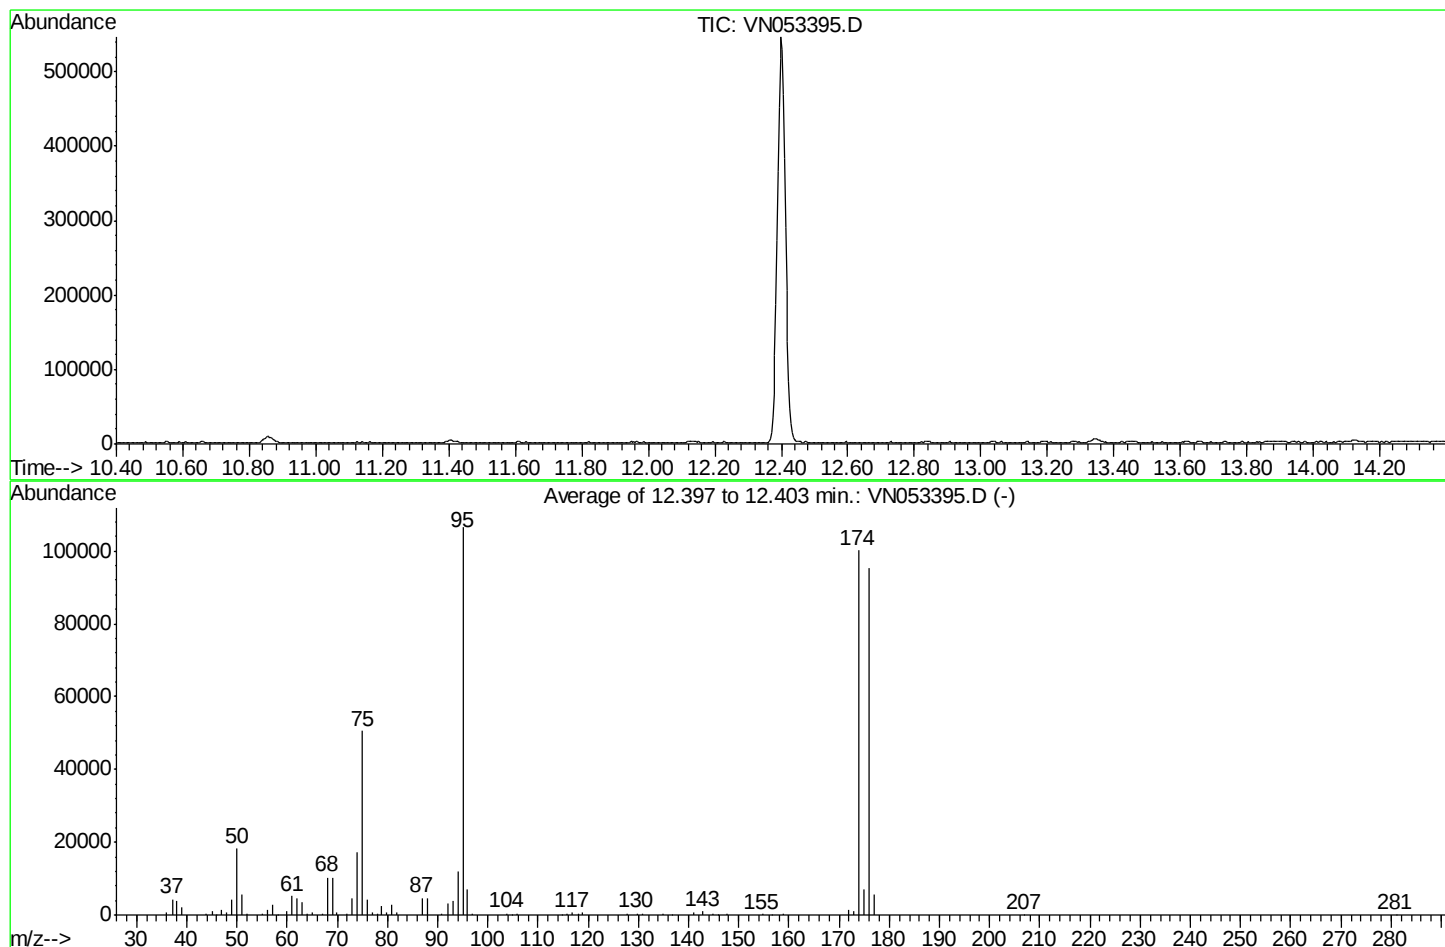

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	18146	PASS
75	95	30	60	47.5	50634	PASS
95	95	100	100	100.0	106493	PASS
96	95	5	9	6.5	6935	PASS
173	174	0.00	2	1.0	1021	PASS
174	95	50	100	94.0	100117	PASS
175	174	5	9	7.1	7107	PASS
176	174	95	101	95.2	95266	PASS
177	176	5	9	6.0	5748	PASS