
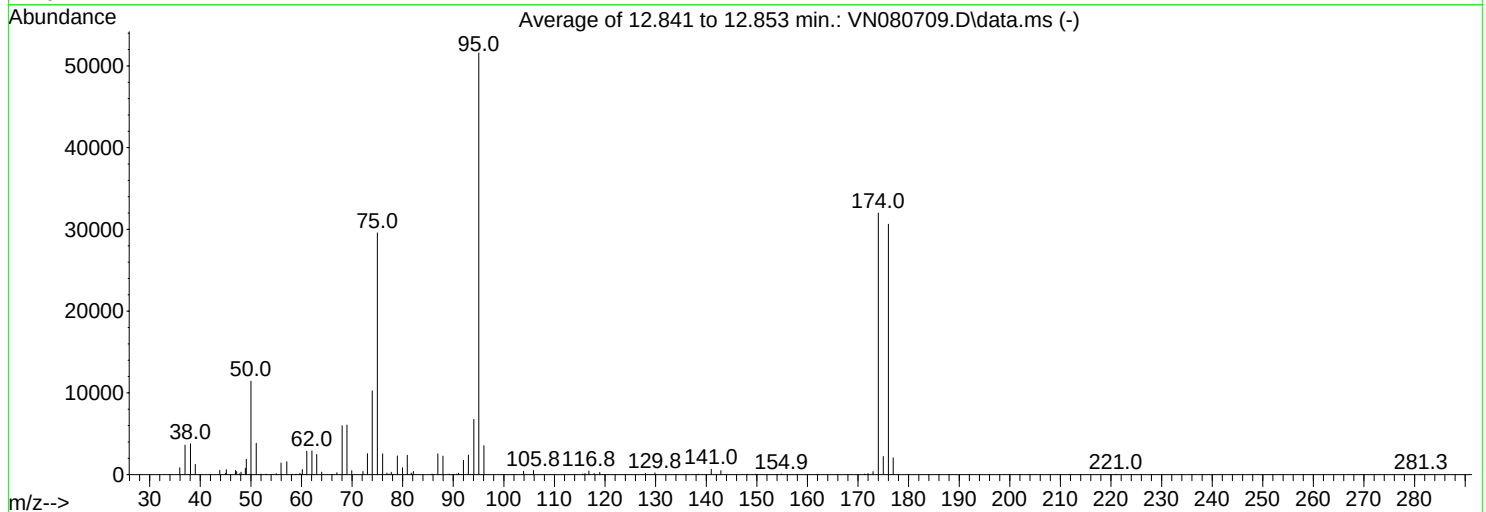


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011524\
Data File : VN080709.D
Acq On : 15 Jan 2024 09:03
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M
Title : SW846 8260
Last Update : Thu Jan 11 06:34:36 2024

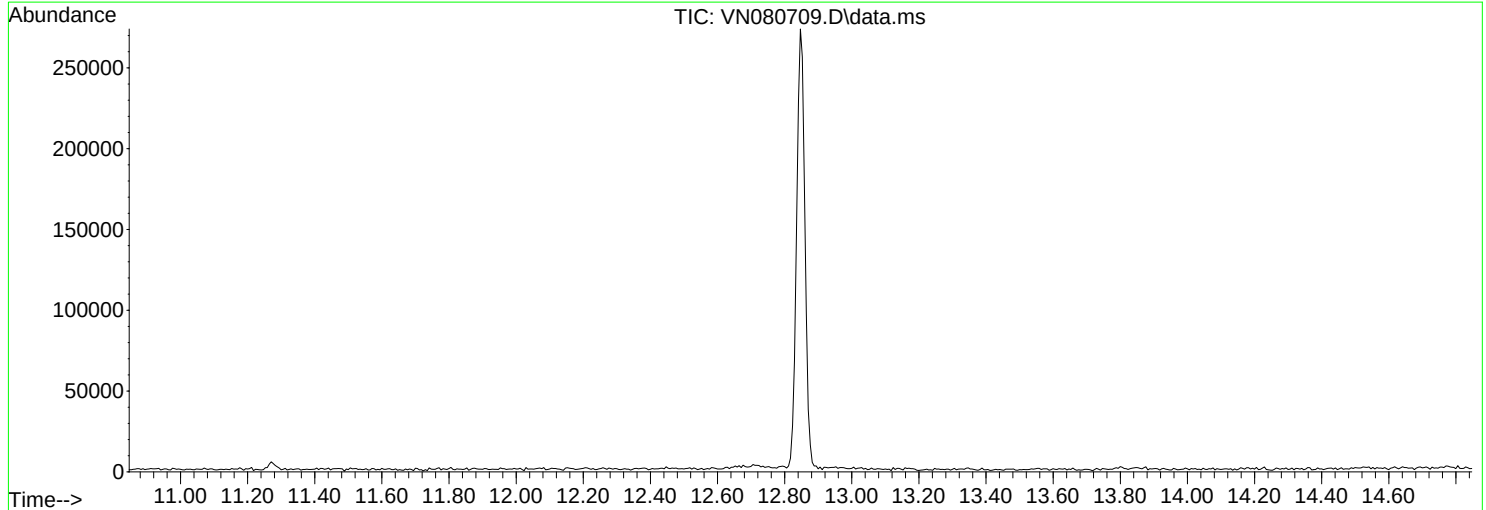

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	11426	PASS
75	95	30	60	57.3	29573	PASS
95	95	100	100	100.0	51600	PASS
96	95	5	9	6.9	3543	PASS
173	174	0.00	2	1.2	382	PASS
174	95	50	100	62.0	32011	PASS
175	174	5	9	6.9	2206	PASS
176	174	95	101	95.7	30627	PASS
177	176	5	9	6.7	2052	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	853	48.05	286	58.90	58	72.15	391
37.00	3614	48.90	793	59.70	174	73.05	256
38.05	3779	49.10	1885	60.15	625	74.00	1025
39.00	1254	50.00	11426	61.05	2861	75.00	2957
39.95	14	51.05	3845	62.05	2913	76.05	2548
43.85	528	52.00	57	63.00	2461	76.90	192
45.00	158	53.00	60	64.00	306	77.30	74
45.15	617	55.00	130	67.00	234	77.75	298
46.95	513	55.95	1424	68.05	5998	78.10	52
47.20	369	57.10	1592	69.00	6073	78.95	2283
47.80	120	58.10	55	69.95	493	79.95	849

Average of 12.841 to 12.853 min.: VN080709.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.90	2371	94.05	6763	129.85	210	175.00	2206
81.70	195	95.05	51600	138.50	54	176.00	30627
82.10	397	96.05	3543	141.00	664	176.95	2052
85.80	70	103.90	415	142.90	485	221.00	53
86.95	2551	105.85	509	148.10	61	281.30	51
87.95	2266	115.60	84	149.80	50		
89.20	57	116.05	140	154.90	85		
90.70	84	116.80	457	171.30	73		
91.05	178	117.85	132	171.95	145		
92.00	1739	118.95	274	172.95	382		
93.00	2381	127.95	161	174.00	32011		

Instrument :

MSVOA_N

ClientSampleId :

BFB