
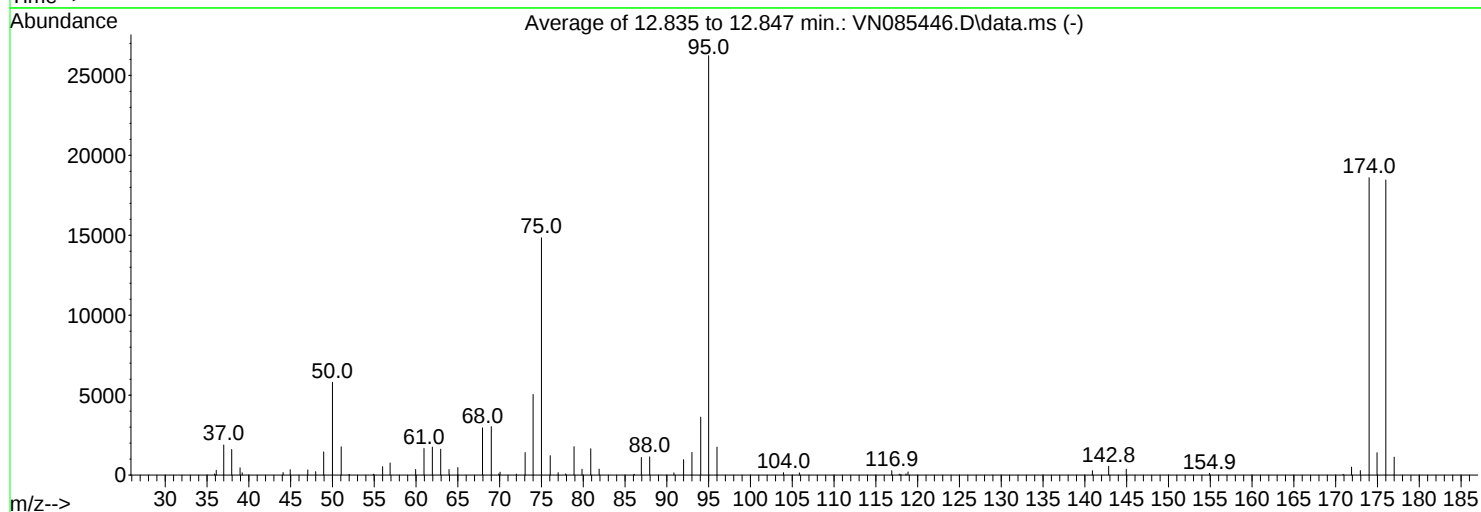


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011525\
Data File : VN085446.D
Acq On : 15 Jan 2025 08:25
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Title : SW846 8260
Last Update : Wed Jan 15 02:16:08 2025

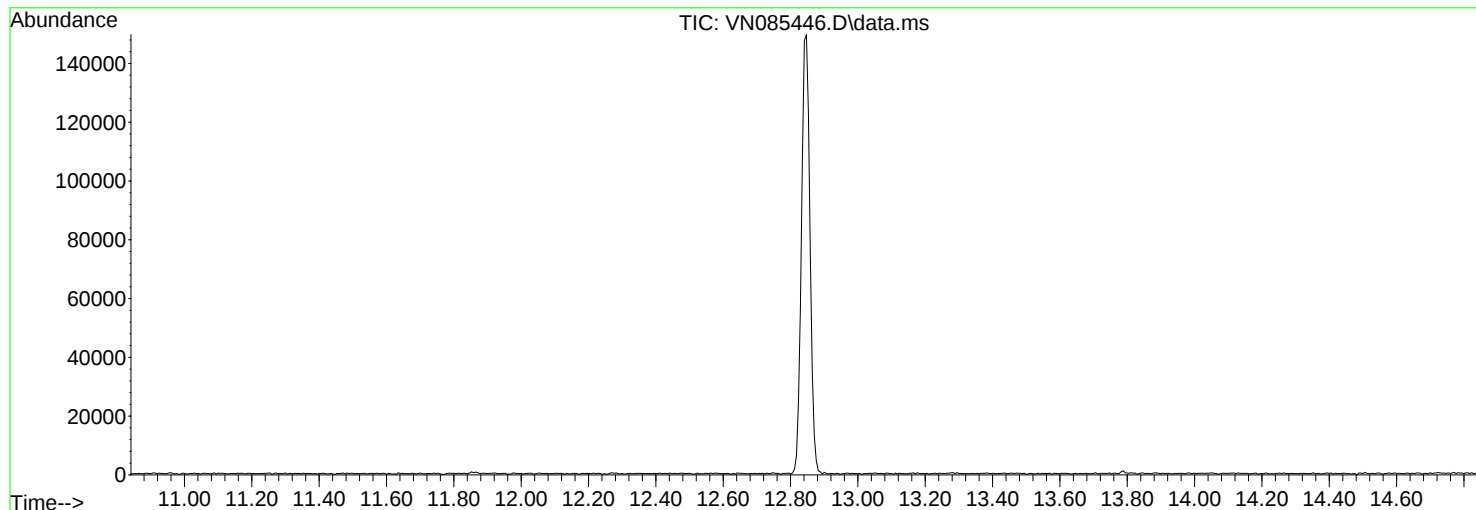

AutoFind: Scans 1850, 1851, 1852; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	5803	PASS
75	95	30	60	56.6	14841	PASS
95	95	100	100	100.0	26229	PASS
96	95	5	9	6.7	1751	PASS
173	174	0.00	2	1.5	282	PASS
174	95	50	100	70.9	18601	PASS
175	174	5	9	7.5	1400	PASS
176	174	95	101	99.2	18460	PASS
177	176	5	9	6.1	1123	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	68	50.00	5803	65.00	470	77.90	74
36.10	301	51.05	1765	67.95	2957	78.90	1776
37.00	1886	52.00	51	69.00	3028	79.85	366
37.95	1600	54.90	57	69.90	78	80.90	1647
38.95	455	56.00	526	70.05	183	81.90	371
39.20	148	56.90	756	72.00	63	86.10	50
44.10	162	59.95	348	73.05	1410	86.95	1098
44.95	335	60.95	1665	74.00	5045	87.95	1141
47.05	324	61.95	1750	75.00	14841	90.85	141
48.00	215	62.95	1619	76.05	1214	92.00	968
48.95	1451	63.95	348	77.00	157	93.00	1420

Average of 12.835 to 12.847 min.: VN085446.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	3627	142.85	553				
95.00	26229	144.95	368				
96.00	1751	154.90	115				
103.95	154	170.90	51				
105.85	141	171.90	499				
116.90	277	172.95	282				
117.80	60	174.00	18601				
118.00	50	174.95	1400				
118.60	78	176.00	18460				
118.85	195	177.00	1123				
140.90	275						

Instrument :

MSVOA_N

ClientSampleId :

BFB