

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN011620\
 Data File : VN059733.D
 Acq On : 16 Jan 2020 15:41
 Operator : JC/MD
 Sample : PB126118TB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB126118TB

Quant Time: Jan 17 04:37:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011320W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 14 08:58:21 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.64	168	194994	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.57	114	293075	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.40	117	255813	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	111119	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.00	65	101115	46.69	ug/l	0.00
Spiked Amount			Recovery	=	93.38%	
35) Dibromofluoromethane	7.57	113	87279	49.94	ug/l	0.00
Spiked Amount			Recovery	=	99.88%	
50) Toluene-d8	10.08	98	334323	49.37	ug/l	0.00
Spiked Amount			Recovery	=	98.74%	
62) 4-Bromofluorobenzene	12.40	95	114839	47.04	ug/l	0.00
Spiked Amount			Recovery	=	94.08%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Acetone	3.79	43	4269	Below Cal		100
17) Carbon Disulfide	4.03	76	1500	0.295	ug/l #	75
18) Methyl Acetate	4.31	43	1864	0.737	ug/l #	54
20) Methylene Chloride	4.53	84	3760	0.642	ug/l #	84
25) 2-Butanone	6.81	43	1935	1.578	ug/l #	50
31) Cyclohexane	7.64	56	3773	1.178	ug/l #	1
36) 1,1-Dichloropropene	7.64	75	13210	5.176	ug/l #	50
38) Carbon Tetrachloride	7.64	117	18010	6.487	ug/l #	16
43) Isopropyl Acetate	8.14	43	45601	11.075	ug/l #	90
45) 1,2-Dichloropropane	9.25	63	814	0.432	ug/l #	44
48) Methyl methacrylate	9.17	41	2580	1.401	ug/l #	13
51) 4-Methyl-2-Pentanone	9.97	43	3395	1.426	ug/l	95
52) Toluene	10.14	92	1842	0.383	ug/l	96
54) cis-1,3-Dichloropropene	9.89	75	21979	6.987	ug/l #	57
57) 1,3-Dichloropropane	10.75	76	3637	1.203	ug/l #	42
59) 2-Hexanone	10.75	43	47064	26.841	ug/l #	56
74) N-amyl acetate	12.03	43	1727	0.546	ug/l #	45
76) 1,2,3-Trichloropropane	12.40	75	56835	30.393	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.73	105	3816	0.557	ug/l	98
81) trans-1,4-Dichloro-2-buten	12.40	75	56835	65.268	ug/l #	11
92) 1,2-Dibromo-3-Chloropropan	14.26	75	410	Below Cal	#	6
93) 1,2,4-Trichlorobenzene	14.91	180	1152	0.541	ug/l	93
95) Naphthalene	15.13	128	4824	0.796	ug/l	97
96) 1,2,3-Trichlorobenzene	15.31	180	1656	0.799	ug/l #	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN011620\
Data File : VN059733.D
Acq On : 16 Jan 2020 15:41
Operator : JC/MD
Sample : PB126118TB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB126118TB

Quant Time: Jan 17 04:37:45 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N011320W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 14 08:58:21 2020
Response via : Initial Calibration

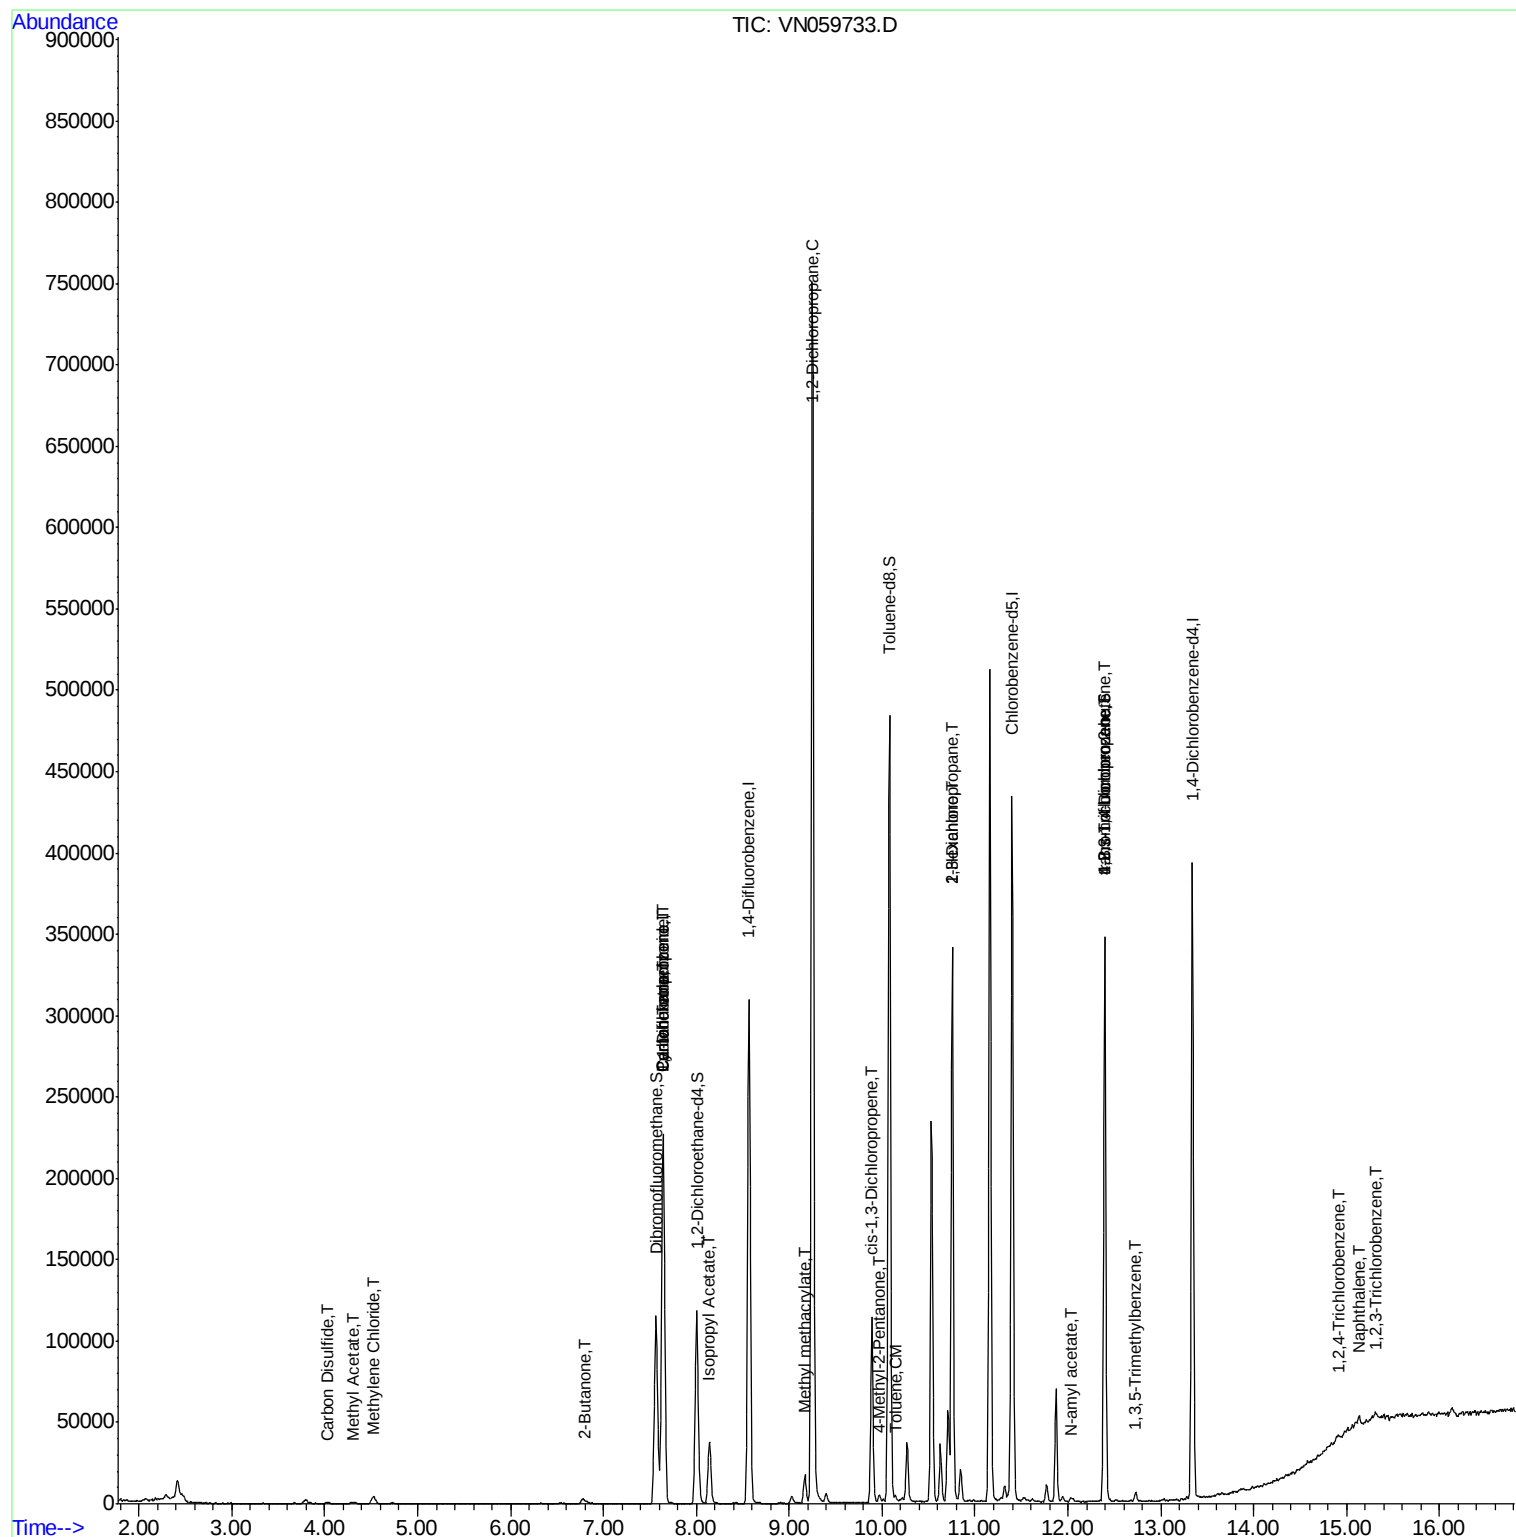

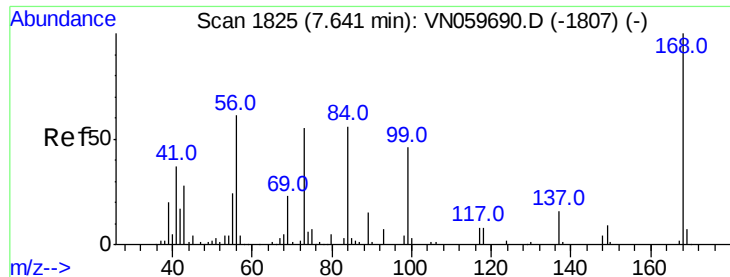

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.64 min Scan# 1826

Delta R.T. 0.00 min

Lab File: VN059733.D

Acq: 16 Jan 2020 15:41

Instrument :

MSVOA_N

ClientSampleId :


PB126118TB

Tgt Ion:168 Resp: 194994

Ion Ratio Lower Upper




168 100

99 50.8 48.2 72.4

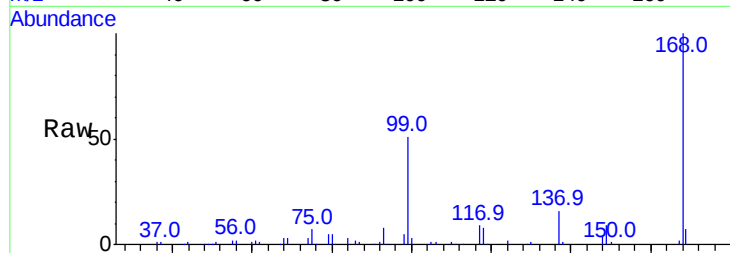

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

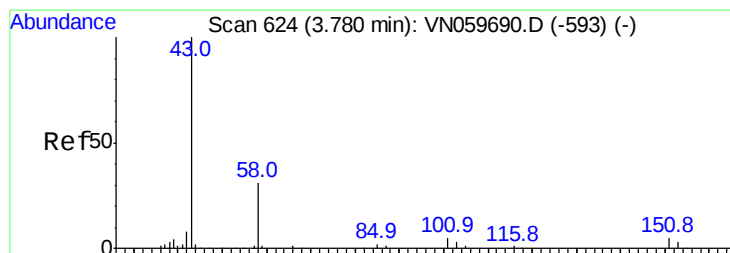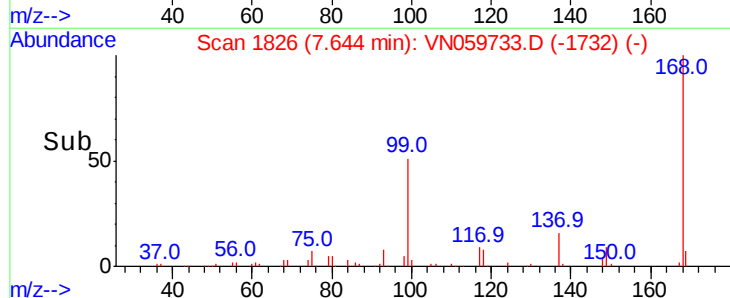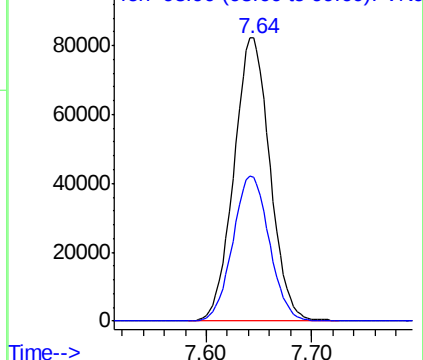

#16

Acetone

Concen: Below Cal

RT: 3.79 min Scan# 627

Delta R.T. 0.01 min

Lab File: VN059733.D


Acq: 16 Jan 2020 15:41

Tgt Ion: 43 Resp: 4269

Ion Ratio Lower Upper



43 100


58 29.4 23.6 35.4

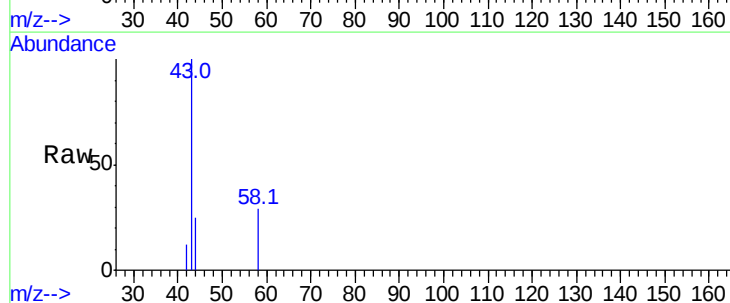

Abundance Ion 43.00 (42.70 to 43.70): VN

Ion 58.00 (57.70 to 58.70): VN



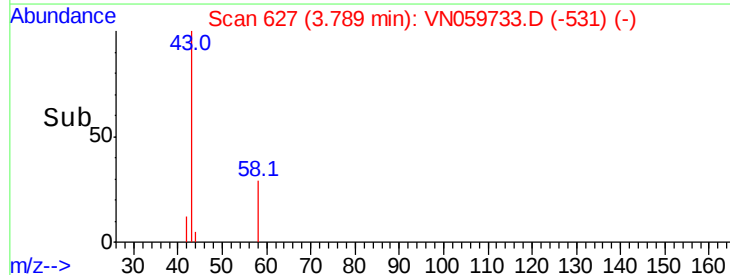
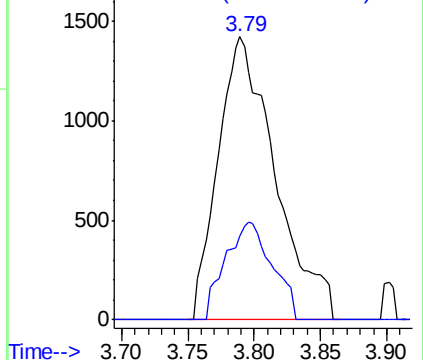


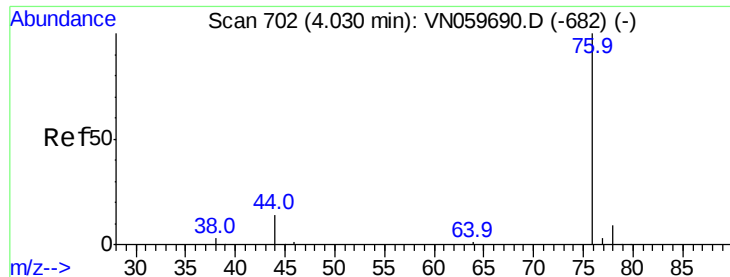

#17
Carbon Disulfide
Concen: 0.295 ug/l
RT: 4.03 min Scan# 702
Delta R.T. 0.00 min
Lab File: VN059733.D
Acq: 16 Jan 2020 15:41




Instrument :
MSVOA_N
ClientSampled :
PB126118TB


Tgt Ion: 76 Resp: 1500
Ion Ratio Lower Upper
76 100
78 0.0 7.4 11.0#

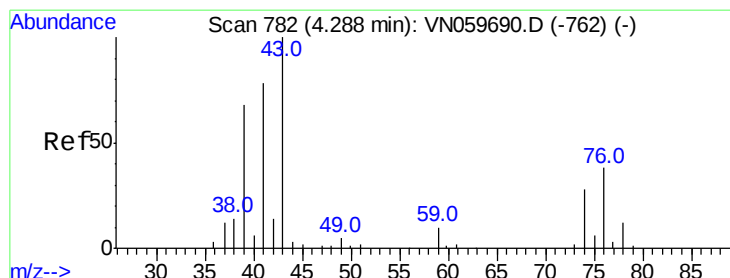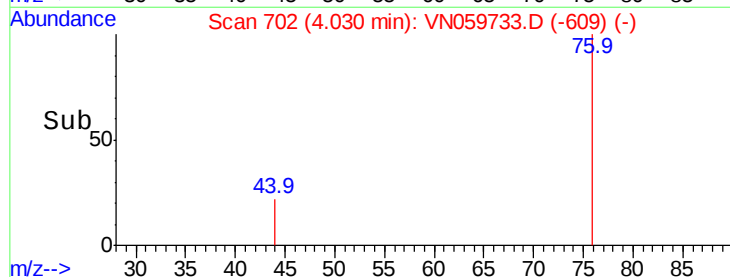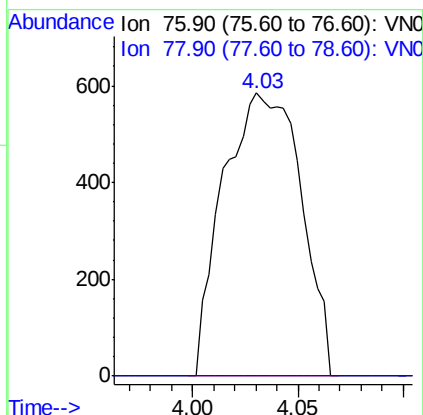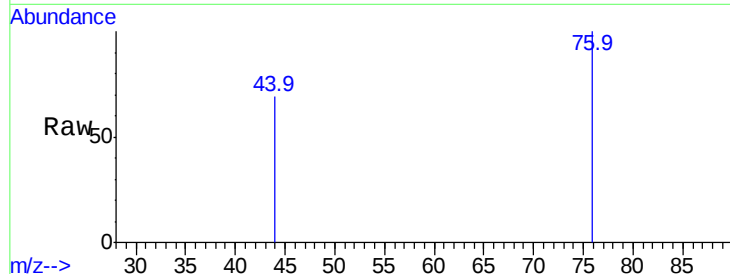

#18
Methyl Acetate
Concen: 0.737 ug/l
RT: 4.31 min Scan# 788
Delta R.T. 0.02 min
Lab File: VN059733.D
Acq: 16 Jan 2020 15:41

Tgt Ion: 43 Resp: 1864
Ion Ratio Lower Upper
43 100
74 0.0 17.5 26.3#


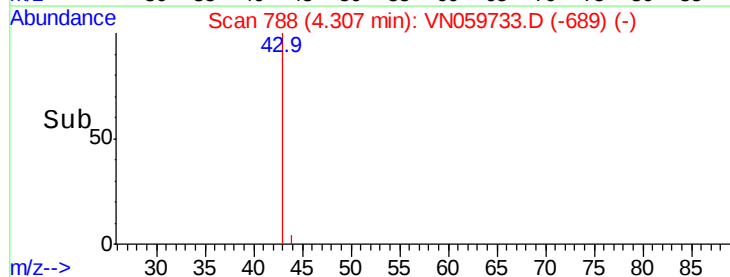
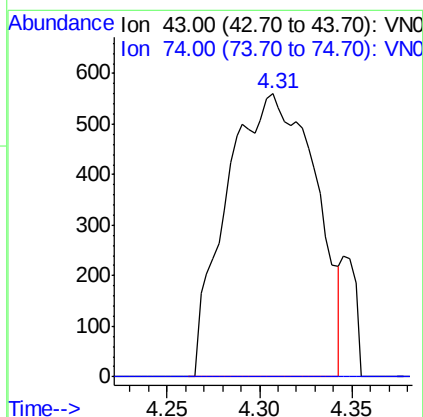
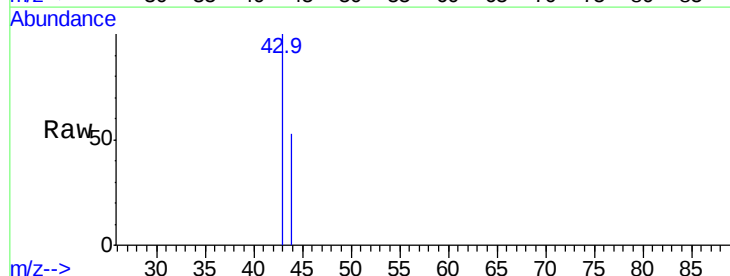


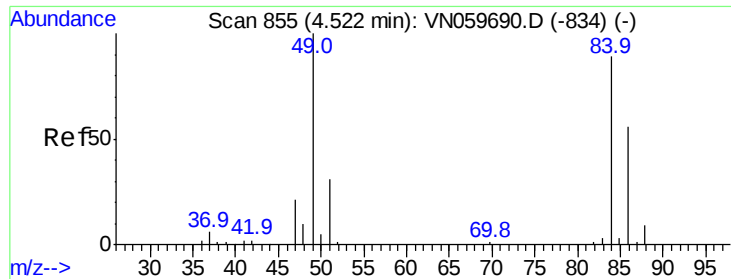

#20
Methylene Chloride
Concen: 0.642 ug/l
RT: 4.53 min Scan# 856
Delta R.T. 0.00 min
Lab File: VN059733.D
Acq: 16 Jan 2020 15:41




Instrument :
MSVOA_N
ClientSampled :
PB126118TB


Tgt Ion: 84 Resp: 3760
Ion Ratio Lower Upper
84 100
49 105.9 106.6 160.0#
51 36.5 31.9 47.9
86 68.7 50.8 76.2

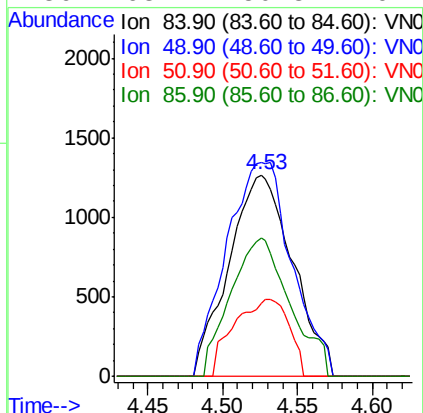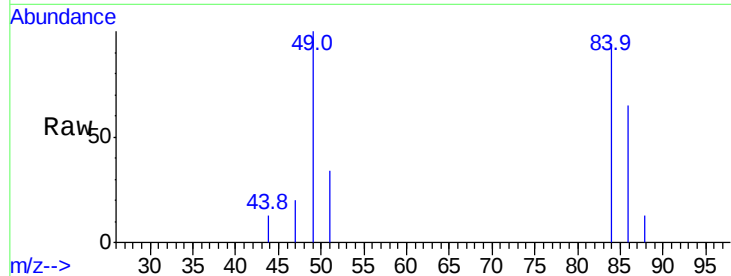

#25
2-Butanone
Concen: 1.578 ug/l
RT: 6.81 min Scan# 1568
Delta R.T. 0.02 min
Lab File: VN059733.D
Acq: 16 Jan 2020 15:41

Tgt Ion: 43 Resp: 1935
Ion Ratio Lower Upper
43 100
72 0.0 19.9 29.9#

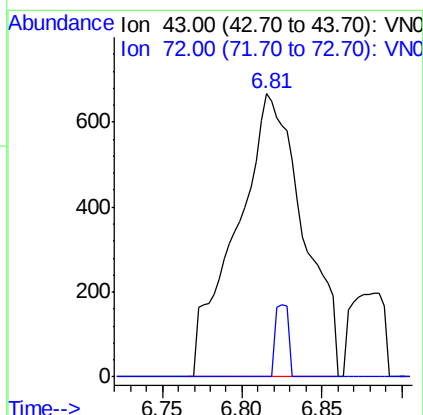


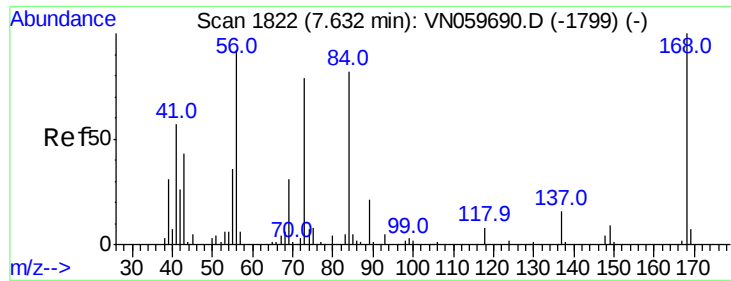




#31
Cyclohexane
Concen: 1.178 ug/l
RT: 7.64 min Scan# 1824
Delta R.T. 0.01 min
Lab File: VN059733.D
Acq: 16 Jan 2020 15:41

Instrument :
MSVOA_N
ClientSampled :
PB126118TB

Tgt Ion: 56 Resp: 3773
Ion Ratio Lower Upper
56 100
69 166.5 26.5 39.7#
84 128.6 65.3 97.9#

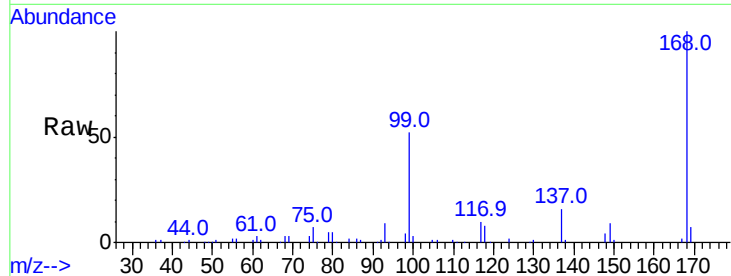


Abundance Ion 56.00 (55.70 to 56.70): VNC
Ion 69.00 (68.70 to 69.70): VNC
Ion 84.00 (83.70 to 84.70): VNC


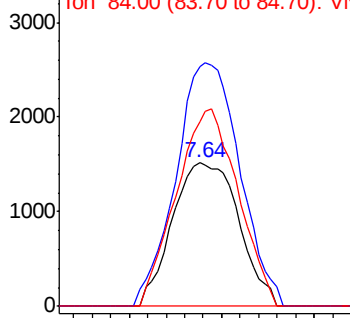



#33
1,2-Dichloroethane-d4
Concen: 46.695 ug/l
RT: 8.00 min Scan# 1938
Delta R.T. 0.00 min
Lab File: VN059733.D
Acq: 16 Jan 2020 15:41

Tgt Ion: 65 Resp: 101115
Ion Ratio Lower Upper
65 100
67 51.5 0.0 103.0



Abundance Ion 64.90 (64.60 to 65.60): VNC
Ion 66.90 (66.60 to 67.60): VNC

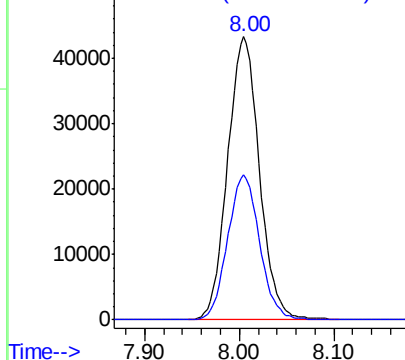


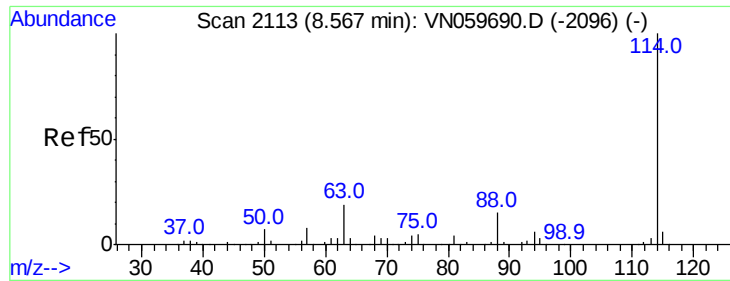

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.57 min Scan# 2113
 Delta R.T. 0.00 min
 Lab File: VN059733.D
 Acq: 16 Jan 2020 15:41

Instrument :
 MSVOA_N
 ClientSampleId :
 PB126118TB

Tgt Ion	Ratio	Lower	Upper
114	100		
63	18.9	0.0	43.6
88	15.1	0.0	31.4



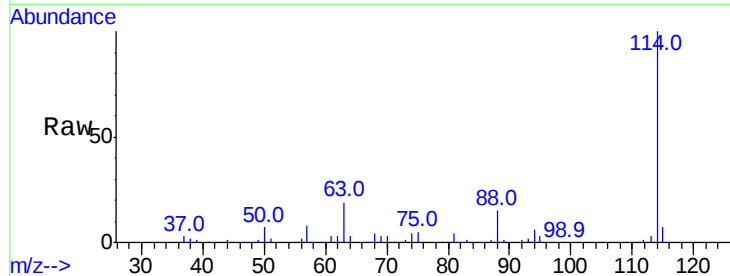


Abundance

Ion 113.90 (113.60 to 114.60): V


Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

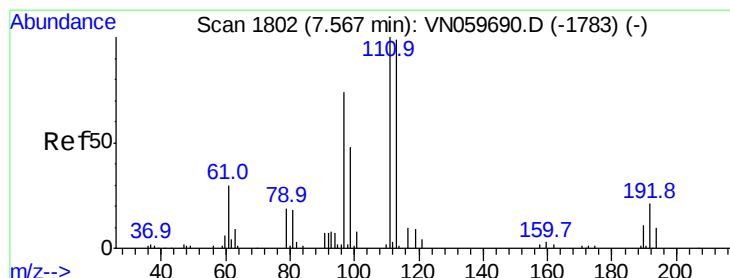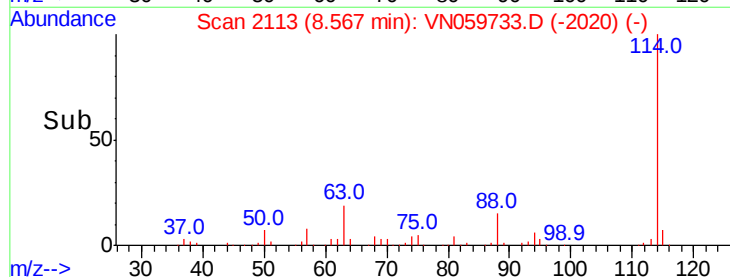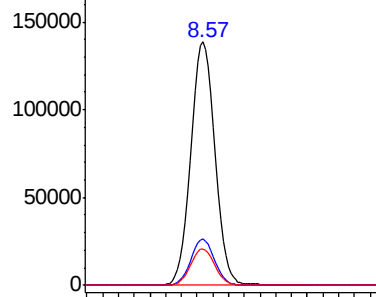

#35
 Dibromofluoromethane
 Concen: 49.938 ug/l
 RT: 7.57 min Scan# 1802
 Delta R.T. 0.00 min
 Lab File: VN059733.D
 Acq: 16 Jan 2020 15:41

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.2	83.5	125.3
192	21.4	15.4	23.2


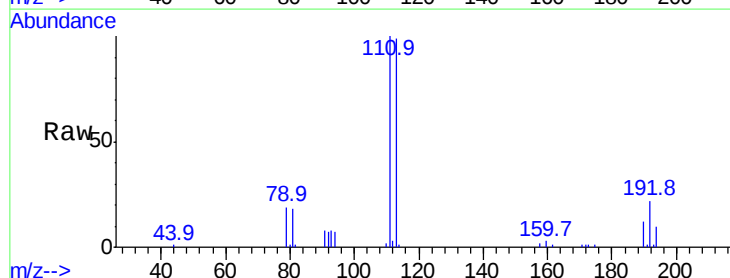



Abundance

Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

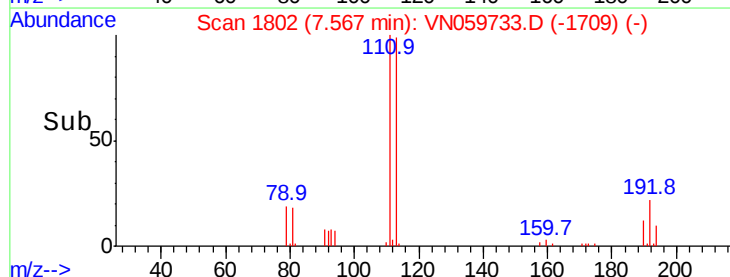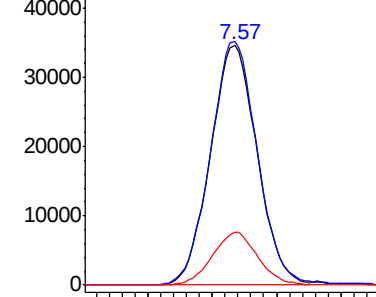


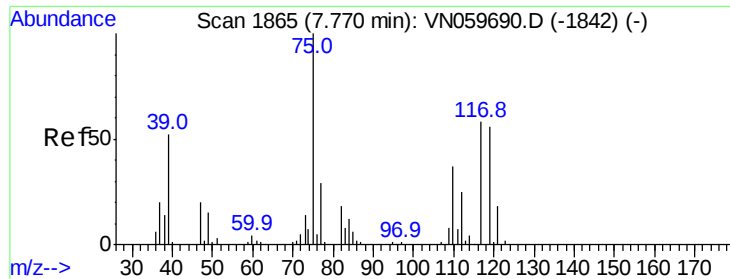




#36
 1,1-Dichloropropene
 Concen: 5.176 ug/l
 RT: 7.64 min Scan# 1826
 Delta R.T. -0.13 min
 Lab File: VN059733.D
 Acq: 16 Jan 2020 15:41

Instrument :
 MSVOA_N
 ClientSampleId :
 PB126118TB

Tgt Ion: 75 Resp: 13210
 Ion Ratio Lower Upper
 75 100
 110 8.7 16.6 49.7#
 77 0.0 25.1 37.7#

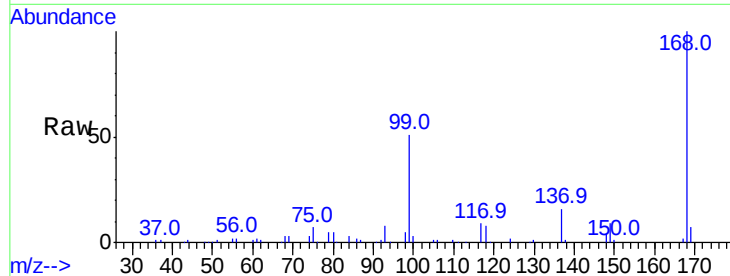


Abundance Ion 74.90 (74.60 to 75.60): VN0
 Ion 109.90 (109.60 to 110.60): V
 Ion 76.90 (76.60 to 77.60): VN0

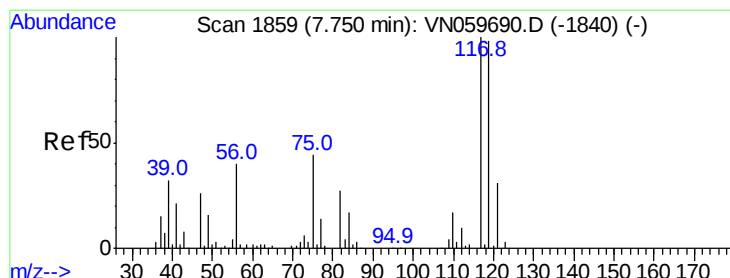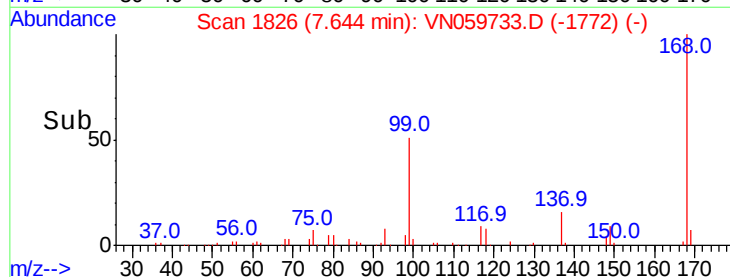
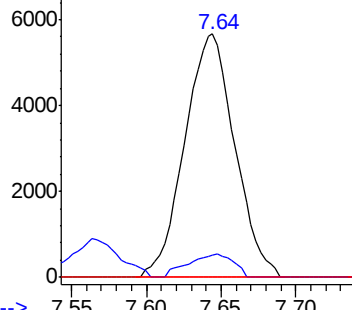



#38
 Carbon Tetrachloride
 Concen: 6.487 ug/l
 RT: 7.64 min Scan# 1825
 Delta R.T. -0.11 min
 Lab File: VN059733.D
 Acq: 16 Jan 2020 15:41

Tgt Ion: 117 Resp: 18010
 Ion Ratio Lower Upper
 117 100
 119 5.0 76.5 114.7#
 121 0.0 25.1 37.7#

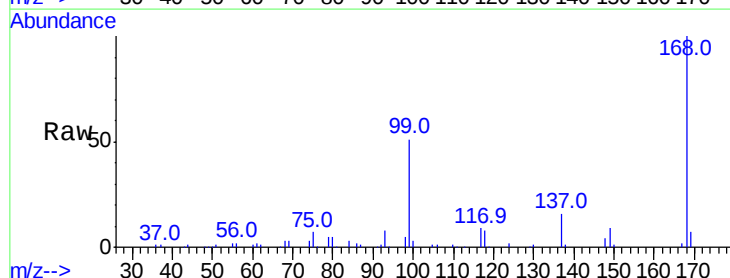

Abundance Ion 116.80 (116.50 to 117.50): V
 Ion 118.80 (118.50 to 119.50): V
 Ion 120.80 (120.50 to 121.50): V

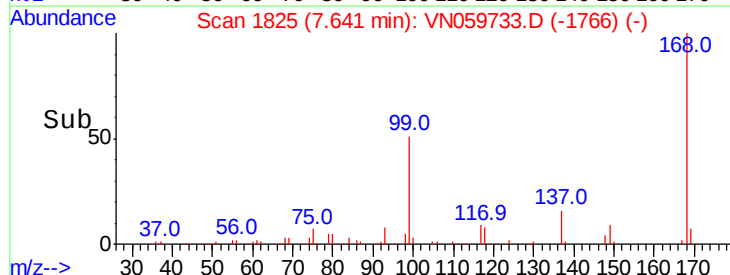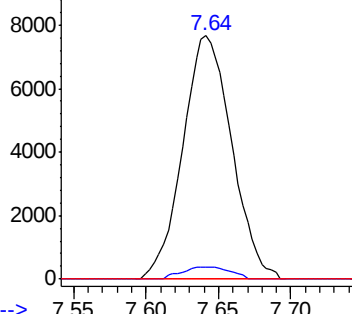

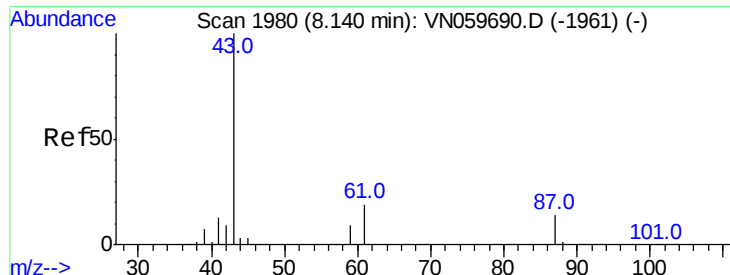

#43

Isopropyl Acetate

Concen: 11.075 ug/l

RT: 8.14 min Scan# 1981

Delta R.T. 0.00 min

Lab File: VN059733.D

Acq: 16 Jan 2020 15:41

Instrument :

MSVOA_N

ClientSampled :

PB126118TB


Tgt Ion: 43 Resp: 45601

Ion Ratio Lower Upper

43 100

61 19.2 20.2 30.2#

87 13.9 9.5 14.3



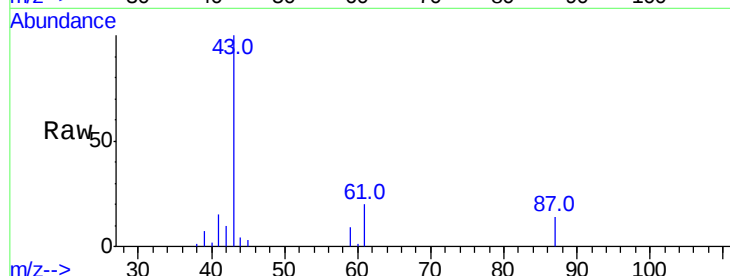


Abundance

Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

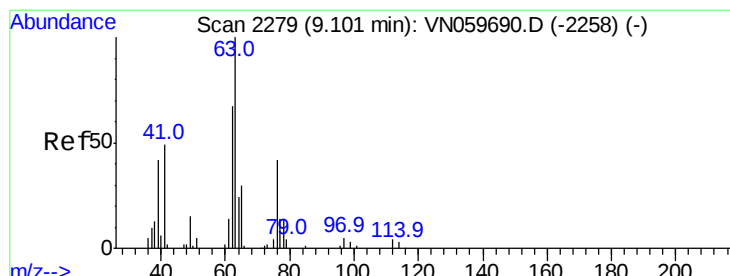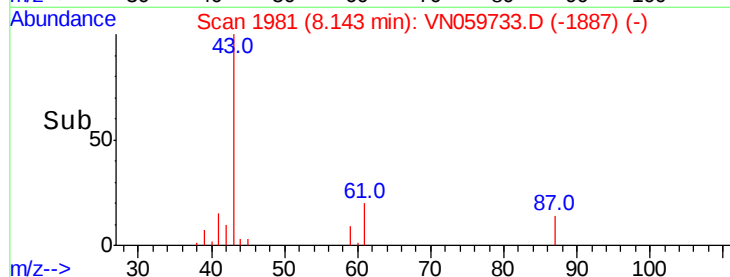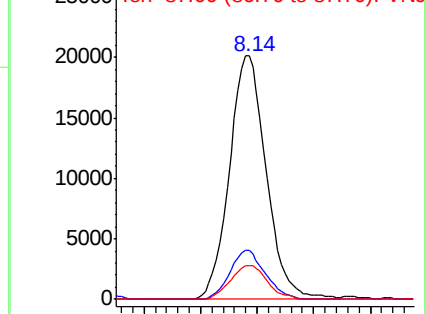

#45

1,2-Dichloropropane

Concen: 0.432 ug/l

RT: 9.25 min Scan# 2326

Delta R.T. 0.15 min

Lab File: VN059733.D


Acq: 16 Jan 2020 15:41

Tgt Ion: 63 Resp: 814

Ion Ratio Lower Upper

63 100



65 0.0 24.9 37.3#

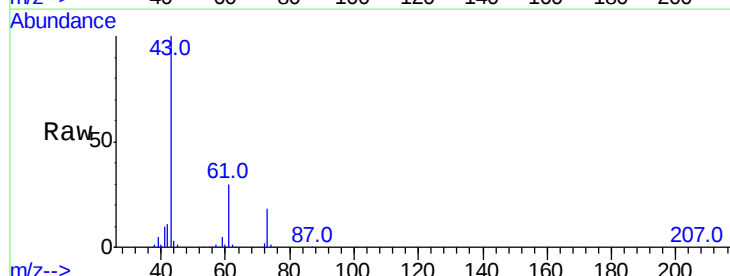


Abundance

Ion 62.90 (62.60 to 63.60): VN0

Ion 64.90 (64.60 to 65.60): VN0

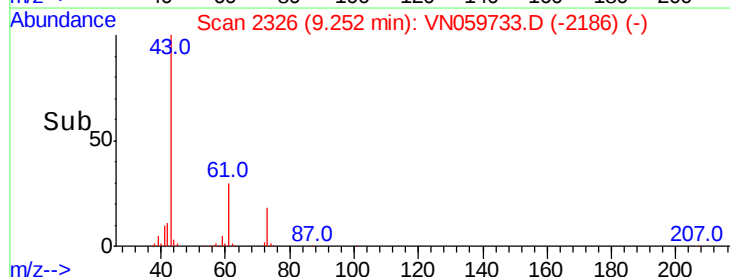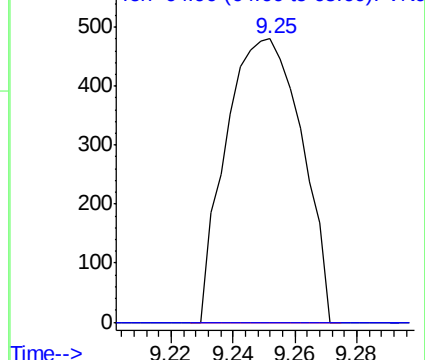


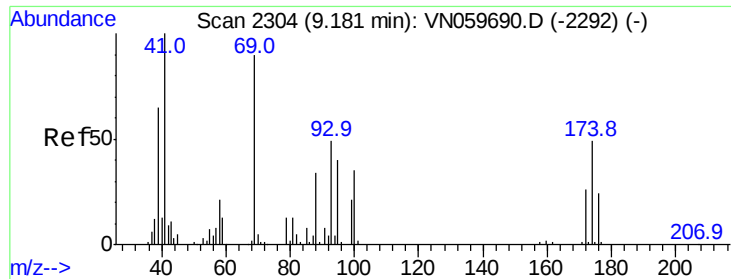




#48
Methyl methacrylate
Concen: 1.401 ug/l
RT: 9.17 min Scan# 2299
Delta R.T. -0.02 min
Lab File: VN059733.D
Acq: 16 Jan 2020 15:41

Instrument :
MSVOA_N
ClientSampleId :
PB126118TB

Tgt Ion: 41 Resp: 2580
Ion Ratio Lower Upper
41 100
69 0.0 64.4 96.6#
39 0.0 51.3 76.9#




Abundance Ion 41.00 (40.70 to 41.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 39.00 (38.70 to 39.70): VN0


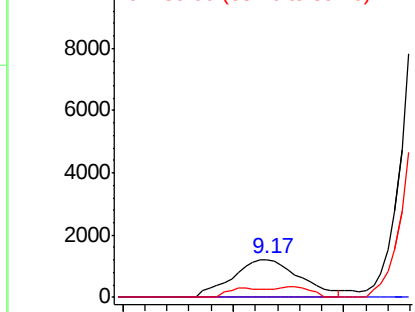



#50
Toluene-d8
Concen: 49.371 ug/l
RT: 10.08 min Scan# 2583
Delta R.T. 0.00 min
Lab File: VN059733.D
Acq: 16 Jan 2020 15:41

Tgt Ion: 98 Resp: 334323
Ion Ratio Lower Upper
98 100
100 65.0 51.2 76.8



Abundance Ion 98.00 (97.70 to 98.70): VN0
Ion 100.00 (99.70 to 100.70): VN0

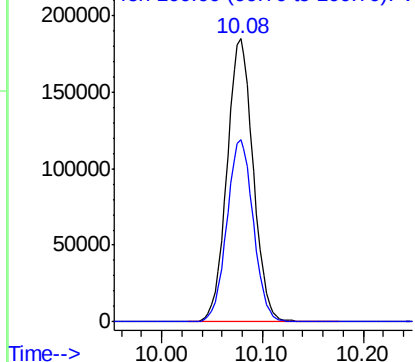


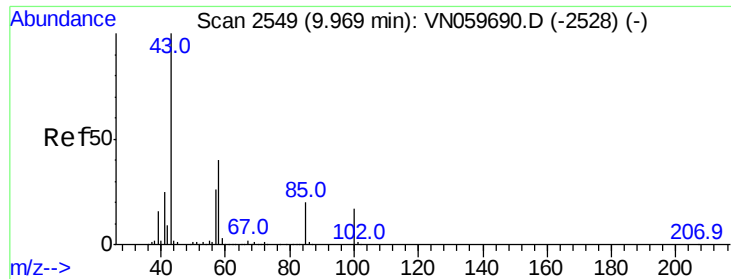




#51
4-Methyl-2-Pentanone
Concen: 1.426 ug/l
RT: 9.97 min Scan# 2550
Delta R.T. 0.00 min
Lab File: VN059733.D
Acq: 16 Jan 2020 15:41

Instrument :
MSVOA_N
ClientSampleId :
PB126118TB

Tgt Ion: 43 Resp: 3395
Ion Ratio Lower Upper
43 100
58 34.4 29.8 44.8

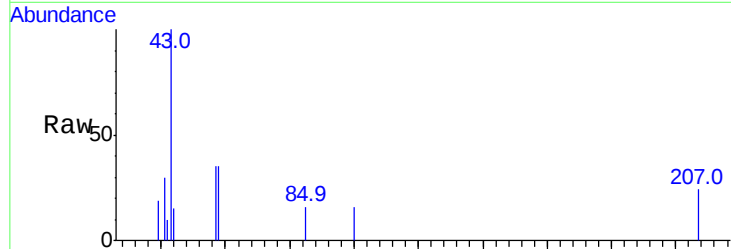


Abundance Ion 43.00 (42.70 to 43.70): VN0
Ion 58.00 (57.70 to 58.70): VN0

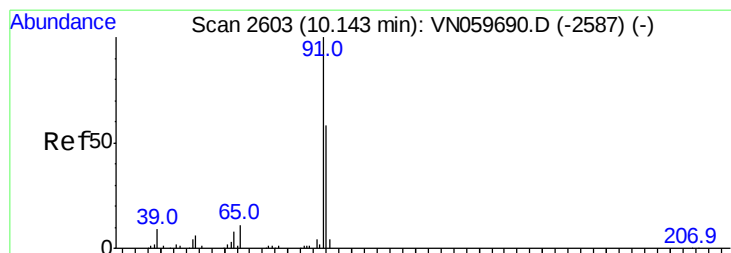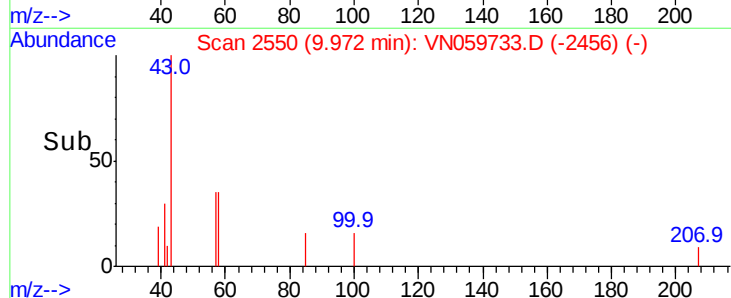
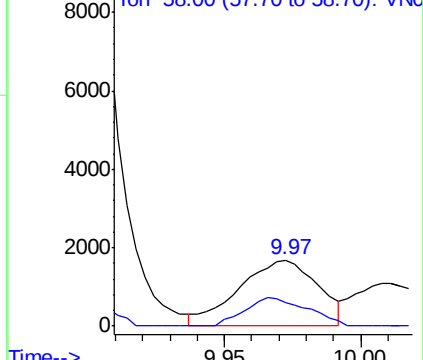



#52
Toluene
Concen: 0.383 ug/l
RT: 10.14 min Scan# 2603
Delta R.T. 0.00 min
Lab File: VN059733.D
Acq: 16 Jan 2020 15:41

Tgt Ion: 92 Resp: 1842
Ion Ratio Lower Upper
92 100
91 170.2 140.4 210.6



Abundance Ion 92.00 (91.70 to 92.70): VN0
Ion 91.00 (90.70 to 91.70): VN0

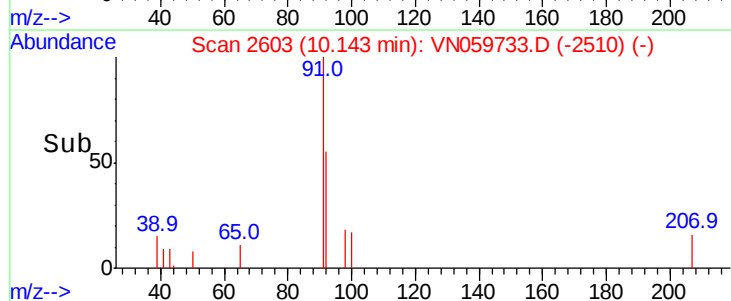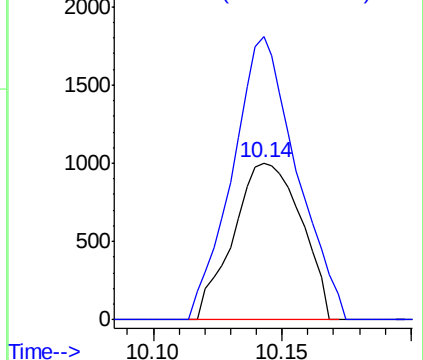


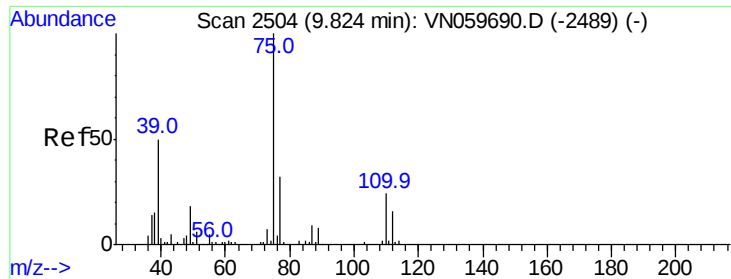




#54
 cis-1,3-Dichloropropene
 Concen: 6.987 ug/l
 RT: 9.89 min Scan# 2524
 Delta R.T. 0.06 min
 Lab File: VN059733.D
 Acq: 16 Jan 2020 15:41

Instrument :
 MSVOA_N
 ClientSampleId :
 PB126118TB

Tgt Ion: 75 Resp: 21979
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.1 37.7#
 39 30.9 46.1 69.1#

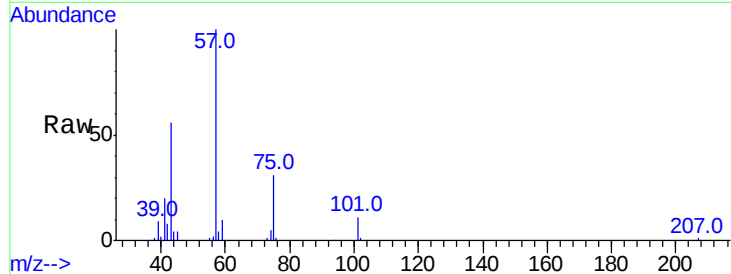


Abundance Ion 74.90 (74.60 to 75.60): VN0
 Ion 76.90 (76.60 to 77.60): VN0
 Ion 39.00 (38.70 to 39.70): VN0


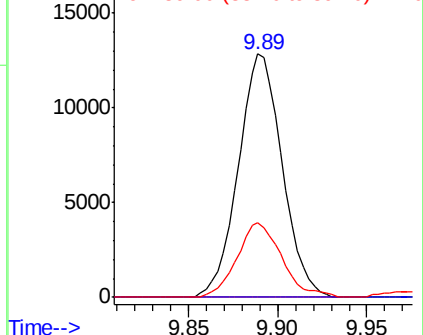



#57
 1,3-Dichloropropane
 Concen: 1.203 ug/l
 RT: 10.75 min Scan# 2793
 Delta R.T. 0.06 min
 Lab File: VN059733.D
 Acq: 16 Jan 2020 15:41

Tgt Ion: 76 Resp: 3637
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.8 38.8#



Abundance Ion 75.90 (75.60 to 76.60): VN0
 Ion 77.90 (77.60 to 78.60): VN0



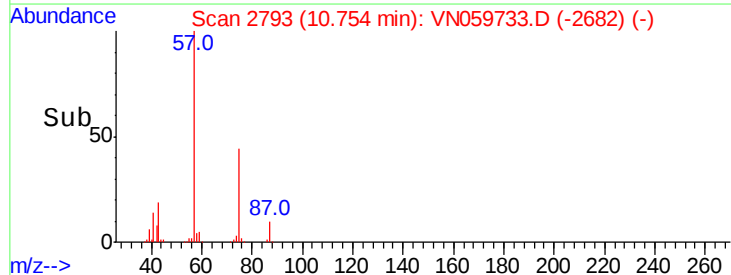
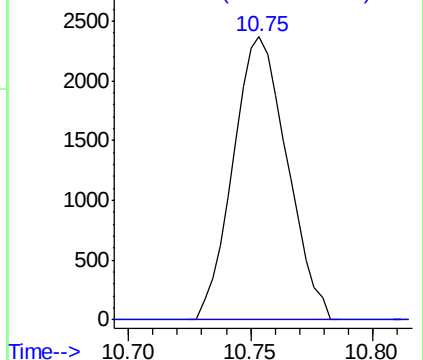


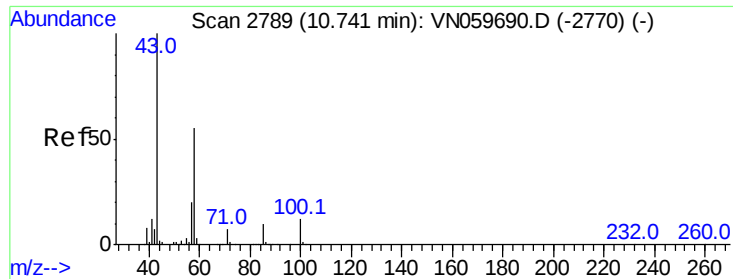

#59
2-Hexanone
Concen: 26.841 ug/l
RT: 10.75 min Scan# 2793
Delta R.T. 0.01 min
Lab File: VN059733.D
Acq: 16 Jan 2020 15:41




Instrument :
MSVOA_N
ClientSampleId :
PB126118TB


Tgt Ion: 43 Resp: 47064
Ion Ratio Lower Upper
43 100
58 20.7 25.8 77.3#

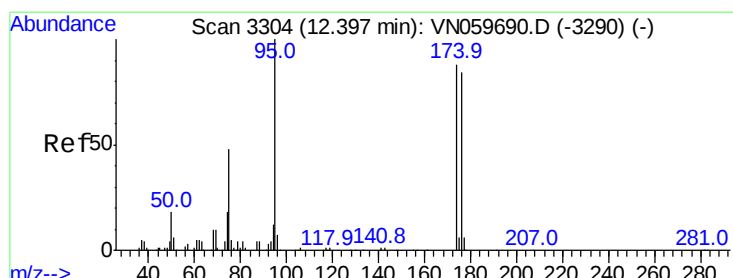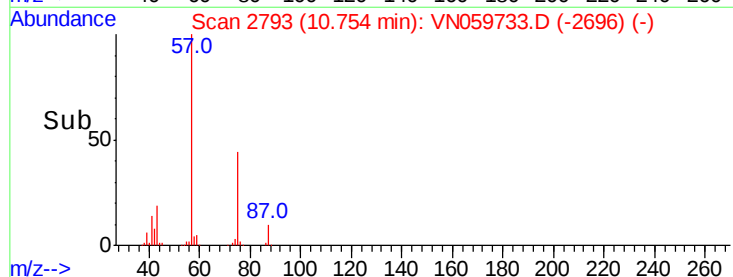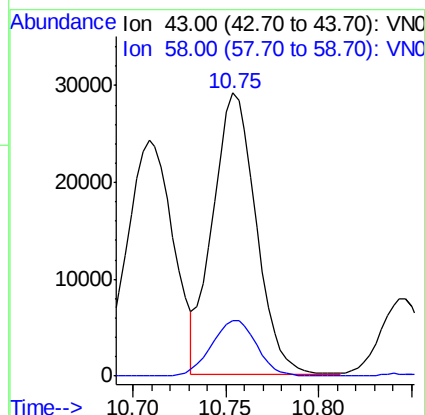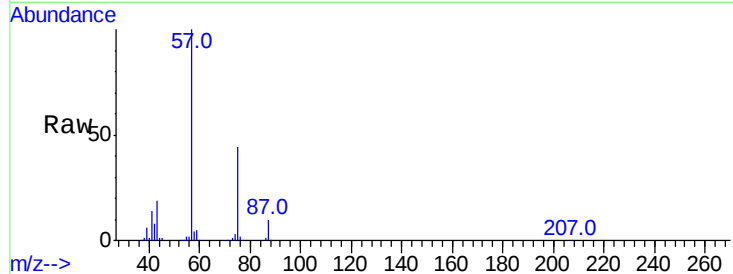

#62
4-Bromofluorobenzene
Concen: 47.043 ug/l
RT: 12.40 min Scan# 3304
Delta R.T. 0.00 min
Lab File: VN059733.D
Acq: 16 Jan 2020 15:41

Tgt Ion: 95 Resp: 114839
Ion Ratio Lower Upper
95 100
174 89.4 0.0 151.4
176 85.8 0.0 146.0


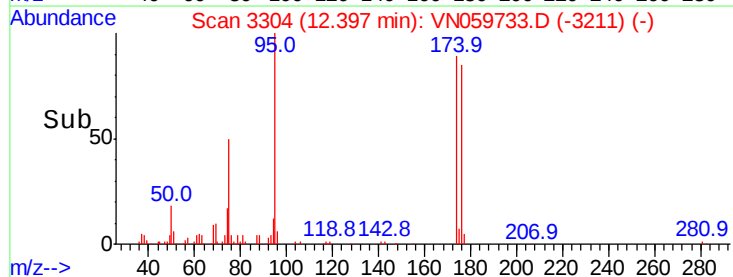
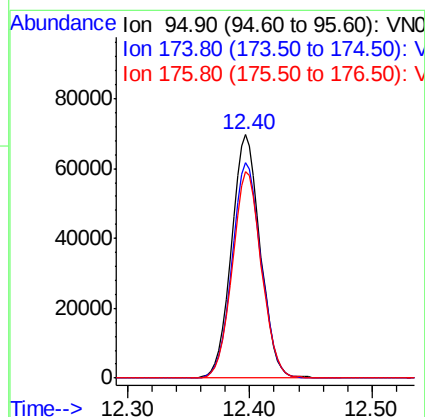
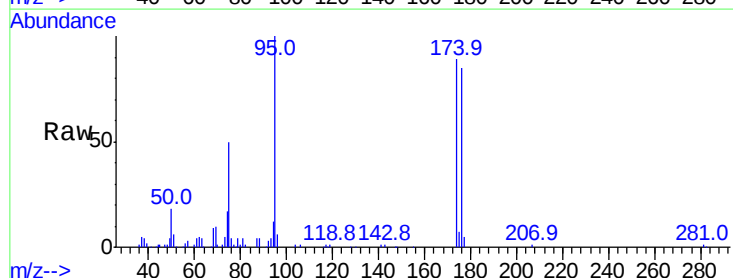


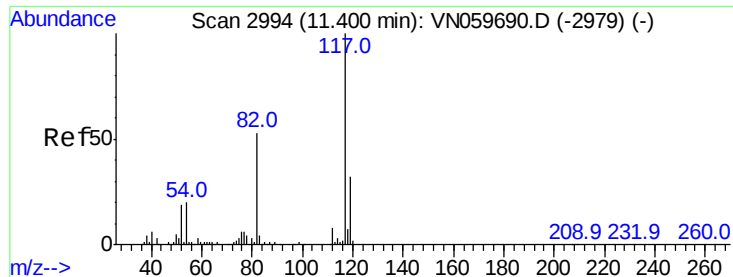

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.40 min Scan# 2994
Delta R.T. 0.00 min
Lab File: VN059733.D
Acq: 16 Jan 2020 15:41




Instrument :
MSVOA_N
ClientSampleId :
PB126118TB


Tgt Ion:117 Resp: 255813
Ion Ratio Lower Upper
117 100
82 52.1 45.9 68.9
119 31.8 25.5 38.3

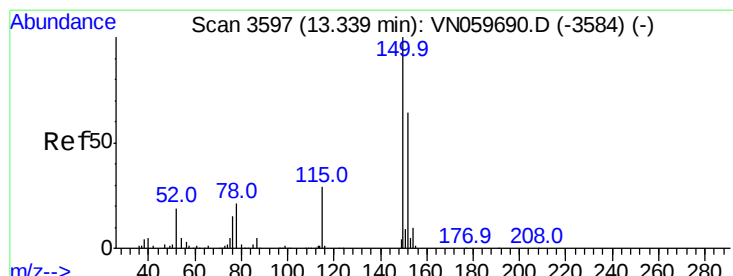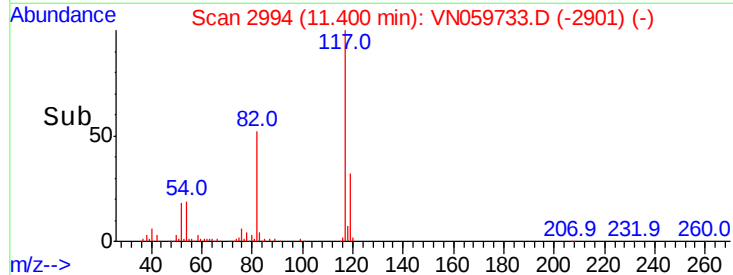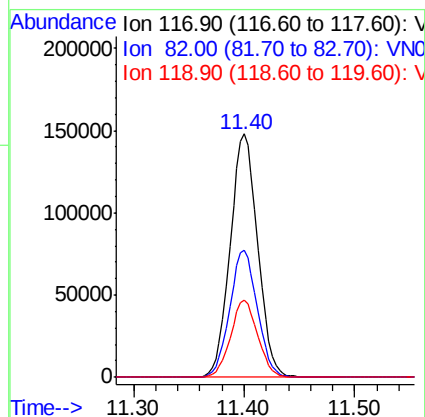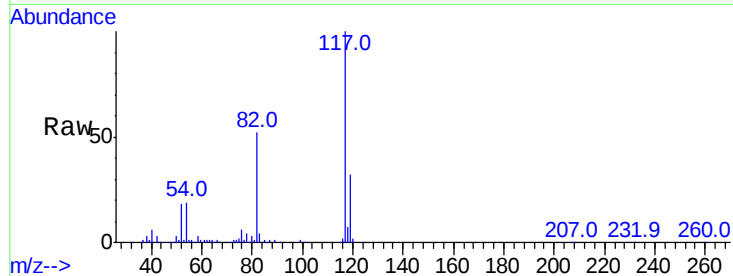

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3597
Delta R.T. 0.00 min
Lab File: VN059733.D
Acq: 16 Jan 2020 15:41

Tgt Ion:152 Resp: 111119
Ion Ratio Lower Upper
152 100
115 56.7 30.3 90.9
150 154.2 0.0 345.2

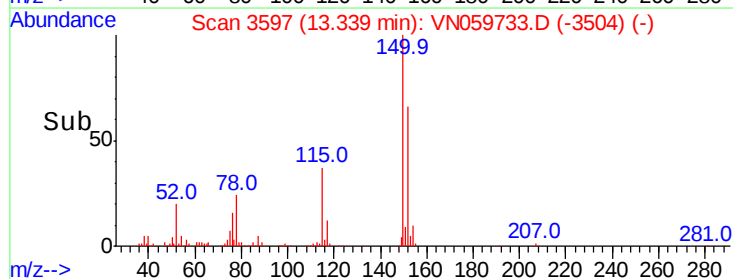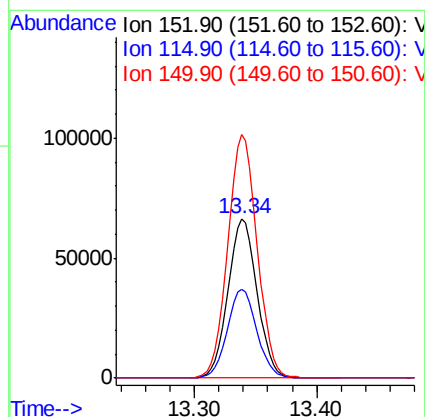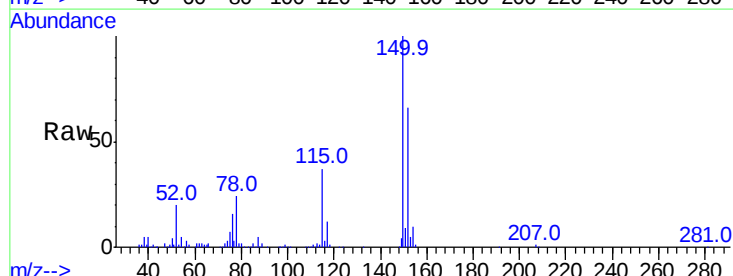

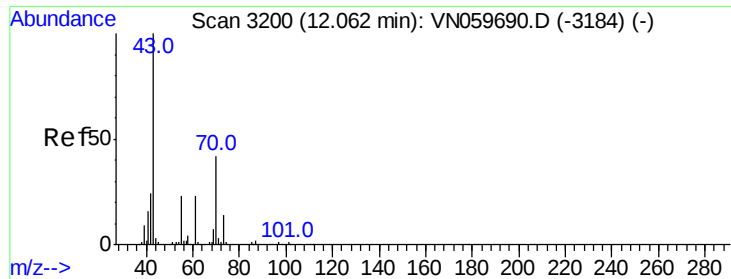

#74

N-ethyl acetate

Concen: 0.546 ug/l

RT: 12.03 min Scan# 3189

Delta R.T. -0.04 min

Lab File: VN059733.D

Acq: 16 Jan 2020 15:41

Instrument :

MSVOA_N

ClientSampled :

PB126118TB

Tgt Ion: 43 Resp: 1727


Ion Ratio Lower Upper

43 100

70 0.0 31.3 46.9#

55 0.0 19.8 29.6#

61 0.0 18.3 27.5#

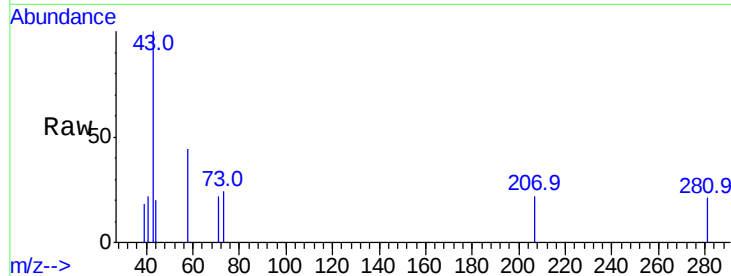



Abundance

Ion 43.00 (42.70 to 43.70): VNC


Ion 70.00 (69.70 to 70.70): VNC

Ion 55.00 (54.70 to 55.70): VNC

Ion 61.00 (60.70 to 61.70): VNC

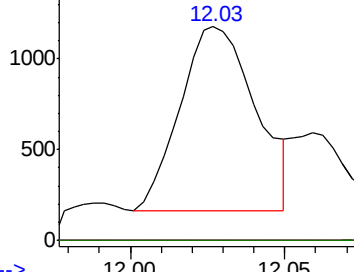

Time-->



#76

1,2,3-Trichloropropane

Concen: 30.393 ug/l

RT: 12.40 min Scan# 3304

Delta R.T. -0.15 min

Lab File: VN059733.D


Acq: 16 Jan 2020 15:41

Tgt Ion: 75 Resp: 56835

Ion Ratio Lower Upper

75 100



77 1.0 0.0 0.0#




Abundance

Ion 74.90 (74.60 to 75.60): VNC

Ion 77.00 (76.70 to 77.70): VNC




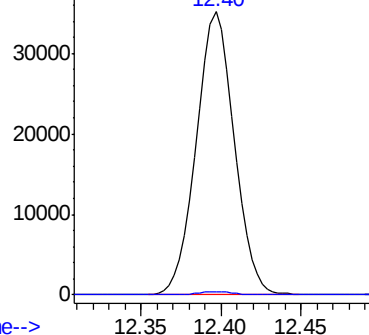


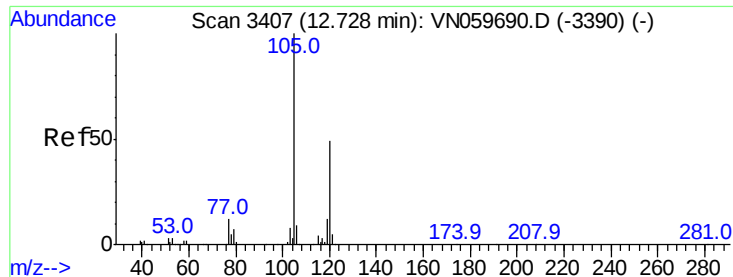

#80
 1,3,5-Trimethylbenzene
 Concen: 0.557 ug/l
 RT: 12.73 min Scan# 3408
 Delta R.T. 0.00 min
 Lab File: VN059733.D
 Acq: 16 Jan 2020 15:41




Instrument :
 MSVOA_N
 ClientSampled :
 PB126118TB


Tgt Ion: 105 Resp: 3816
 Ion Ratio Lower Upper
 105 100
 120 49.8 24.1 72.4

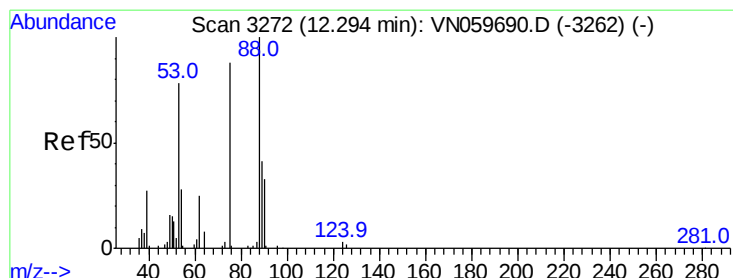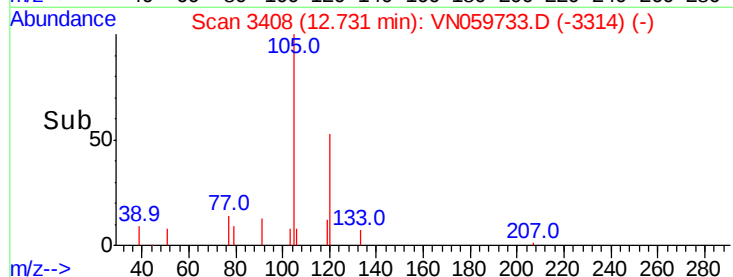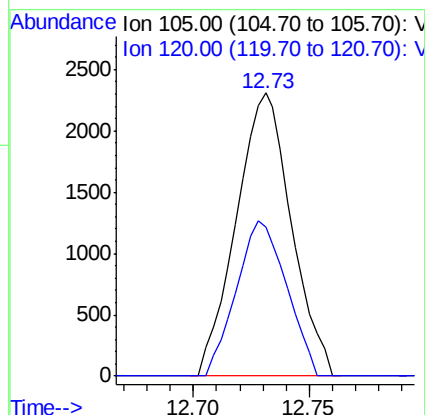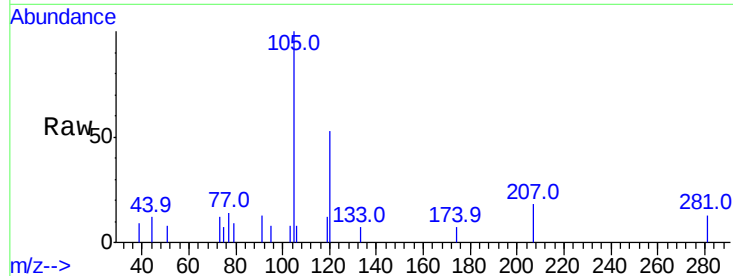

#81
 trans-1,4-Dichloro-2-butene
 Concen: 65.268 ug/l
 RT: 12.40 min Scan# 3304
 Delta R.T. 0.10 min
 Lab File: VN059733.D
 Acq: 16 Jan 2020 15:41

Tgt Ion: 75 Resp: 56835
 Ion Ratio Lower Upper
 75 100
 53 0.0 78.1 117.1#
 89 0.0 35.4 53.2#


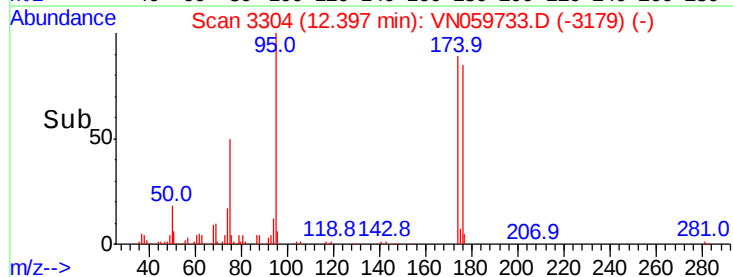
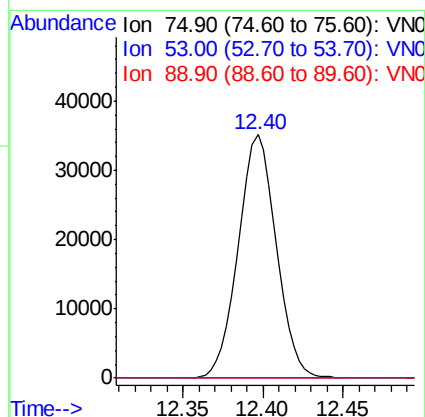
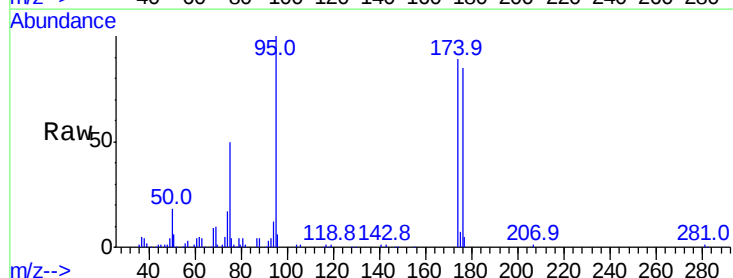


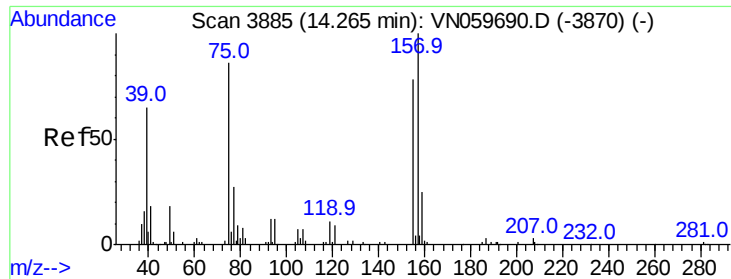

#92
 1,2-Dibromo-3-Chloropropane
 Concen: Below Cal
 RT: 14.26 min Scan# 3883
 Delta R.T. -0.01 min
 Lab File: VN059733.D
 Acq: 16 Jan 2020 15:41




Instrument :
 MSVOA_N
 ClientSampleId :
 PB126118TB


Tgt Ion: 75 Resp: 410
 Ion Ratio Lower Upper
 75 100
 155 0.0 37.0 110.9#
 157 0.0 48.4 145.2#

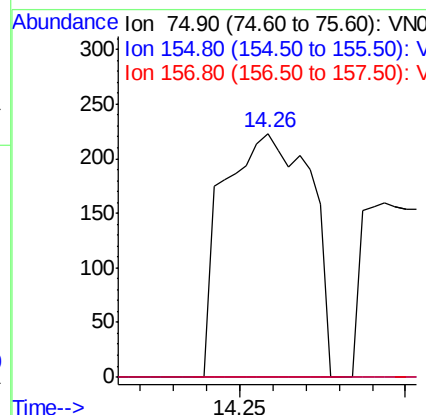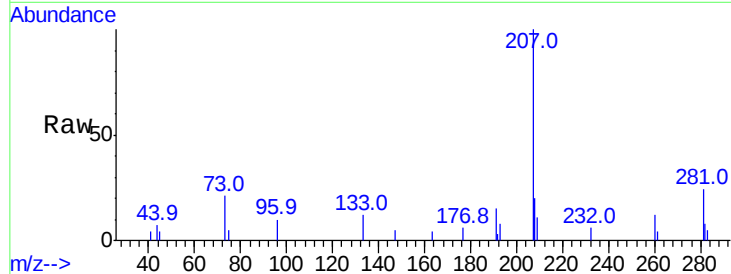

#93
 1,2,4-Trichlorobenzene
 Concen: 0.541 ug/l
 RT: 14.91 min Scan# 4085
 Delta R.T. 0.00 min
 Lab File: VN059733.D
 Acq: 16 Jan 2020 15:41

Tgt Ion: 180 Resp: 1152
 Ion Ratio Lower Upper
 180 100
 182 85.9 46.9 140.7
 145 29.3 15.0 45.1

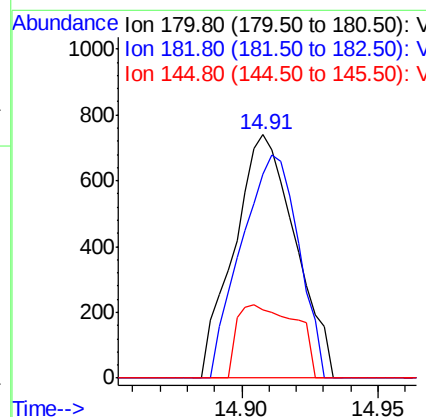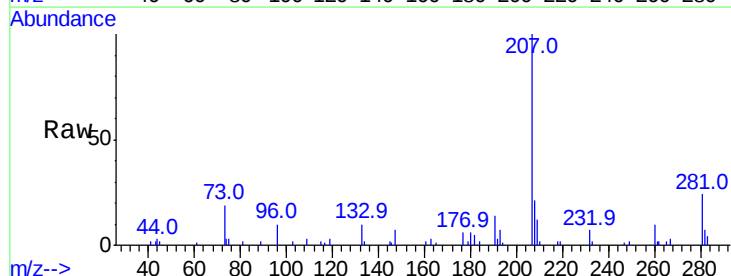



#95

Naphthalene

Concen: 0.796 ug/l

RT: 15.13 min Scan# 4155

Delta R.T. 0.00 min

Lab File: VN059733.D

Acq: 16 Jan 2020 15:41

Instrument :

MSVOA_N

ClientSampleId :

PB126118TB


Tgt Ion:128 Resp: 4824

Ion Ratio Lower Upper

128 100

127 11.1 10.4 15.6

129 10.7 8.6 12.8






Abundance

Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

15.13

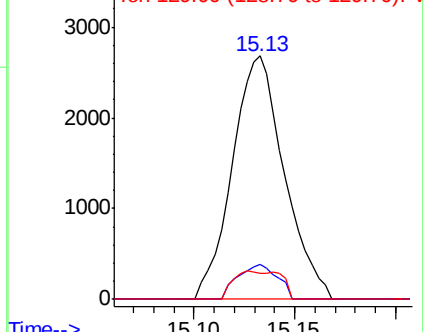

#96

1,2,3-Trichlorobenzene

Concen: 0.799 ug/l

RT: 15.31 min Scan# 4210

Delta R.T. 0.00 min

Lab File: VN059733.D

Acq: 16 Jan 2020 15:41


Tgt Ion:180 Resp: 1656

Ion Ratio Lower Upper

180 100

182 78.5 47.4 142.3

145 50.7 16.3 48.9#



Abundance

Ion 179.80 (179.50 to 180.50): V

Ion 181.80 (181.50 to 182.50): V

Ion 144.90 (144.60 to 145.60): V

15.31

