
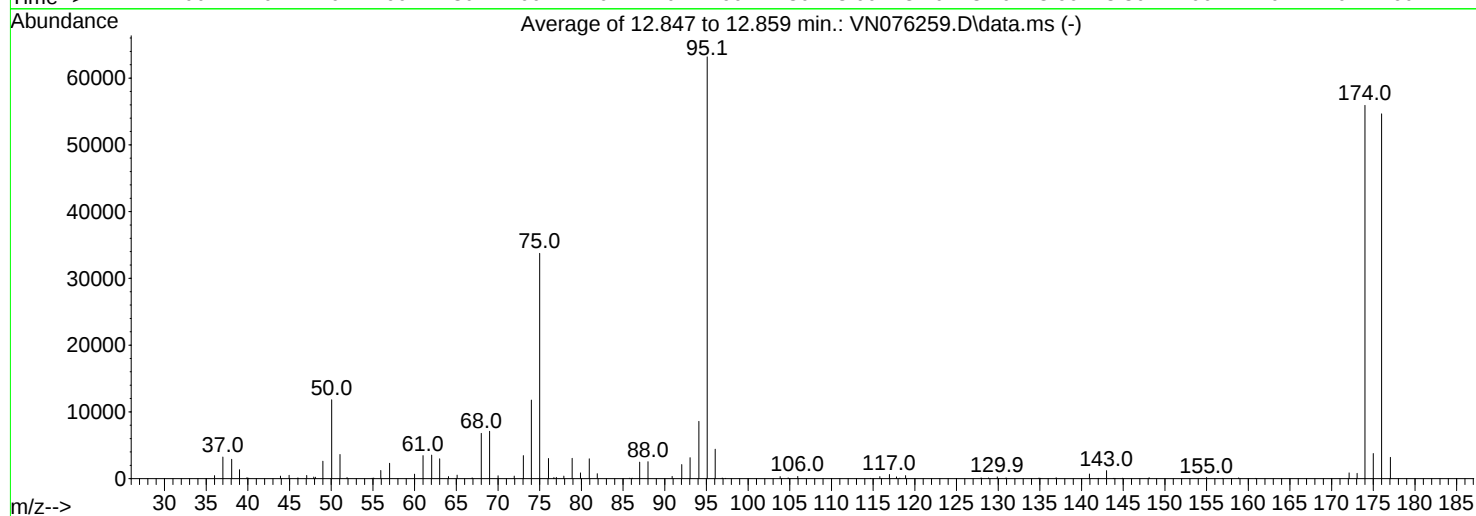


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011623\
Data File : VN076259.D
Acq On : 16 Jan 2023 09:57
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Title : SW846 8260
Last Update : Tue Jan 17 03:59:22 2023

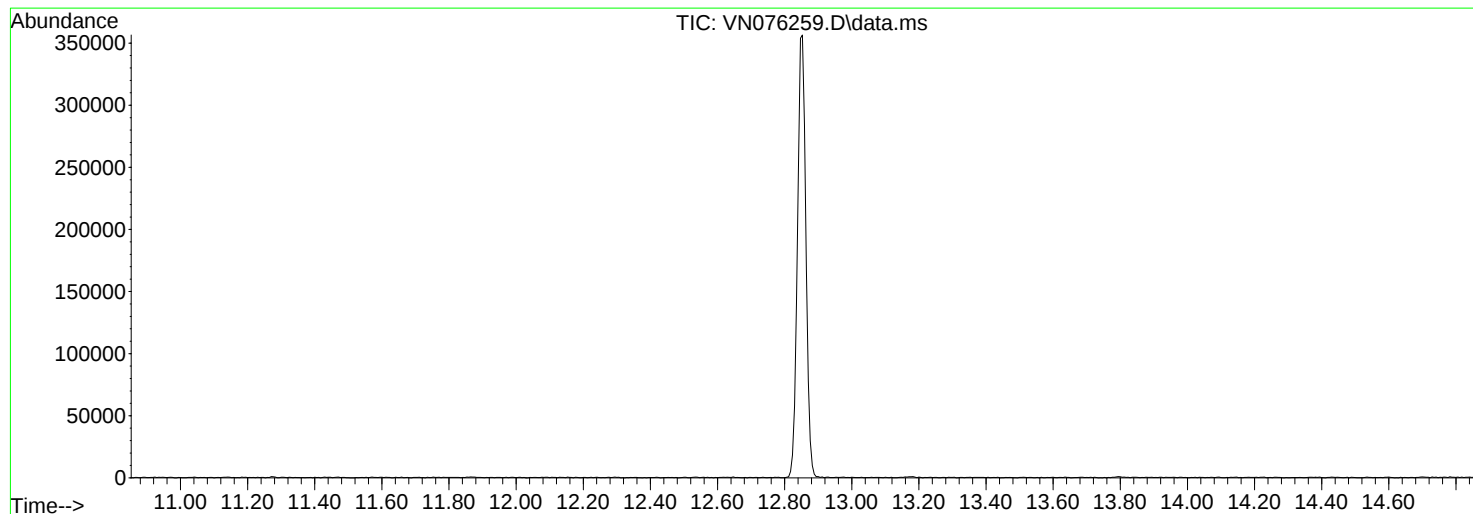

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	11810	PASS
75	95	30	60	53.4	33757	PASS
95	95	100	100	100.0	63187	PASS
96	95	5	9	7.0	4408	PASS
173	174	0.00	2	1.4	785	PASS
174	95	50	100	88.5	55925	PASS
175	174	5	9	6.7	3766	PASS
176	174	95	101	97.7	54648	PASS
177	176	5	9	5.9	3201	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	468	48.10	217	62.05	3534	75.00	3375
37.00	3230	49.00	2627	63.00	2980	76.05	3011
38.05	2896	50.05	11810	64.05	320	76.70	161
39.00	1344	51.05	3614	65.10	536	77.00	191
39.90	171	51.90	178	66.90	130	77.90	393
40.10	66	54.90	76	68.00	6793	78.90	3042
43.90	396	55.10	96	69.00	7089	79.90	867
44.95	515	55.95	1235	70.00	445	80.95	2983
46.00	128	57.00	2292	71.95	397	81.90	736
47.05	492	60.00	661	73.05	3451	85.80	64
47.90	254	61.00	3466	74.00	11767	86.10	66

Average of 12.847 to 12.859 min.: VN076259.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.00	2469	104.80	120	130.95	121	155.00	179
88.00	2544	105.95	345	134.90	98	156.90	63
90.90	328	114.70	55	135.10	61	158.85	122
92.05	2123	115.80	324	136.95	139	160.90	58
93.05	3133	116.95	620	140.95	691	172.10	860
94.10	8590	117.80	278	142.00	52	173.05	785
95.10	63187	118.20	84	143.00	1193	174.00	55925
96.05	4408	118.90	461	143.80	51	175.00	3766
96.90	102	127.95	127	144.00	51	176.00	54648
97.30	51	128.85	118	144.90	87	177.05	3201
103.85	326	129.90	260	148.10	136		

Instrument :

MSVOA_N

ClientSampleId :

BFB