
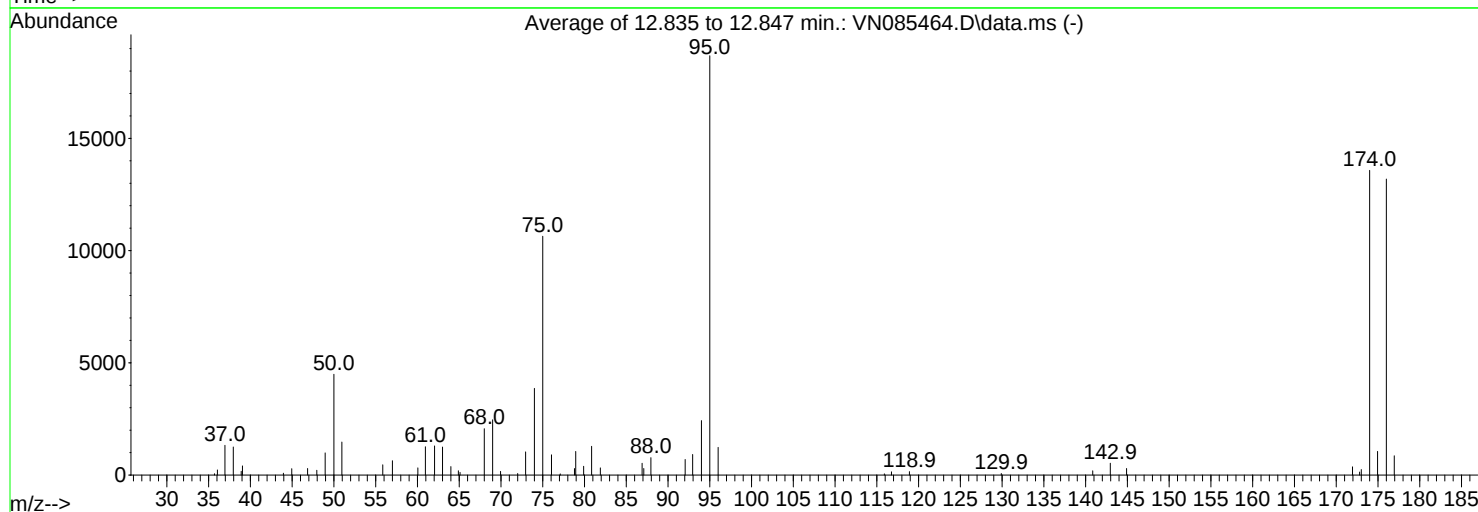


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011625\
Data File : VN085464.D
Acq On : 16 Jan 2025 11:42
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Title : SW846 8260
Last Update : Wed Jan 15 02:16:08 2025

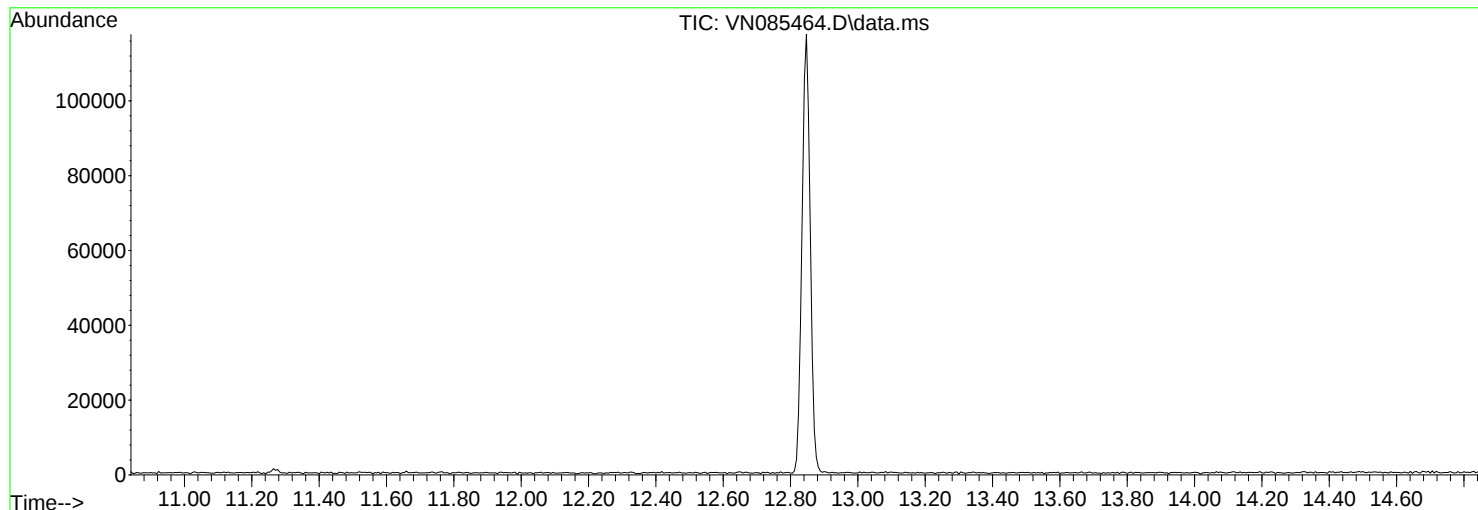

AutoFind: Scans 1850, 1851, 1852; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.0	4490	PASS
75	95	30	60	56.9	10638	PASS
95	95	100	100	100.0	18682	PASS
96	95	5	9	6.6	1233	PASS
173	174	0.00	2	1.8	246	PASS
174	95	50	100	72.7	13574	PASS
175	174	5	9	7.8	1055	PASS
176	174	95	101	97.1	13187	PASS
177	176	5	9	6.5	860	PASS

Average of 12.835 to 12.847 min.: VN085464.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.70	61	50.00	4490	68.00	2065	79.90	392
36.05	228	50.95	1471	69.00	2463	80.85	1282
36.95	1325	55.85	458	69.95	165	81.90	320
37.95	1252	57.00	640	72.00	70	86.90	520
38.90	170	60.05	320	72.95	1032	87.10	293
39.05	409	60.95	1261	74.00	3863	87.95	777
43.95	84	62.05	1299	75.00	10638	92.05	694
44.95	285	63.00	1248	76.05	902	92.95	918
46.85	293	64.00	379	77.10	54	94.00	2428
47.95	214	64.90	192	78.80	291	95.00	18682
48.95	988	65.10	119	78.95	1053	96.00	1233

Average of 12.835 to 12.847 min.: VN085464.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
115.90	56	174.95	1055				
116.75	145	176.00	13187				
118.90	153	176.95	860				
129.90	71						
140.85	190						
142.95	528						
144.90	292						
171.95	367						
172.80	135						
173.00	246						
174.00	13574						

Instrument :

MSVOA_N

ClientSampleId :

BFB