

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN011719\
 Data File : VN053438.D
 Acq On : 17 Jan 2019 16:53
 Operator : JC/SP
 Sample : PB116439TB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 6 Sample Multiplier: 28


Quant Time: Jan 18 00:34:38 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011519W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 16 03:10:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	904256	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1406739	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1347154	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	575008	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	454553	50.86	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.72%	
35) Dibromofluoromethane	7.59	113	409700	51.03	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.06%	
50) Toluene-d8	10.09	98	1768235	52.08	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.16%	
62) 4-Bromofluorobenzene	12.40	95	609615	51.20	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.40%	
Target Compounds						
16) Acetone	3.82	43	11568	5.517	ug/l	99
20) Methylene Chloride	4.56	84	16290	1.702	ug/l	95
43) Isopropyl Acetate	8.17	43	37582	2.836	ug/l #	86
95) Naphthalene	15.14	128	12928	4.796	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN011719\
Data File : VN053438.D
Acq On : 17 Jan 2019 16:53
Operator : JC/SP
Sample : PB116439TB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 6 Sample Multiplier: 28

Quant Time: Jan 18 00:34:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011519W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 16 03:10:53 2019
Response via : Initial Calibration

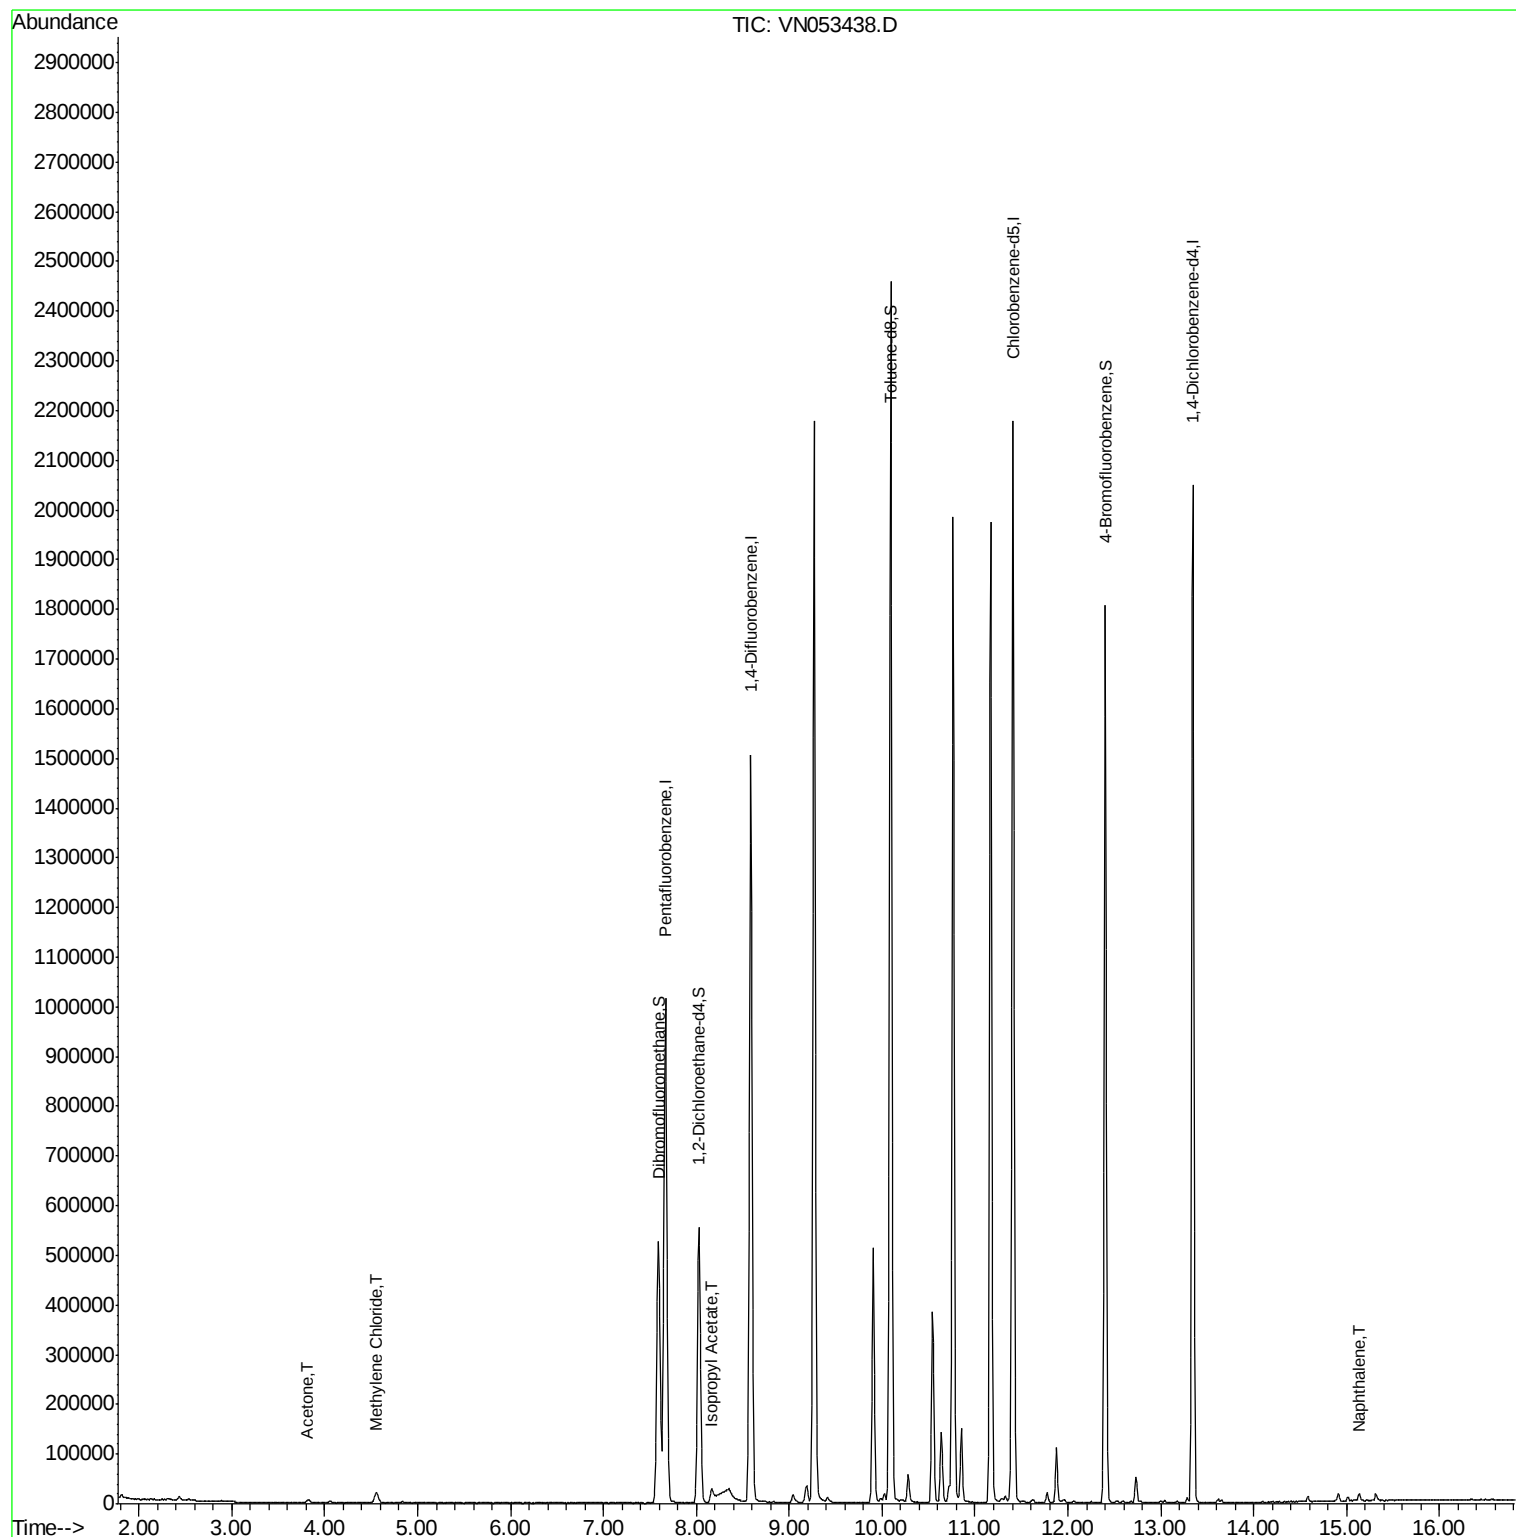



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: VN053438.D


Acq: 17 Jan 2019 16:53

Tot Ion:168 Resp: 904256

Ion Ratio Lower Upper

168 100

99 50.1 39.1 58.7

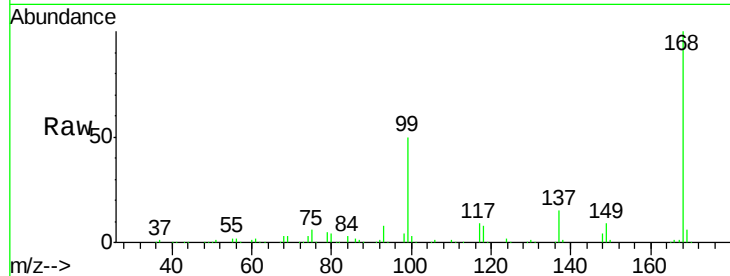

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

7.67

400000

300000



200000

100000

0

Time-->

7.60 7.70 7.80

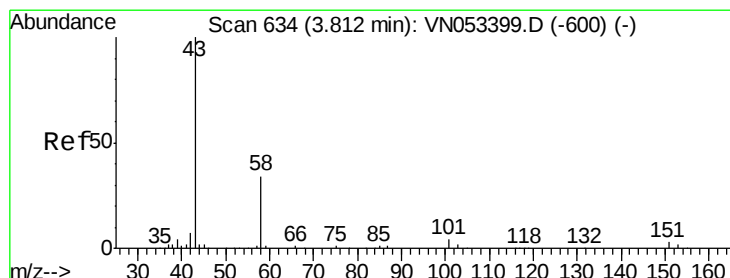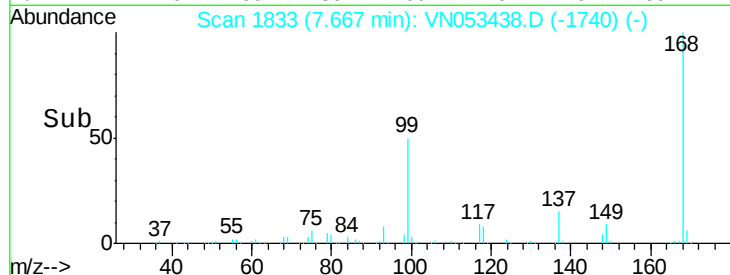

#16

Acetone

Concen: 5.517 ug/l

RT: 3.82 min Scan# 636

Delta R.T. 0.01 min

Lab File: VN053438.D


Acq: 17 Jan 2019 16:53

Tgt Ion: 43 Resp: 11568

Ion Ratio Lower Upper

43 100

58 34.7 27.1 40.7

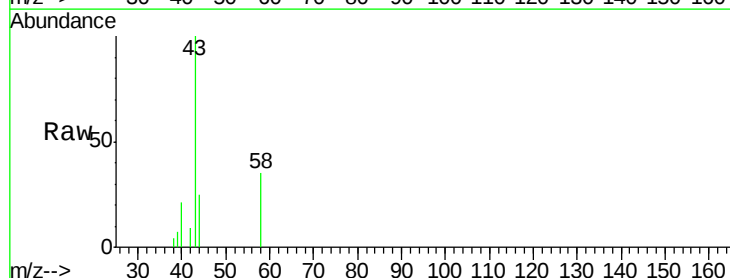

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

3.82

4000

3000


2000


1000

0

Time-->

3.75 3.80 3.85 3.90




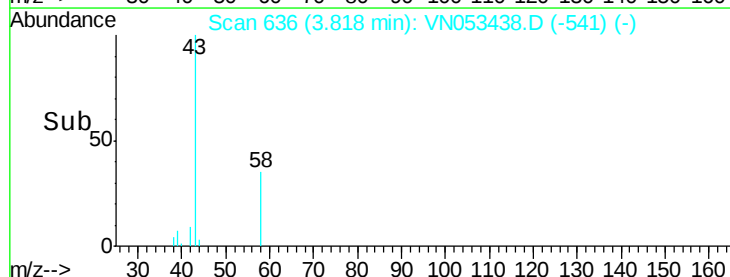


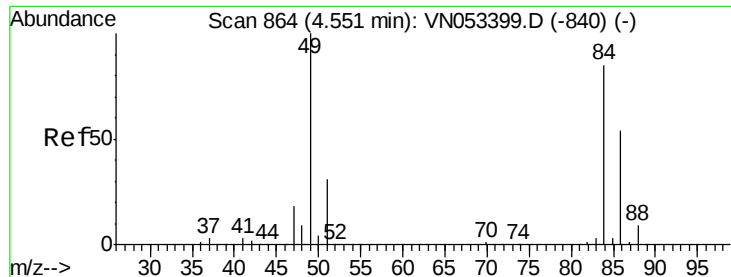

#20
Methvlene Chloride
Concen: 1.702 ug/l
RT: 4.56 min Scan# 866
Delta R.T. 0.01 min
Lab File: VN053438.D
Acq: 17 Jan 2019 16:53

Tot Ion: 84 Resp: 16290




Ion	Ratio	Lower	Upper
84	100		
49	110.1	94.3	141.5
51	32.3	29.4	44.2
86	65.0	51.4	77.0

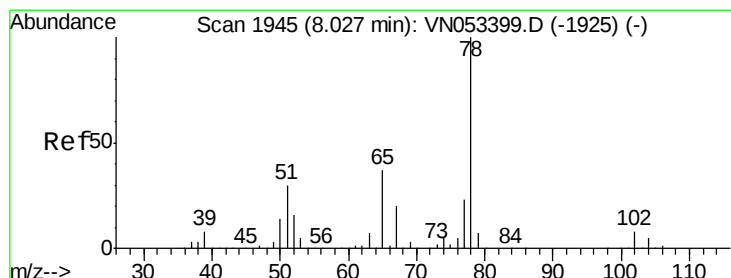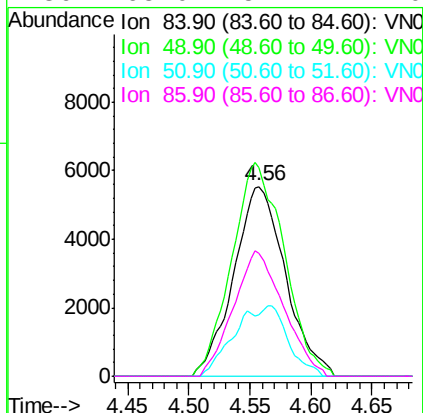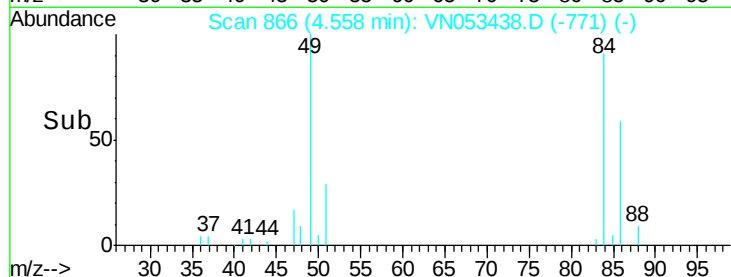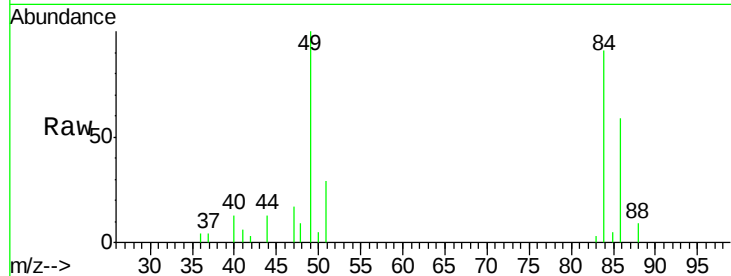


#33
1,2-Dichloroethane-d4
Concen: N.D. ug/l
RT: 8.03 min Scan# 1945
Delta R.T. -0.00 min
Lab File: VN053438.D
Acq: 17 Jan 2019 16:53

Tgt Ion: 65 Resp: 454553

Ion	Ratio	Lower	Upper
65	100		
67	55.1	0.0	111.2

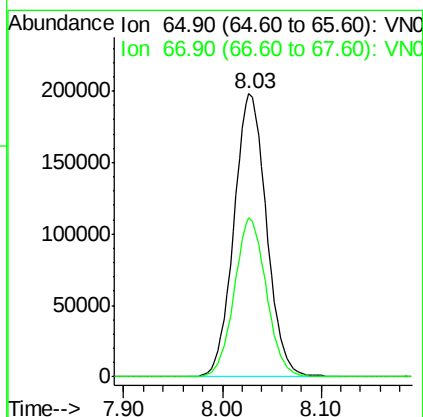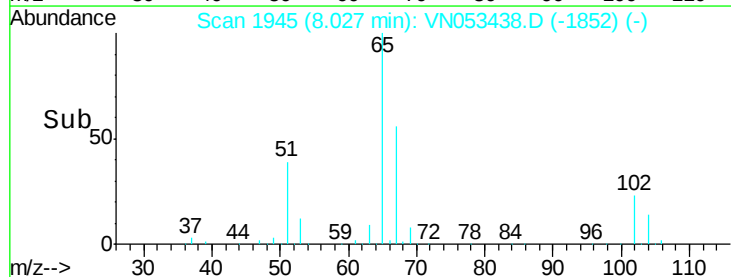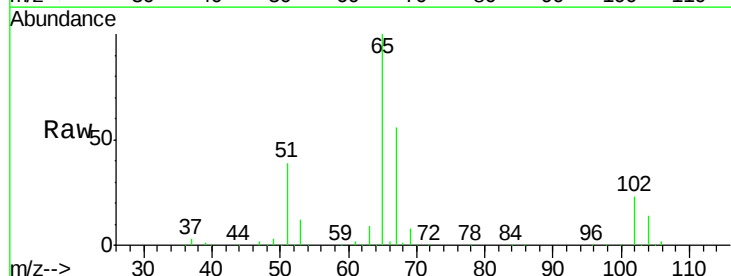


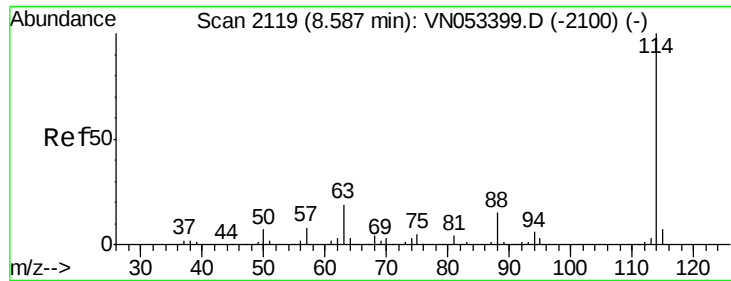

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. -0.00 min
 Lab File: VN053438.D
 Acq: 17 Jan 2019 16:53

Tot Ion:114 Resp: 1406739




Ion	Ratio	Lower	Upper
114	100		
63	19.6	0.0	38.6
88	15.7	0.0	30.4

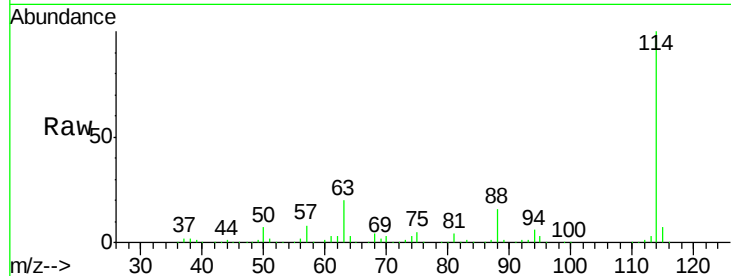

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN


Ion 87.90 (87.60 to 88.60): VN

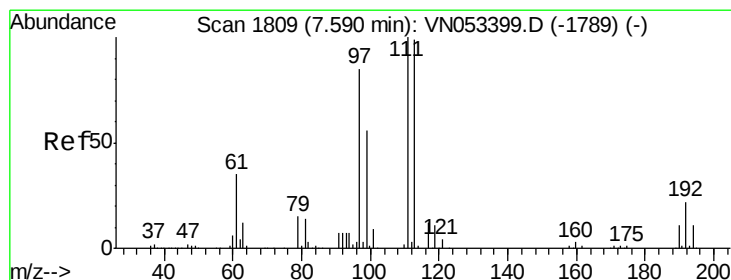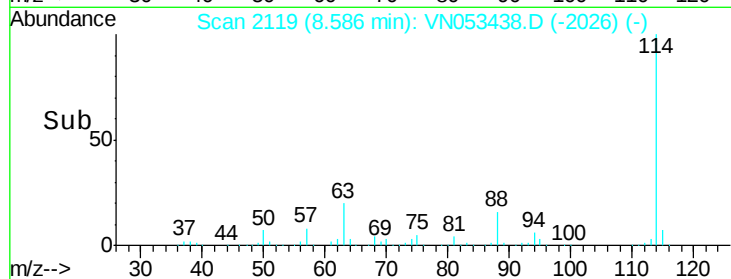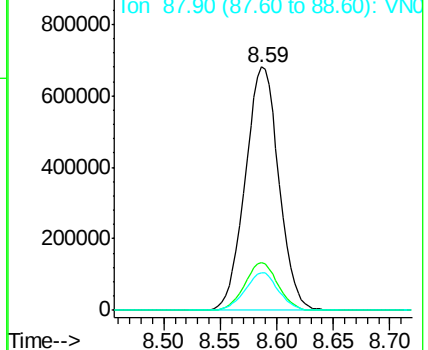

#35
 Dibromofluoromethane
 Concen: 50.000 ug/l
 RT: 7.59 min Scan# 1810
 Delta R.T. 0.00 min
 Lab File: VN053438.D
 Acq: 17 Jan 2019 16:53

Tgt Ion:113 Resp: 409700



Ion	Ratio	Lower	Upper
113	100		
111	102.7	81.1	121.7
192	22.9	18.2	27.2

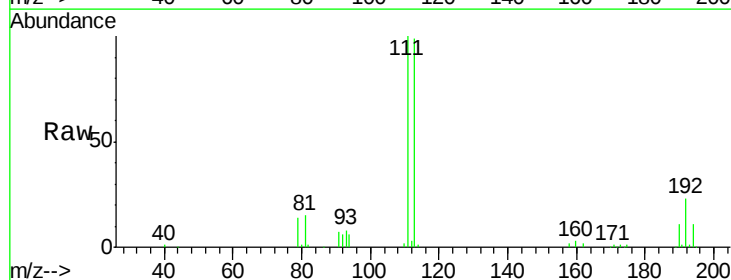


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

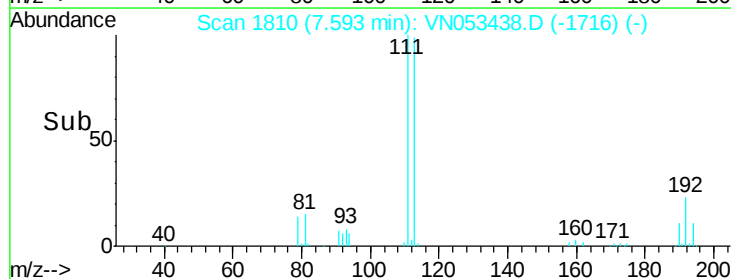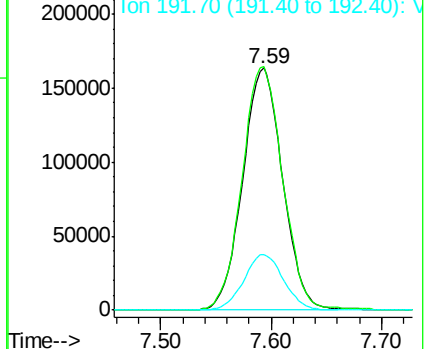

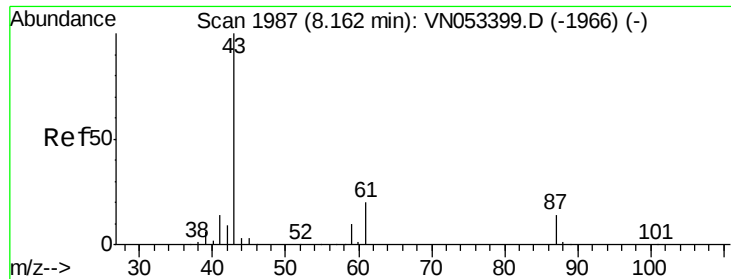

#43

Isopropyl Acetate

Concen: 2.836 ug/l

RT: 8.17 min Scan# 1988


Delta R.T. 0.00 min

Lab File: VN053438.D

Acq: 17 Jan 2019 16:53

Tot Ion: 43 Resp: 37582




Ion	Ratio	Lower	Upper
43	100		
61	19.2	23.9	35.9#
87	12.9	11.0	16.6

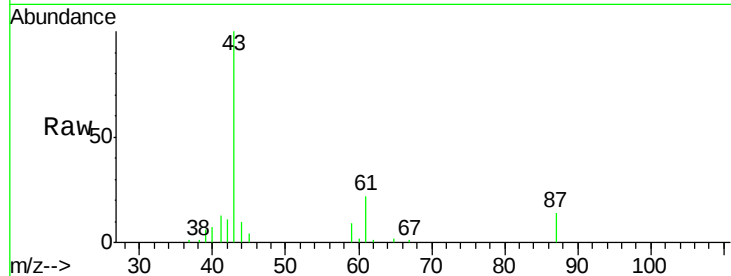

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

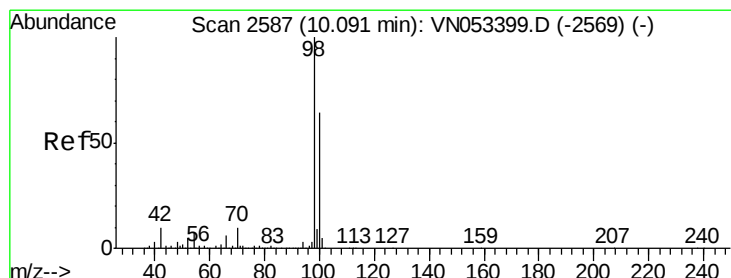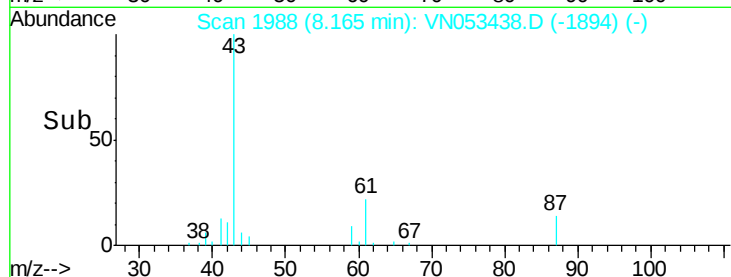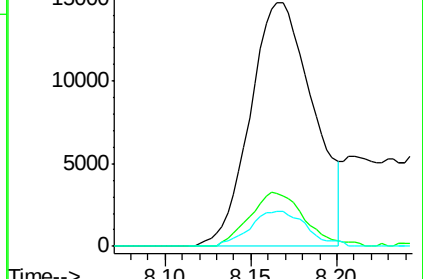

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.09 min Scan# 2587


Delta R.T. -0.00 min

Lab File: VN053438.D

Acq: 17 Jan 2019 16:53



Tgt Ion: 98 Resp: 1768235


Ion	Ratio	Lower	Upper
98	100		
100	64.8	51.4	77.0

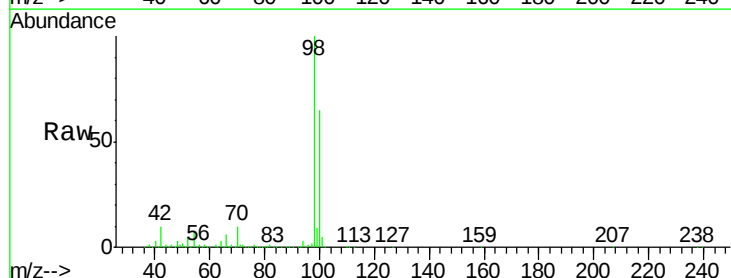

Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN0

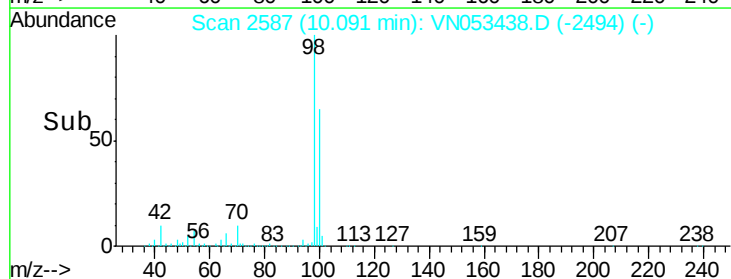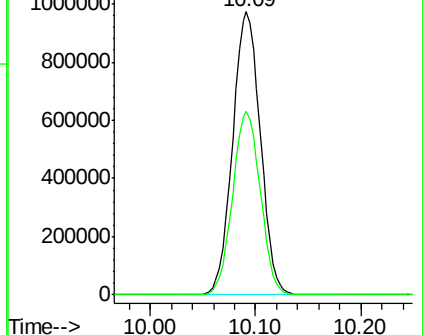

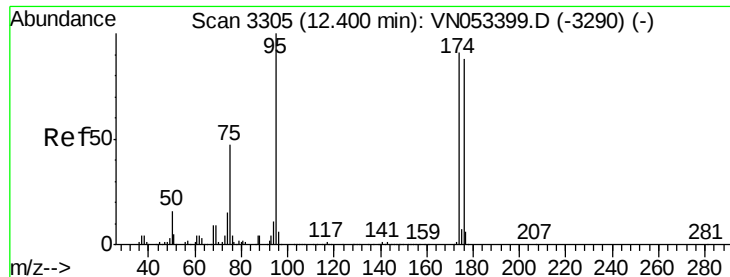

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.00 min

Lab File: VN053438.D

Acq: 17 Jan 2019 16:53


Tot Ion: 95 Resp: 609615

Ion Ratio Lower Upper

95 100

174 91.2 0.0 183.2




176 88.6 0.0 177.4

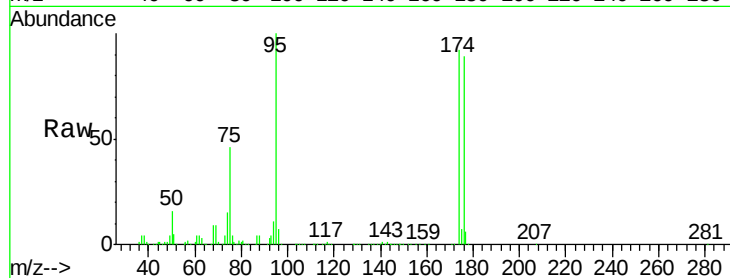

Abundance Ion 94.90 (94.60 to 95.60): VN053399.D (-3290) (-)

Ion 173.80 (173.50 to 174.50): VN053399.D (-3290) (-)

Ion 175.80 (175.50 to 176.50): VN053399.D (-3290) (-)

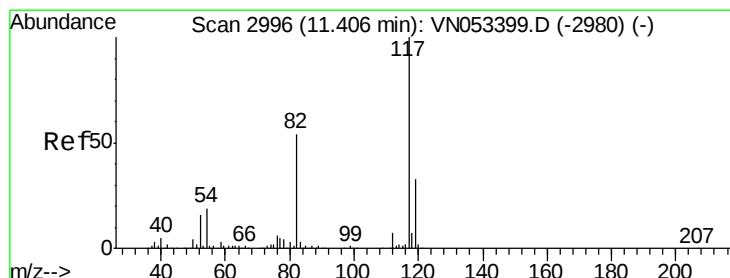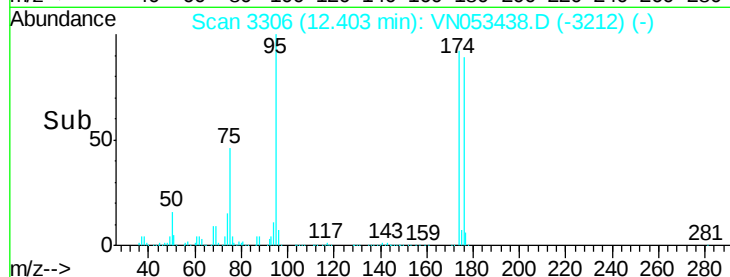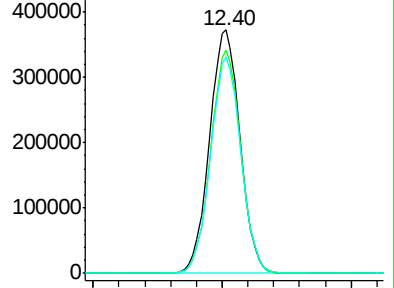

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2997

Delta R.T. 0.00 min

Lab File: VN053438.D

Acq: 17 Jan 2019 16:53


Tgt Ion: 117 Resp: 1347154

Ion Ratio Lower Upper

117 100

82 52.6 42.9 64.3



119 32.4 26.0 39.0

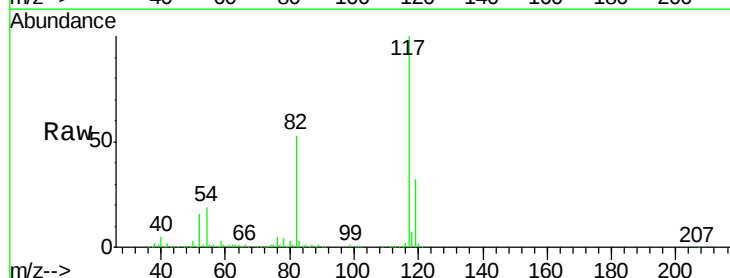


Abundance Ion 116.90 (116.60 to 117.60): VN053399.D (-2980) (-)

Ion 82.00 (81.70 to 82.70): VN053399.D (-2980) (-)

Ion 118.90 (118.60 to 119.60): VN053399.D (-2980) (-)

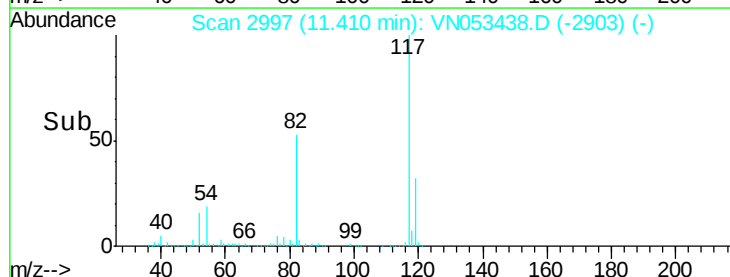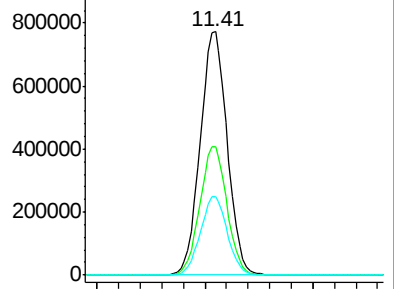


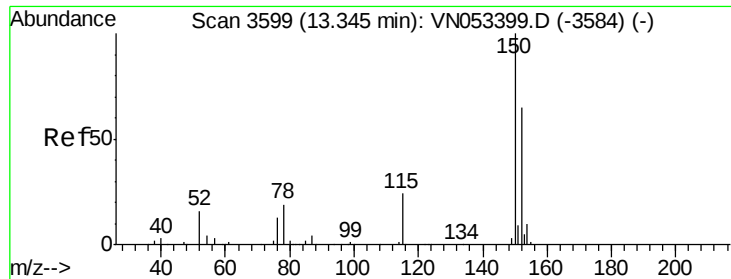




#72

1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.35 min Scan# 3599
Delta R.T. -0.00 min
Lab File: VN053438.D
Acq: 17 Jan 2019 16:53

Tot Ion	Ratio	Lower	Upper
152	100		
115	55.4	27.8	83.4
150	156.3	0.0	349.0

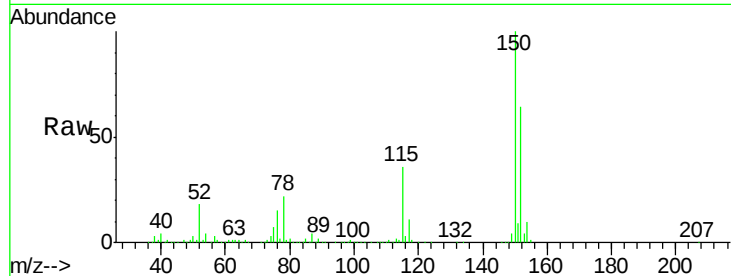


Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

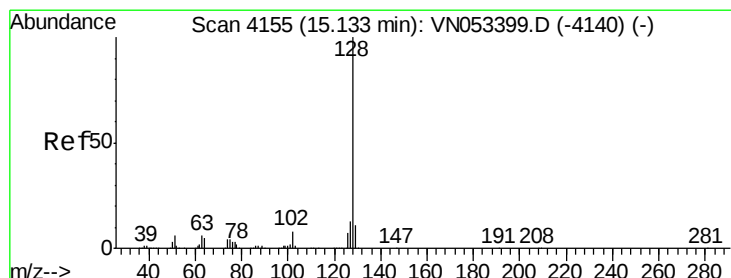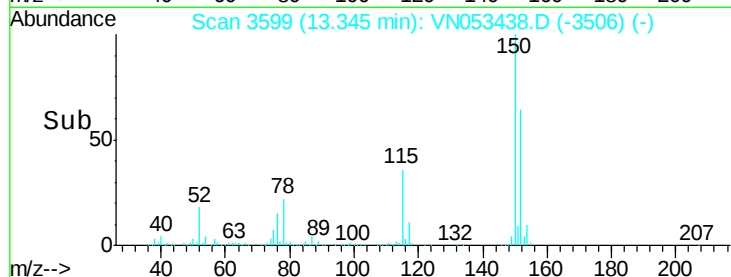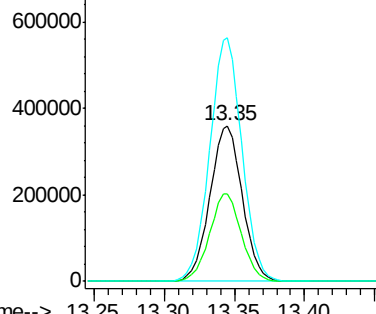

#95

Naphthalene
Concen: 4.796 ug/l
RT: 15.14 min Scan# 4156
Delta R.T. 0.00 min
Lab File: VN053438.D
Acq: 17 Jan 2019 16:53

Tgt Ion	Ratio	Lower	Upper
128	100		
127	12.5	10.3	15.5
129	10.3	8.6	13.0

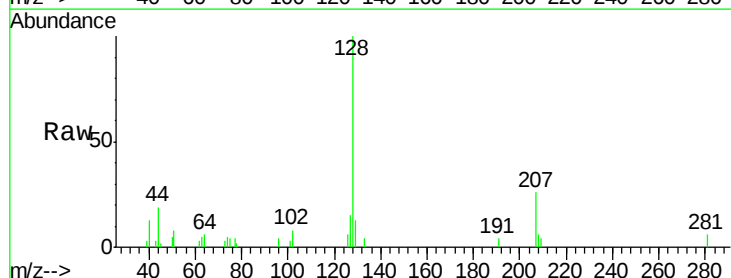

Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

