

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN011719\
 Data File : VN053449.D
 Acq On : 17 Jan 2019 21:47
 Operator : JC/SP
 Sample : PB116439ZHE#11
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 17 Sample Multiplier: 28


Quant Time: Jan 18 01:13:55 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011519W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 16 03:10:53 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	907359	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1419826	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1358282	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	593514	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	464596	51.80	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.60%	
35) Dibromofluoromethane	7.59	113	413042	50.97	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.94%	
50) Toluene-d8	10.09	98	1782036	52.00	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.00%	
62) 4-Bromofluorobenzene	12.40	95	614097	51.10	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.20%	
Target Compounds						
16) Acetone	3.82	43	12677	6.025	ug/l	92
20) Methylene Chloride	4.56	84	17147	1.785	ug/l	97
43) Isopropyl Acetate	8.17	43	46739	3.494	ug/l #	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN011719\
Data File : VN053449.D
Acq On : 17 Jan 2019 21:47
Operator : JC/SP
Sample : PB116439ZHE#11
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 17 Sample Multiplier: 28

Quant Time: Jan 18 01:13:55 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011519W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 16 03:10:53 2019
Response via : Initial Calibration

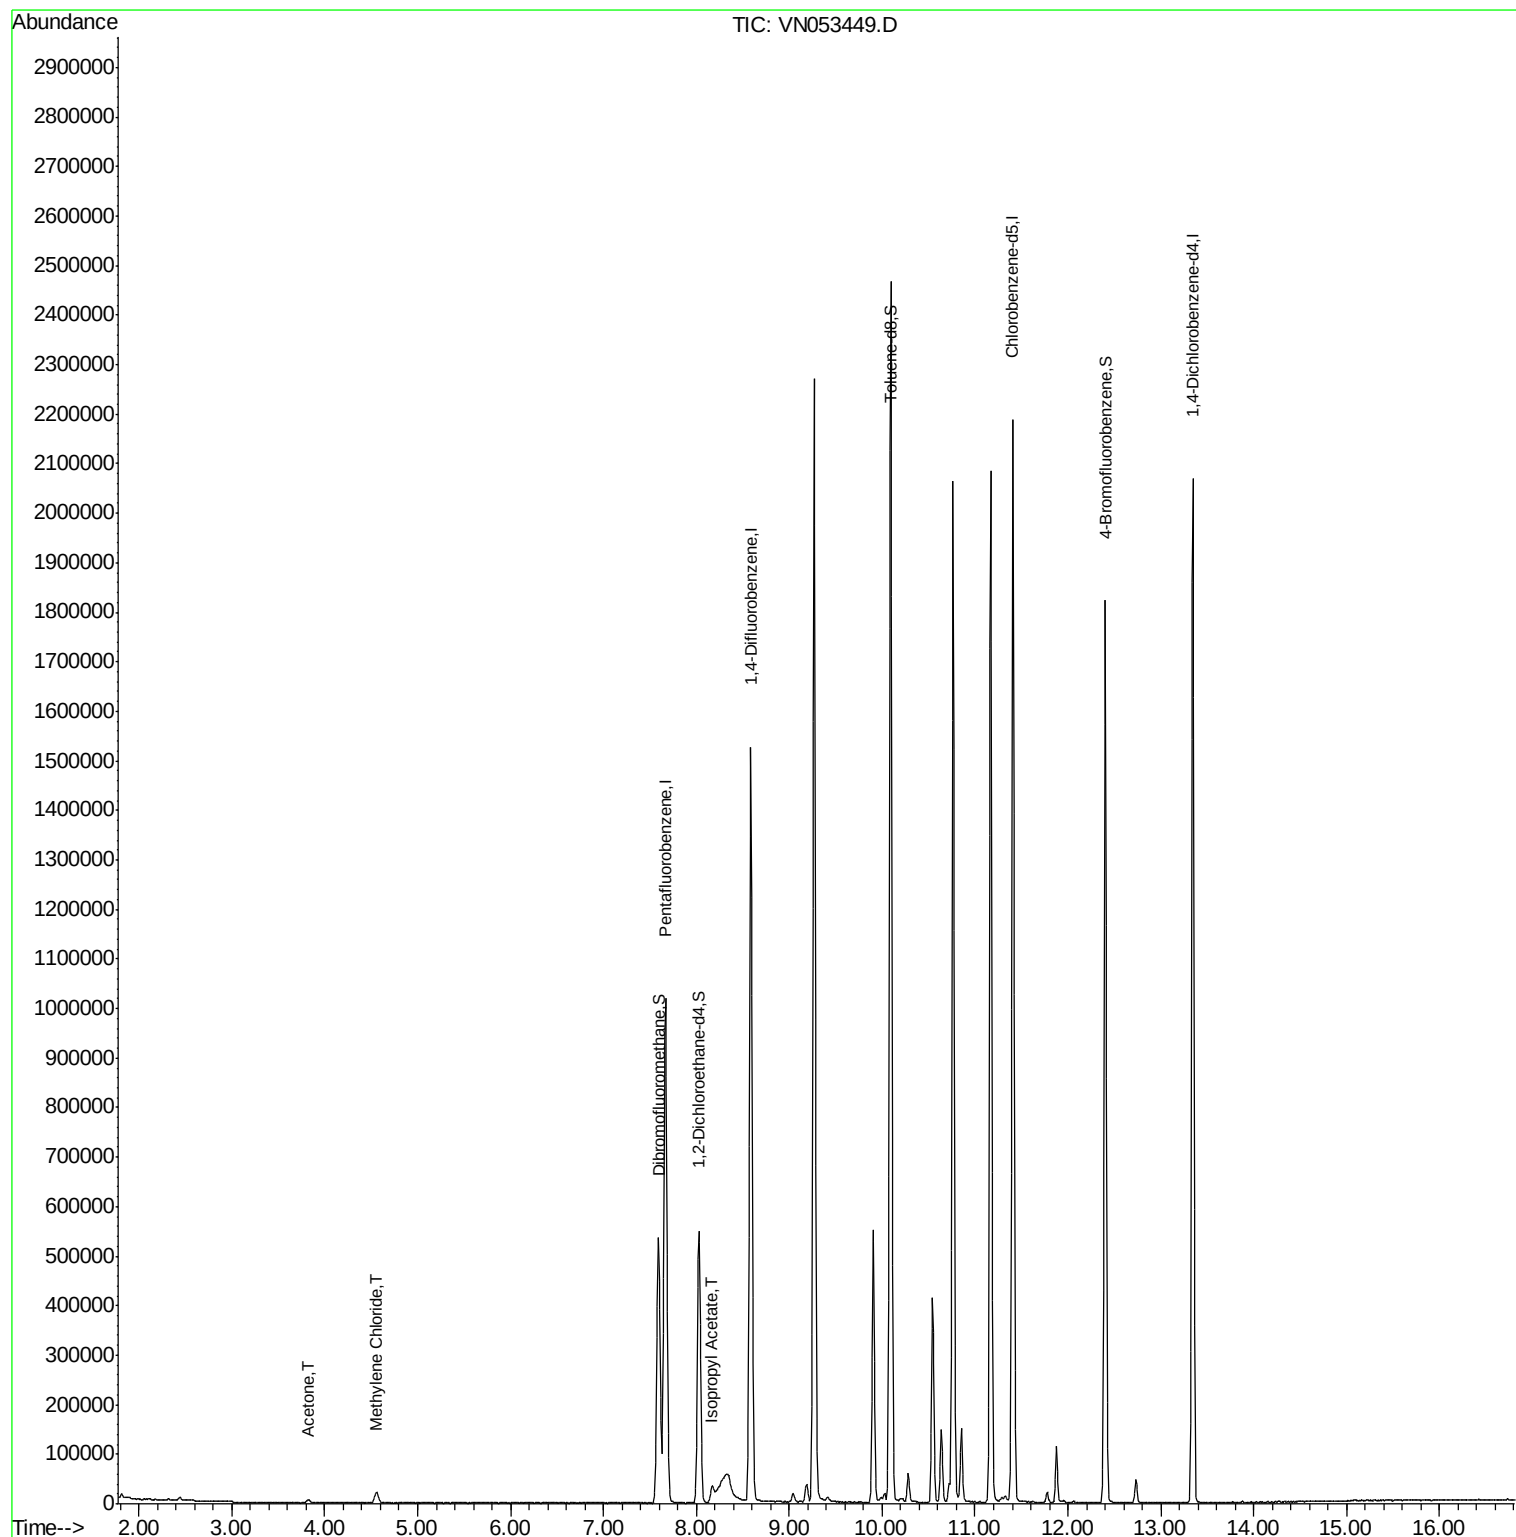

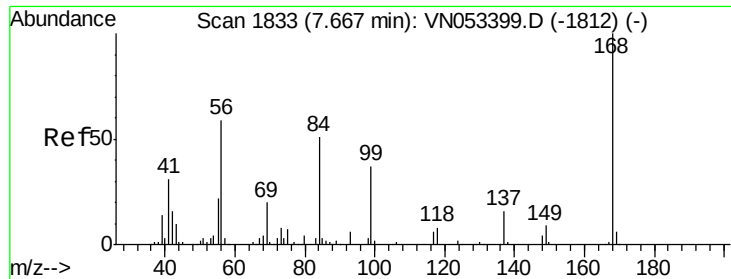

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: VN053449.D


Acq: 17 Jan 2019 21:47

Tot Ion:168 Resp: 907359

Ion Ratio Lower Upper

168 100

99 50.0 39.1 58.7

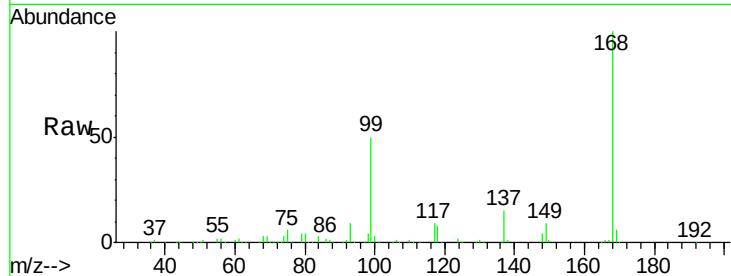

Abundance Ion 167.90 (167.60 to 168.60): VN053399.D (-1812) (-)

Ion 98.90 (98.60 to 99.60): VN053399.D (-1812) (-)

7.67

400000



300000

200000

100000

0

Time-->

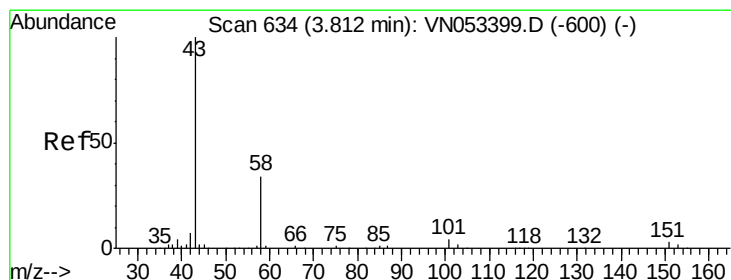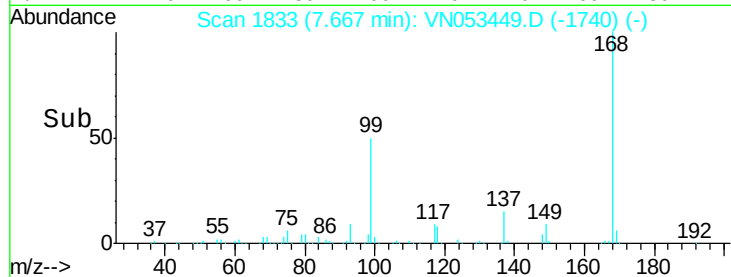

#16

Acetone

Concen: 6.025 ug/l

RT: 3.82 min Scan# 637

Delta R.T. 0.01 min

Lab File: VN053449.D


Acq: 17 Jan 2019 21:47

Tgt Ion: 43 Resp: 12677

Ion Ratio Lower Upper

43 100

58 29.3 27.1 40.7

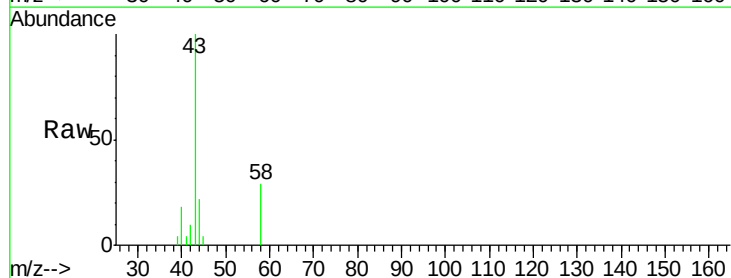

Abundance Ion 43.00 (42.70 to 43.70): VN053399.D (-600) (-)

Ion 58.00 (57.70 to 58.70): VN053399.D (-600) (-)

3.82

5000

4000


3000


2000

1000

0

Time-->




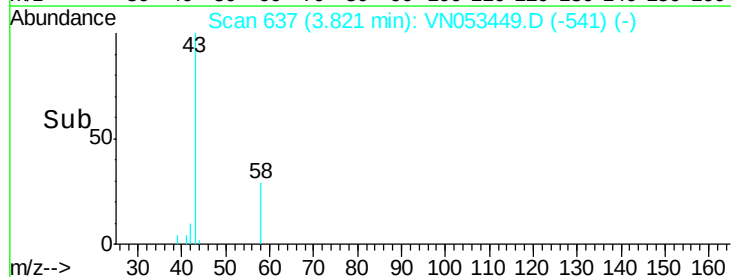


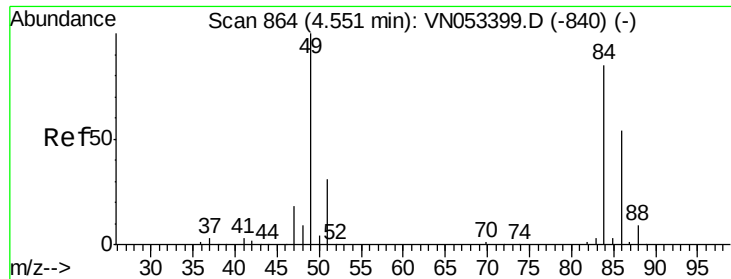

#20
Methylene Chloride
Concen: 1.785 ug/l
RT: 4.56 min Scan# 866
Delta R.T. 0.01 min
Lab File: VN053449.D
Acq: 17 Jan 2019 21:47

Tot Ion: 84 Resp: 17147




Ion	Ratio	Lower	Upper
84	100		
49	118.8	94.3	141.5
51	39.3	29.4	44.2
86	70.2	51.4	77.0

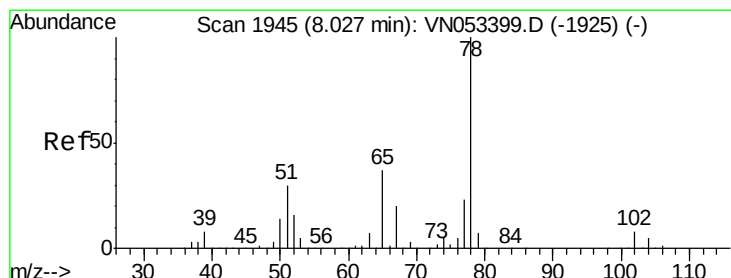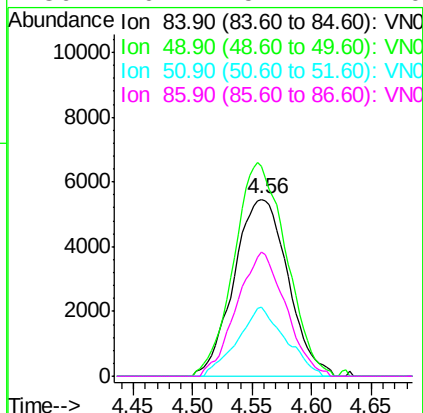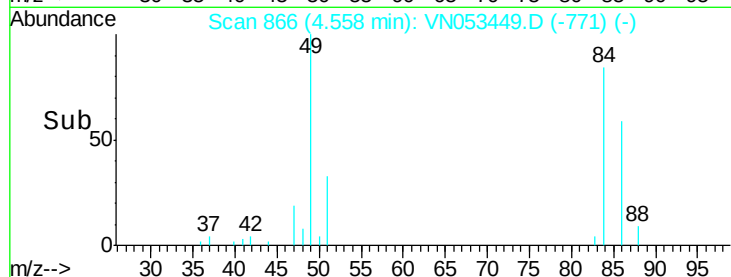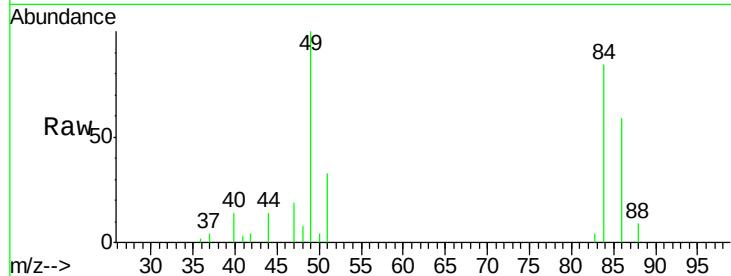


#33
1,2-Dichloroethane-d4
Concen: Below ug/l
RT: 8.03 min Scan# 1945
Delta R.T. 0.00 min
Lab File: VN053449.D
Acq: 17 Jan 2019 21:47

Tgt Ion: 65 Resp: 464596

Ion	Ratio	Lower	Upper
65	100		
67	55.5	0.0	111.2

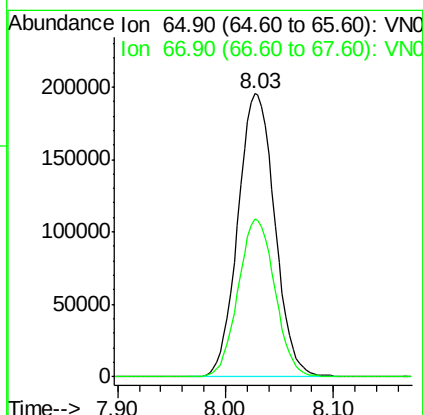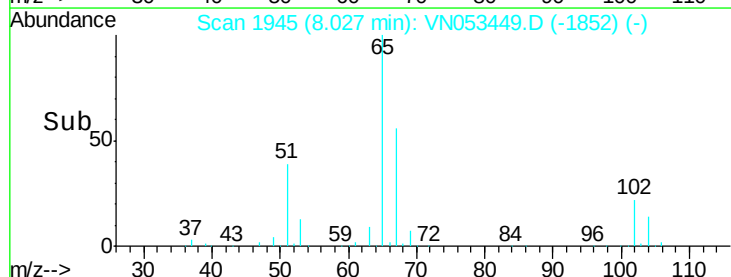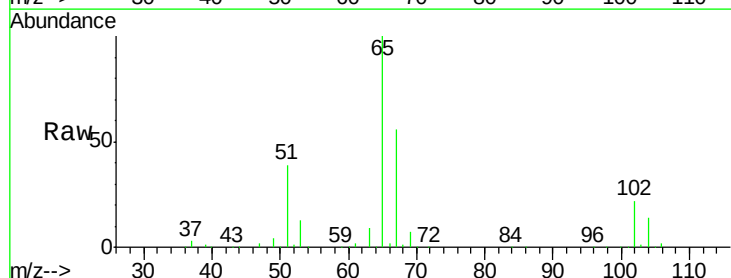


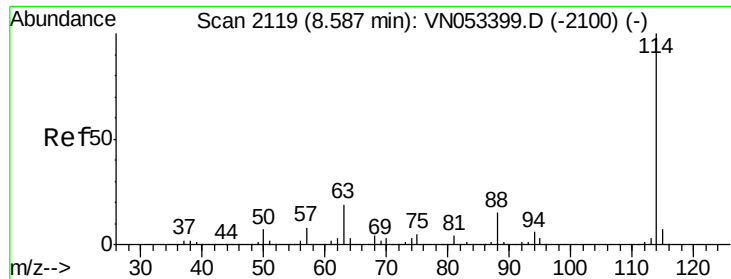

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.59 min Scan# 2119
Delta R.T. 0.00 min
Lab File: VN053449.D
Acq: 17 Jan 2019 21:47

Tot Ion:114 Resp: 1419826




Ion	Ratio	Lower	Upper
114	100		
63	19.8	0.0	38.6
88	15.8	0.0	30.4

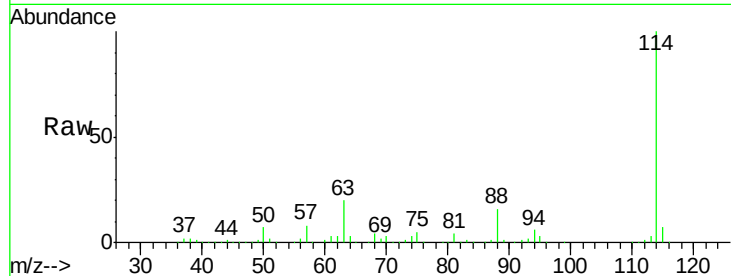

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN


Ion 87.90 (87.60 to 88.60): VN

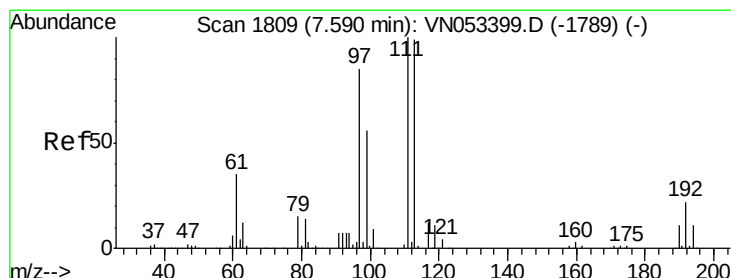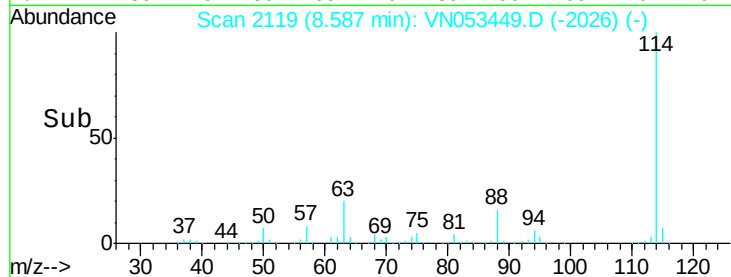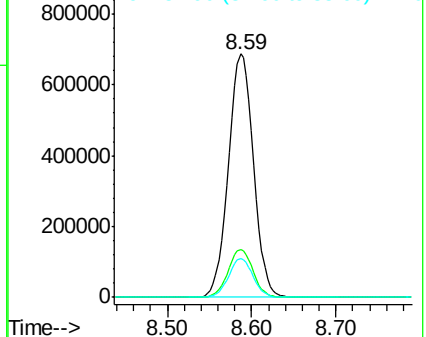

#35
Dibromofluoromethane
Concen: 50.000 ug/l
RT: 7.59 min Scan# 1810
Delta R.T. 0.00 min
Lab File: VN053449.D
Acq: 17 Jan 2019 21:47

Tgt Ion:113 Resp: 413042



Ion	Ratio	Lower	Upper
113	100		
111	101.9	81.1	121.7
192	22.8	18.2	27.2

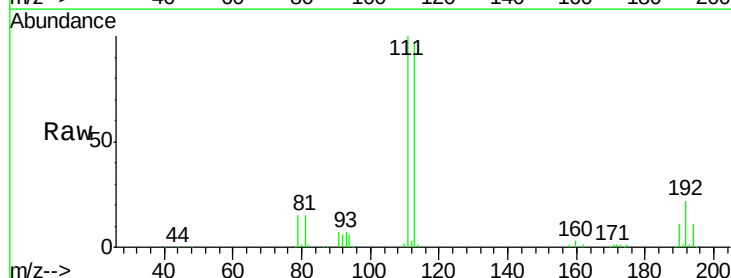


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

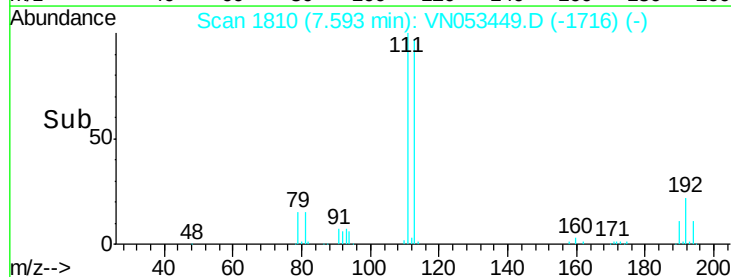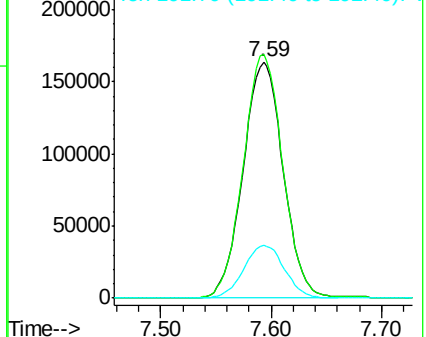

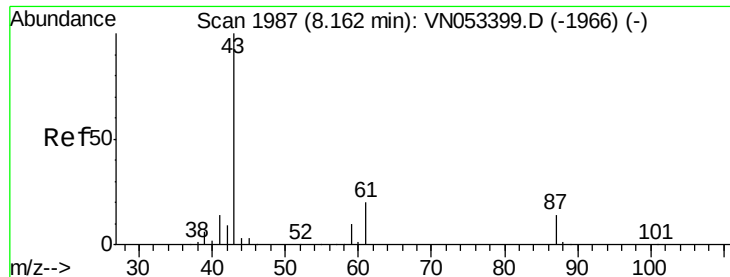

#43

Isopropyl Acetate

Concen: 3.494 ug/l

RT: 8.17 min Scan# 1989


Delta R.T. 0.01 min

Lab File: VN053449.D

Acq: 17 Jan 2019 21:47

Tot Ion: 43 Resp: 46739




Ion	Ratio	Lower	Upper
43	100		
61	16.7	23.9	35.9#
87	10.1	11.0	16.6#

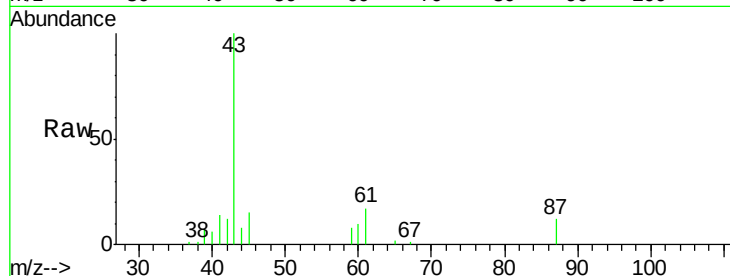

Abundance Ion 43.00 (42.70 to 43.70): VN053399.D (-1966) (-)

Ion 61.00 (60.70 to 61.70): VN053399.D (-1966) (-)

Ion 87.00 (86.70 to 87.70): VN053399.D (-1966) (-)

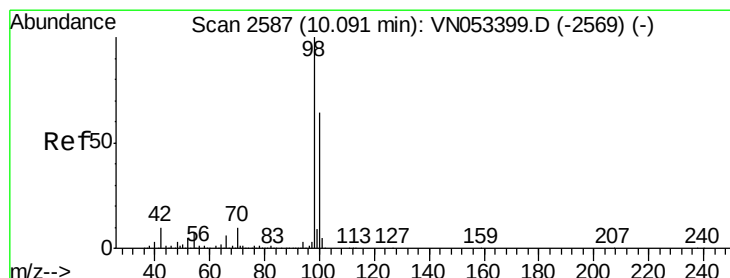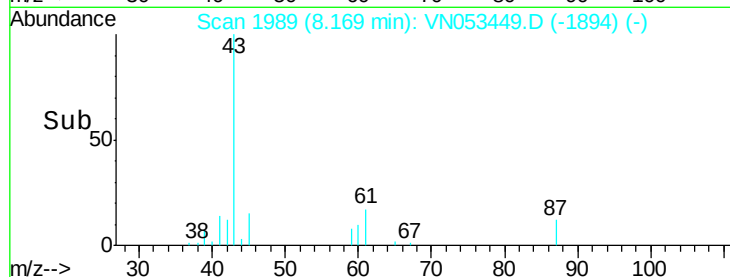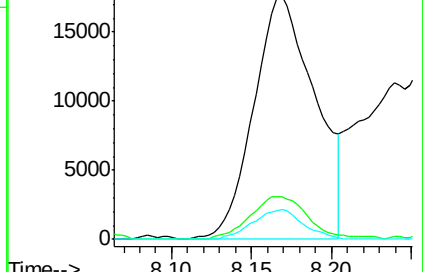

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.09 min Scan# 2587


Delta R.T. 0.00 min

Lab File: VN053449.D

Acq: 17 Jan 2019 21:47



Tgt Ion: 98 Resp: 1782036


Ion	Ratio	Lower	Upper
98	100		
100	64.1	51.4	77.0

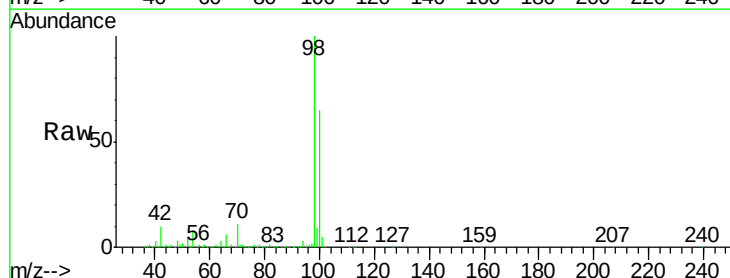

Abundance Ion 98.00 (97.70 to 98.70): VN053399.D (-2569) (-)

Ion 100.00 (99.70 to 100.70): VN053399.D (-2569) (-)

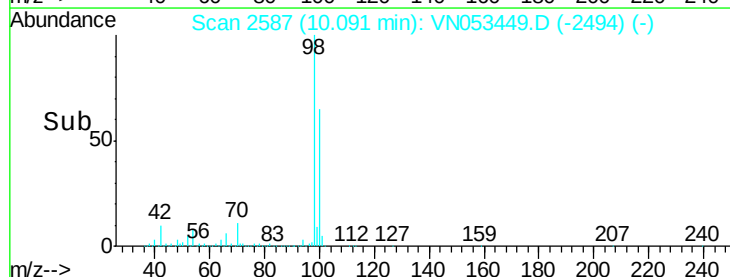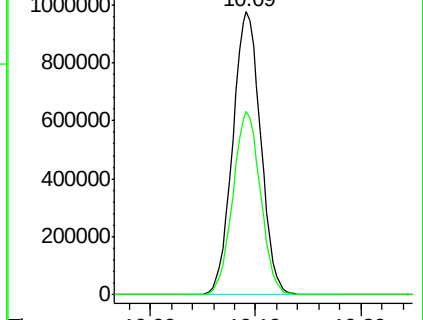

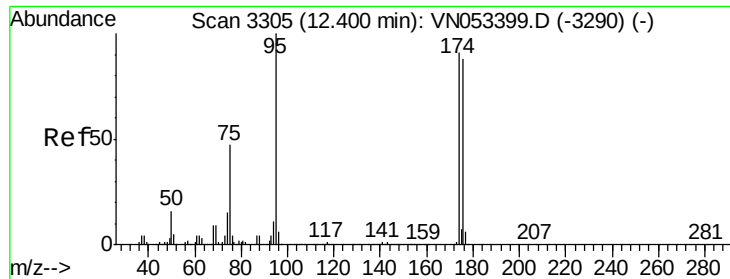

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.00 min

Lab File: VN053449.D

Acq: 17 Jan 2019 21:47


Tot Ion: 95 Resp: 614097

Ion Ratio Lower Upper

95 100

174 92.8 0.0 183.2




176 89.4 0.0 177.4

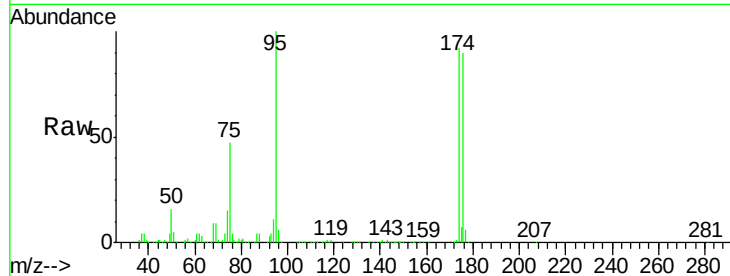

Abundance Ion 94.90 (94.60 to 95.60): VN053399.D (-3290) (-)

Ion 173.80 (173.50 to 174.50): VN053399.D (-3290) (-)

Ion 175.80 (175.50 to 176.50): VN053399.D (-3290) (-)

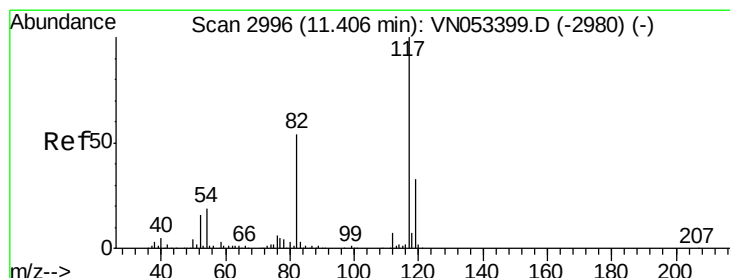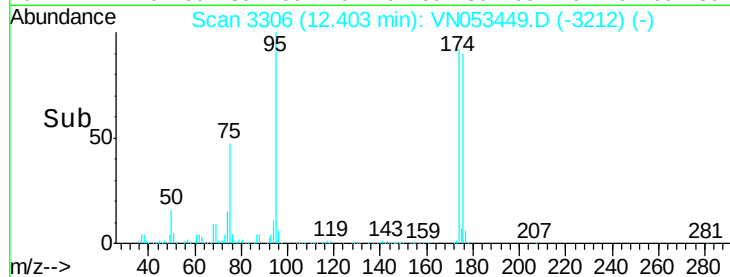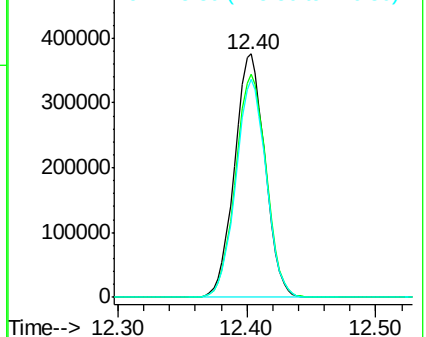

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2997

Delta R.T. 0.00 min

Lab File: VN053449.D

Acq: 17 Jan 2019 21:47


Tgt Ion: 117 Resp: 1358282

Ion Ratio Lower Upper

117 100

82 52.4 42.9 64.3



119 32.4 26.0 39.0

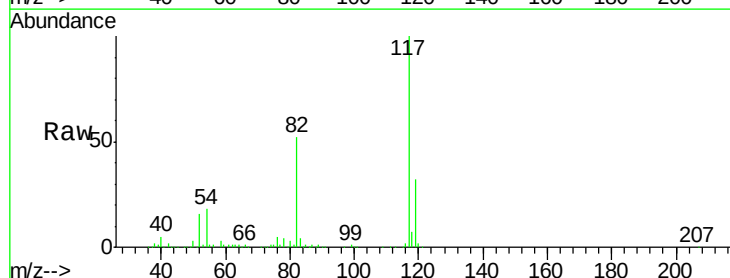


Abundance Ion 116.90 (116.60 to 117.60): VN053399.D (-2980) (-)

Ion 82.00 (81.70 to 82.70): VN053399.D (-2980) (-)

Ion 118.90 (118.60 to 119.60): VN053399.D (-2980) (-)

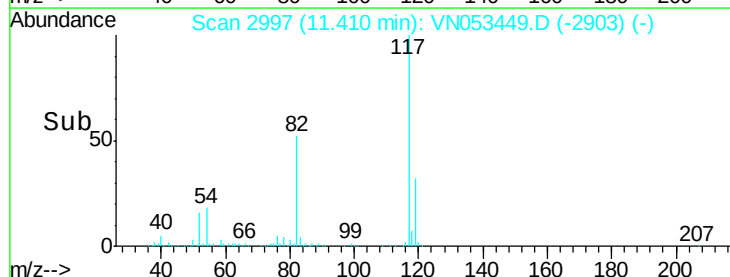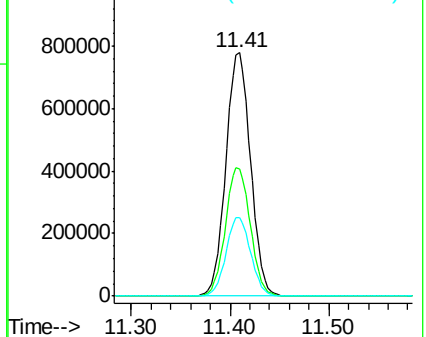


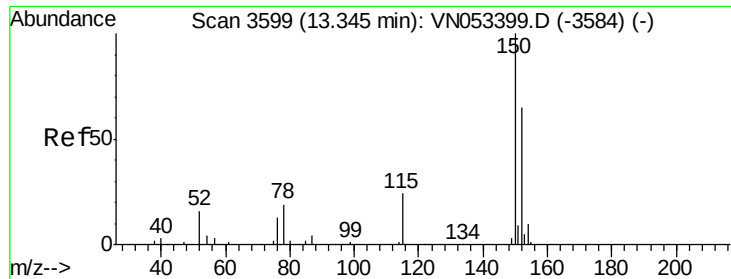

#72

1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.35 min Scan# 3599
 Delta R.T. 0.00 min
 Lab File: VN053449.D
 Acq: 17 Jan 2019 21:47

Tot Ion	Ratio	Lower	Upper
152	100		
115	56.9	27.8	83.4
150	158.2	0.0	349.0

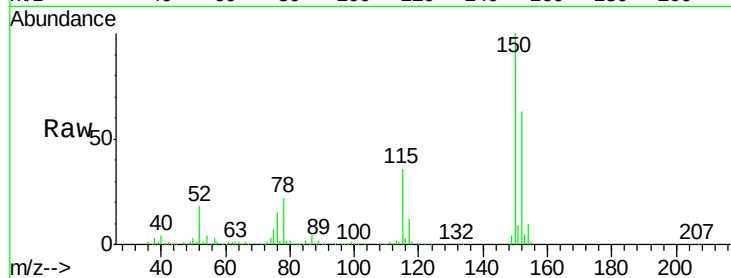

Abundance Ion 151.90 (151.60 to 152.60): V
 Ion 114.90 (114.60 to 115.60): V
 Ion 149.90 (149.60 to 150.60): V

