

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN011720\
 Data File : VN059754.D
 Acq On : 17 Jan 2020 12:38
 Operator : JC/MD
 Sample : PB126145TB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB126145TB

Quant Time: Jan 18 01:21:41 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011320W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 14 08:58:21 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.64	168	195763	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.57	114	286979	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.40	117	250999	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	103803	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.00	65	100006	46.00	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.00%	
35) Dibromofluoromethane	7.56	113	87270	50.99	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.98%	
50) Toluene-d8	10.08	98	333688	50.32	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.64%	
62) 4-Bromofluorobenzene	12.40	95	111585	46.68	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.36%	
Target Compounds						
43) Isopropyl Acetate	8.14	43	42773	10.609	ug/l #	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN011720\
Data File : VN059754.D
Acq On : 17 Jan 2020 12:38
Operator : JC/MD
Sample : PB126145TB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB126145TB

Quant Time: Jan 18 01:21:41 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N011320W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 14 08:58:21 2020
Response via : Initial Calibration

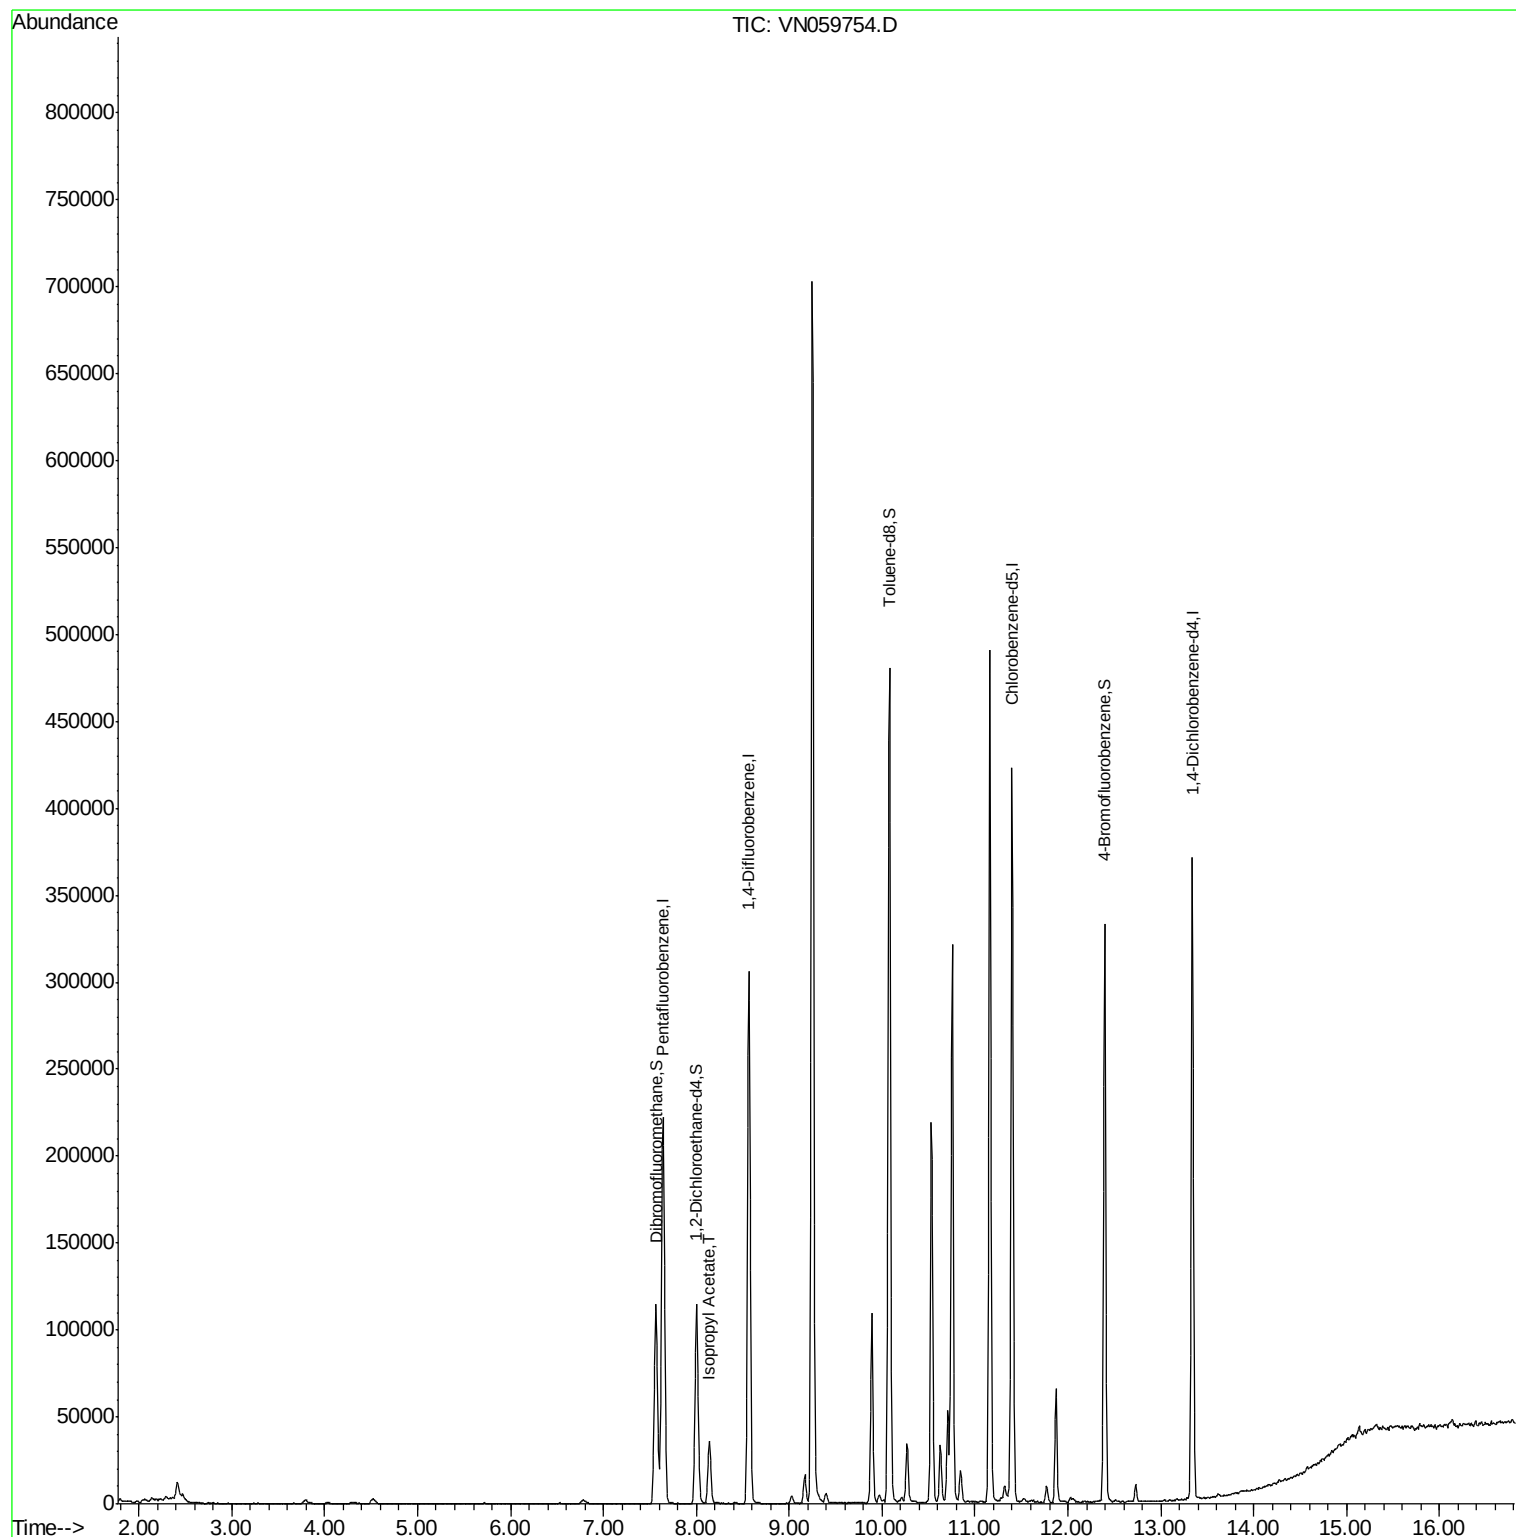

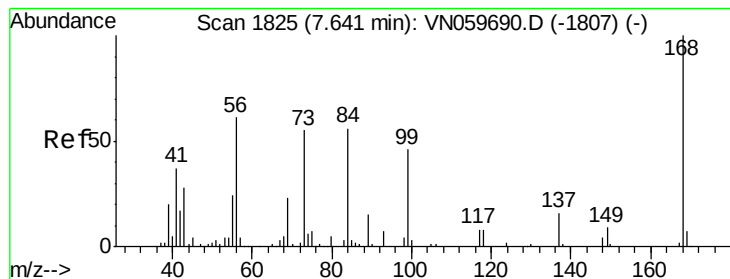

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.64 min Scan# 1825

Delta R.T. 0.00 min

Lab File: VN059754.D

Acq: 17 Jan 2020 12:38

Instrument :

MSVOA_N

ClientSampled :


PB126145TB

Tot Ion:168 Resp: 195763

Ion Ratio Lower Upper




168 100

99 51.1 48.2 72.4

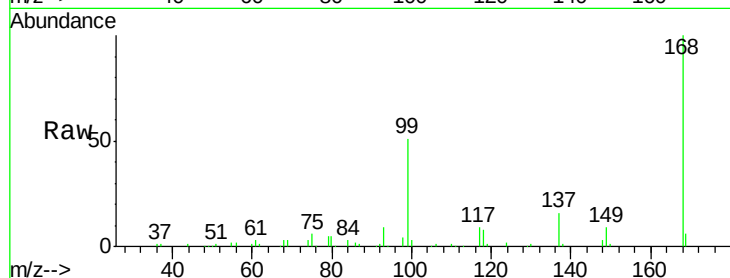

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

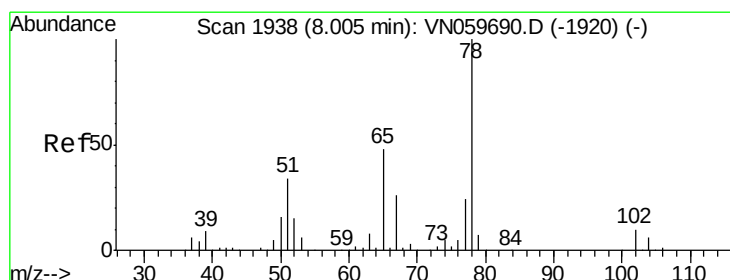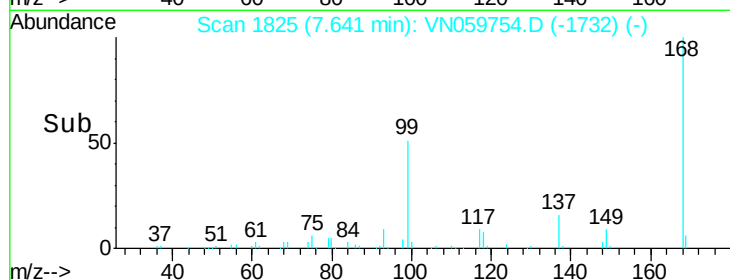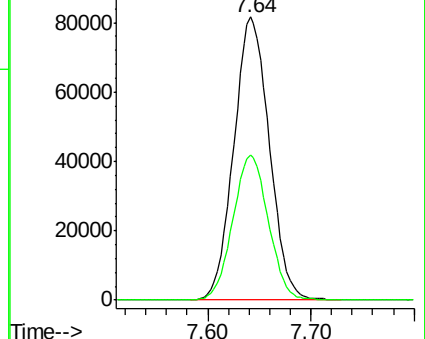

#33

1,2-Dichloroethane-d4

Concen: 46.001 ug/l

RT: 8.00 min Scan# 1937

Delta R.T. -0.00 min

Lab File: VN059754.D


Acq: 17 Jan 2020 12:38

Tgt Ion: 65 Resp: 100006

Ion Ratio Lower Upper



65 100


67 51.6 0.0 103.0

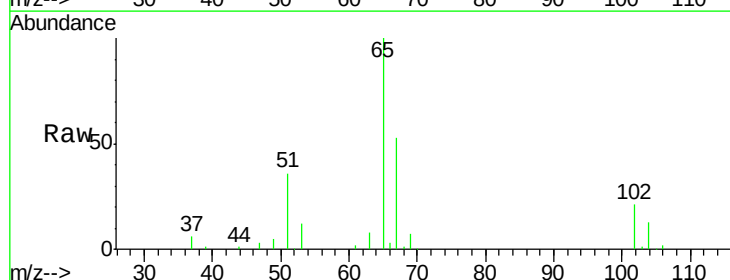

Abundance Ion 64.90 (64.60 to 65.60): VNO

Ion 66.90 (66.60 to 67.60): VNO

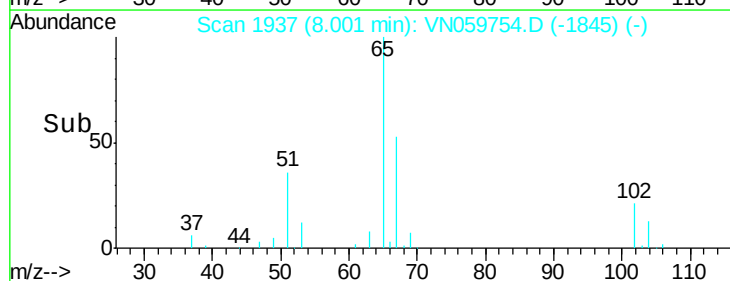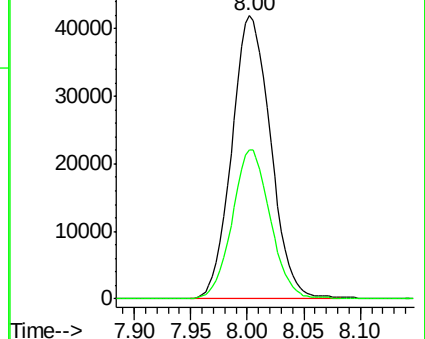


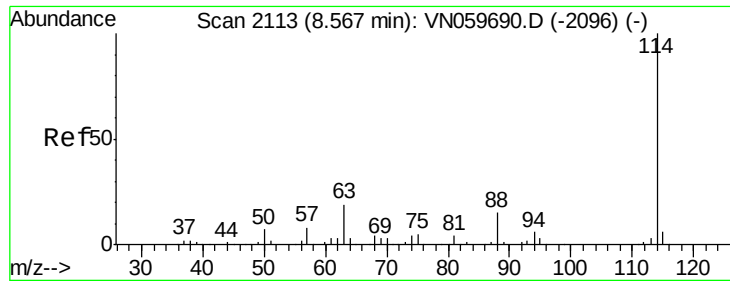




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.57 min Scan# 2113
 Delta R.T. 0.00 min
 Lab File: VN059754.D
 Acq: 17 Jan 2020 12:38

Instrument :
 MSVOA_N
 ClientSampleId :
 PB126145TB

Tot Ion:114 Resp: 286979
 Ion Ratio Lower Upper
 114 100
 63 18.3 0.0 43.6
 88 14.9 0.0 31.4

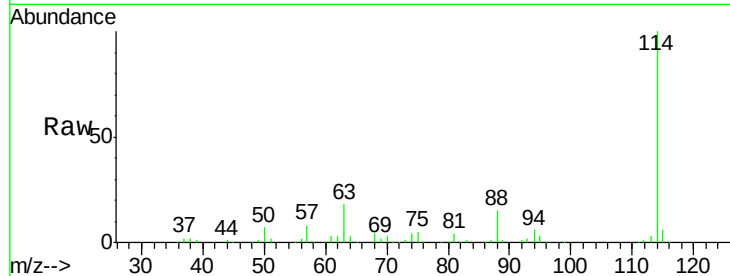


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): V
 Ion 87.90 (87.60 to 88.60): V

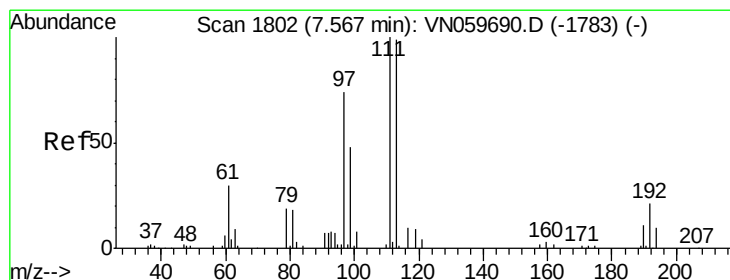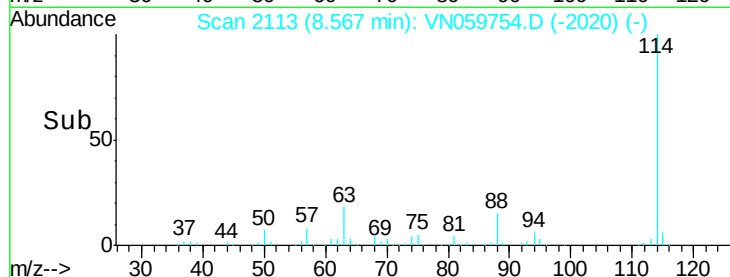
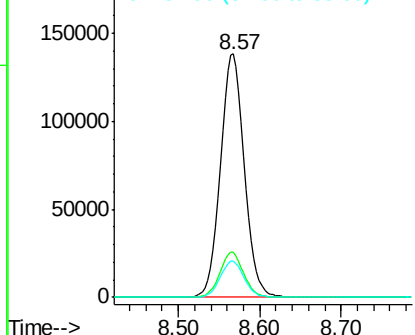



#35
 Dibromofluoromethane
 Concen: 50.994 ug/l
 RT: 7.56 min Scan# 1801
 Delta R.T. -0.00 min
 Lab File: VN059754.D
 Acq: 17 Jan 2020 12:38

Tgt Ion:113 Resp: 87270
 Ion Ratio Lower Upper
 113 100
 111 102.9 83.5 125.3
 192 21.9 15.4 23.2

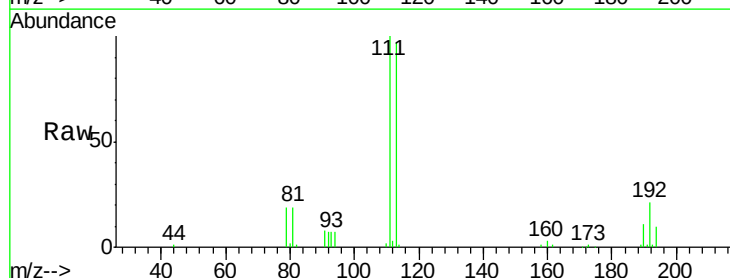

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

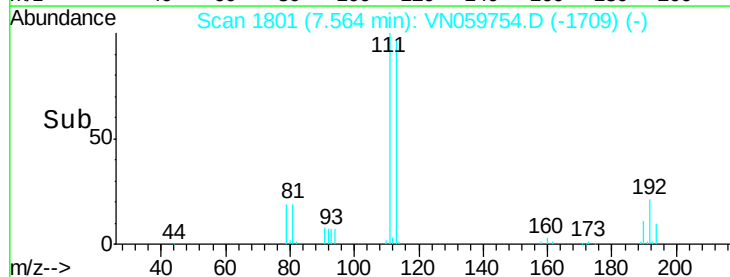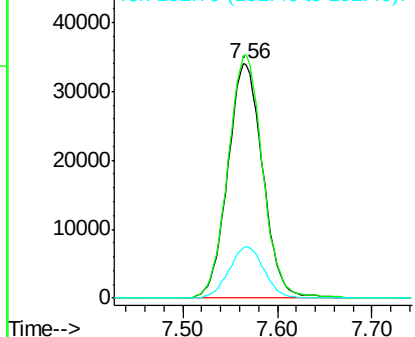

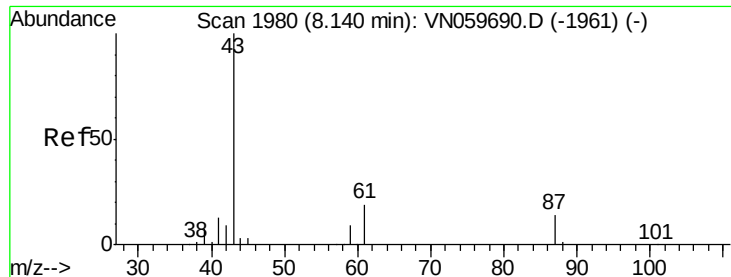

#43

Isopropyl Acetate

Concen: 10.609 ug/l

RT: 8.14 min Scan# 1980

Delta R.T. 0.00 min

Lab File: VN059754.D

Acq: 17 Jan 2020 12:38

Instrument :

MSVOA_N

ClientSampleId :

PB126145TB





Tot Ion: 43 Resp: 42773

Ion Ratio Lower Upper

43 100

61 19.7 20.2 30.2#

87 15.3 9.5 14.3#

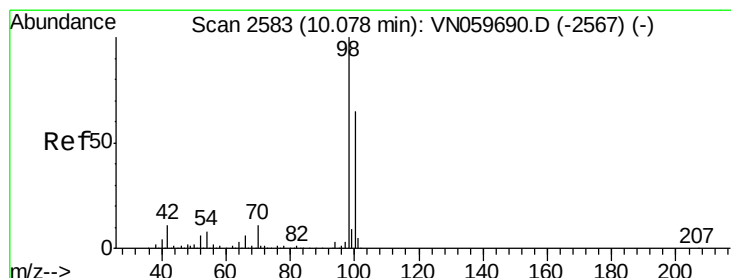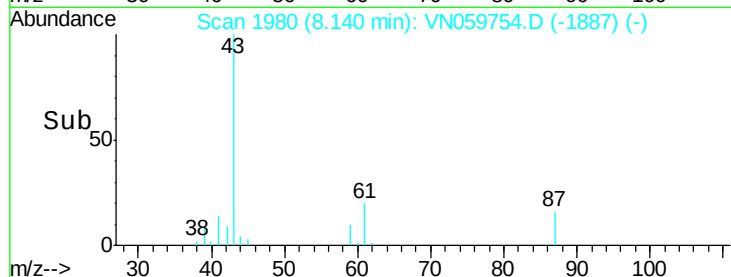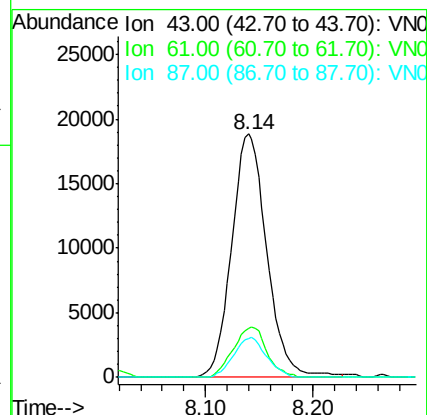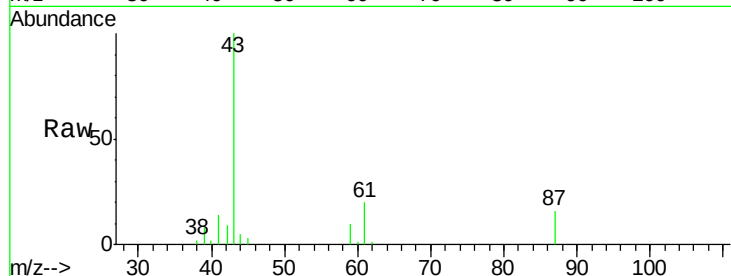

#50

Toluene-d8

Concen: 50.324 ug/l

RT: 10.08 min Scan# 2583

Delta R.T. 0.00 min

Lab File: VN059754.D




Acq: 17 Jan 2020 12:38


Tgt Ion: 98 Resp: 333688

Ion Ratio Lower Upper

98 100

100 64.5 51.2 76.8


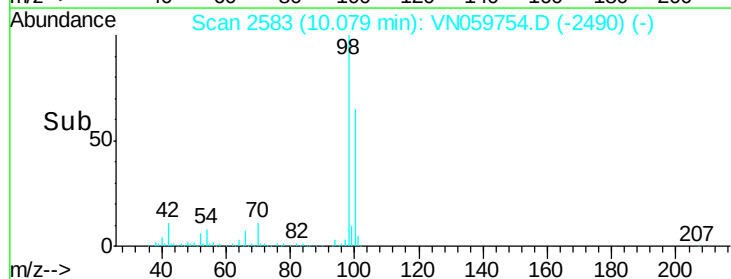
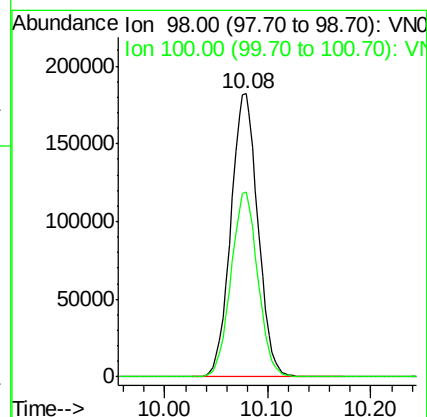
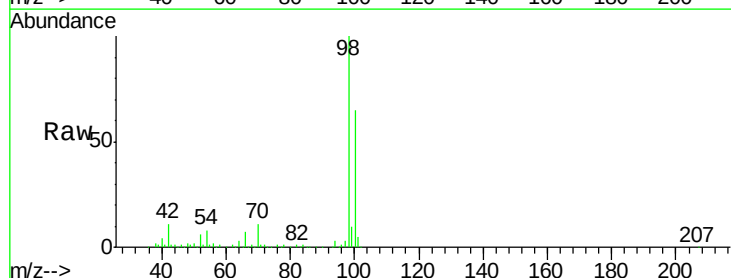


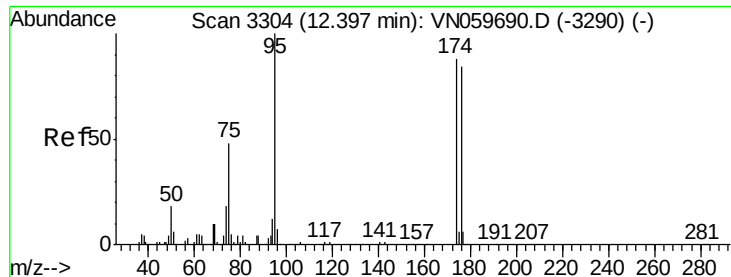

#62
4-Bromofluorobenzene
Concen: 46.681 ug/l
RT: 12.40 min Scan# 3304
Delta R.T. 0.00 min
Lab File: VN059754.D
Acq: 17 Jan 2020 12:38




Instrument :
MSVOA_N
ClientSampleId :
PB126145TB


Tot Ion: 95 Resp: 111585
Ion Ratio Lower Upper
95 100
174 88.9 0.0 151.4
176 87.2 0.0 146.0

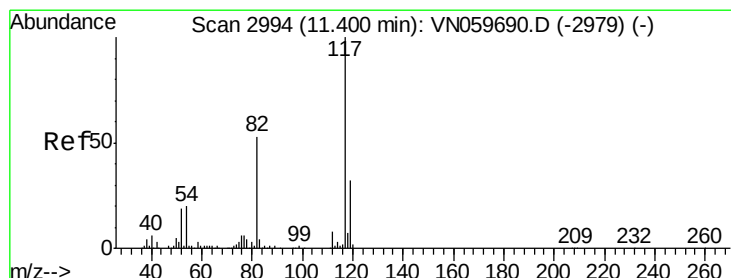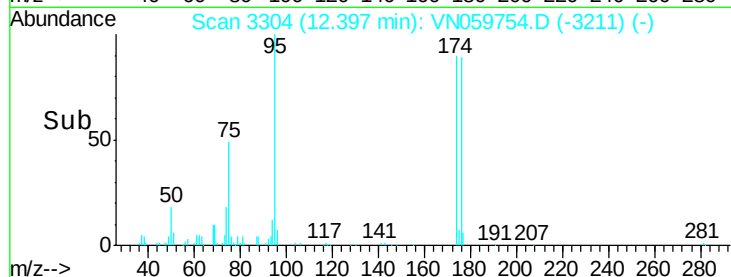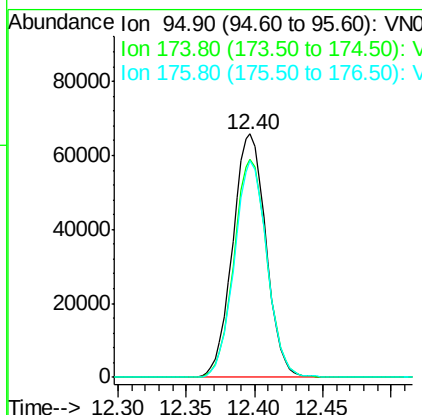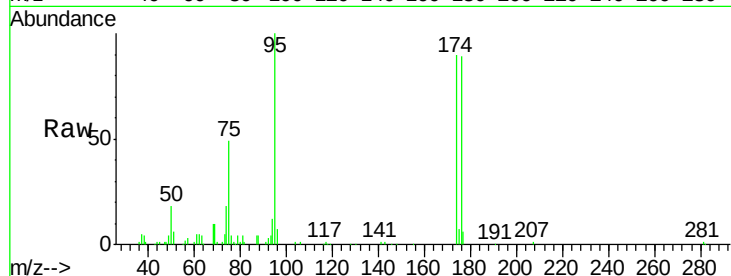

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.40 min Scan# 2994
Delta R.T. 0.00 min
Lab File: VN059754.D
Acq: 17 Jan 2020 12:38

Tgt Ion: 117 Resp: 250999
Ion Ratio Lower Upper
117 100
82 51.7 45.9 68.9
119 32.0 25.5 38.3

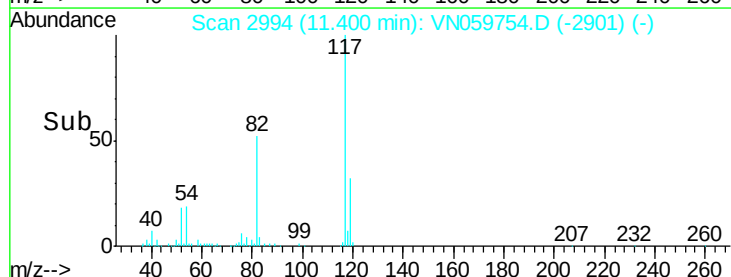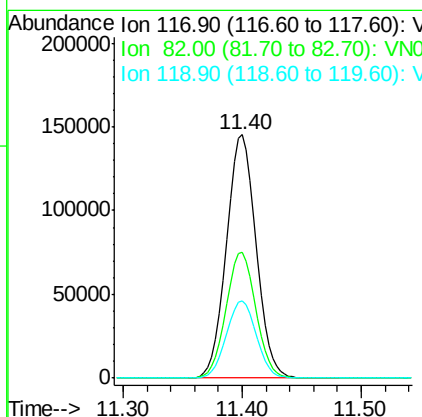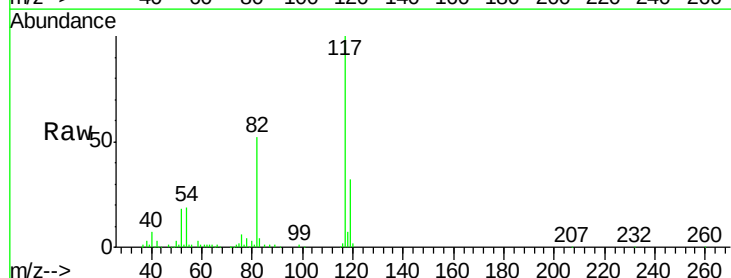

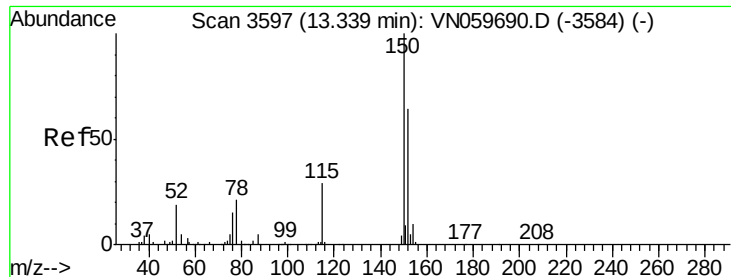

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.34 min Scan# 3597

Delta R.T. 0.00 min

Lab File: VN059754.D

Acq: 17 Jan 2020 12:38

Instrument :

MSVOA_N

ClientSampleId :

PB126145TB


Tot Ion:152 Resp: 103803

Ion Ratio Lower Upper

152 100

115 57.7 30.3 90.9

150 157.8 0.0 345.2

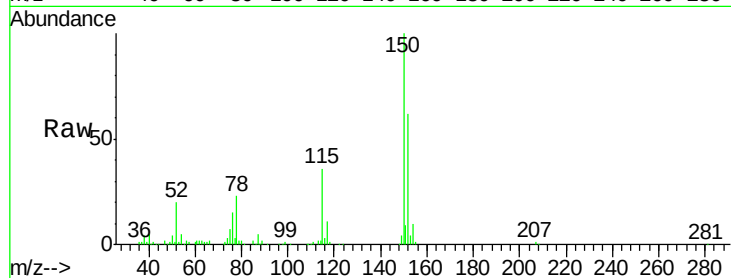

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

