


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN011720\
Data File : VN059748.D
Acq On : 17 Jan 2020 8:39
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011320W.M
Title : SW846 8260
Last Update : Sat Jan 18 03:09:32 2020

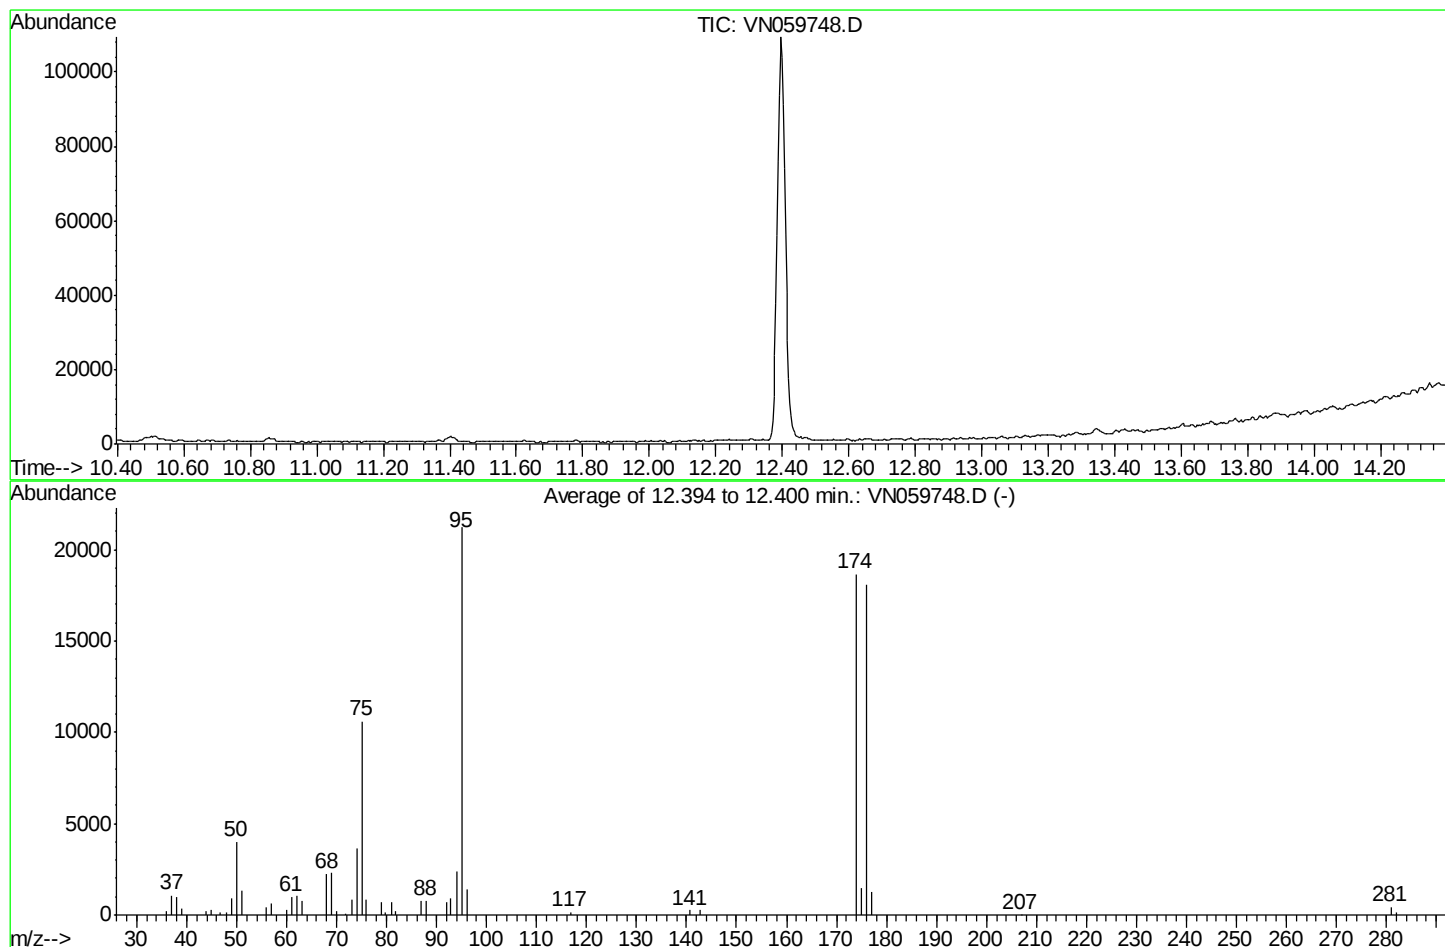

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	4005	PASS
75	95	30	60	49.9	10591	PASS
95	95	100	100	100.0	21224	PASS
96	95	5	9	6.8	1438	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.8	18645	PASS
175	174	5	9	8.0	1500	PASS
176	174	95	101	97.1	18112	PASS
177	176	5	9	7.0	1262	PASS