

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011722\
 Data File : VN070646.D
 Acq On : 17 Jan 2022 15:38
 Operator : JC/MD
 Sample : N1143-01ME
 Misc : 5.06g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 WEST-BOILER-ROOM-SOUTH-SIDEWALLME

Quant Time: Jan 17 17:05:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 27 18:47:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.080	168	1189602	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.965	114	1980642	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	1611345	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	726964	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	895074	52.331	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 104.660%	
35) Dibromofluoromethane	8.016	113	614779	51.301	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 102.600%	
50) Toluene-d8	10.441	98	2491087	50.885	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 101.760%	
62) 4-Bromofluorobenzene	12.731	95	1020009	57.687	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 115.380%	

Target Compounds				Qvalue		
11) Tert butyl alcohol	5.305	59	11610	4.077	ug/l #	72
16) Acetone	4.310	43	36281	3.268	ug/l	94
18) Methyl Acetate	4.859	43	6960	0.217	ug/l	93
25) 2-Butanone	7.348	43	150965	10.798	ug/l	90
29) Tetrahydrofuran	7.705	42	8997	1.079	ug/l #	58
31) Cyclohexane	8.078	56	26796	0.993	ug/l #	1
36) 1,1-Dichloropropene	8.080	75	92794	4.681	ug/l #	43
37) Ethyl Acetate	7.348	43	150965	5.875	ug/l #	68
38) Carbon Tetrachloride	8.080	117	113479	5.995	ug/l #	16
41) Methacrylonitrile	7.708	41	5232	0.407	ug/l #	31
55) 1,1,2-Trichloroethane	10.875	97	11765	0.808	ug/l #	28
58) 2-Chloroethyl Vinyl ether	10.060	63	151	18.536	ug/l #	45
59) 2-Hexanone	11.049	43	92045	4.958	ug/l #	29
67) Ethyl Benzene	11.843	91	16046	0.256	ug/l	94
68) m/p-Xylenes	11.950	106	33638	1.475	ug/l	81
69) o-Xylene	12.280	106	21212	0.935	ug/l	55
73) Isopropylbenzene	12.578	105	85087	1.260	ug/l	97
74) N-amyl acetate	12.366	43	1819252	64.091	ug/l #	66
75) 1,1,2,2-Tetrachloroethane	12.862	83	17521	1.156	ug/l #	1
76) 1,2,3-Trichloropropane	12.731	75	486944	24.122	ug/l #	1
77) Bromobenzene	12.827	156	3129	0.202	ug/l #	1
78) n-propylbenzene	12.919	91	374115	5.002	ug/l	95
79) 2-Chlorotoluene	12.983	91	136041	2.835	ug/l #	38
80) 1,3,5-Trimethylbenzene	13.058	105	1219681	22.545	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.731	75	486944	81.838	ug/l #	7
82) 4-Chlorotoluene	13.058	91	141519	3.148	ug/l #	56
83) tert-Butylbenzene	13.324	119	87310	1.833	ug/l	96
84) 1,2,4-Trimethylbenzene	13.367	105	2906353	55.791	ug/l	98
85) sec-Butylbenzene	13.501	105	395087	6.109	ug/l #	65
86) p-Isopropyltoluene	13.613	119	402055	7.914	ug/l	97
89) n-Butylbenzene	13.940	91	270909	6.393	ug/l #	73
90) Hexachloroethane	14.217	117	35679	4.043	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.260	180	5369	0.448	ug/l #	37
95) Naphthalene	15.507	128	89641	4.406	ug/l	99
96) 1,2,3-Trichlorobenzene	15.705	180	5614	1.308	ug/l #	87

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011722\
Data File : VN070646.D
Acq On : 17 Jan 2022 15:38
Operator : JC/MD
Sample : N1143-01ME
Misc : 5.06g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WEST-BOILER-ROOM-SOUTH-SIDEWALLME

Quant Time: Jan 17 17:05:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260
QLast Update : Mon Dec 27 18:47:12 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011722\
Data File : VN070646.D
Acq On : 17 Jan 2022 15:38
Operator : JC/MD
Sample : N1143-01ME
Misc : 5.06g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WEST-BOILER-ROOM-SOUTH-SIDEWALLME

Quant Time: Jan 17 17:05:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260
QLast Update : Mon Dec 27 18:47:12 2021
Response via : Initial Calibration




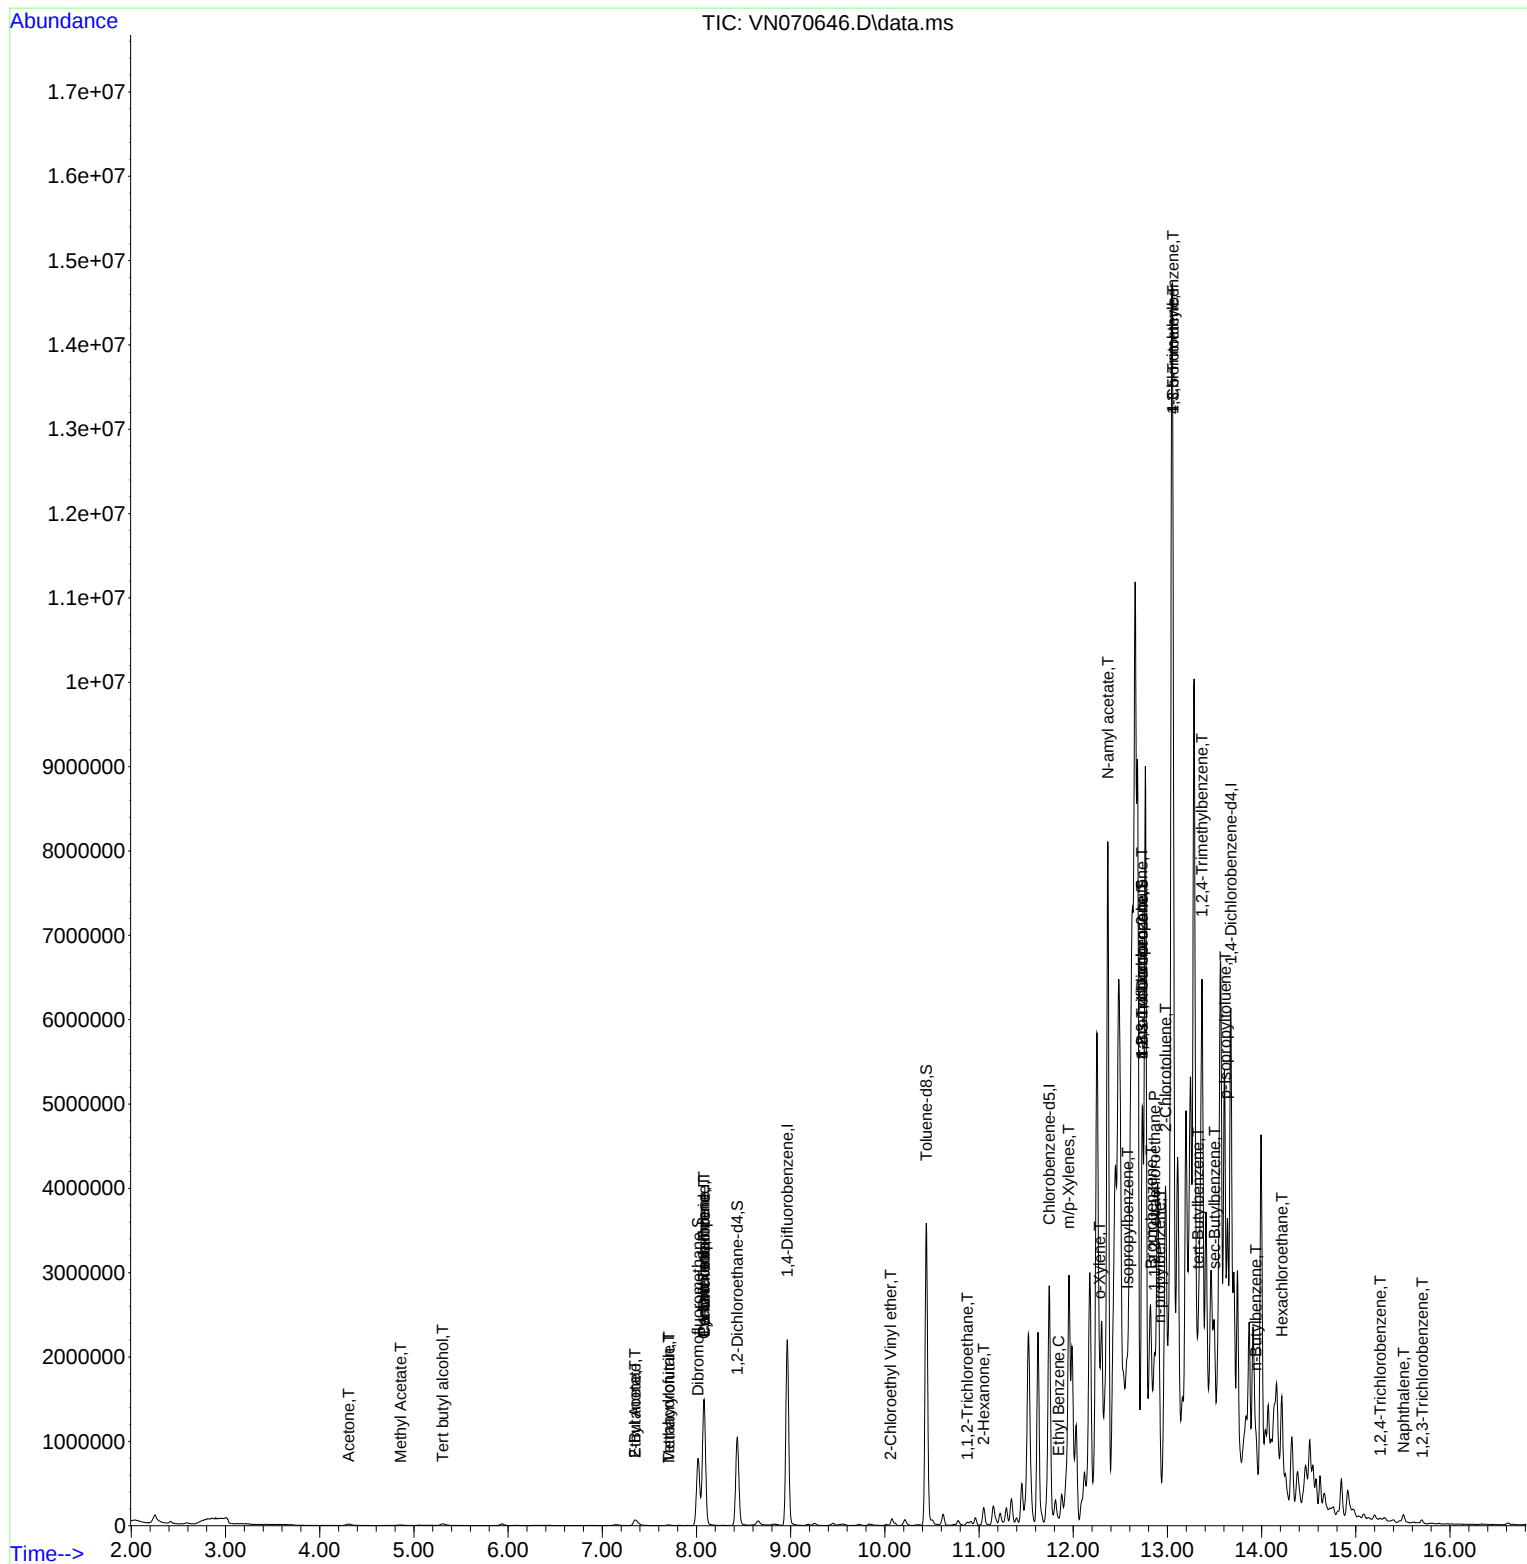


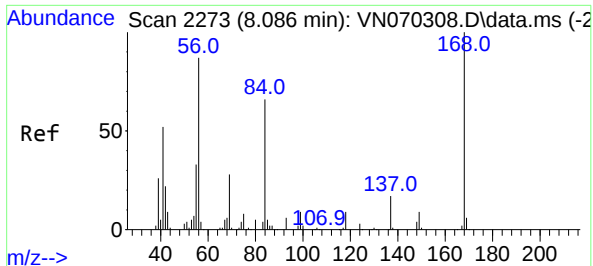

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.080 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38




Instrument :
MSVOA_N
ClientSampleId :
WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion:168 Resp: 1189602
Ion Ratio Lower Upper
168 100
99 57.8 41.3 61.9

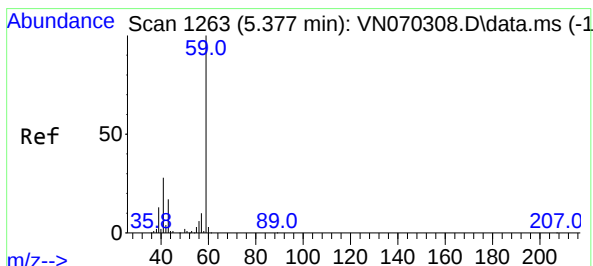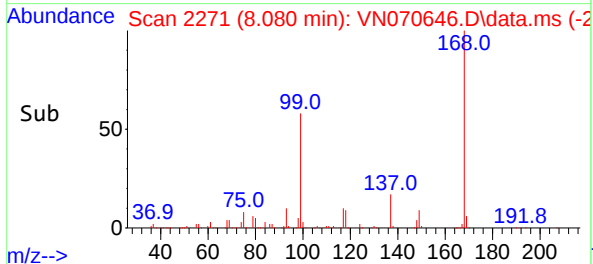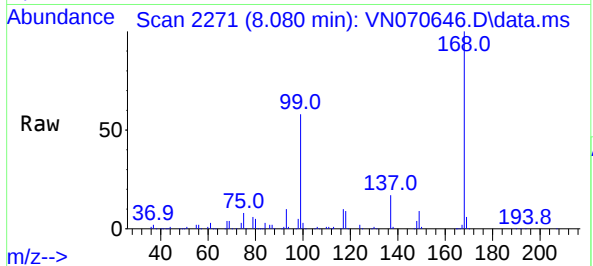

#11
Tert butyl alcohol
Concen: 4.077 ug/l
RT: 5.305 min Scan# 1236
Delta R.T. -0.072 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38

Tgt Ion: 59 Resp: 11610
Ion Ratio Lower Upper
59 100
57 0.4 8.7 13.1#


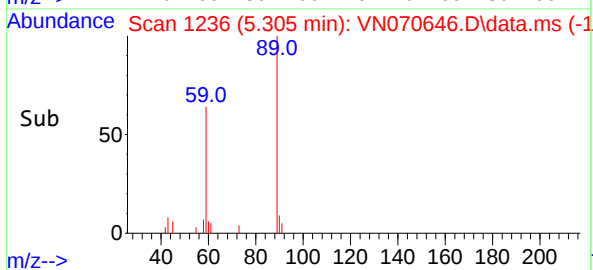

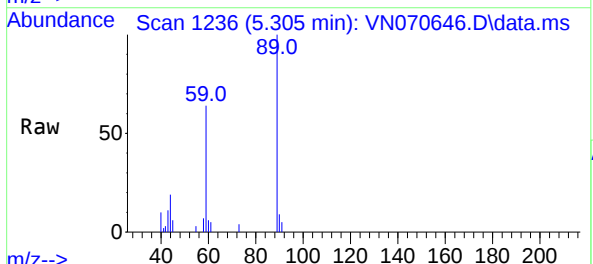




#16
Acetone
Concen: 3.268 ug/l
RT: 4.310 min Scan# 80
Delta R.T. 0.025 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38




Instrument :
MSVOA_N
ClientSampleId :
WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion: 43 Resp: 36281
Ion Ratio Lower Upper
43 100
58 32.2 23.1 34.7

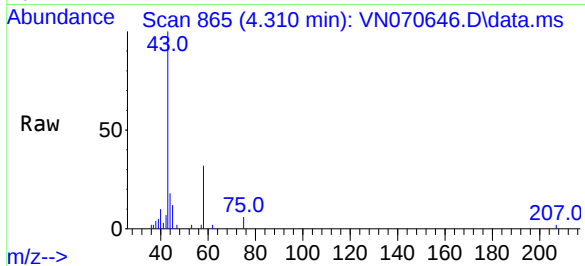

#18
Methyl Acetate
Concen: 0.217 ug/l
RT: 4.859 min Scan# 1070
Delta R.T. 0.005 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38

Tgt Ion: 43 Resp: 6960
Ion Ratio Lower Upper
43 100
74 21.0 19.4 29.2

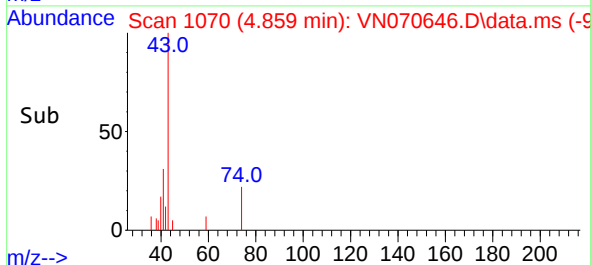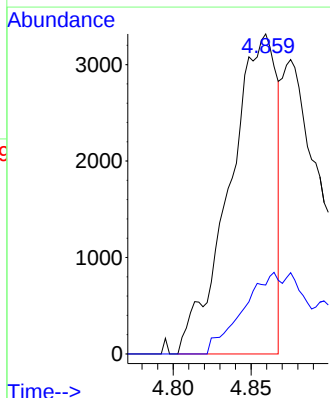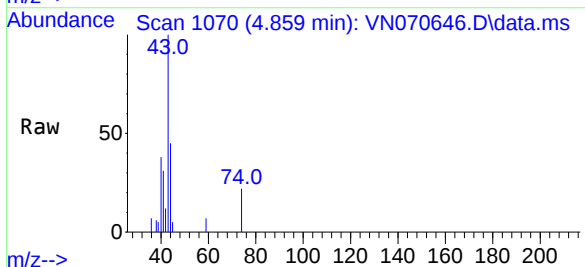

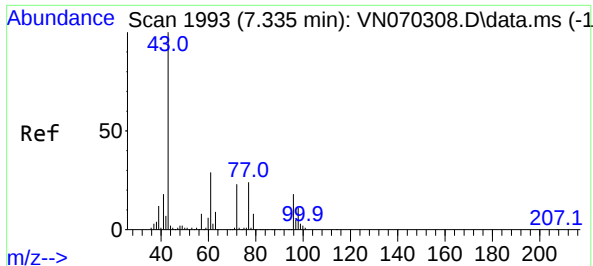

#25

2-Butanone

Concen: 10.798 ug/l

RT: 7.348 min Scan# 1998

Delta R.T. 0.013 min

Lab File: VN070646.D

Acq: 17 Jan 2022 15:38

Instrument :

MSVOA_N

ClientSampleId :





WEST-BOILER-ROOM-SOUTH-SIDEWALLME

Tgt Ion: 43 Resp: 150965

Ion Ratio Lower Upper

43 100

72 21.8 21.7 32.5

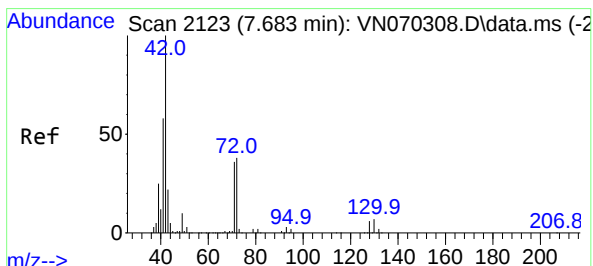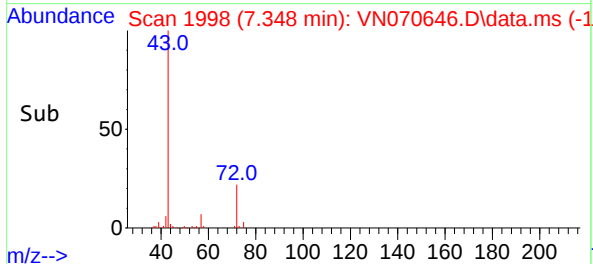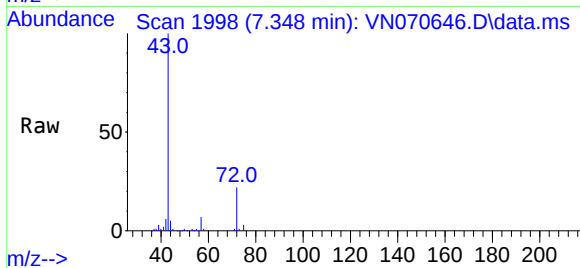

#29

Tetrahydrofuran

Concen: 1.079 ug/l

RT: 7.705 min Scan# 2131

Delta R.T. 0.022 min

Lab File: VN070646.D

Acq: 17 Jan 2022 15:38




Tgt Ion: 42 Resp: 8997


Ion Ratio Lower Upper

42 100

72 19.8 36.3 54.5#

71 14.8 34.7 52.1#


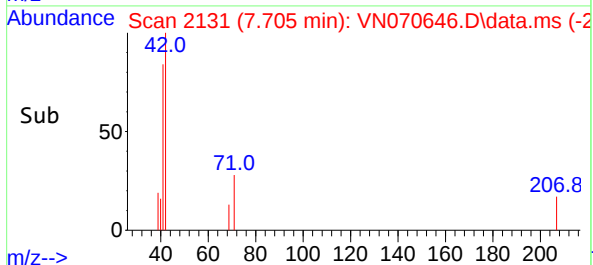
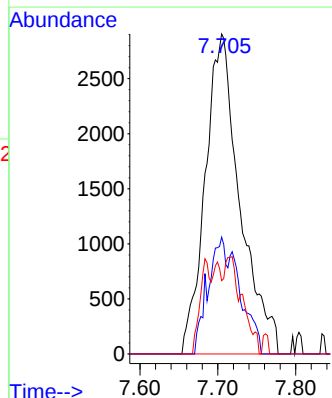
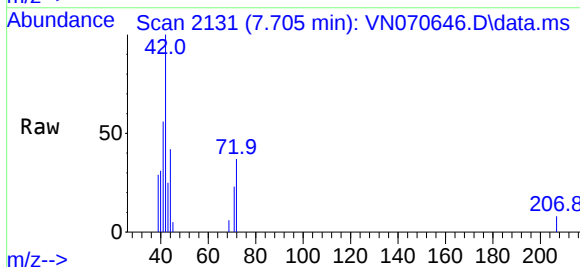




#31
Cyclohexane
Concen: 0.993 ug/l
RT: 8.078 min Scan# 21
Delta R.T. -0.016 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38




Instrument :
MSVOA_N
ClientSampleId :
WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion: 56 Resp: 26796
Ion Ratio Lower Upper
56 100
69 174.2 27.1 40.7#
84 150.5 73.4 110.0#

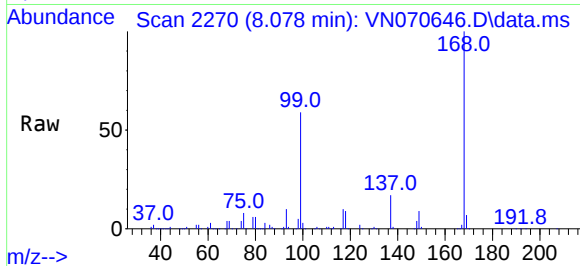

#33
1,2-Dichloroethane-d4
Concen: 52.331 ug/l
RT: 8.434 min Scan# 2403
Delta R.T. -0.003 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38

Tgt Ion: 65 Resp: 895074
Ion Ratio Lower Upper
65 100
67 53.8 0.0 103.0


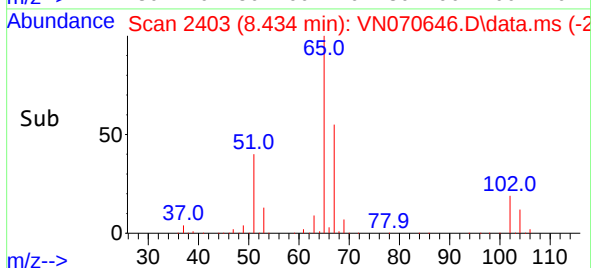

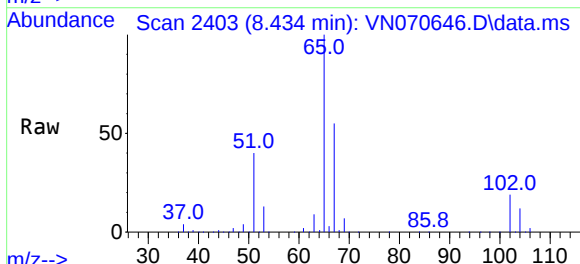




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.965 min Scan# 2061
Delta R.T. -0.003 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38




Instrument : MSVOA_N
ClientSampleId : WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion:114 Resp: 1980642
Ion Ratio Lower Upper
114 100
63 23.5 0.0 37.8
88 17.0 0.0 27.4



#35
Dibromofluoromethane
Concen: 51.301 ug/l
RT: 8.016 min Scan# 2247
Delta R.T. -0.005 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38

Tgt Ion:113 Resp: 614779
Ion Ratio Lower Upper
113 100
111 103.4 82.2 123.2
192 19.4 16.9 25.3


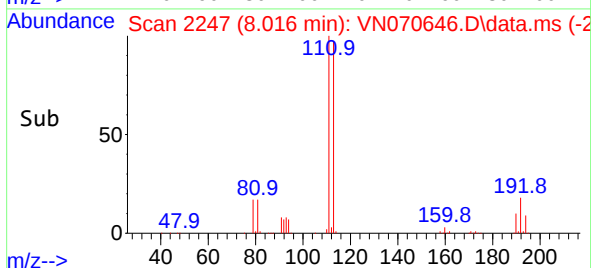
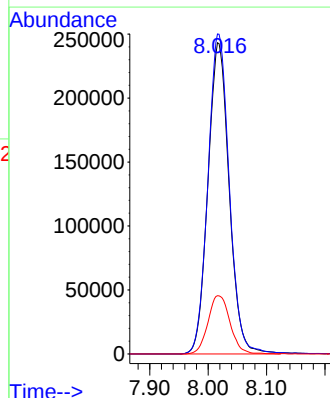





#36
1,1-Dichloropropene
Concen: 4.681 ug/l
RT: 8.080 min Scan# 21
Delta R.T. -0.140 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38




Instrument : MSVOA_N
ClientSampleId : WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion: 75 Resp: 92794
Ion Ratio Lower Upper
75 100
110 2.0 18.4 55.2#
77 0.0 24.4 36.6#



#37
Ethyl Acetate
Concen: 5.875 ug/l
RT: 7.348 min Scan# 1998
Delta R.T. -0.064 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38

Tgt Ion: 43 Resp: 150965
Ion Ratio Lower Upper
43 100
61 0.0 11.5 17.3#
70 0.0 7.9 11.9#


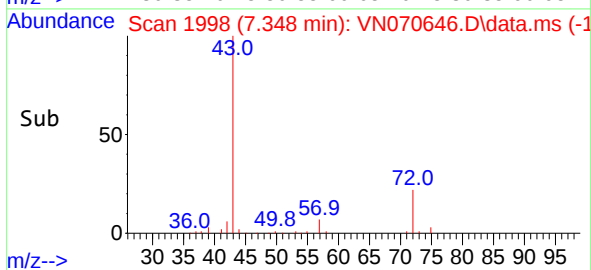






#38
Carbon Tetrachloride
Concen: 5.995 ug/l
RT: 8.080 min Scan# 2132
Delta R.T. -0.126 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38




Instrument : MSVOA_N
ClientSampleId : WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion:117 Resp: 113479
Ion Ratio Lower Upper
117 100
119 5.1 76.1 114.1#
121 0.0 24.2 36.2#

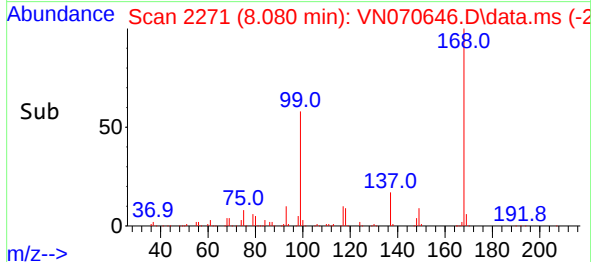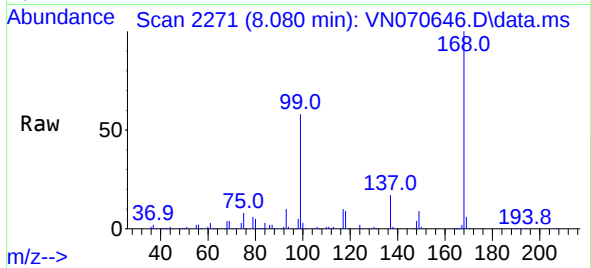

#41
Methacrylonitrile
Concen: 0.407 ug/l
RT: 7.708 min Scan# 2132
Delta R.T. 0.070 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38

Tgt Ion: 41 Resp: 5232
Ion Ratio Lower Upper
41 100
39 30.3 48.1 72.1#
67 0.0 68.3 102.5#
52 0.0 29.6 44.4#


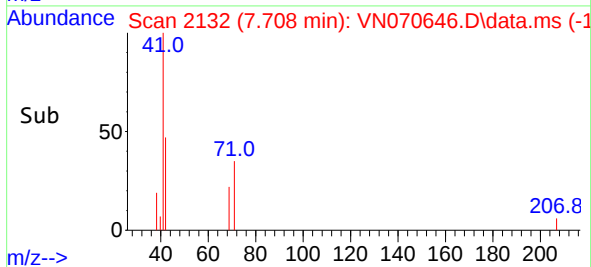

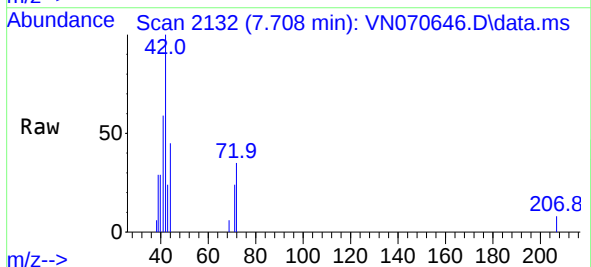


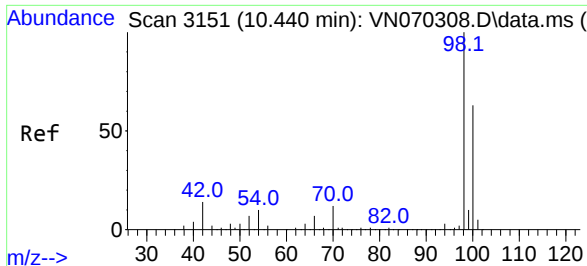

#50
Toluene-d8
Concen: 50.885 ug/l
RT: 10.441 min Scan# 3151
Delta R.T. 0.001 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38




Instrument : MSVOA_N
ClientSampleId : WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion: 98 Resp: 2491087
Ion Ratio Lower Upper
98 100
100 64.2 50.4 75.6

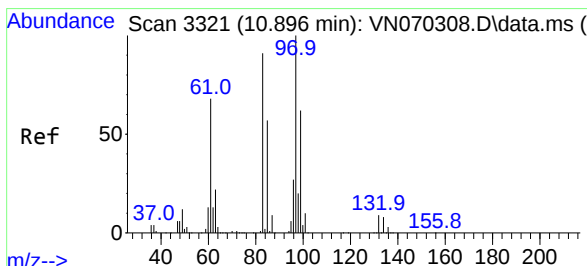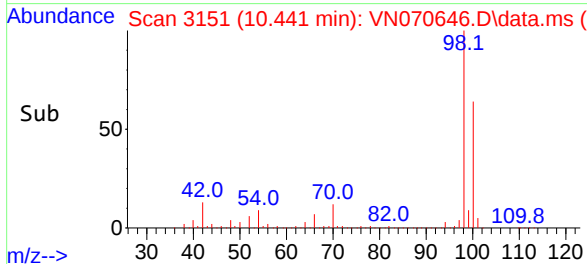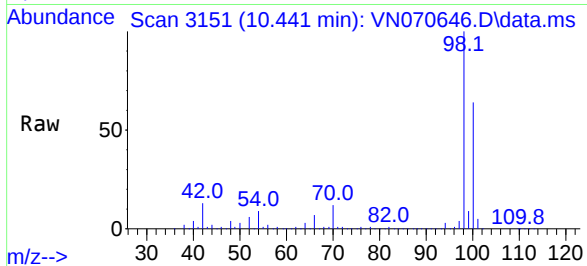

#55
1,1,2-Trichloroethane
Concen: 0.808 ug/l
RT: 10.875 min Scan# 3313
Delta R.T. -0.021 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38

Tgt Ion: 97 Resp: 11765
Ion Ratio Lower Upper
97 100
83 13.0 67.8 101.6#
85 17.1 45.4 68.2#
99 0.0 49.4 74.0#


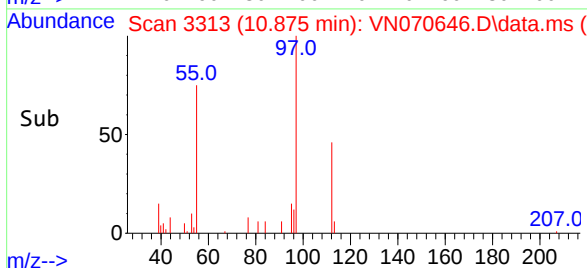
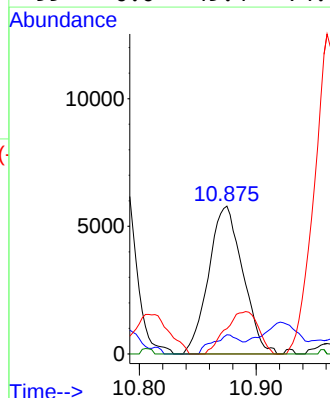
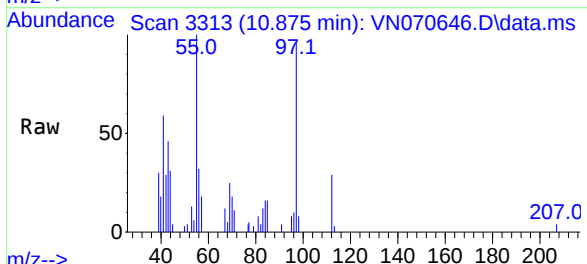




#58
2-Chloroethyl Vinyl ether
Concen: 18.536 ug/l
RT: 10.060 min Scan# 3009
Delta R.T. 0.019 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38




Instrument : MSVOA_N
ClientSampleId : WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion: 63 Resp: 151
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#

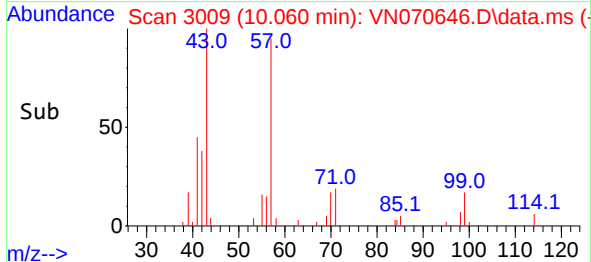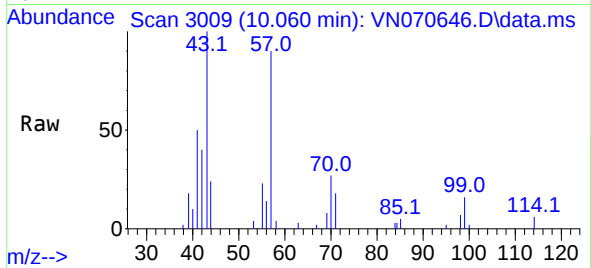

#59
2-Hexanone
Concen: 4.958 ug/l
RT: 11.049 min Scan# 3378
Delta R.T. -0.035 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38

Tgt Ion: 43 Resp: 92045
Ion Ratio Lower Upper
43 100
58 3.1 26.9 80.7#


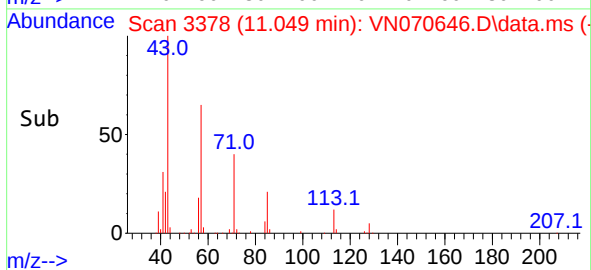






#62
4-Bromofluorobenzene
Concen: 57.687 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.000 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38




Instrument : MSVOA_N
ClientSampleId : WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion: 95 Resp: 1020009
Ion Ratio Lower Upper
95 100
174 68.9 0.0 187.2
176 66.9 0.0 181.4

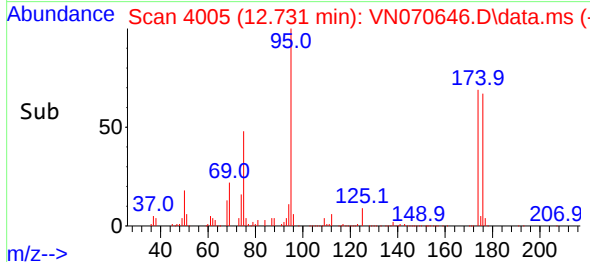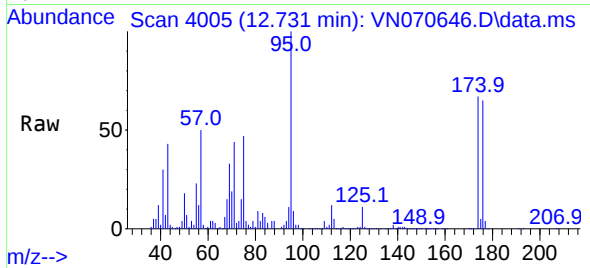

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. 0.003 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38

Tgt Ion: 117 Resp: 1611345
Ion Ratio Lower Upper
117 100
82 59.7 42.4 63.6
119 32.0 25.4 38.2


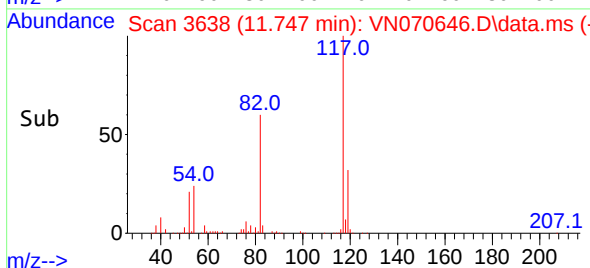
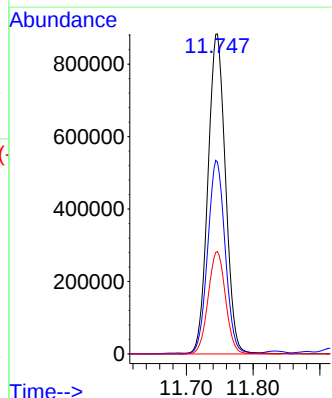





#67
Ethyl Benzene
Concen: 0.256 ug/l
RT: 11.843 min Scan# 3674
Delta R.T. 0.000 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38




Instrument : MSVOA_N
ClientSampleId : WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion: 91 Resp: 16046
Ion Ratio Lower Upper
91 100
106 28.8 25.7 38.5



#68
m/p-Xylenes
Concen: 1.475 ug/l
RT: 11.950 min Scan# 3714
Delta R.T. -0.003 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38

Tgt Ion:106 Resp: 33638
Ion Ratio Lower Upper
106 100
91 228.9 160.6 240.8


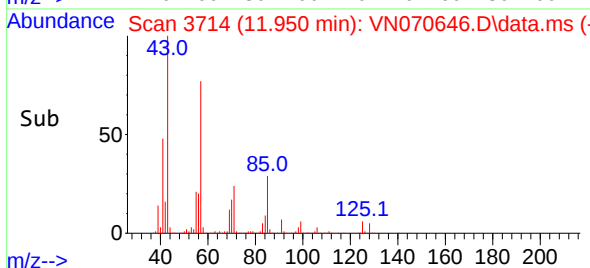
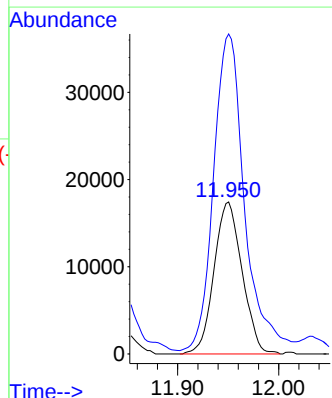





#69
o-Xylene
Concen: 0.935 ug/l
RT: 12.280 min Scan# 3836
Delta R.T. 0.002 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38




Instrument :
MSVOA_N
ClientSampleId :
WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion:106 Resp: 21212
Ion Ratio Lower Upper
106 100
91 282.7 105.8 317.3



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. 0.003 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38

Tgt Ion:152 Resp: 726964
Ion Ratio Lower Upper
152 100
115 65.9 27.5 82.5
150 154.8 0.0 344.4


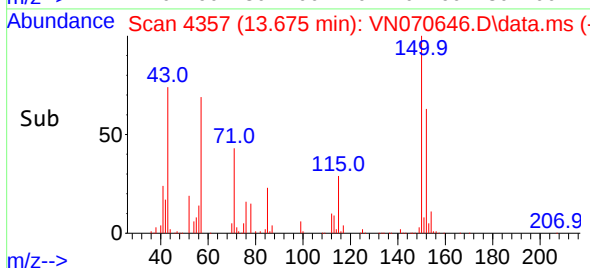
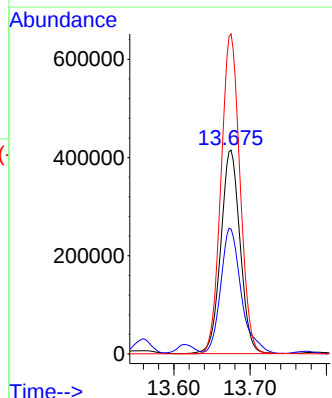





#73
Isopropylbenzene
Concen: 1.260 ug/l
RT: 12.578 min Scan# 3948
Delta R.T. 0.000 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38




Instrument : MSVOA_N
ClientSampleId : WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion:105 Resp: 85087
Ion Ratio Lower Upper
105 100
120 25.2 13.4 40.1



#74
N-ethyl acetate
Concen: 64.091 ug/l
RT: 12.366 min Scan# 3869
Delta R.T. -0.019 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38

Tgt Ion: 43 Resp: 1819252
Ion Ratio Lower Upper
43 100
70 14.5 33.4 50.0#
55 26.3 19.3 28.9
61 0.0 18.5 27.7#


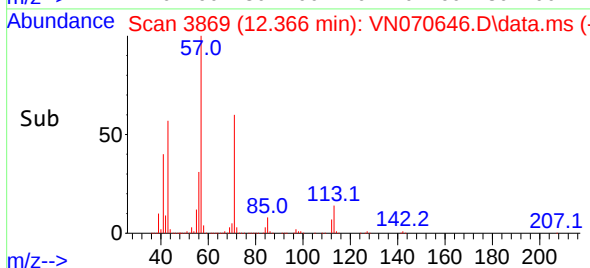
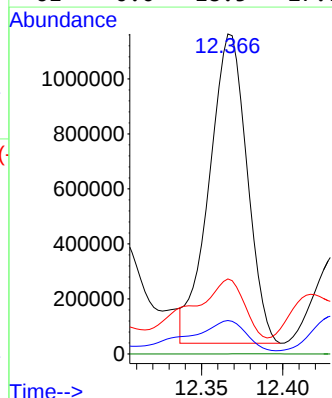





#75
1,1,2,2-Tetrachloroethane
Concen: 1.156 ug/l
RT: 12.862 min Scan# 4005
Delta R.T. 0.037 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38




Instrument : MSVOA_N
ClientSampleId : WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion: 83 Resp: 17521
Ion Ratio Lower Upper
83 100
131 0.5 5.5 16.5#
85 691.8 32.4 97.2#

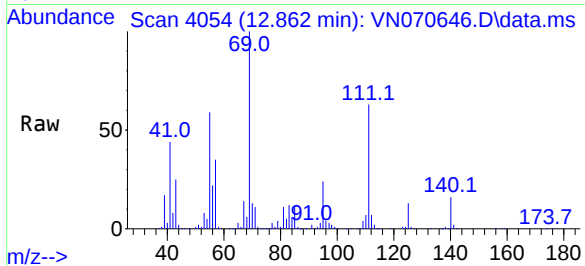

#76
1,2,3-Trichloropropane
Concen: 24.122 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.147 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38

Tgt Ion: 75 Resp: 486944
Ion Ratio Lower Upper
75 100
77 2.7 82.6 247.8#


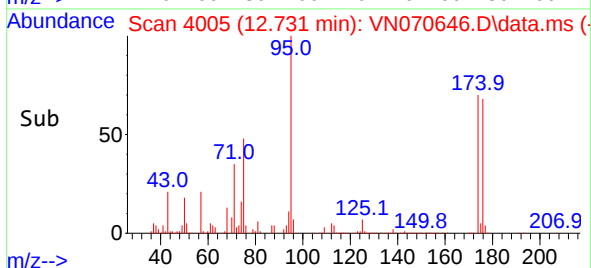
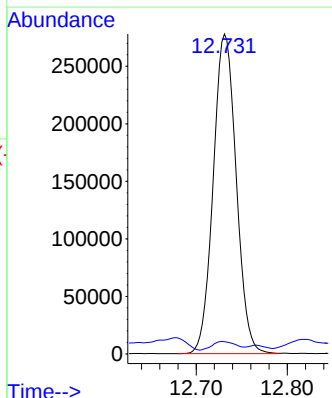
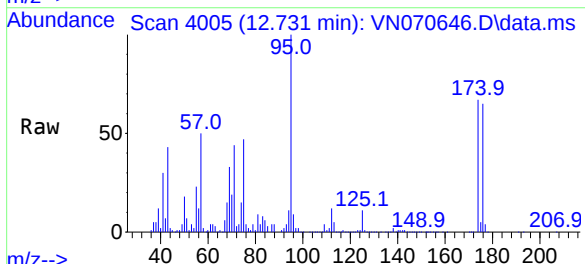




#77
Bromobenzene
Concen: 0.202 ug/l
RT: 12.827 min Scan# 4053
Delta R.T. -0.033 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38




Instrument : MSVOA_N
ClientSampleId : WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion:156 Resp: 3129
Ion Ratio Lower Upper
156 100
77 608.1 90.6 271.8#
158 0.0 48.9 146.7#



#78
n-propylbenzene
Concen: 5.002 ug/l
RT: 12.919 min Scan# 4075
Delta R.T. -0.000 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38

Tgt Ion: 91 Resp: 374115
Ion Ratio Lower Upper
91 100
120 21.5 11.9 35.9


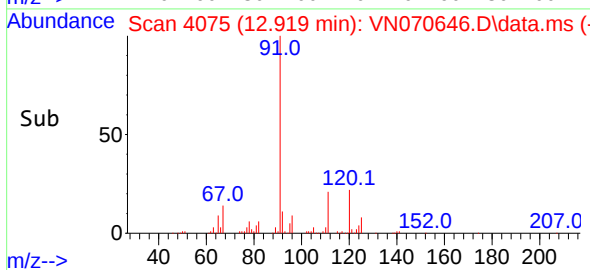






#79
2-Chlorotoluene
Concen: 2.835 ug/l
RT: 12.983 min Scan# 4108
Delta R.T. -0.024 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38




Instrument : MSVOA_N
ClientSampleId : WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion: 91 Resp: 136041
Ion Ratio Lower Upper
91 100
126 0.0 18.3 54.8#

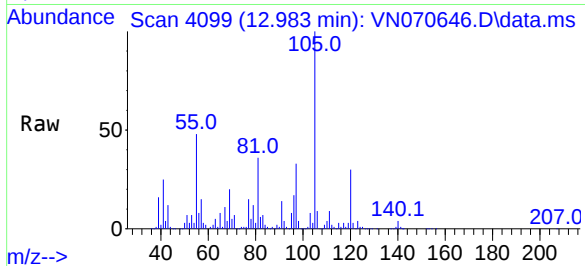

#80
1,3,5-Trimethylbenzene
Concen: 22.545 ug/l
RT: 13.058 min Scan# 4127
Delta R.T. 0.000 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38

Tgt Ion:105 Resp: 1219681
Ion Ratio Lower Upper
105 100
120 47.4 24.6 73.6


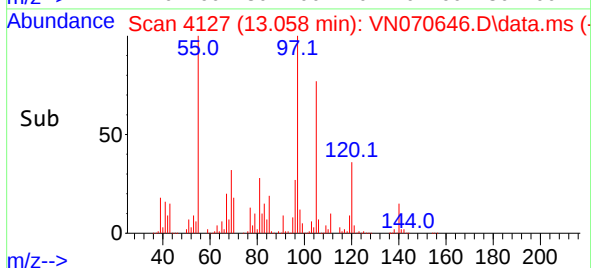
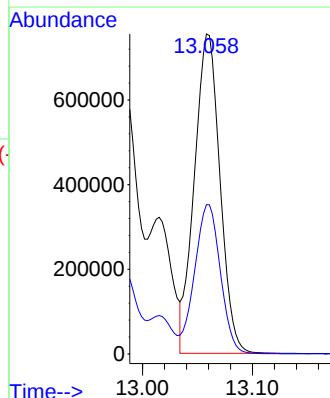
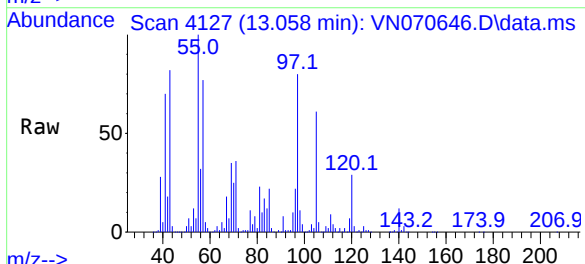




#81
trans-1,4-Dichloro-2-butene
Concen: 81.838 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.107 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38




Instrument : MSVOA_N
ClientSampleId : WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion: 75 Resp: 486944
Ion Ratio Lower Upper
75 100
53 3.4 90.5 135.7#
89 0.0 38.2 57.4#



#82
4-Chlorotoluene
Concen: 3.148 ug/l
RT: 13.058 min Scan# 4127
Delta R.T. -0.046 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38

Tgt Ion: 91 Resp: 141519
Ion Ratio Lower Upper
91 100
126 10.5 18.2 54.6#


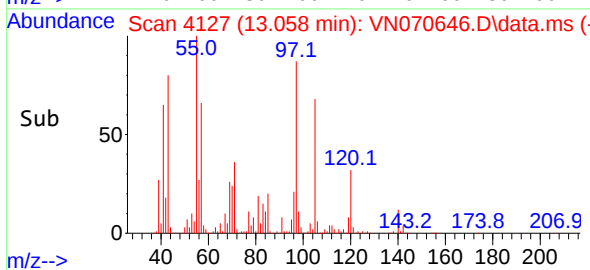






#83
 tert-Butylbenzene
 Concen: 1.833 ug/l
 RT: 13.324 min Scan# 4225
 Delta R.T. 0.003 min
 Lab File: VN070646.D
 Acq: 17 Jan 2022 15:38




Instrument : MSVOA_N
 ClientSampleId : WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion:119 Resp: 87310
 Ion Ratio Lower Upper
 119 100
 91 59.0 31.5 94.5
 134 24.3 12.4 37.4

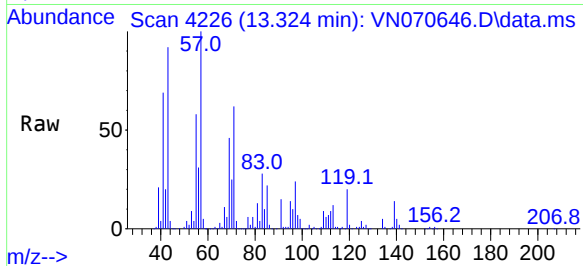

#84
 1,2,4-Trimethylbenzene
 Concen: 55.791 ug/l
 RT: 13.367 min Scan# 4242
 Delta R.T. 0.001 min
 Lab File: VN070646.D
 Acq: 17 Jan 2022 15:38

Tgt Ion:105 Resp: 2906353
 Ion Ratio Lower Upper
 105 100
 120 44.2 22.8 68.4


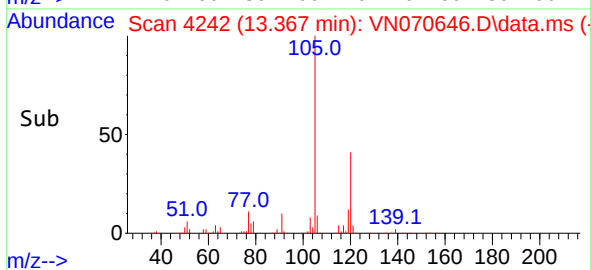

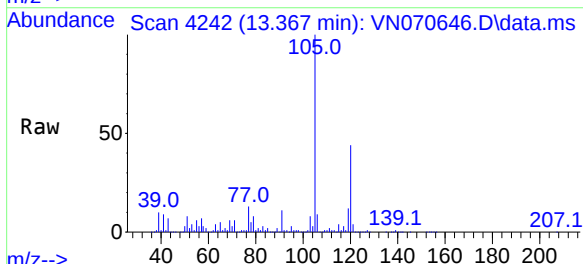




#85
 sec-Butylbenzene
 Concen: 6.109 ug/l
 RT: 13.501 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: VN070646.D
 Acq: 17 Jan 2022 15:38




Instrument :
 MSVOA_N
 ClientSampleId :
 WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion:105 Resp: 395087
 Ion Ratio Lower Upper
 105 100
 134 37.2 10.4 31.1#



#86
 p-Isopropyltoluene
 Concen: 7.914 ug/l
 RT: 13.613 min Scan# 4334
 Delta R.T. 0.000 min
 Lab File: VN070646.D
 Acq: 17 Jan 2022 15:38

Tgt Ion:119 Resp: 402055
 Ion Ratio Lower Upper
 119 100
 134 25.3 13.6 40.7
 91 24.1 11.4 34.1


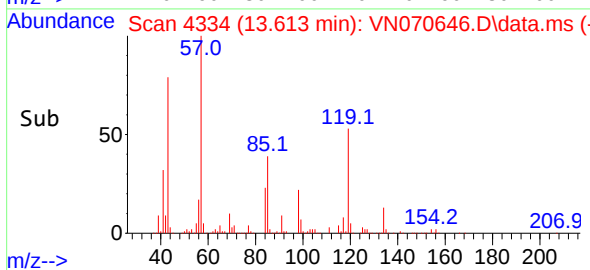






#89
n-Butylbenzene
Concen: 6.393 ug/l
RT: 13.940 min Scan# 4456
Delta R.T. 0.000 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38




Instrument : MSVOA_N
ClientSampleId : WEST-BOILER-ROOM-SOUTH-SIDEWALLME


Tgt Ion: 91 Resp: 270909
Ion Ratio Lower Upper
91 100
92 60.3 25.4 76.0
134 0.0 13.6 40.8#

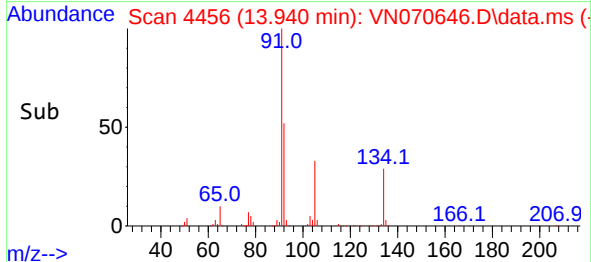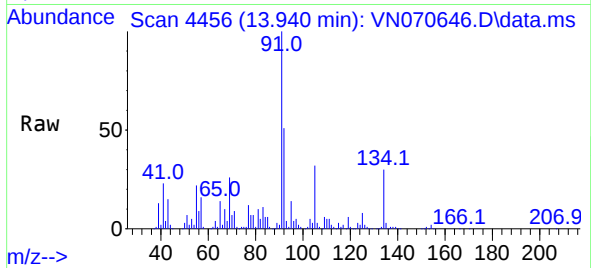

#90
Hexachloroethane
Concen: 4.043 ug/l
RT: 14.217 min Scan# 4559
Delta R.T. 0.008 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38


Tgt Ion: 117 Resp: 35679
Ion Ratio Lower Upper
117 100
201 0.0 43.9 131.6#

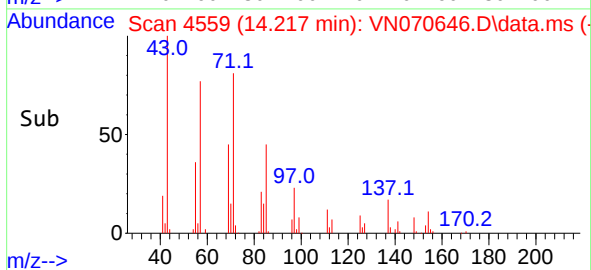






#93
1,2,4-Trichlorobenzene
Concen: 0.448 ug/l
RT: 15.260 min Scan# 4949
Delta R.T. -0.003 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38

Instrument :
MSVOA_N
ClientSampleId :
WEST-BOILER-ROOM-SOUTH-SIDEWALLME



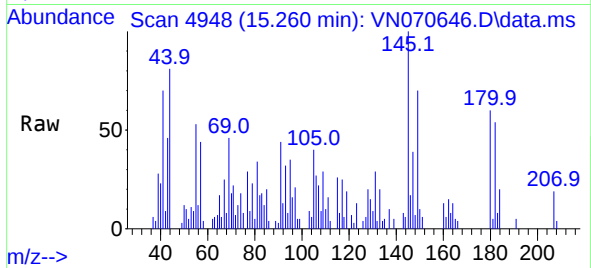



Tgt Ion:180 Resp: 5369
Ion Ratio Lower Upper
180 100
182 89.9 48.3 144.9
145 163.3 14.5 43.5#

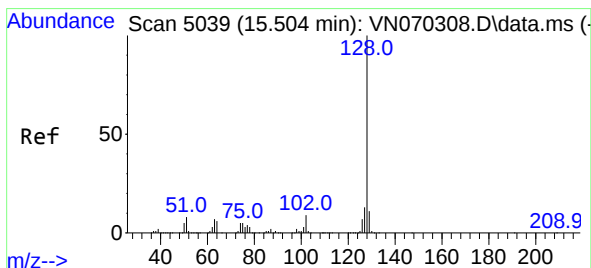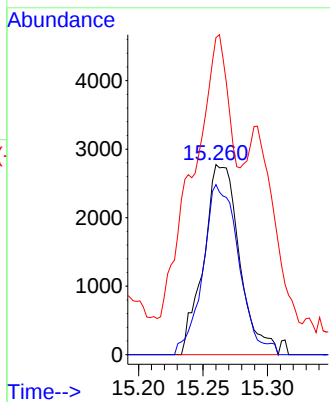

#95
Naphthalene
Concen: 4.406 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. 0.003 min
Lab File: VN070646.D
Acq: 17 Jan 2022 15:38


Tgt Ion:128 Resp: 89641
Ion Ratio Lower Upper
128 100
127 14.1 10.5 15.7
129 10.9 8.7 13.1

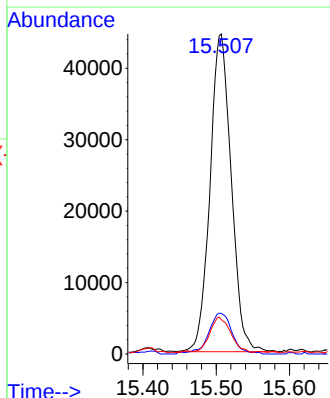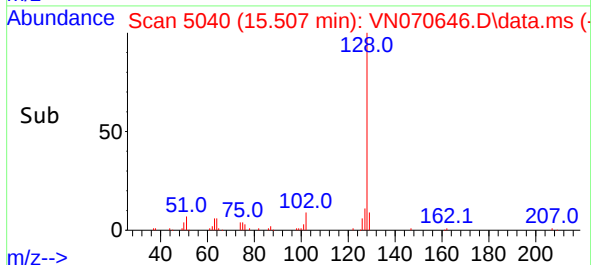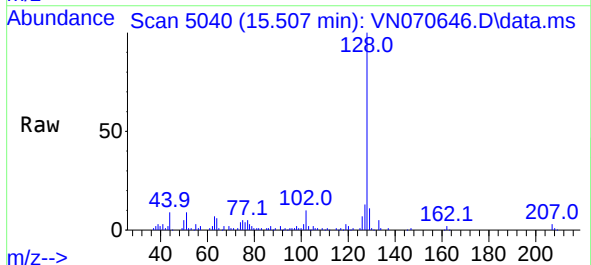



#96
 1,2,3-Trichlorobenzene
 Concen: 1.308 ug/l
 RT: 15.705 min Scan# 5112
 Delta R.T. 0.005 min
 Lab File: VN070646.D
 Acq: 17 Jan 2022 15:38

Instrument :
 MSVOA_N
 ClientSampleId :
 WEST-BOILER-ROOM-SOUTH-SIDEWALLME



Tgt Ion:180 Resp: 5614
 Ion Ratio Lower Upper
 180 100
 182 87.9 47.4 142.2
 145 47.1 15.0 45.1#

