

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011722\
 Data File : VN070647.D
 Acq On : 17 Jan 2022 16:03
 Operator : JC/MD
 Sample : N1160-01 50X
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FMI-114DL

Quant Time: Jan 17 17:06:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 27 18:47:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	1088828	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	1839922	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	1624118	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	568267	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	763180	48.749	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	97.500%
35) Dibromofluoromethane	8.021	113	528429	47.467	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	94.940%
50) Toluene-d8	10.440	98	2229451	49.024	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	98.040%
62) 4-Bromofluorobenzene	12.731	95	815917	49.674	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	99.340%
Target Compounds						
					Qvalue	
3) Chloromethane	2.306	50	4079	0.243	ug/l	95
11) Tert butyl alcohol	5.320	59	3962	1.520	ug/l #	71
13) Acrolein	4.041	56	718	0.339	ug/l #	14
16) Acetone	4.301	43	19622	1.931	ug/l	100
25) 2-Butanone	7.345	43	7327	0.573	ug/l	91
30) Chloroform	7.817	83	18935	0.773	ug/l	99
31) Cyclohexane	8.086	56	26574	1.076	ug/l #	1
36) 1,1-Dichloropropene	8.086	75	87996	4.778	ug/l #	49
37) Ethyl Acetate	7.345	43	7327	0.307	ug/l #	68
38) Carbon Tetrachloride	8.083	117	106736	6.070	ug/l #	17
40) Benzene	8.461	78	74157	1.313	ug/l	99
52) Toluene	10.505	92	826505	24.185	ug/l	97
53) t-1,3-Dichloropropene	10.502	75	9074	0.447	ug/l #	1
67) Ethyl Benzene	11.846	91	337732	5.349	ug/l	96
68) m/p-Xylenes	11.950	106	378868	16.485	ug/l	93
69) o-Xylene	12.280	106	187791	8.215	ug/l	91
70) Styrene	12.280	104	11754	0.325	ug/l #	1
73) Isopropylbenzene	12.578	105	16850	0.319	ug/l	99
75) 1,1,2,2-Tetrachloroethane	12.811	83	98	0.452	ug/l #	1
76) 1,2,3-Trichloropropane	12.731	75	415785	26.097	ug/l #	1
78) n-propylbenzene	12.924	91	51413	0.879	ug/l	95
79) 2-Chlorotoluene	12.980	91	17618	0.470	ug/l #	38
80) 1,3,5-Trimethylbenzene	13.061	105	67684	1.601	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.731	75	415785	89.393	ug/l #	5
83) tert-Butylbenzene	13.369	119	33323	0.895	ug/l #	61
84) 1,2,4-Trimethylbenzene	13.369	105	269697	6.623	ug/l	98
85) sec-Butylbenzene	13.369	105	269697	5.335	ug/l #	56
89) n-Butylbenzene	13.943	91	7045	0.213	ug/l #	70
90) Hexachloroethane	14.214	117	2192	0.318	ug/l #	6
95) Naphthalene	15.507	128	29392	2.891	ug/l #	93
96) 1,2,3-Trichlorobenzene	15.705	180	2138	1.061	ug/l	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011722\
Data File : VN070647.D
Acq On : 17 Jan 2022 16:03
Operator : JC/MD
Sample : N1160-01 50X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FMI-114DL

Quant Time: Jan 17 17:06:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260
QLast Update : Mon Dec 27 18:47:12 2021
Response via : Initial Calibration




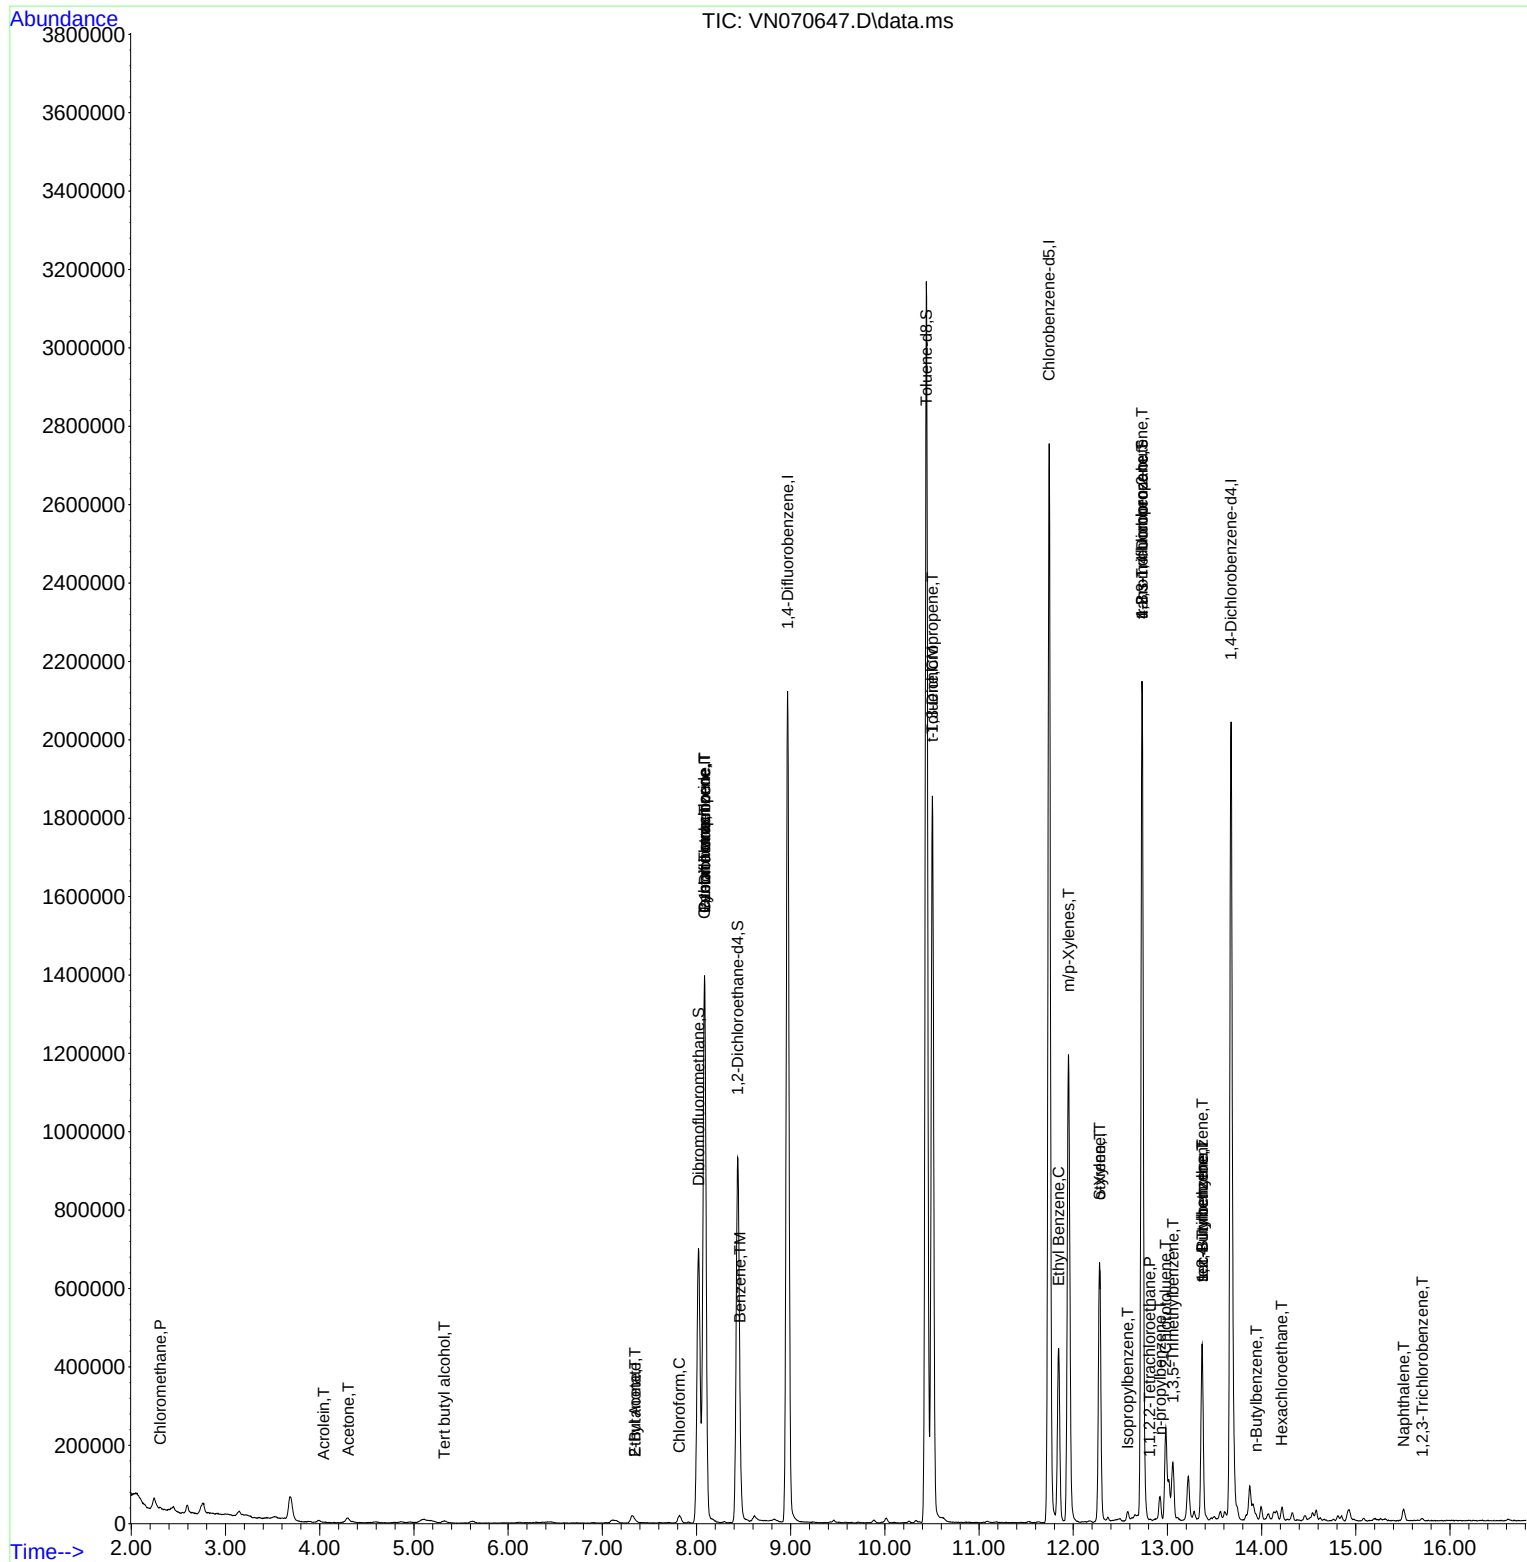




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03




Instrument :
MSVOA_N
ClientSampleId :
FMI-114DL


Tgt Ion:168 Resp: 1088828
Ion Ratio Lower Upper
168 100
99 59.1 41.3 61.9

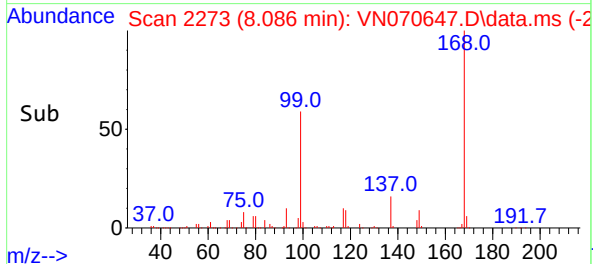

#3
Chloromethane
Concen: 0.243 ug/l
RT: 2.306 min Scan# 118
Delta R.T. 0.003 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03

Tgt Ion: 50 Resp: 4079
Ion Ratio Lower Upper
50 100
52 28.9 25.4 38.0


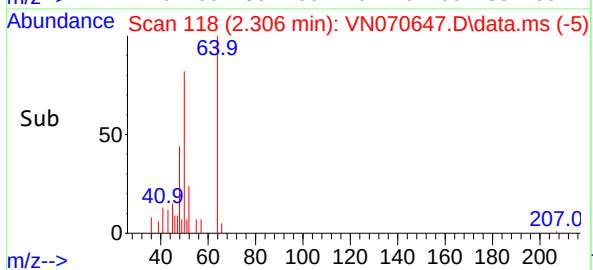

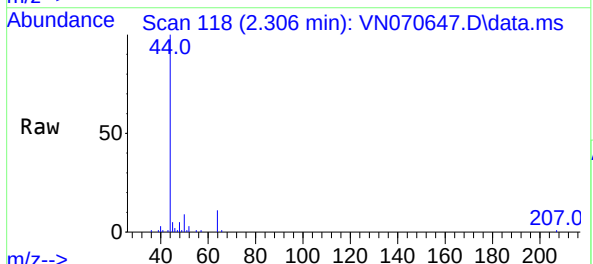




#11
Tert butyl alcohol
Concen: 1.520 ug/l
RT: 5.320 min Scan# 11
Delta R.T. -0.057 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03




Instrument :
MSVOA_N
ClientSampleId :
FMI-114DL


Tgt Ion: 59 Resp: 3962
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#

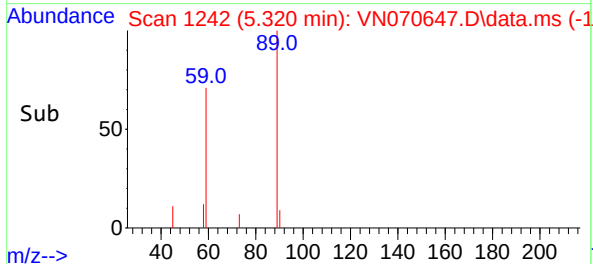

#13
Acrolein
Concen: 0.339 ug/l
RT: 4.041 min Scan# 765
Delta R.T. 0.000 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03

Tgt Ion: 56 Resp: 718
Ion Ratio Lower Upper
56 100
55 0.0 56.6 85.0#


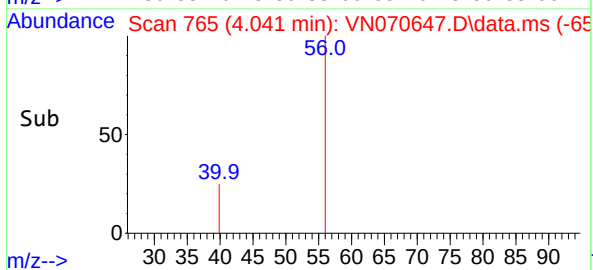

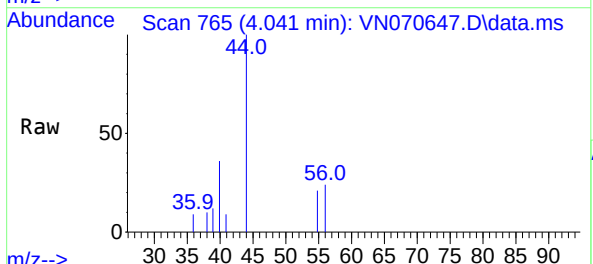




#16
Acetone
Concen: 1.931 ug/l
RT: 4.301 min Scan# 80
Delta R.T. 0.016 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03




Instrument :
MSVOA_N
ClientSampleId :
FMI-114DL


Tgt Ion: 43 Resp: 19622
Ion Ratio Lower Upper
43 100
58 29.0 23.1 34.7

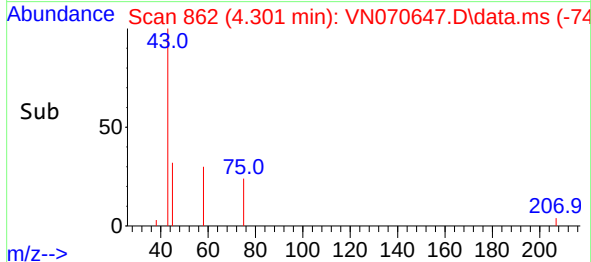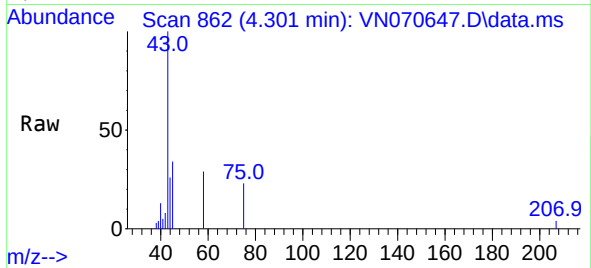

#25
2-Butanone
Concen: 0.573 ug/l
RT: 7.345 min Scan# 1997
Delta R.T. 0.010 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03

Tgt Ion: 43 Resp: 7327
Ion Ratio Lower Upper
43 100
72 22.3 21.7 32.5

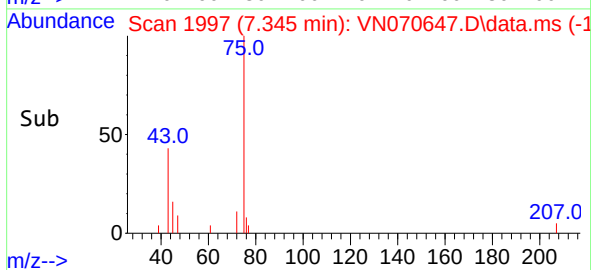



#30

Chloroform

Concen: 0.773 ug/l

RT: 7.817 min Scan# 2173

Delta R.T. 0.000 min

Lab File: VN070647.D

Acq: 17 Jan 2022 16:03

Instrument :

MSVOA_N

ClientSampleId :





FMI-114DL

Tgt Ion: 83 Resp: 18935

Ion Ratio Lower Upper

83 100

85 64.4 51.9 77.9

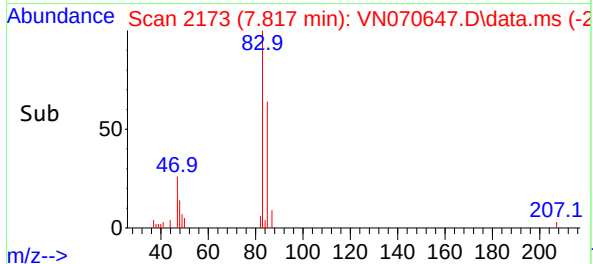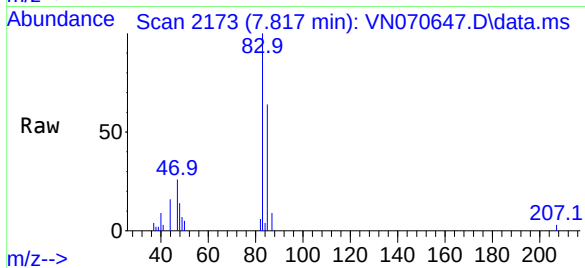

#31

Cyclohexane

Concen: 1.076 ug/l

RT: 8.086 min Scan# 2273

Delta R.T. -0.008 min

Lab File: VN070647.D

Acq: 17 Jan 2022 16:03




Tgt Ion: 56 Resp: 26574


Ion Ratio Lower Upper

56 100

69 168.8 27.1 40.7#

84 151.1 73.4 110.0#

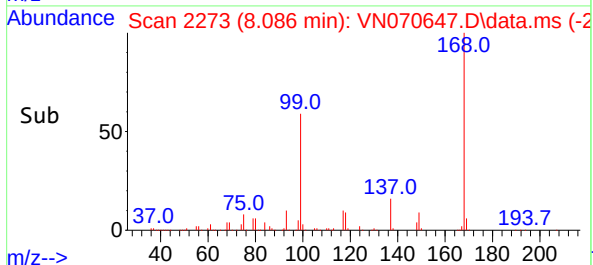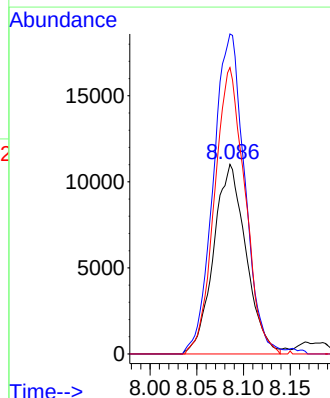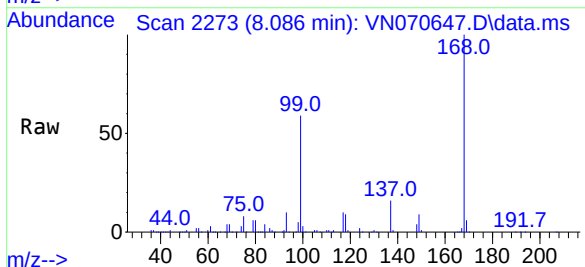



#33

1,2-Dichloroethane-d4

Concen: 48.749 ug/l

RT: 8.437 min Scan# 2404

Delta R.T. -0.000 min

Lab File: VN070647.D

Acq: 17 Jan 2022 16:03

Instrument :

MSVOA_N

ClientSampleId :





FMI-114DL

Tgt Ion: 65 Resp: 763180

Ion Ratio Lower Upper

65 100

67 53.0 0.0 103.0

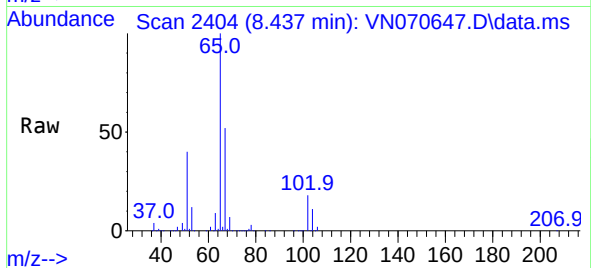

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.968 min Scan# 2602

Delta R.T. -0.000 min

Lab File: VN070647.D

Acq: 17 Jan 2022 16:03




Tgt Ion: 114 Resp: 1839922


Ion Ratio Lower Upper

114 100

63 23.3 0.0 37.8

88 16.8 0.0 27.4


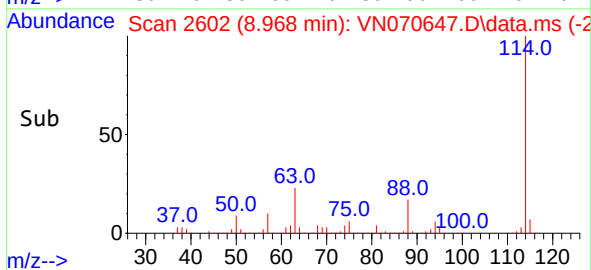






#35
Dibromofluoromethane
Concen: 47.467 ug/l
RT: 8.021 min Scan# 211
Delta R.T. 0.000 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03




Instrument :
MSVOA_N
ClientSampleId :
FMI-114DL


Tgt Ion:113 Resp: 528429
Ion Ratio Lower Upper
113 100
111 102.7 82.2 123.2
192 19.6 16.9 25.3

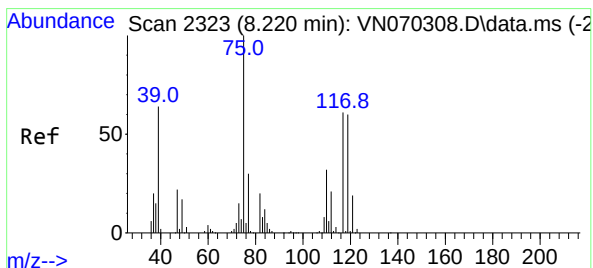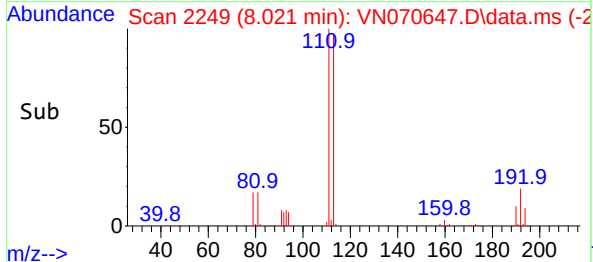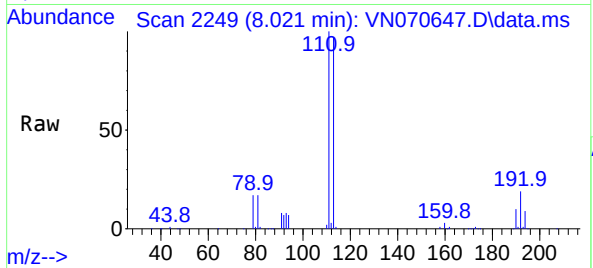

#36
1,1-Dichloropropene
Concen: 4.778 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.134 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03

Tgt Ion: 75 Resp: 87996
Ion Ratio Lower Upper
75 100
110 8.4 18.4 55.2#
77 0.0 24.4 36.6#


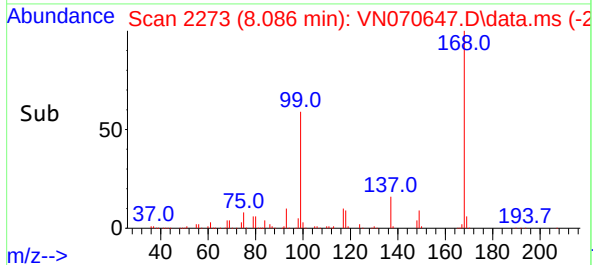

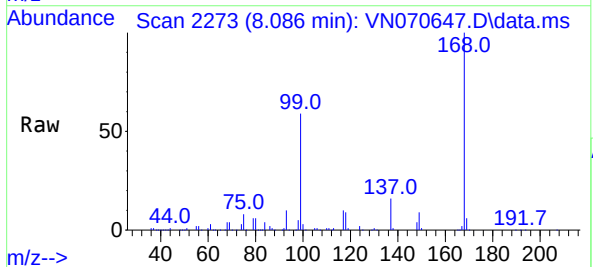




#37
Ethyl Acetate
Concen: 0.307 ug/l
RT: 7.345 min Scan# 1997
Delta R.T. -0.067 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03




Instrument :
MSVOA_N
ClientSampleId :
FMI-114DL


Tgt Ion: 43 Resp: 7327
Ion Ratio Lower Upper
43 100
61 0.0 11.5 17.3#
70 0.0 7.9 11.9#

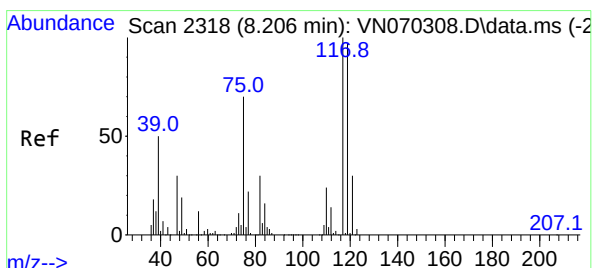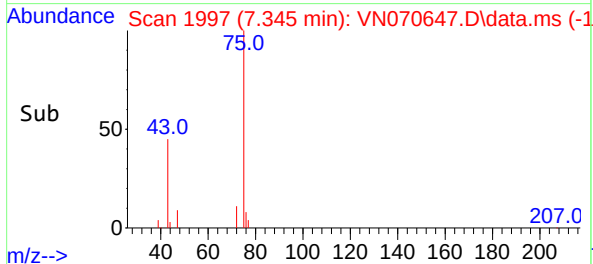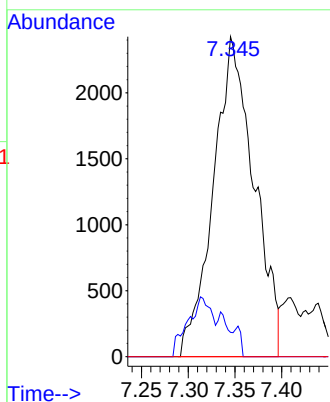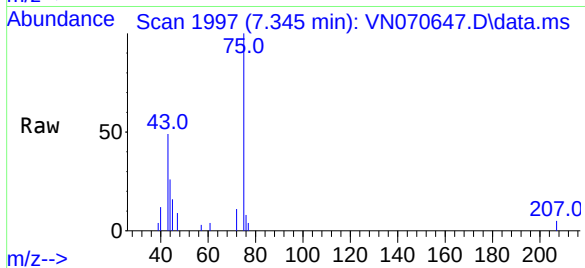

#38
Carbon Tetrachloride
Concen: 6.070 ug/l
RT: 8.083 min Scan# 2272
Delta R.T. -0.123 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03

Tgt Ion: 117 Resp: 106736
Ion Ratio Lower Upper
117 100
119 5.7 76.1 114.1#
121 0.0 24.2 36.2#


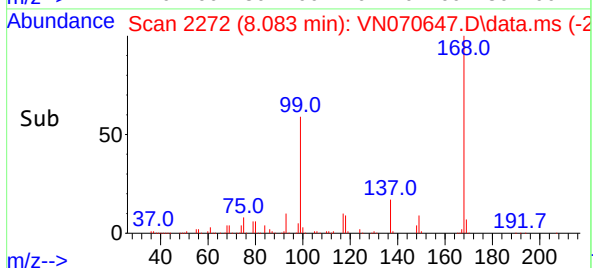

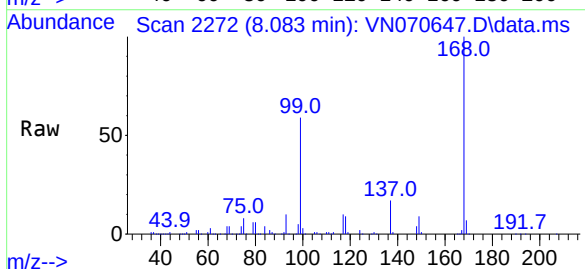




#40
Benzene
Concen: 1.313 ug/l
RT: 8.461 min Scan# 2412
Delta R.T. 0.003 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03




Instrument :
MSVOA_N
ClientSampleId :
FMI-114DL


Tgt Ion: 78 Resp: 74157
Ion Ratio Lower Upper
78 100
77 23.9 18.6 27.8

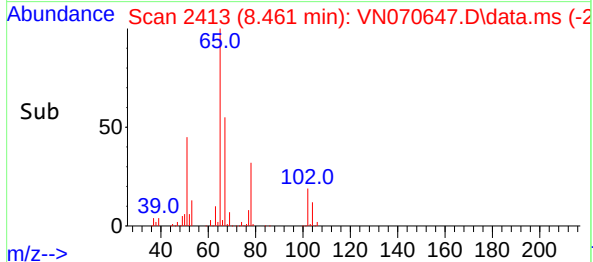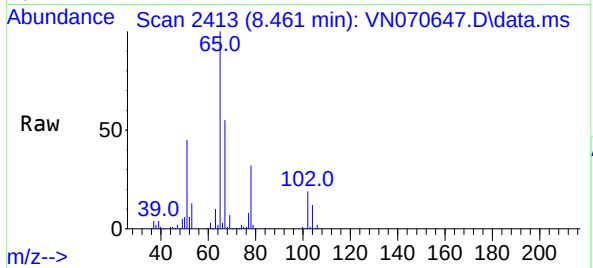

#50
Toluene-d8
Concen: 49.024 ug/l
RT: 10.440 min Scan# 3151
Delta R.T. 0.000 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03

Tgt Ion: 98 Resp: 2229451
Ion Ratio Lower Upper
98 100
100 64.7 50.4 75.6


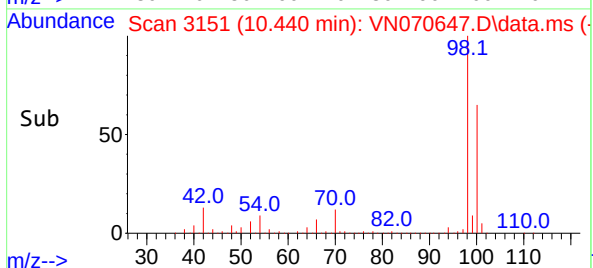
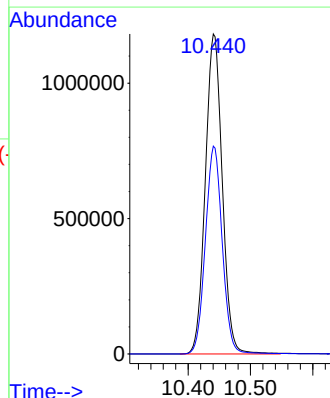
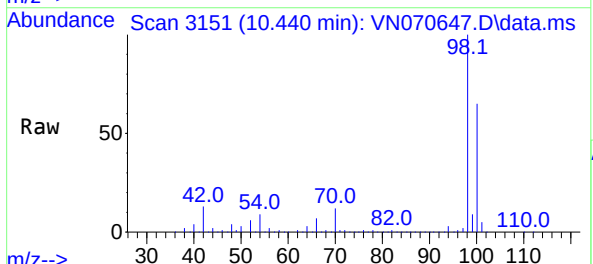




#52
Toluene
Concen: 24.185 ug/l
RT: 10.505 min Scan# 3175
Delta R.T. -0.000 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03




Instrument :
MSVOA_N
ClientSampleId :
FMI-114DL


Tgt Ion: 92 Resp: 826505
Ion Ratio Lower Upper
92 100
91 173.4 142.0 213.0

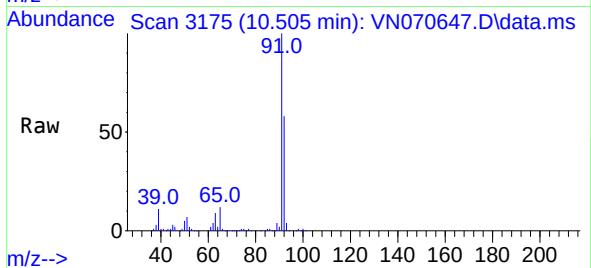

#53
t-1,3-Dichloropropene
Concen: 0.447 ug/l
RT: 10.502 min Scan# 3174
Delta R.T. -0.215 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03

Tgt Ion: 75 Resp: 9074
Ion Ratio Lower Upper
75 100
77 165.4 25.6 38.4#


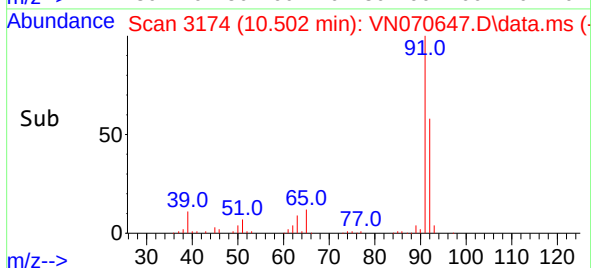






#62
4-Bromofluorobenzene
Concen: 49.674 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.000 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03




Instrument :
MSVOA_N
ClientSampleId :
FMI-114DL


Tgt Ion: 95 Resp: 815917
Ion Ratio Lower Upper
95 100
174 73.9 0.0 187.2
176 71.0 0.0 181.4



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. -0.000 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03

Tgt Ion: 117 Resp: 1624118
Ion Ratio Lower Upper
117 100
82 60.7 42.4 63.6
119 32.2 25.4 38.2

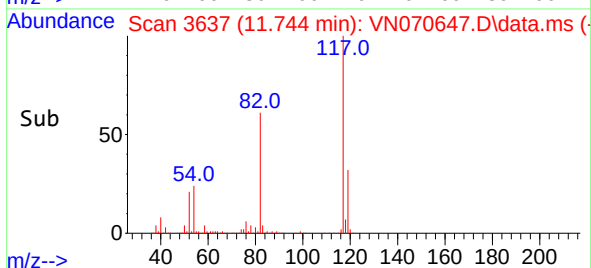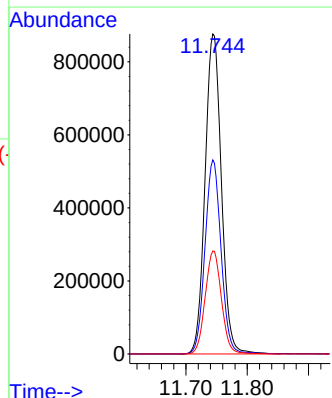



#67

Ethyl Benzene

Concen: 5.349 ug/l

RT: 11.846 min Scan# 3

Delta R.T. 0.003 min

Lab File: VN070647.D

Acq: 17 Jan 2022 16:03

Instrument :

MSVOA_N

ClientSampleId :





FMI-114DL

Tgt Ion: 91 Resp: 337732

Ion Ratio Lower Upper

91 100

106 30.0 25.7 38.5

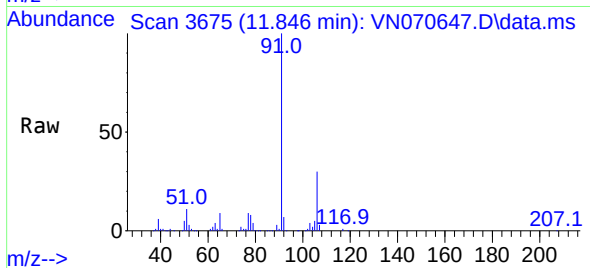

#68

m/p-Xylenes

Concen: 16.485 ug/l

RT: 11.950 min Scan# 3714

Delta R.T. -0.003 min

Lab File: VN070647.D




Acq: 17 Jan 2022 16:03


Tgt Ion:106 Resp: 378868

Ion Ratio Lower Upper

106 100

91 212.0 160.6 240.8


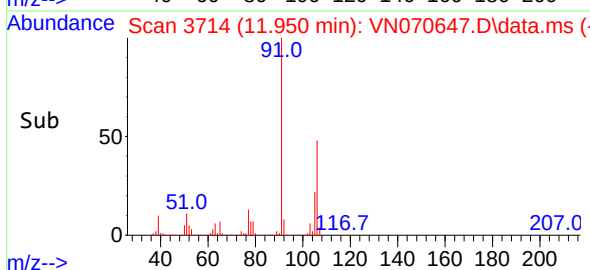






#69
o-Xylene
Concen: 8.215 ug/l
RT: 12.280 min Scan# 3837
Delta R.T. 0.002 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03




Instrument :
MSVOA_N
ClientSampleId :
FMI-114DL


Tgt Ion:106 Resp: 187791
Ion Ratio Lower Upper
106 100
91 224.9 105.8 317.3

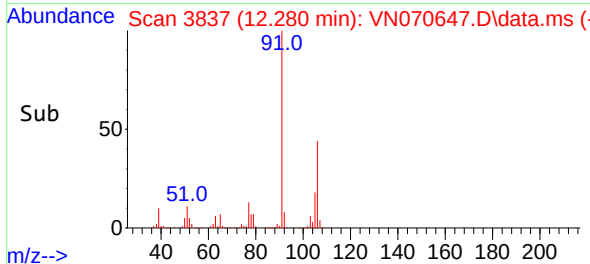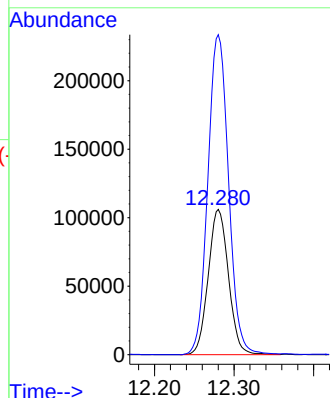

#70
Styrene
Concen: 0.325 ug/l
RT: 12.280 min Scan# 3837
Delta R.T. -0.014 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03

Tgt Ion:104 Resp: 11754
Ion Ratio Lower Upper
104 100
78 258.2 38.7 58.1#
103 236.9 45.0 67.6#


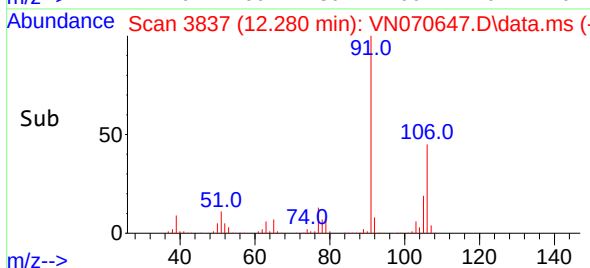
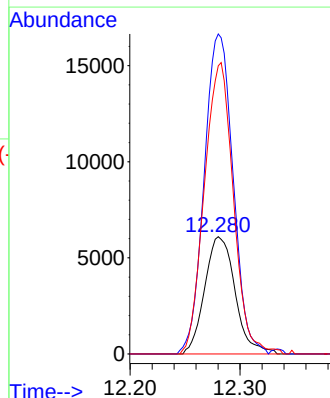
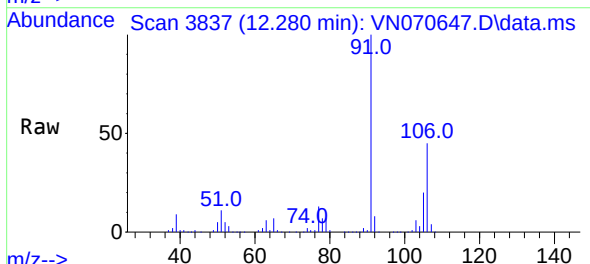




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 41
Delta R.T. 0.003 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03




Instrument :
MSVOA_N
ClientSampleId :
FMI-114DL


Tgt Ion:152 Resp: 568267
Ion Ratio Lower Upper
152 100
115 61.1 27.5 82.5
150 156.7 0.0 344.4



#73
Isopropylbenzene
Concen: 0.319 ug/l
RT: 12.578 min Scan# 3948
Delta R.T. -0.000 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03

Tgt Ion:105 Resp: 16850
Ion Ratio Lower Upper
105 100
120 26.4 13.4 40.1


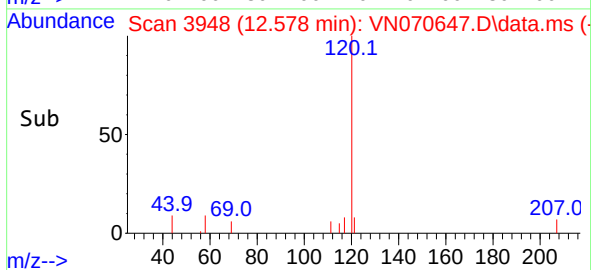






#75
1,1,2,2-Tetrachloroethane
Concen: 0.452 ug/l
RT: 12.811 min Scan# 4035
Delta R.T. -0.014 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03




Instrument :
MSVOA_N
ClientSampleId :
FMI-114DL


Tgt Ion: 83 Resp: 98
Ion Ratio Lower Upper
83 100
131 0.0 5.5 16.5#
85 606.1 32.4 97.2#

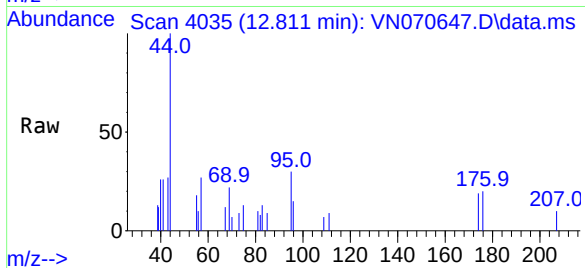

#76
1,2,3-Trichloropropane
Concen: 26.097 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.147 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03

Tgt Ion: 75 Resp: 415785
Ion Ratio Lower Upper
75 100
77 1.2 82.6 247.8#


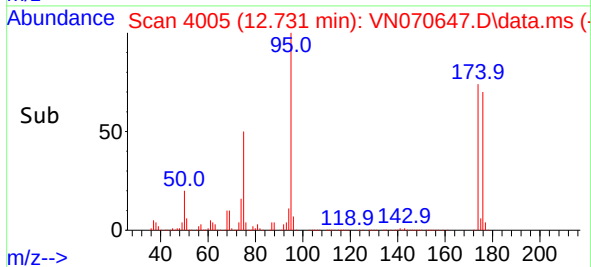

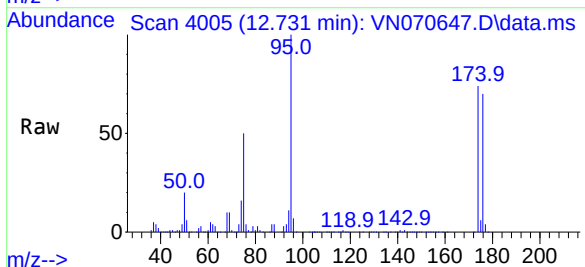




#78
n-propylbenzene
Concen: 0.879 ug/l
RT: 12.924 min Scan# 4077
Delta R.T. 0.005 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03




Instrument :
MSVOA_N
ClientSampleId :
FMI-114DL


Tgt Ion: 91 Resp: 51413
Ion Ratio Lower Upper
91 100
120 21.4 11.9 35.9

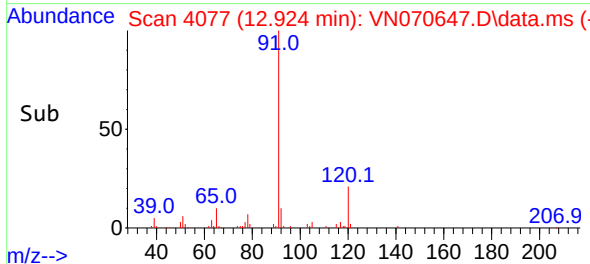

#79
2-Chlorotoluene
Concen: 0.470 ug/l
RT: 12.980 min Scan# 4098
Delta R.T. -0.027 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03

Tgt Ion: 91 Resp: 17618
Ion Ratio Lower Upper
91 100
126 0.0 18.3 54.8#


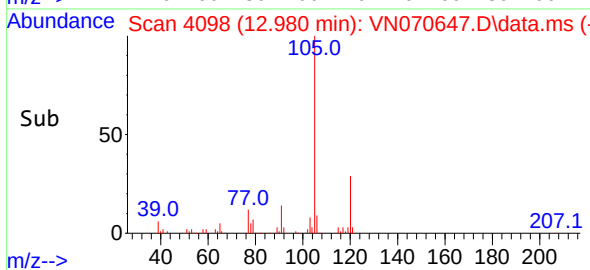

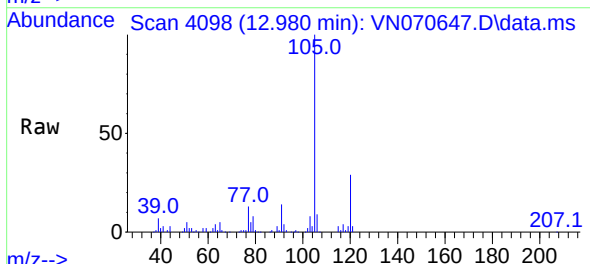




#80
1,3,5-Trimethylbenzene
Concen: 1.601 ug/l
RT: 13.061 min Scan# 41
Delta R.T. 0.003 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03




Instrument :
MSVOA_N
ClientSampleId :
FMI-114DL


Tgt Ion:105 Resp: 67684
Ion Ratio Lower Upper
105 100
120 48.4 24.6 73.6

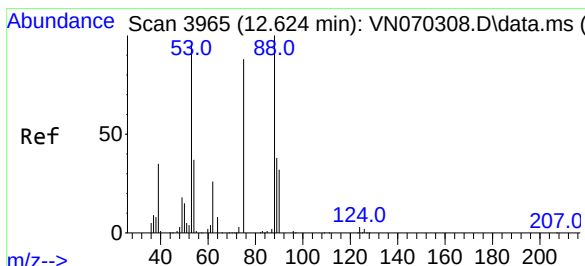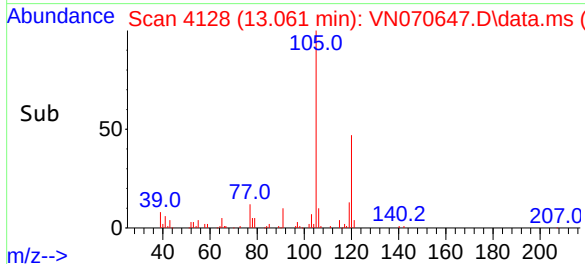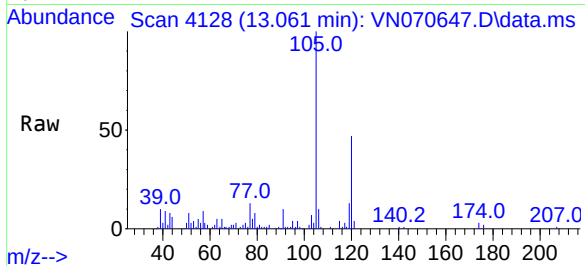

#81
trans-1,4-Dichloro-2-butene
Concen: 89.393 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.107 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03

Tgt Ion: 75 Resp: 415785
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#


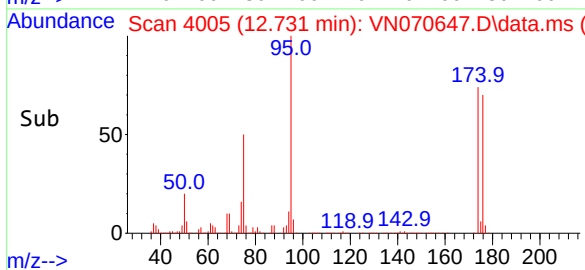

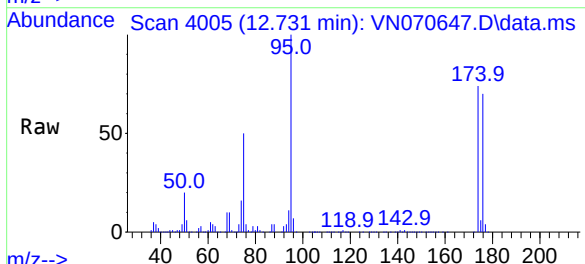




#83
tert-Butylbenzene
Concen: 0.895 ug/l
RT: 13.369 min Scan# 4225
Delta R.T. 0.048 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03




Instrument :
MSVOA_N
ClientSampleId :
FMI-114DL


Tgt Ion:119 Resp: 33323
Ion Ratio Lower Upper
119 100
91 90.3 31.5 94.5
134 0.0 12.4 37.4#

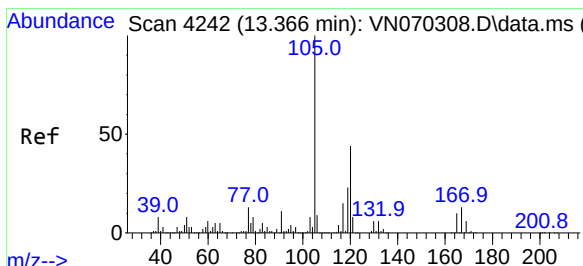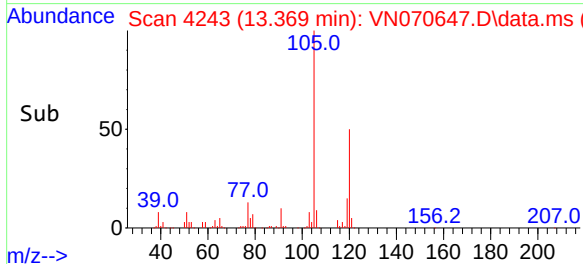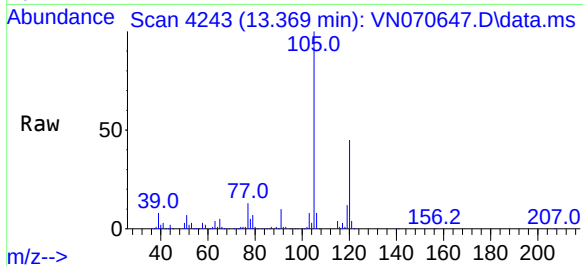

#84
1,2,4-Trimethylbenzene
Concen: 6.623 ug/l
RT: 13.369 min Scan# 4243
Delta R.T. 0.003 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03

Tgt Ion:105 Resp: 269697
Ion Ratio Lower Upper
105 100
120 44.3 22.8 68.4


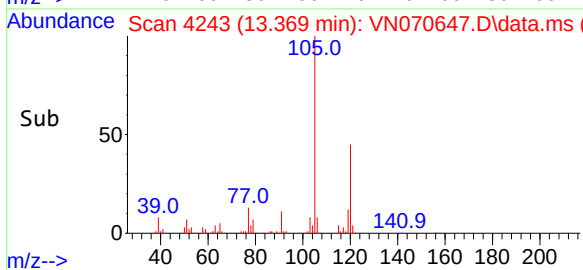

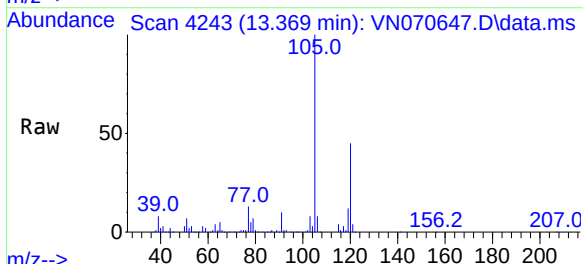




#85
sec-Butylbenzene
Concen: 5.335 ug/l
RT: 13.369 min Scan# 41
Delta R.T. -0.132 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03




Instrument :
MSVOA_N
ClientSampleId :
FMI-114DL


Tgt Ion:105 Resp: 269697
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#

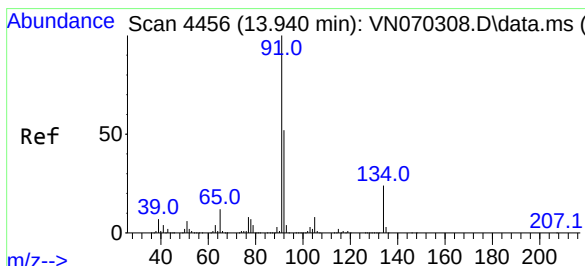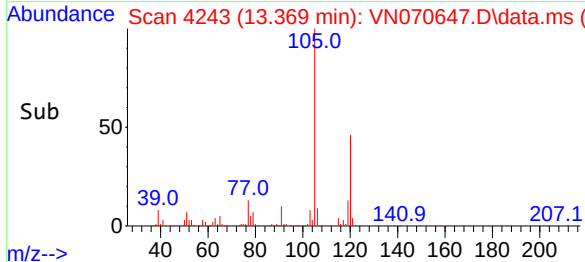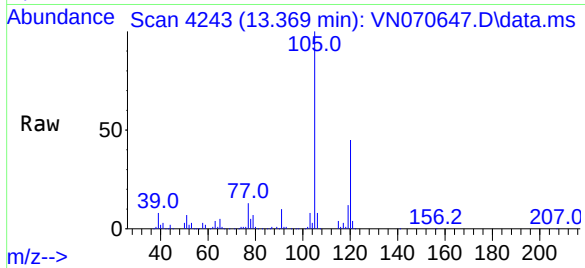

#89
n-Butylbenzene
Concen: 0.213 ug/l
RT: 13.943 min Scan# 4457
Delta R.T. 0.003 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03

Tgt Ion: 91 Resp: 7045
Ion Ratio Lower Upper
91 100
92 63.0 25.4 76.0
134 0.0 13.6 40.8#


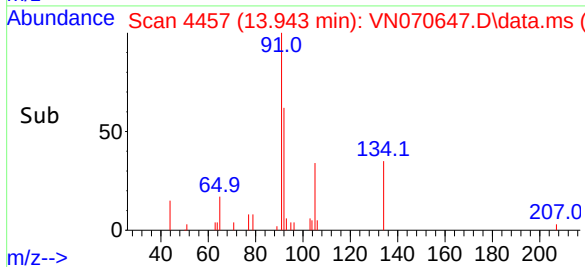

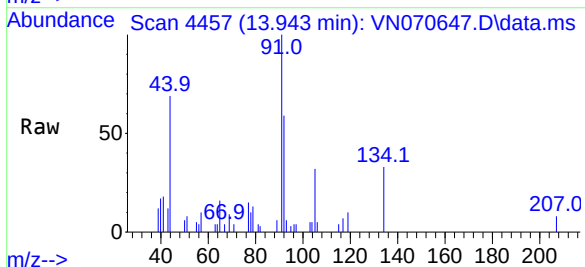




#90
Hexachloroethane
Concen: 0.318 ug/l
RT: 14.214 min Scan# 4558
Delta R.T. 0.005 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03




Instrument :
MSVOA_N
ClientSampleId :
FMI-114DL


Tgt Ion:117 Resp: 2192
Ion Ratio Lower Upper
117 100
201 0.0 43.9 131.6#

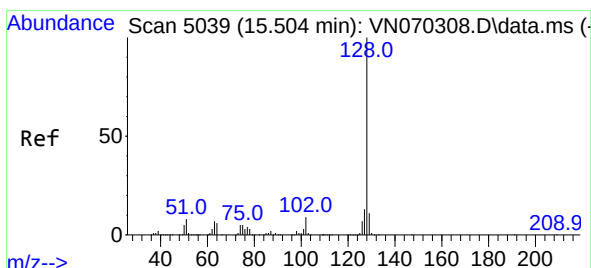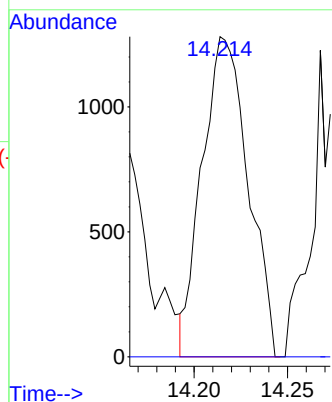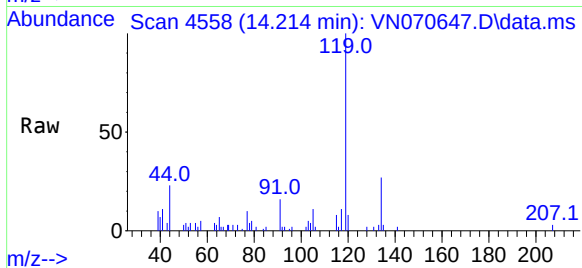

#95
Naphthalene
Concen: 2.891 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. 0.003 min
Lab File: VN070647.D
Acq: 17 Jan 2022 16:03


Tgt Ion:128 Resp: 29392
Ion Ratio Lower Upper
128 100
127 8.5 10.5 15.7#
129 11.2 8.7 13.1

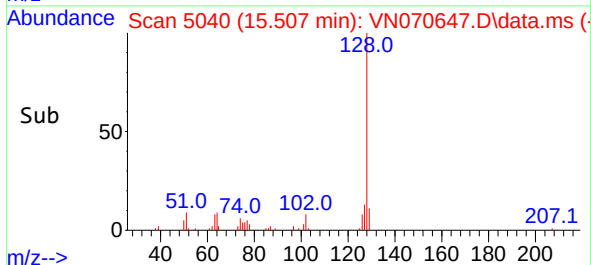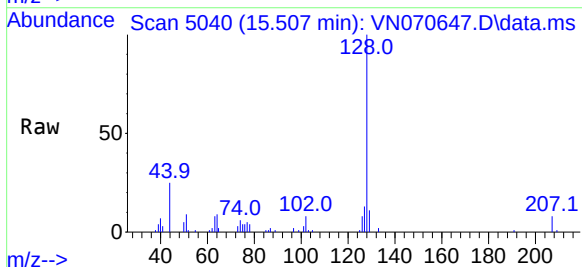



#96
 1,2,3-Trichlorobenzene
 Concen: 1.061 ug/l
 RT: 15.705 min Scan# 5114
 Delta R.T. 0.005 min
 Lab File: VN070647.D
 Acq: 17 Jan 2022 16:03

Instrument :
 MSVOA_N
 ClientSampleId :
 FMI-114DL

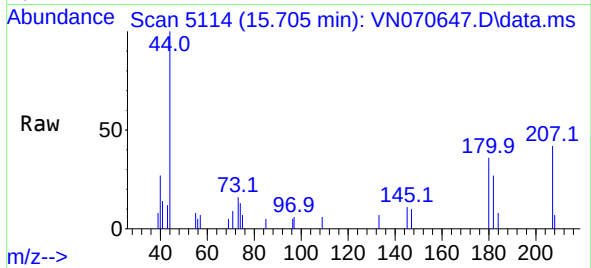

Tgt Ion:	180	Resp:	2138
Ion	Ratio	Lower	Upper
180	100		
182	80.7	47.4	142.2
145	19.9	15.0	45.1

