

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011723\
 Data File : VN076278.D
 Acq On : 17 Jan 2023 14:24
 Operator : JC\MD
 Sample : PB150289ZHE#03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB150289ZHE#03

Quant Time: Jan 18 00:54:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 17 03:59:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.229	168	368528	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	597891	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	535345	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	220848	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	200206	48.519	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	97.040%
35) Dibromofluoromethane	8.171	113	177499	47.459	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.920%
50) Toluene-d8	10.570	98	701476	50.786	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	101.580%
62) 4-Bromofluorobenzene	12.853	95	221612	49.147	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	98.300%
Target Compounds						
					Qvalue	
16) Acetone	4.441	43	39183	29.557	ug/l	99
18) Methyl Acetate	5.030	43	1304	0.291	ug/l #	46
20) Methylene Chloride	5.283	84	18939	4.288	ug/l #	95
25) 2-Butanone	7.500	43	5650	2.797	ug/l	95
29) Tetrahydrofuran	7.859	42	479	0.384	ug/l #	51
31) Cyclohexane	8.229	56	7125	1.124	ug/l #	1
36) 1,1-Dichloropropene	8.235	75	27535	5.181	ug/l #	49
37) Ethyl Acetate	7.565	43	34114	8.034	ug/l	97
38) Carbon Tetrachloride	8.229	117	36107	6.092	ug/l #	17
42) 1,2-Dichloroethane	8.694	62	1538	0.283	ug/l #	73
43) Isopropyl Acetate	8.694	43	276952	39.937	ug/l #	76
45) 1,2-Dichloropropane	9.741	63	2529	0.665	ug/l #	42
48) Methyl methacrylate	9.741	41	145331	44.268	ug/l #	35
49) 1,4-Dioxane	9.735	88	138	1.992	ug/l #	1
51) 4-Methyl-2-Pentanone	10.453	43	15018	3.689	ug/l #	75
53) t-1,3-Dichloropropene	10.729	75	1383	0.260	ug/l #	42
54) cis-1,3-Dichloropropene	10.359	75	75513	12.358	ug/l #	61
56) Ethyl methacrylate	10.988	69	1639	0.313	ug/l #	1
57) 1,3-Dichloropropane	11.206	76	9577	1.451	ug/l #	42
59) 2-Hexanone	11.170	43	150161	50.902	ug/l #	21
71) Bromoform	12.841	173	1591	0.523	ug/l #	1
74) N-amyl acetate	12.488	43	1767	0.360	ug/l #	37
76) 1,2,3-Trichloropropane	12.853	75	115630	28.329	ug/l #	1
77) Bromobenzene	12.976	156	63	Below Cal		69
81) trans-1,4-Dichloro-2-b...	12.853	75	115630	87.114	ug/l #	11
88) 1,4-Dichlorobenzene	13.806	146	842	0.211	ug/l #	75
93) 1,2,4-Trichlorobenzene	15.394	180	456	1.420	ug/l #	64
95) Naphthalene	15.641	128	2465	2.046	ug/l #	85
96) 1,2,3-Trichlorobenzene	15.853	180	316	1.237	ug/l #	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011723\
Data File : VN076278.D
Acq On : 17 Jan 2023 14:24
Operator : JC\MD
Sample : PB150289ZHE#03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB150289ZHE#03

Quant Time: Jan 18 00:54:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 17 03:59:22 2023
Response via : Initial Calibration




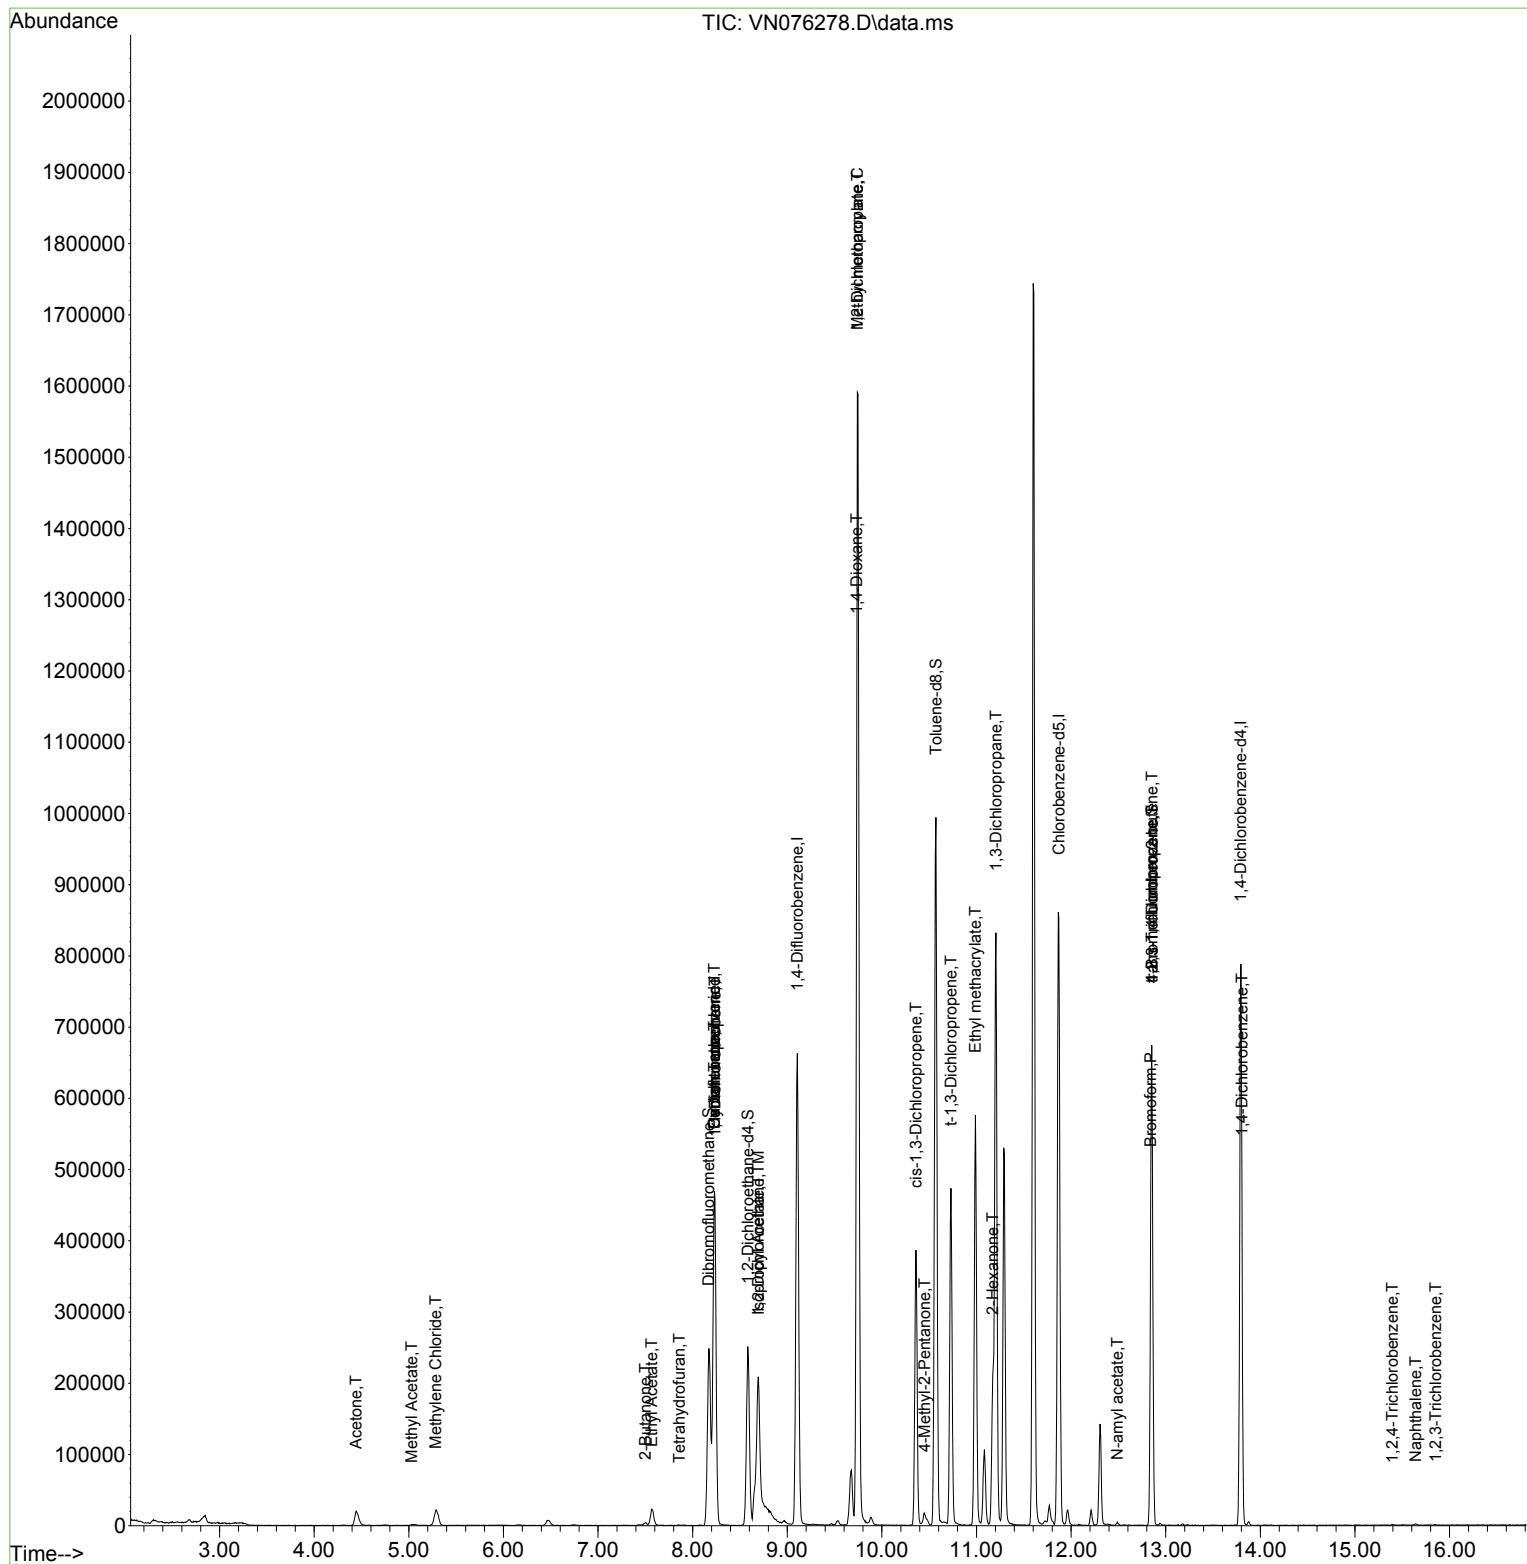




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 1050
Delta R.T. -0.001 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24




Instrument :
MSVOA_N
ClientSampleId :
PB150289ZHE#03


Tgt Ion:168 Resp: 368528
Ion Ratio Lower Upper
168 100
99 56.5 41.6 62.4

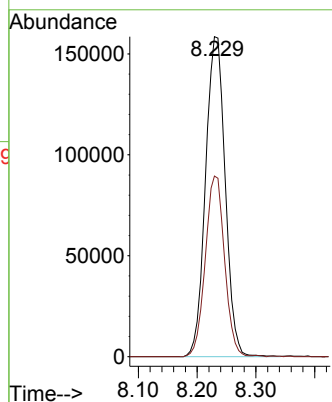

#16
Acetone
Concen: 29.557 ug/l
RT: 4.441 min Scan# 406
Delta R.T. -0.001 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24

Tgt Ion: 43 Resp: 39183
Ion Ratio Lower Upper
43 100
58 34.0 26.7 40.1


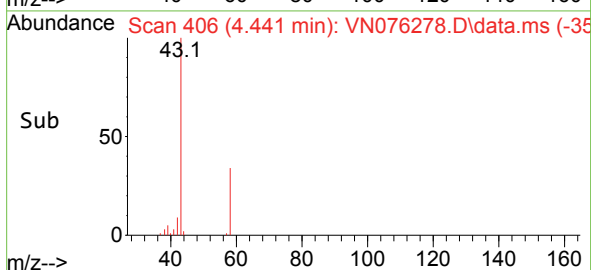






#18
Methyl Acetate
Concen: 0.291 ug/l
RT: 5.030 min Scan# 507
Delta R.T. -0.006 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24




Instrument :
MSVOA_N
ClientSampleId :
PB150289ZHE#03


Tgt Ion: 43 Resp: 1304
Ion Ratio Lower Upper
43 100
74 0.0 23.3 34.9#

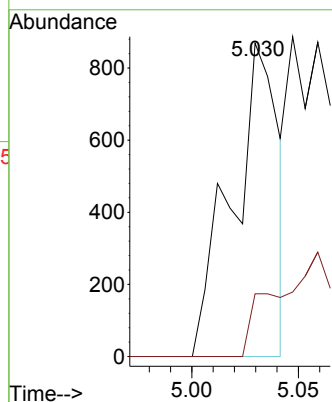

#20
Methylene Chloride
Concen: 4.288 ug/l
RT: 5.283 min Scan# 549
Delta R.T. -0.006 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24

Tgt Ion: 84 Resp: 18939
Ion Ratio Lower Upper
84 100
49 103.6 84.5 126.7
51 23.3 26.0 39.0#
86 61.8 52.0 78.0


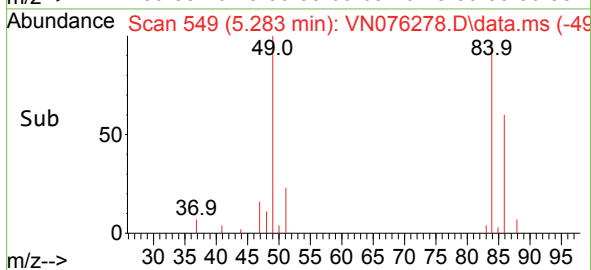




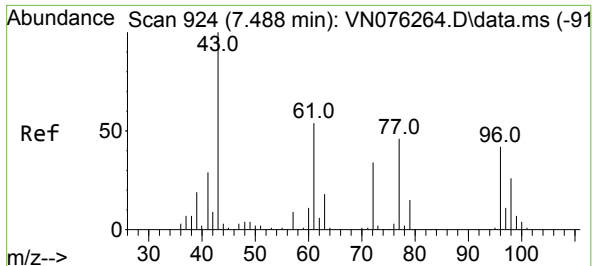

#25
2-Butanone
Concen: 2.797 ug/l
RT: 7.500 min Scan# 91
Delta R.T. 0.012 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24




Instrument :
MSVOA_N
ClientSampleId :
PB150289ZHE#03


Tgt Ion: 43 Resp: 5650
Ion Ratio Lower Upper
43 100
72 31.6 27.4 41.2

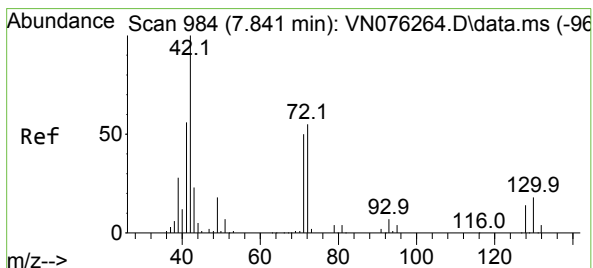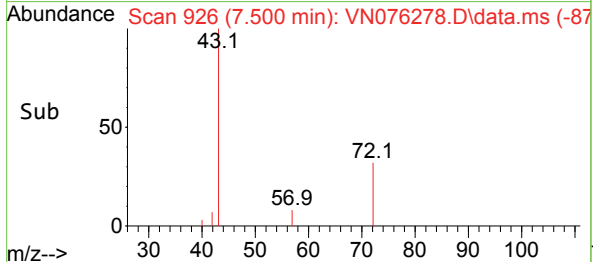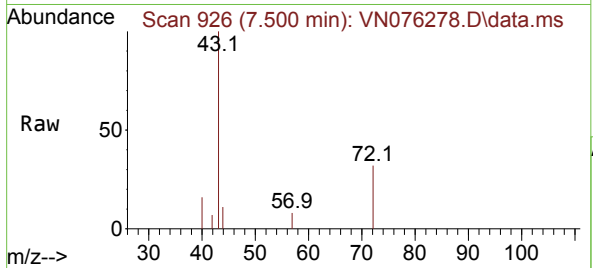

#29
Tetrahydrofuran
Concen: 0.384 ug/l
RT: 7.859 min Scan# 987
Delta R.T. 0.018 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24


Tgt Ion: 42 Resp: 479
Ion Ratio Lower Upper
42 100
72 24.2 44.0 66.0#
71 12.5 41.1 61.7#

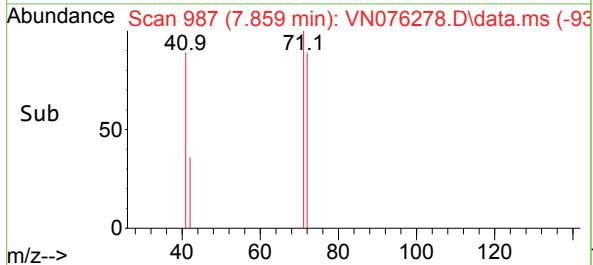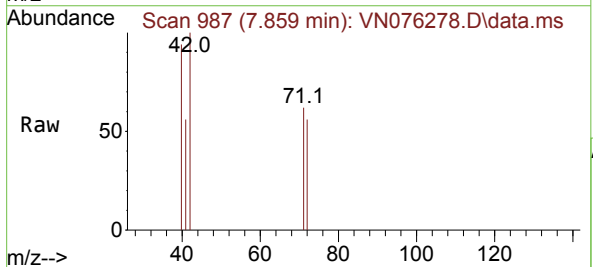






#31
Cyclohexane
Concen: 1.124 ug/l
RT: 8.229 min Scan# 1050
Delta R.T. -0.030 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24

Instrument :
MSVOA_N
ClientSampleId :
PB150289ZHE#03







Tgt Ion: 56 Resp: 7125
Ion Ratio Lower Upper
56 100
69 156.3 25.8 38.8#
84 177.1 79.0 118.4#



#33
1,2-Dichloroethane-d4
Concen: 48.519 ug/l
RT: 8.582 min Scan# 1110
Delta R.T. 0.000 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24

Tgt Ion: 65 Resp: 200206
Ion Ratio Lower Upper
65 100
67 51.3 0.0 104.6





#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. -0.000 min

Lab File: VN076278.D

Acq: 17 Jan 2023 14:24

Instrument :

MSVOA_N

ClientSampleId :

PB150289ZHE#03





Tgt Ion:114 Resp: 597891

Ion Ratio Lower Upper

114 100

63 18.1 0.0 35.8

88 15.0 0.0 28.0

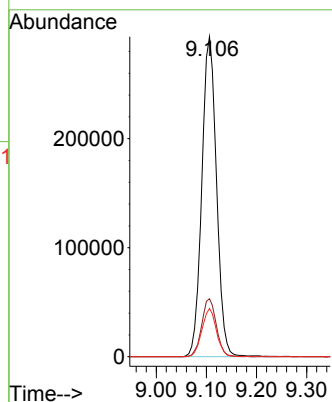

#35

Dibromofluoromethane

Concen: 47.459 ug/l

RT: 8.171 min Scan# 1040

Delta R.T. -0.000 min

Lab File: VN076278.D

Acq: 17 Jan 2023 14:24




Tgt Ion:113 Resp: 177499


Ion Ratio Lower Upper

113 100

111 102.7 82.7 124.1

192 20.3 15.6 23.4


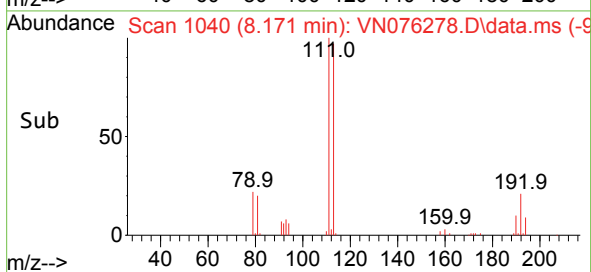
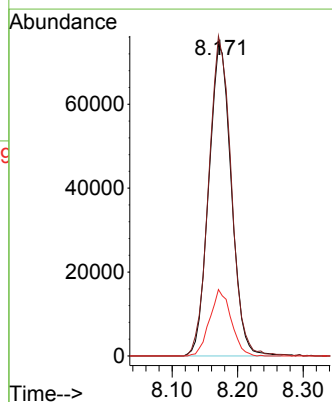





#36
1,1-Dichloropropene
Concen: 5.181 ug/l
RT: 8.235 min Scan# 1075
Delta R.T. -0.142 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24




Instrument :
MSVOA_N
ClientSampleId :
PB150289ZHE#03


Tgt Ion: 75 Resp: 27535
Ion Ratio Lower Upper
75 100
110 9.4 18.8 56.3#
77 0.0 25.0 37.4#



#37
Ethyl Acetate
Concen: 8.034 ug/l
RT: 7.565 min Scan# 937
Delta R.T. -0.000 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24

Tgt Ion: 43 Resp: 34114
Ion Ratio Lower Upper
43 100
61 16.4 11.1 16.7
70 12.6 10.0 15.0

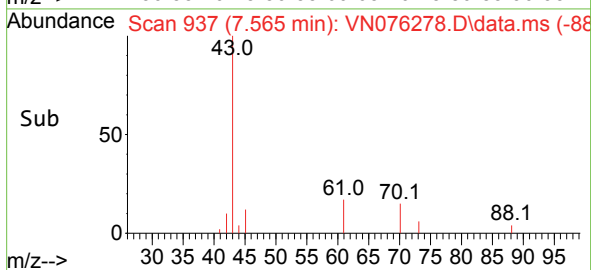



#38

Carbon Tetrachloride

Concen: 6.092 ug/l

RT: 8.229 min Scan# 1

Delta R.T. -0.136 min

Lab File: VN076278.D


Acq: 17 Jan 2023 14:24

Instrument :

MSVOA_N

ClientSampleId :

PB150289ZHE#03

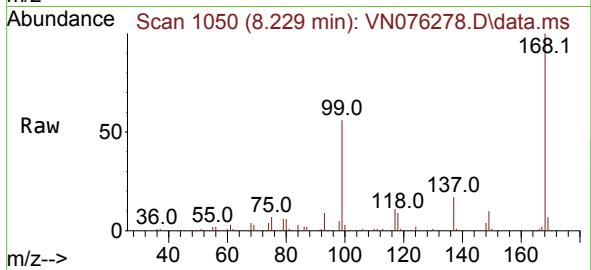




Tgt Ion:117 Resp: 36107

Ion Ratio Lower Upper

117 100

119 5.7 75.4 113.0#

121 0.0 24.2 36.2#

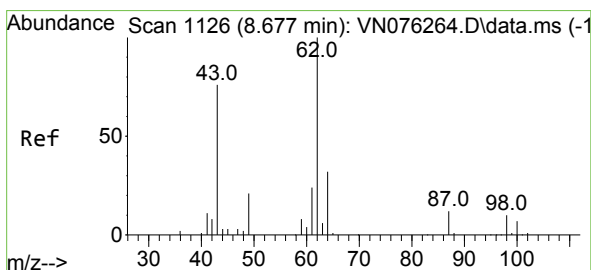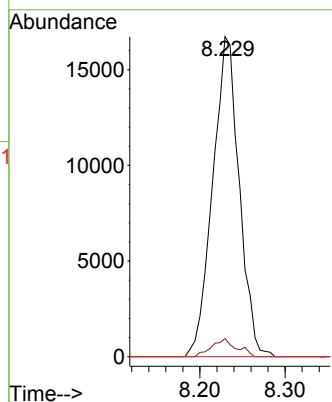

#42

1,2-Dichloroethane

Concen: 0.283 ug/l

RT: 8.694 min Scan# 1129

Delta R.T. 0.017 min

Lab File: VN076278.D




Acq: 17 Jan 2023 14:24


Tgt Ion: 62 Resp: 1538

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.4



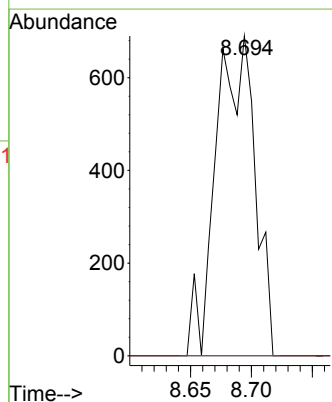





#43
Isopropyl Acetate
Concen: 39.937 ug/l
RT: 8.694 min Scan# 1129
Delta R.T. 0.000 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24




Instrument :
MSVOA_N
ClientSampleId :
PB150289ZHE#03


Tgt Ion: 43 Resp: 276952
Ion Ratio Lower Upper
43 100
61 14.1 23.5 35.3#
87 10.5 13.8 20.6#

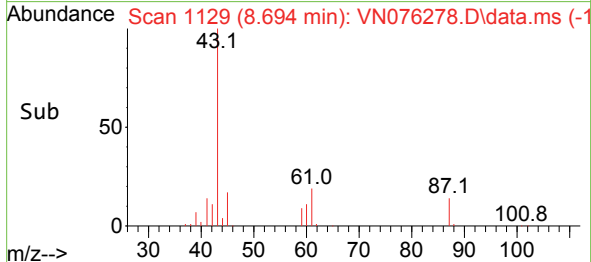

#45
1,2-Dichloropropane
Concen: 0.665 ug/l
RT: 9.741 min Scan# 1307
Delta R.T. 0.117 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24

Tgt Ion: 63 Resp: 2529
Ion Ratio Lower Upper
63 100
65 0.0 26.4 39.6#




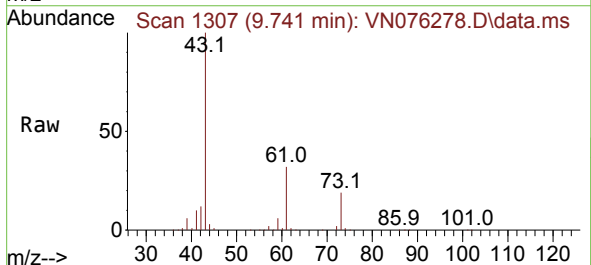




#48
Methyl methacrylate
Concen: 44.268 ug/l
RT: 9.741 min Scan# 11
Delta R.T. 0.059 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24




Instrument :
MSVOA_N
ClientSampleId :
PB150289ZHE#03


Tgt Ion: 41 Resp: 145331
Ion Ratio Lower Upper
41 100
69 0.2 80.8 121.2#
39 57.3 54.4 81.6



#49
1,4-Dioxane
Concen: 1.992 ug/l
RT: 9.735 min Scan# 1306
Delta R.T. 0.035 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24

Tgt Ion: 88 Resp: 138
Ion Ratio Lower Upper
88 100
43 1073249.3 18.1 27.1#
58 5287.7 46.5 69.7#









#50
Toluene-d8
Concen: 50.786 ug/l
RT: 10.570 min Scan# 1448
Delta R.T. -0.001 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24




Instrument :
MSVOA_N
ClientSampleId :
PB150289ZHE#03


Tgt Ion: 98 Resp: 701476
Ion Ratio Lower Upper
98 100
100 64.8 52.2 78.4

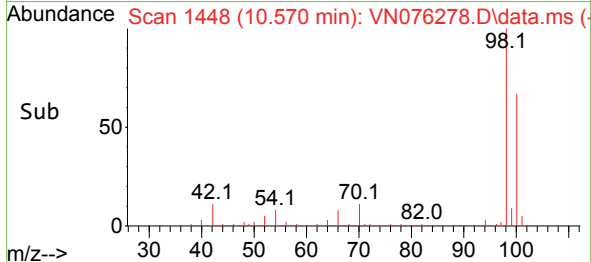

#51
4-Methyl-2-Pentanone
Concen: 3.689 ug/l
RT: 10.453 min Scan# 1428
Delta R.T. 0.006 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24

Tgt Ion: 43 Resp: 15018
Ion Ratio Lower Upper
43 100
58 27.5 35.1 52.7#


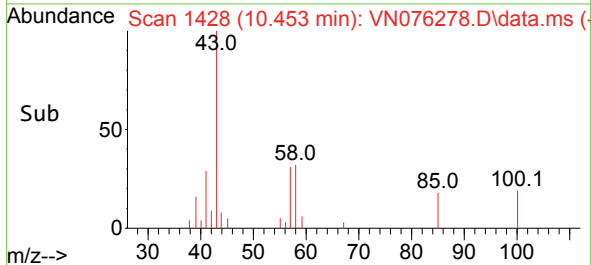






#53
 t-1,3-Dichloropropene
 Concen: 0.260 ug/l
 RT: 10.729 min Scan# 1412
 Delta R.T. -0.106 min
 Lab File: VN076278.D
 Acq: 17 Jan 2023 14:24




Instrument :
 MSVOA_N
 ClientSampleId :
 PB150289ZHE#03


Tgt Ion: 75 Resp: 1383
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.8 38.6#



#54
 cis-1,3-Dichloropropene
 Concen: 12.358 ug/l
 RT: 10.359 min Scan# 1412
 Delta R.T. 0.047 min
 Lab File: VN076278.D
 Acq: 17 Jan 2023 14:24

Tgt Ion: 75 Resp: 75513
 Ion Ratio Lower Upper
 75 100
 77 0.4 26.5 39.7#
 39 29.7 37.1 55.7#


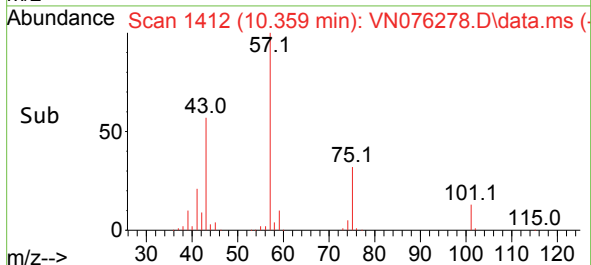
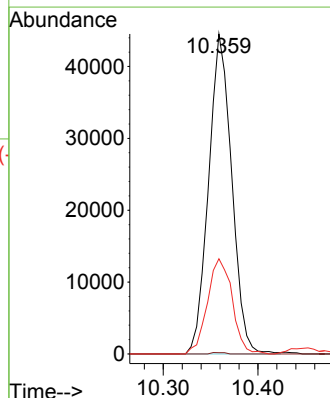





#56
Ethyl methacrylate
Concen: 0.313 ug/l
RT: 10.988 min Scan# 1519
Delta R.T. 0.112 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24




Instrument :
MSVOA_N
ClientSampleId :
PB150289ZHE#03


Tgt Ion: 69 Resp: 1639
Ion Ratio Lower Upper
69 100
41 6352.1 45.3 67.9#
39 2983.2 29.3 43.9#

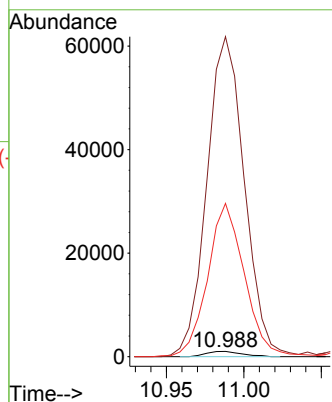

#57
1,3-Dichloropropane
Concen: 1.451 ug/l
RT: 11.206 min Scan# 1556
Delta R.T. 0.041 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24

Tgt Ion: 76 Resp: 9577
Ion Ratio Lower Upper
76 100
78 0.0 26.4 39.6#









#59
2-Hexanone
Concen: 50.902 ug/l
RT: 11.170 min Scan# 1115
Delta R.T. -0.024 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24




Instrument :
MSVOA_N
ClientSampleId :
PB150289ZHE#03


Tgt Ion: 43 Resp: 150161
Ion Ratio Lower Upper
43 100
58 0.0 30.1 90.3#



#62
4-Bromofluorobenzene
Concen: 49.147 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24

Tgt Ion: 95 Resp: 221612
Ion Ratio Lower Upper
95 100
174 85.8 0.0 174.6
176 82.4 0.0 167.8

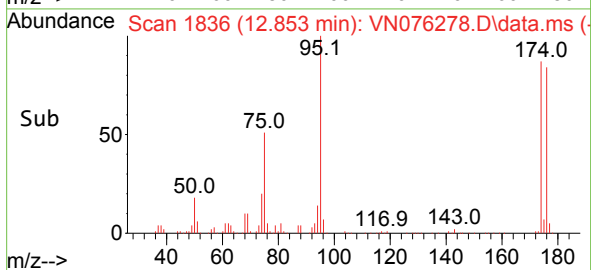



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.870 min Scan# 1

Delta R.T. 0.005 min

Lab File: VN076278.D

Acq: 17 Jan 2023 14:24

Instrument :

MSVOA_N

ClientSampleId :

PB150289ZHE#03





Tgt Ion:117 Resp: 535345

Ion Ratio Lower Upper

117 100

82 52.0 42.2 63.2

119 32.2 26.9 40.3

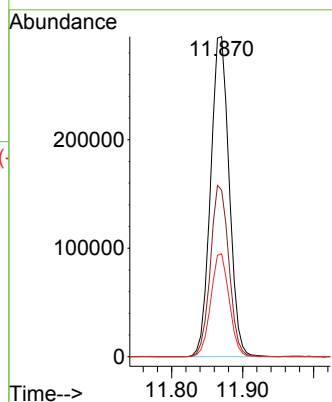

#71

Bromoform

Concen: 0.523 ug/l

RT: 12.841 min Scan# 1834

Delta R.T. 0.259 min

Lab File: VN076278.D

Acq: 17 Jan 2023 14:24




Tgt Ion:173 Resp: 1591


Ion Ratio Lower Upper

173 100

175 731.4 24.1 72.4#

254 0.0 0.0 0.0


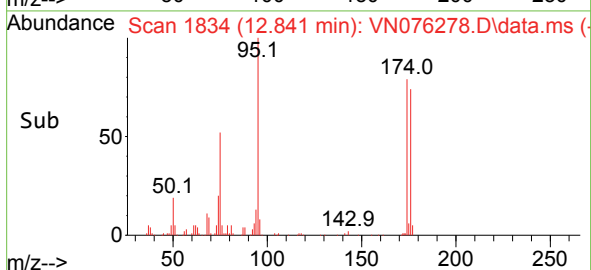




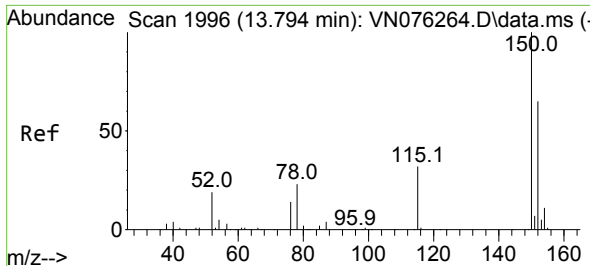

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24




Instrument :
MSVOA_N
ClientSampleId :
PB150289ZHE#03


Tgt Ion:152 Resp: 220848
Ion Ratio Lower Upper
152 100
115 57.4 29.6 88.9
150 155.6 0.0 351.4

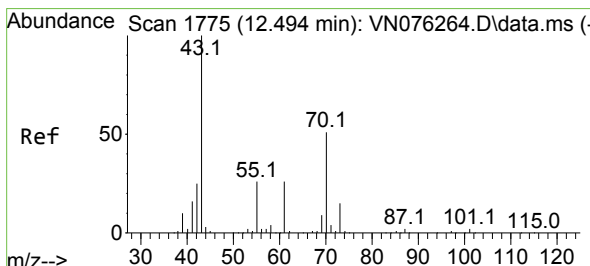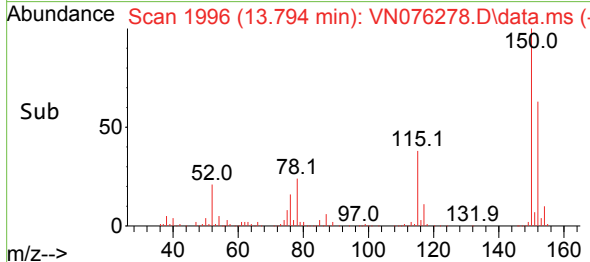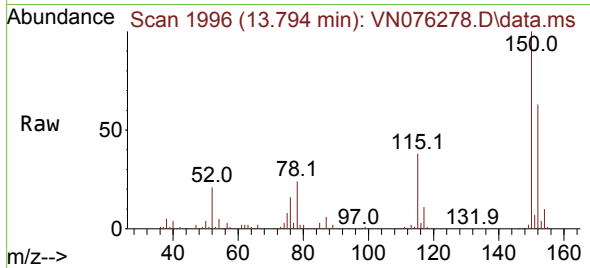

#74
N-ethyl acetate
Concen: 0.360 ug/l
RT: 12.488 min Scan# 1774
Delta R.T. -0.006 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24

Tgt Ion: 43 Resp: 1767
Ion Ratio Lower Upper
43 100
70 0.0 41.2 61.8#
55 0.0 21.0 31.6#
61 0.0 21.6 32.4#


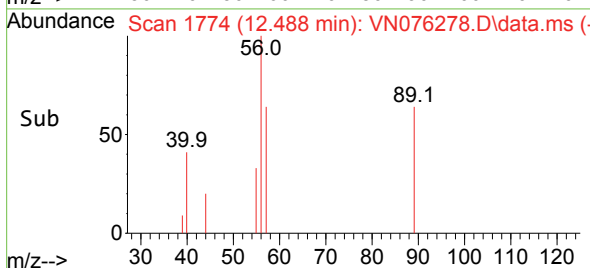
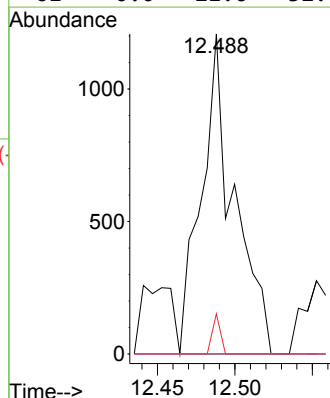
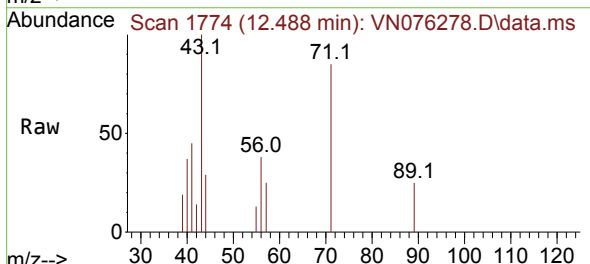




#76
1,2,3-Trichloropropane
Concen: 28.329 ug/l
RT: 12.853 min Scan# 11
Delta R.T. -0.141 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24




Instrument :
MSVOA_N
ClientSampleId :
PB150289ZHE#03


Tgt Ion: 75 Resp: 115630
Ion Ratio Lower Upper
75 100
77 1.2 75.2 225.6#



#77
Bromobenzene
Concen: Below Cal
RT: 12.976 min Scan# 1857
Delta R.T. -0.006 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24

Tgt Ion:156 Resp: 63
Ion Ratio Lower Upper
156 100
77 234.9 93.4 280.2
158 122.2 48.4 145.2


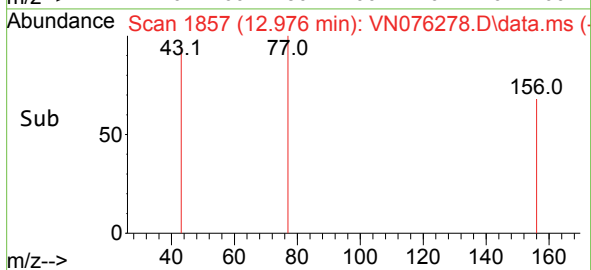






#81
trans-1,4-Dichloro-2-butene
Concen: 87.114 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.118 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24




Instrument :
MSVOA_N
ClientSampleId :
PB150289ZHE#03


Tgt Ion: 75 Resp: 115630
Ion Ratio Lower Upper
75 100
53 0.0 75.8 113.8#
89 0.0 37.0 55.6#

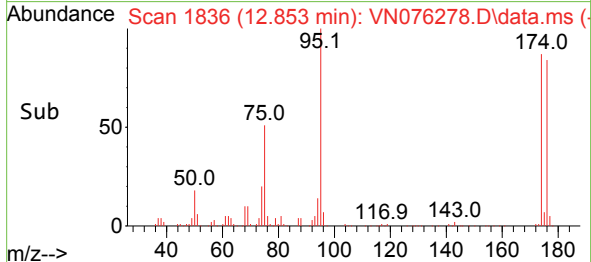

#88
1,4-Dichlorobenzene
Concen: 0.211 ug/l
RT: 13.806 min Scan# 1998
Delta R.T. -0.006 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24

Tgt Ion:146 Resp: 842
Ion Ratio Lower Upper
146 100
111 0.0 19.1 57.5#
148 65.8 31.9 95.9




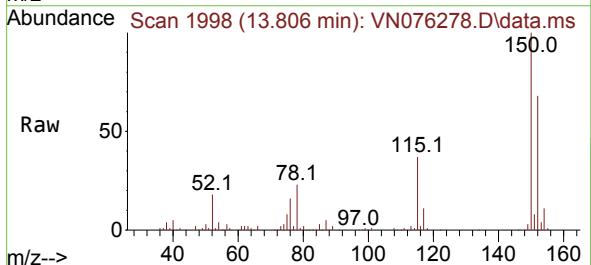




#93
1,2,4-Trichlorobenzene
Concen: 1.420 ug/l
RT: 15.394 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24




Instrument :
MSVOA_N
ClientSampleId :
PB150289ZHE#03


Tgt Ion:180 Resp: 456
Ion Ratio Lower Upper
180 100
182 57.9 47.0 141.2
145 13.4 15.2 45.5#

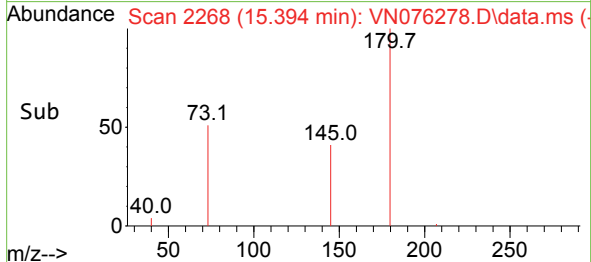

#95
Naphthalene
Concen: 2.046 ug/l
RT: 15.641 min Scan# 2310
Delta R.T. -0.000 min
Lab File: VN076278.D
Acq: 17 Jan 2023 14:24

Tgt Ion:128 Resp: 2465
Ion Ratio Lower Upper
128 100
127 9.2 10.3 15.5#
129 2.3 8.6 13.0#





#96

1,2,3-Trichlorobenzene

Concen: 1.237 ug/l

RT: 15.853 min Scan# 21

Delta R.T. 0.012 min

Lab File: VN076278.D


Acq: 17 Jan 2023 14:24

Instrument :

MSVOA_N

ClientSampleId :

PB150289ZHE#03

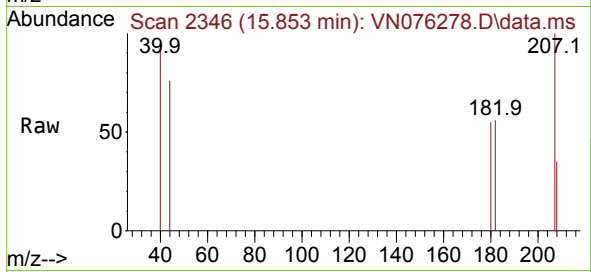

Tgt Ion:180 Resp: 316

Ion Ratio Lower Upper

180 100

182 101.6 47.5 142.5

145 0.0 15.9 47.6#

