
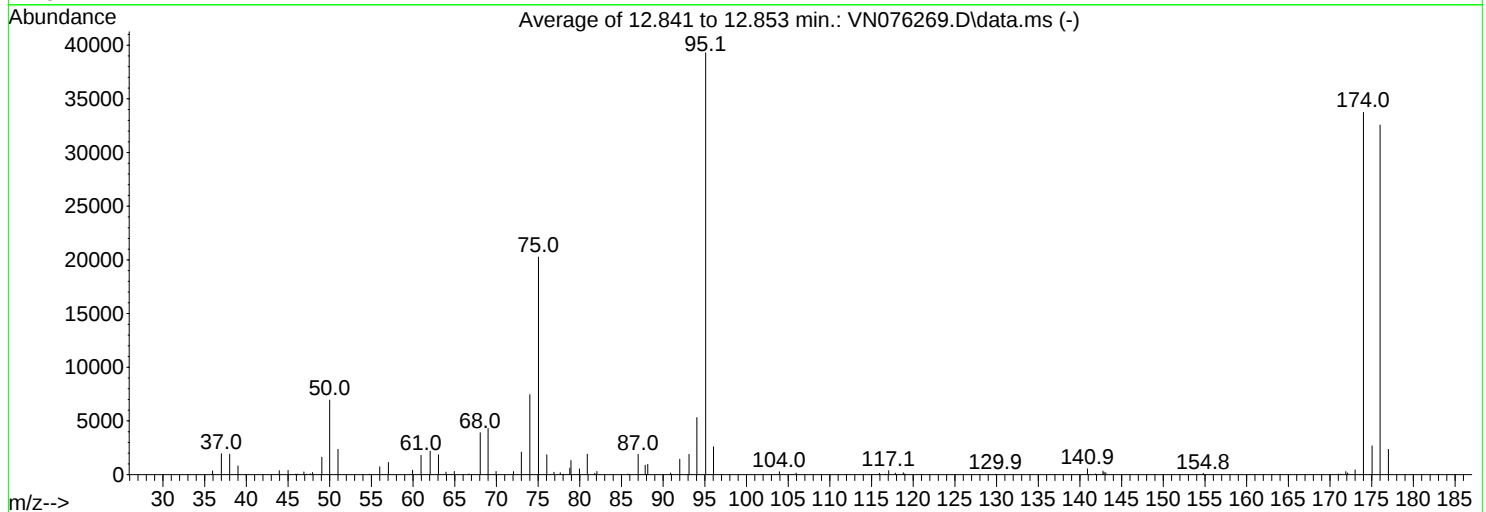


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011723\
Data File : VN076269.D
Acq On : 17 Jan 2023 08:38
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Title : SW846 8260
Last Update : Tue Jan 17 03:59:22 2023

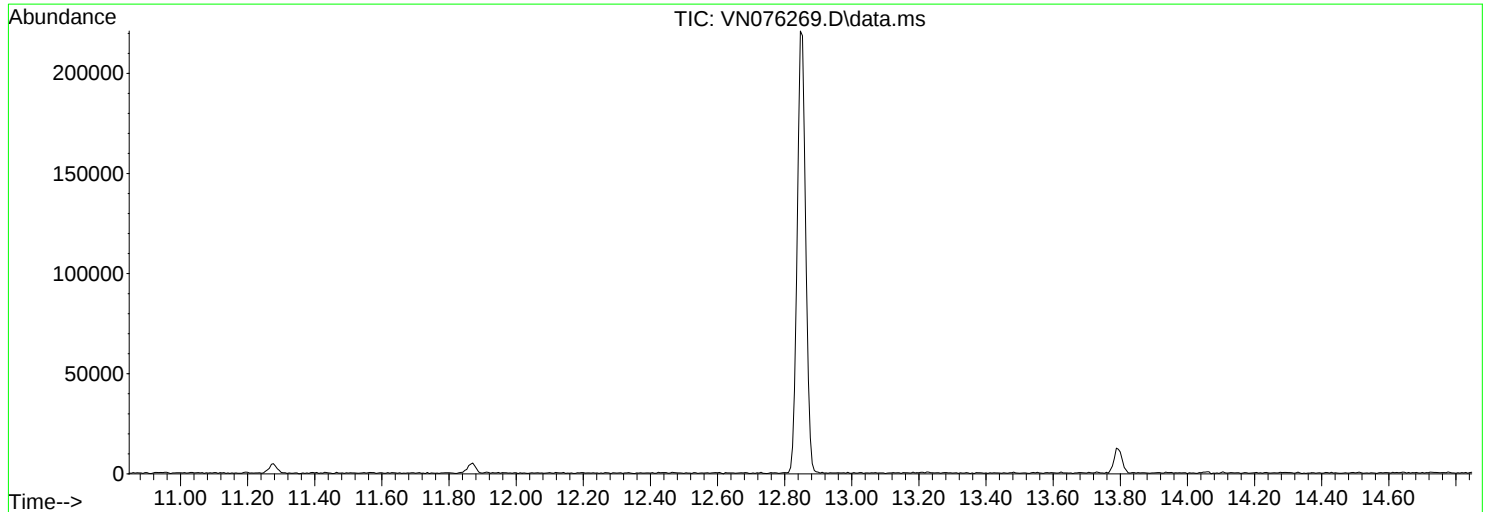

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1826

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.7	6944	PASS
75	95	30	60	51.6	20267	PASS
95	95	100	100	100.0	39285	PASS
96	95	5	9	6.6	2597	PASS
173	174	0.00	2	1.3	453	PASS
174	95	50	100	85.9	33744	PASS
175	174	5	9	8.0	2683	PASS
176	174	95	101	96.5	32557	PASS
177	176	5	9	7.2	2358	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	348	47.70	77	63.05	1843	76.05	1851
37.00	1954	47.95	198	63.95	233	76.90	221
38.00	1905	49.05	1618	64.95	298	77.65	181
39.00	817	50.00	6944	66.70	58	78.00	51
39.90	34	51.00	2355	68.05	3910	78.80	610
43.95	371	54.80	51	69.00	4305	78.95	1308
45.00	404	56.00	729	69.95	305	79.95	533
45.90	53	57.05	1139	72.05	282	80.90	1914
46.10	62	59.95	422	73.00	2107	81.80	124
46.90	261	60.95	1809	74.00	7459	82.05	297
47.20	51	62.05	2190	75.05	20267	85.80	56

Average of 12.841 to 12.853 min.: VN076269.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.00	1892	115.95	114	143.10	187		
87.85	885	116.70	53	154.80	117		
88.15	948	117.05	374	171.00	57		
90.90	144	117.85	154	171.30	52		
92.00	1436	118.80	175	171.90	285		
93.10	1889	119.00	82	172.10	151		
94.05	5316	129.90	51	173.00	453		
95.10	39285	140.90	543	174.00	33744		
96.05	2597	141.90	69	175.05	2683		
103.95	268	142.75	331	176.00	32557		
105.95	153	142.90	218	177.00	2358		

Instrument :

MSVOA_N

ClientSampleId :

BFB