

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN011725\  
 Data File : VN085491.D  
 Acq On : 17 Jan 2025 14:24  
 Operator : JC\MD  
 Sample : PB166090ZHE#03  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :

Quant Time: Jan 17 22:35:37 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N011425W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Jan 15 02:16:08 2025  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 8.224  | 168  | 187273   | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 9.100  | 114  | 365406   | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.865 | 117  | 324540   | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.788 | 152  | 121820   | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |          |
|-----------------------------|--------|-------|----------|----------|------|----------|
| System Monitoring Compounds |        |       |          |          |      |          |
| 33) 1,2-Dichloroethane-d4   | 8.577  | 65    | 166868   | 55.200   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 74 - 125 | Recovery | =    | 110.400% |
| 35) Dibromofluoromethane    | 8.165  | 113   | 121903   | 48.088   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 75 - 124 | Recovery | =    | 96.180%  |
| 50) Toluene-d8              | 10.565 | 98    | 452140   | 50.199   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 86 - 113 | Recovery | =    | 100.400% |
| 62) 4-Bromofluorobenzene    | 12.847 | 95    | 140205   | 45.506   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 77 - 121 | Recovery | =    | 91.020%  |


| Target Compounds              |        |     |        |         | Qvalue |    |
|-------------------------------|--------|-----|--------|---------|--------|----|
| 3) Chloromethane              | 2.359  | 50  | 745    | 0.271   | ug/l # | 41 |
| 11) Tert butyl alcohol        | 5.524  | 59  | 896    | 2.588   | ug/l # | 71 |
| 16) Acetone                   | 4.430  | 43  | 116318 | 119.087 | ug/l   | 97 |
| 18) Methyl Acetate            | 5.018  | 43  | 3073   | 1.035   | ug/l # | 62 |
| 20) Methylene Chloride        | 5.277  | 84  | 2450   | 1.013   | ug/l   | 95 |
| 23) Vinyl Acetate             | 6.453  | 43  | 1197   | 0.236   | ug/l # | 72 |
| 25) 2-Butanone                | 7.482  | 43  | 11282  | 7.849   | ug/l   | 96 |
| 30) Chloroform                | 7.971  | 83  | 3644   | 0.799   | ug/l # | 66 |
| 31) Cyclohexane               | 8.218  | 56  | 5188   | 1.352   | ug/l # | 16 |
| 36) 1,1-Dichloropropene       | 8.218  | 75  | 17779  | 4.997   | ug/l # | 51 |
| 37) Ethyl Acetate             | 7.565  | 43  | 4249   | 1.183   | ug/l # | 77 |
| 38) Carbon Tetrachloride      | 8.224  | 117 | 21400  | 5.254   | ug/l # | 16 |
| 42) 1,2-Dichloroethane        | 8.677  | 62  | 1003   | 0.249   | ug/l # | 76 |
| 43) Isopropyl Acetate         | 8.682  | 43  | 222983 | 38.751  | ug/l # | 79 |
| 48) Methyl methacrylate       | 9.735  | 41  | 141135 | 54.502  | ug/l # | 46 |
| 51) 4-Methyl-2-Pentanone      | 10.441 | 43  | 15071  | 4.513   | ug/l # | 78 |
| 53) t-1,3-Dichloropropene     | 10.718 | 75  | 884    | 0.233   | ug/l # | 88 |
| 54) cis-1,3-Dichloropropene   | 10.353 | 75  | 44737  | 11.041  | ug/l # | 68 |
| 56) Ethyl methacrylate        | 10.823 | 69  | 75     | 1.949   | ug/l # | 23 |
| 57) 1,3-Dichloropropane       | 11.200 | 76  | 6655   | 1.561   | ug/l # | 43 |
| 59) 2-Hexanone                | 11.200 | 43  | 84180  | 35.829  | ug/l # | 59 |
| 71) Bromoform                 | 12.841 | 173 | 817    | 0.438   | ug/l # | 1  |
| 74) N-amyl acetate            | 12.465 | 43  | 1908   | 0.516   | ug/l # | 48 |
| 76) 1,2,3-Trichloropropane    | 12.847 | 75  | 77838  | 31.437  | ug/l # | 1  |
| 81) trans-1,4-Dichloro-2-b... | 12.847 | 75  | 77838  | 85.054  | ug/l # | 3  |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN011725\  
Data File : VN085491.D  
Acq On : 17 Jan 2025 14:24  
Operator : JC\MD  
Sample : PB166090ZHE#03  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :


Quant Time: Jan 17 22:35:37 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N011425W.M  
Quant Title : SW846 8260  
QLast Update : Wed Jan 15 02:16:08 2025  
Response via : Initial Calibration

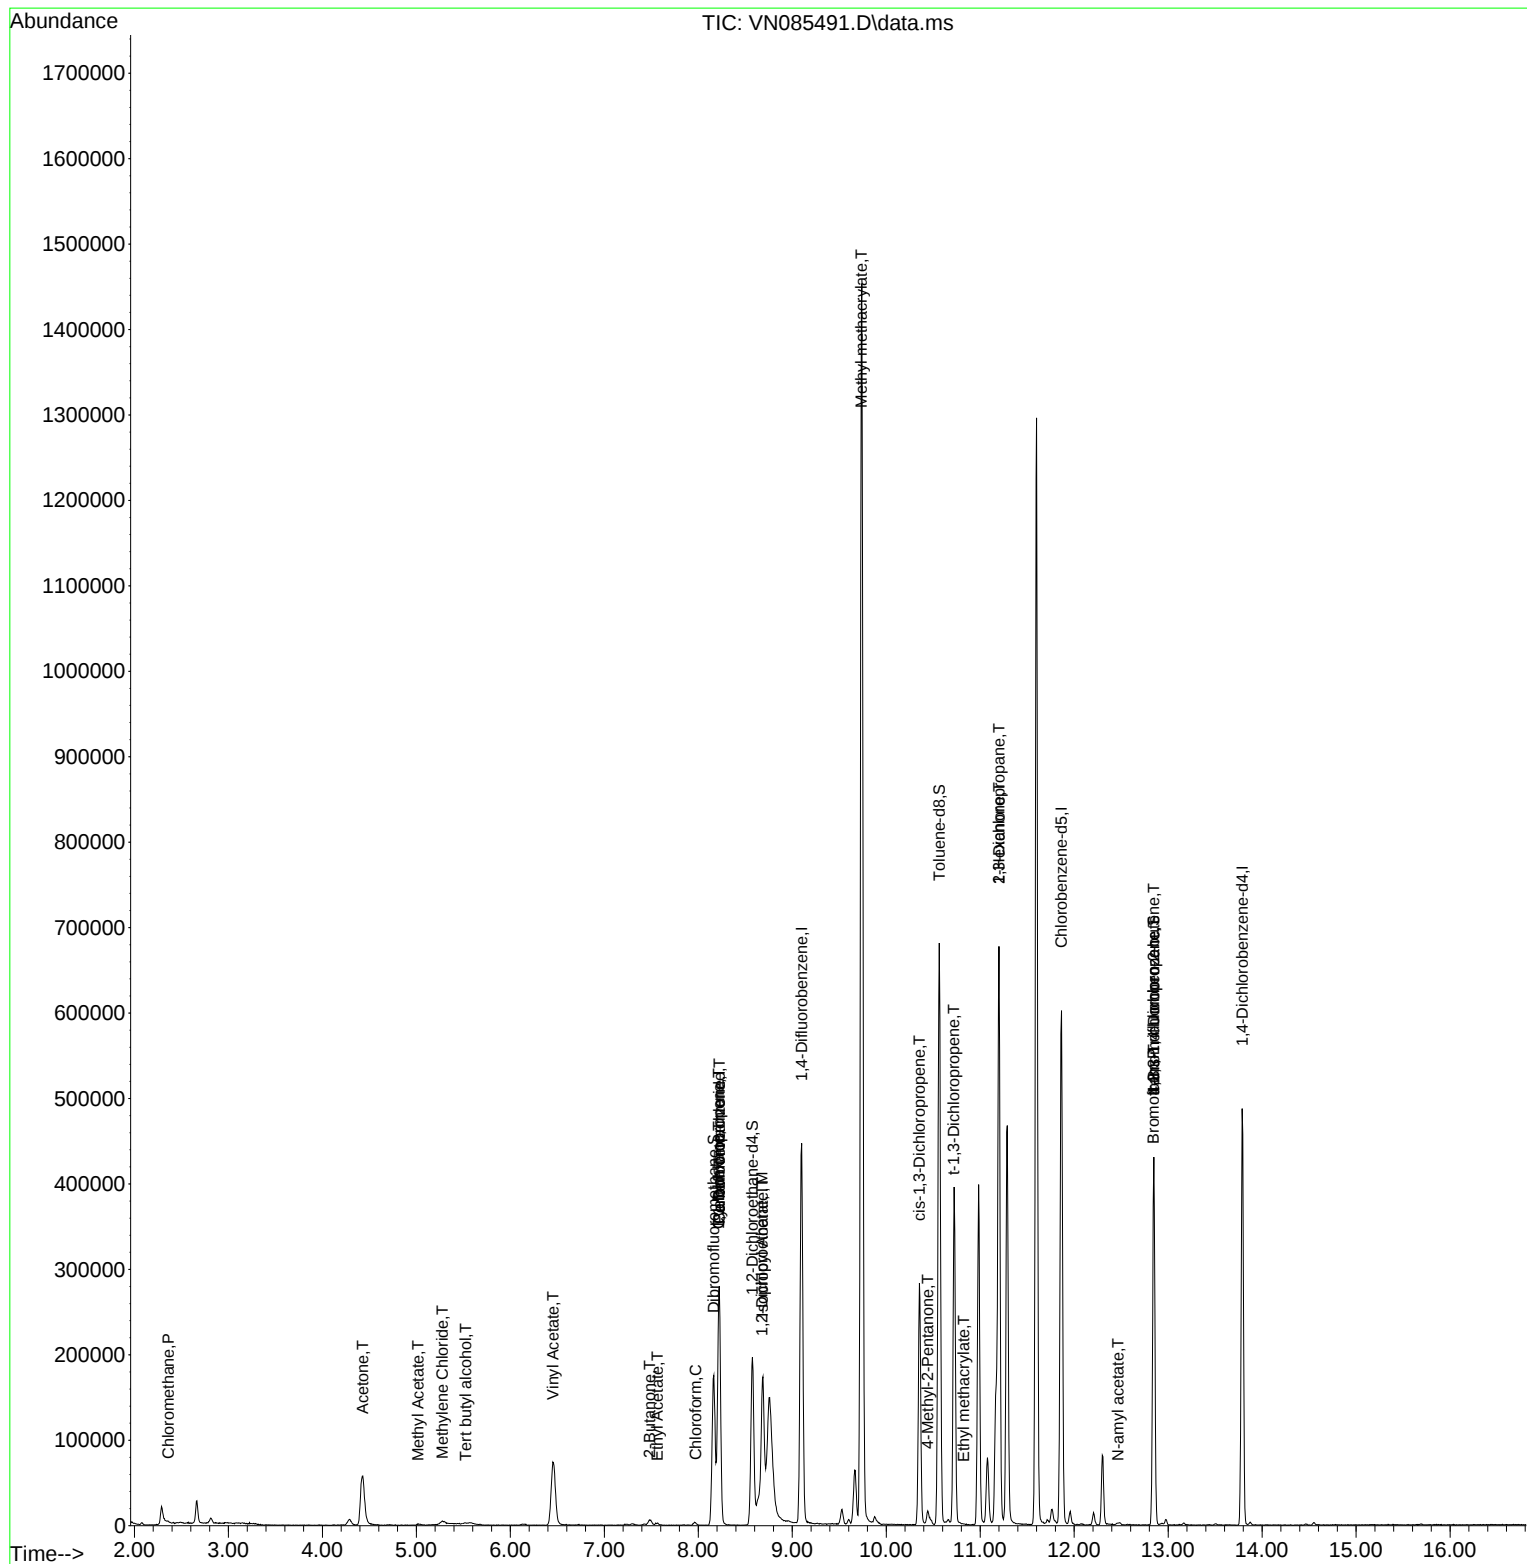






#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 8.224 min Scan# 1066  
Delta R.T. 0.006 min  
Lab File: VN085491.D  
Acq: 17 Jan 2025 14:24

Instrument :  
MSVOA\_N  
ClientSampleId :



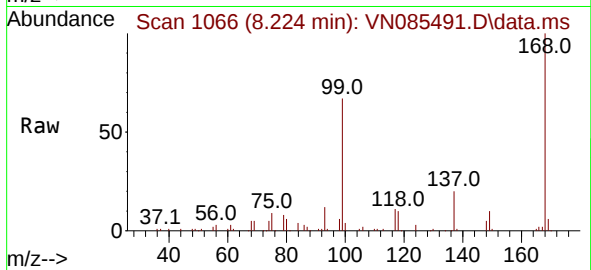


Tgt Ion:168 Resp: 187273  
Ion Ratio Lower Upper  
168 100  
99 67.5 53.6 80.4

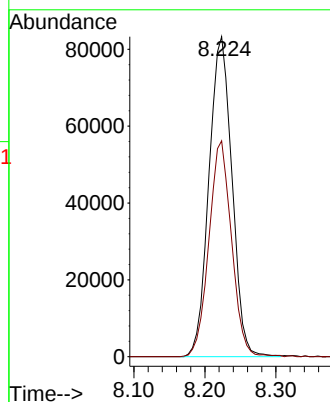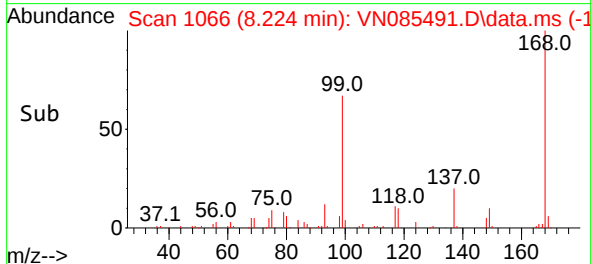

#3  
Chloromethane  
Concen: 0.271 ug/l  
RT: 2.359 min Scan# 69  
Delta R.T. -0.000 min  
Lab File: VN085491.D  
Acq: 17 Jan 2025 14:24


Tgt Ion: 50 Resp: 745  
Ion Ratio Lower Upper  
50 100  
52 0.0 27.0 40.6#

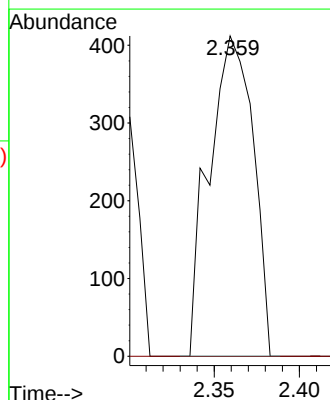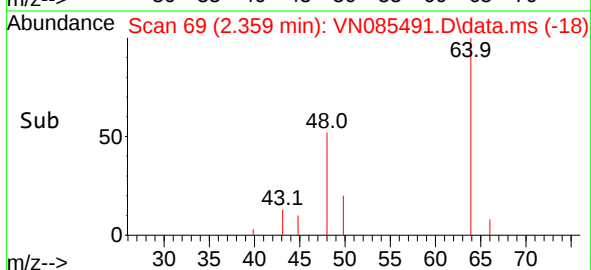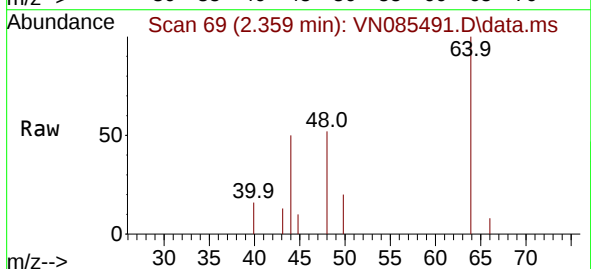






#11  
Tert butyl alcohol  
Concen: 2.588 ug/l  
RT: 5.524 min Scan# 605  
Delta R.T. 0.012 min  
Lab File: VN085491.D  
Acq: 17 Jan 2025 14:24

Instrument :  
MSVOA\_N  
ClientSampleId :






Tgt Ion: 59 Resp: 896  
Ion Ratio Lower Upper  
59 100  
57 0.0 8.6 13.0#

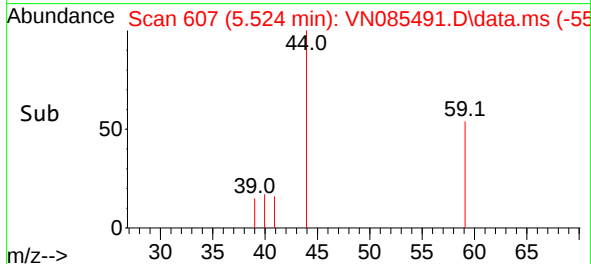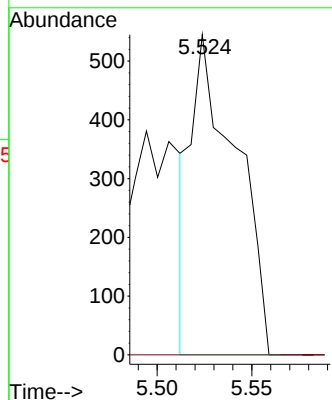

#16  
Acetone  
Concen: 119.087 ug/l  
RT: 4.430 min Scan# 421  
Delta R.T. 0.012 min  
Lab File: VN085491.D  
Acq: 17 Jan 2025 14:24


Tgt Ion: 43 Resp: 116318  
Ion Ratio Lower Upper  
43 100  
58 31.1 23.8 35.6

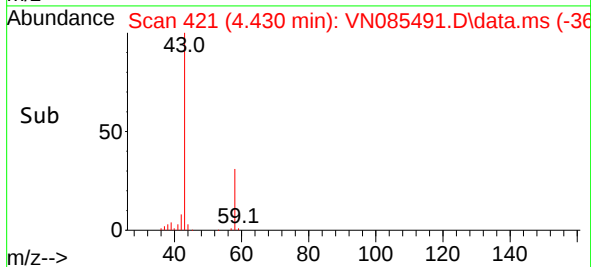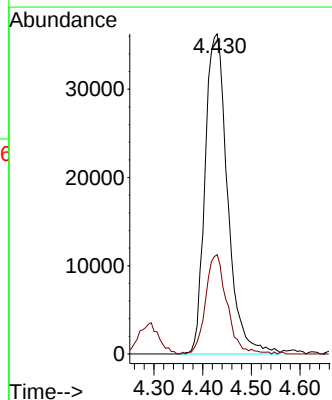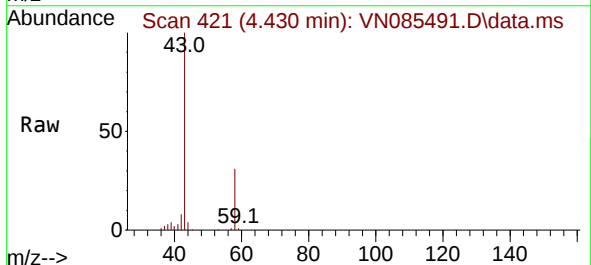






#18  
Methyl Acetate  
Concen: 1.035 ug/l  
RT: 5.018 min Scan# 51  
Delta R.T. -0.000 min  
Lab File: VN085491.D  
Acq: 17 Jan 2025 14:24


Instrument :  
MSVOA\_N  
ClientSampleId :





Tgt Ion: 43 Resp: 3073  
Ion Ratio Lower Upper  
43 100  
74 4.8 18.6 28.0#

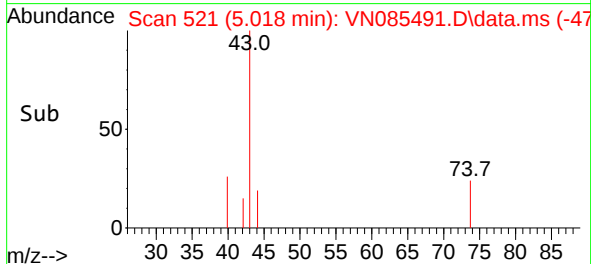


#20  
Methylene Chloride  
Concen: 1.013 ug/l  
RT: 5.277 min Scan# 565  
Delta R.T. 0.006 min  
Lab File: VN085491.D  
Acq: 17 Jan 2025 14:24

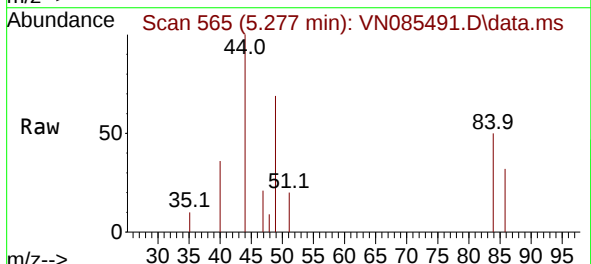

Tgt Ion: 84 Resp: 2450  
Ion Ratio Lower Upper  
84 100  
49 139.9 104.1 156.1  
51 40.9 31.0 46.4  
86 64.7 51.9 77.9



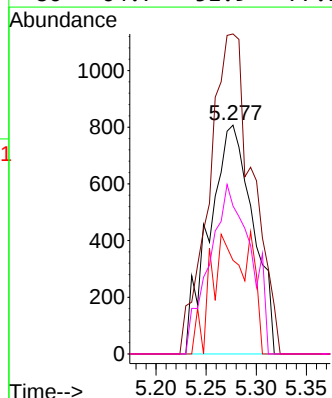





#23  
 Vinyl Acetate  
 Concen: 0.236 ug/l  
 RT: 6.453 min Scan# 71  
 Delta R.T. -0.141 min  
 Lab File: VN085491.D  
 Acq: 17 Jan 2025 14:24




Instrument :  
 MSVOA\_N  
 ClientSampleId :


Tgt Ion: 43 Resp: 1197  
 Ion Ratio Lower Upper  
 43 100  
 86 0.0 8.4 12.6#

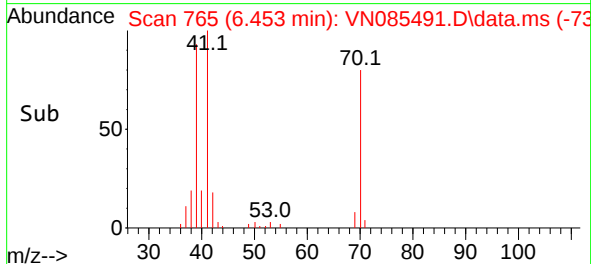

#25  
 2-Butanone  
 Concen: 7.849 ug/l  
 RT: 7.482 min Scan# 940  
 Delta R.T. 0.006 min  
 Lab File: VN085491.D  
 Acq: 17 Jan 2025 14:24

Tgt Ion: 43 Resp: 11282  
 Ion Ratio Lower Upper  
 43 100  
 72 23.5 20.2 30.4

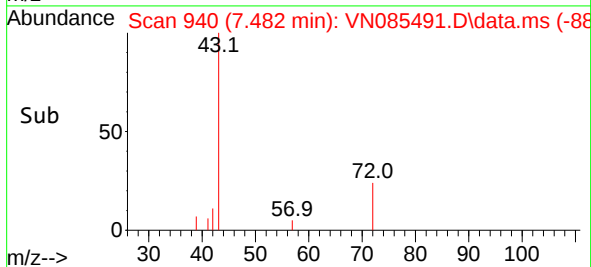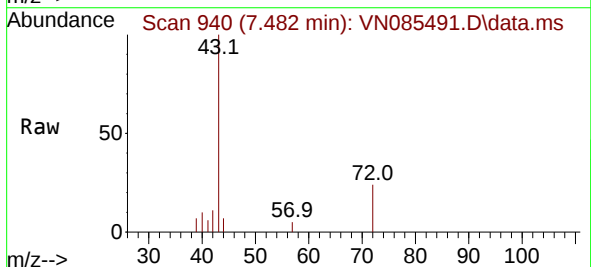



#30

Chloroform

Concen: 0.799 ug/l

RT: 7.971 min Scan# 10

Delta R.T. 0.012 min

Lab File: VN085491.D

Acq: 17 Jan 2025 14:24

Instrument :

MSVOA\_N





ClientSampleId :

Tgt Ion: 83 Resp: 3644

Ion Ratio Lower Upper

83 100

85 38.1 51.8 77.6#

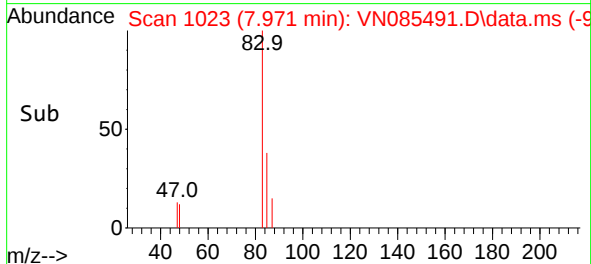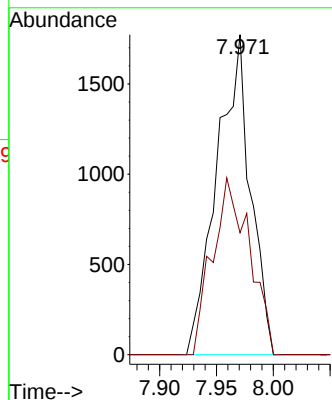

#31

Cyclohexane

Concen: 1.352 ug/l

RT: 8.218 min Scan# 1065

Delta R.T. -0.035 min

Lab File: VN085491.D

Acq: 17 Jan 2025 14:24




Tgt Ion: 56 Resp: 5188


Ion Ratio Lower Upper

56 100

69 161.8 22.2 33.4#

84 106.8 66.4 99.6#

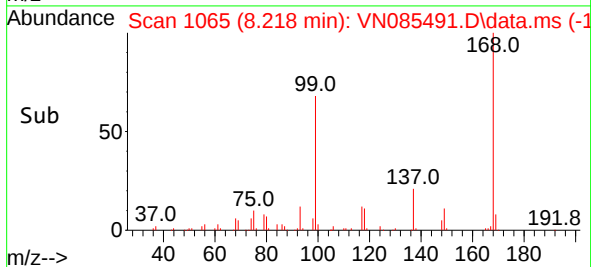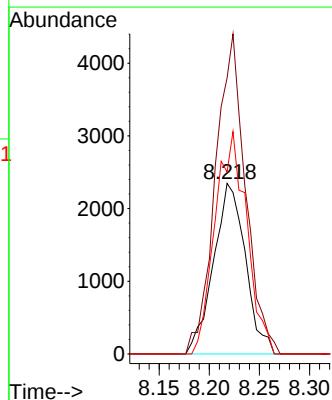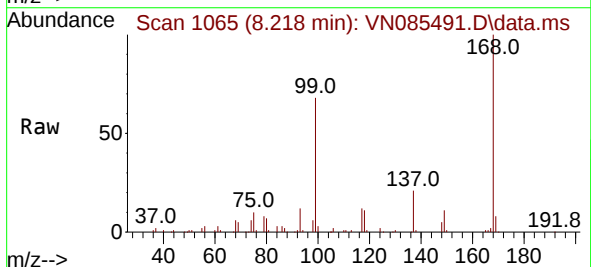

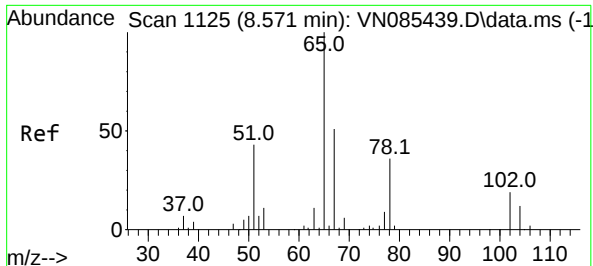

#33

1,2-Dichloroethane-d4

Concen: 55.200 ug/l

RT: 8.577 min Scan# 1125

Delta R.T. 0.006 min

Lab File: VN085491.D

Acq: 17 Jan 2025 14:24

Instrument :

MSVOA\_N





ClientSampleId :

Tgt Ion: 65 Resp: 166868

Ion Ratio Lower Upper

65 100

67 49.9 0.0 101.6

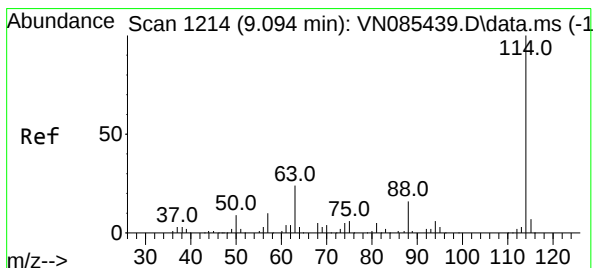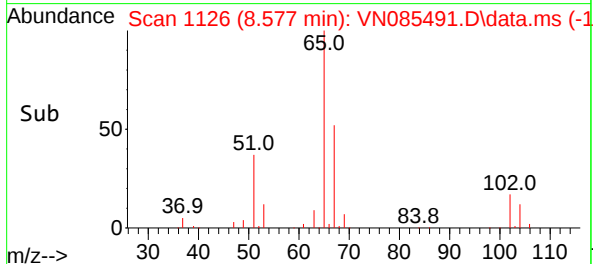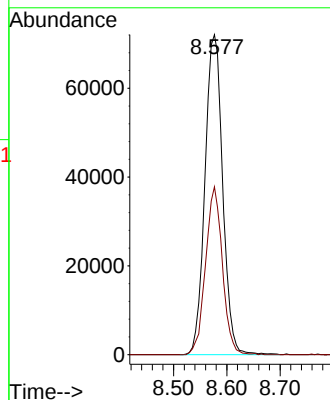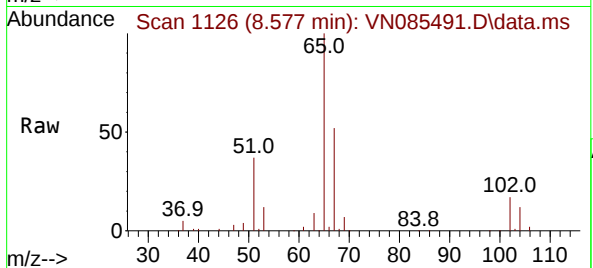

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1215

Delta R.T. 0.006 min

Lab File: VN085491.D

Acq: 17 Jan 2025 14:24




Tgt Ion: 114 Resp: 365406


Ion Ratio Lower Upper

114 100

63 22.7 0.0 47.6

88 15.7 0.0 32.6

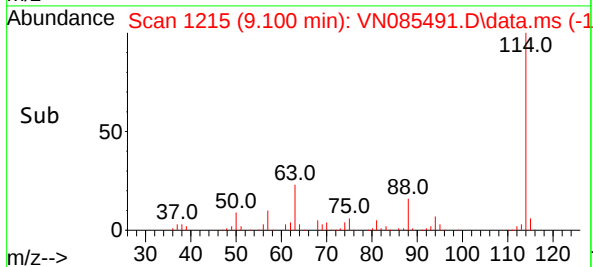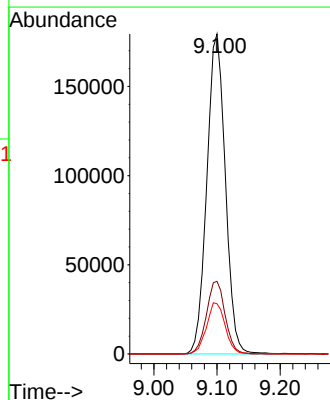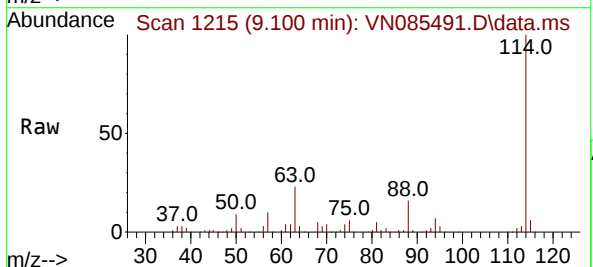

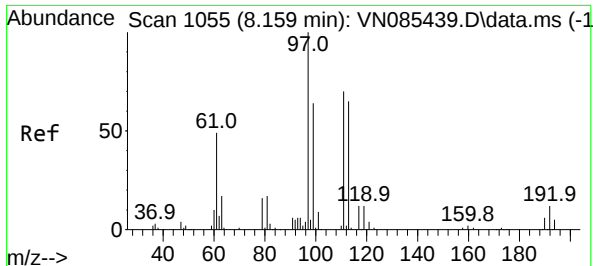

#35

Dibromofluoromethane

Concen: 48.088 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.006 min


Lab File: VN085491.D

Acq: 17 Jan 2025 14:24

Instrument :

MSVOA\_N

ClientSampleId :

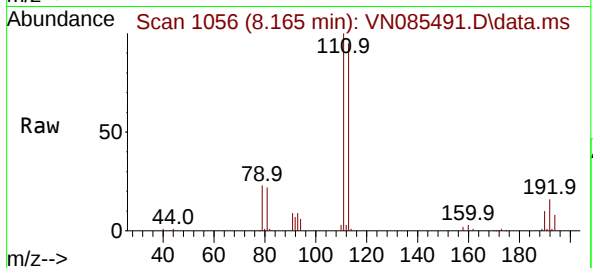




Tgt Ion:113 Resp: 121903

Ion Ratio Lower Upper

113 100

111 103.7 82.7 124.1

192 17.6 14.3 21.5

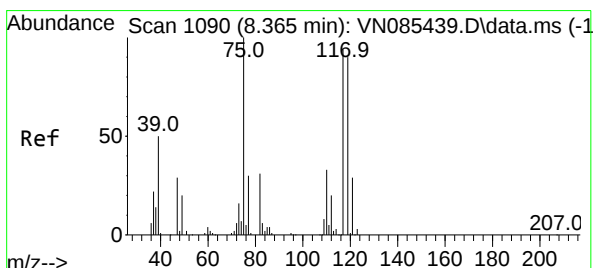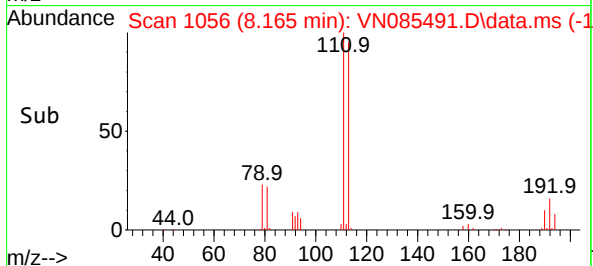

#36

1,1-Dichloropropene

Concen: 4.997 ug/l

RT: 8.218 min Scan# 1065

Delta R.T. -0.147 min

Lab File: VN085491.D

Acq: 17 Jan 2025 14:24




Tgt Ion: 75 Resp: 17779


Ion Ratio Lower Upper

75 100

110 9.1 16.5 49.5#

77 0.0 24.4 36.6#

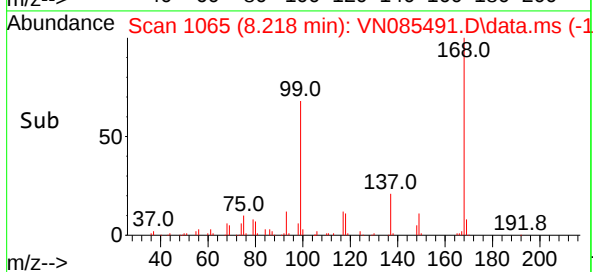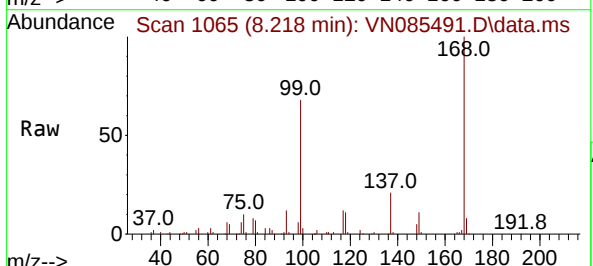



#37

Ethyl Acetate

Concen: 1.183 ug/l

RT: 7.565 min Scan# 91

Delta R.T. 0.012 min


Lab File: VN085491.D

Acq: 17 Jan 2025 14:24




Instrument :

MSVOA\_N

ClientSampleId :



|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 43    | Resp: | 4249  |
| Ion Ratio | Lower | Upper |       |
| 43        | 100   |       |       |
| 61        | 3.0   | 10.9  | 16.3# |
| 70        | 2.8   | 7.5   | 11.3# |



#38

Carbon Tetrachloride

Concen: 5.254 ug/l




RT: 8.224 min Scan# 1066


Delta R.T. -0.135 min

Lab File: VN085491.D

Acq: 17 Jan 2025 14:24

|           |       |       |        |
|-----------|-------|-------|--------|
| Tgt Ion:  | 117   | Resp: | 21400  |
| Ion Ratio | Lower | Upper |        |
| 117       | 100   |       |        |
| 119       | 4.0   | 75.4  | 113.2# |
| 121       | 0.0   | 24.6  | 37.0#  |

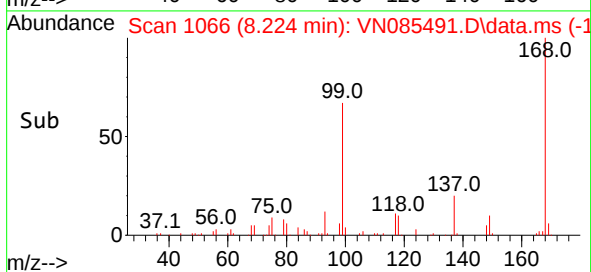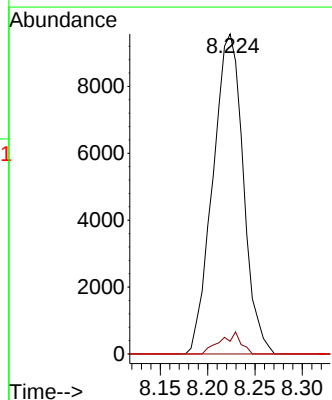

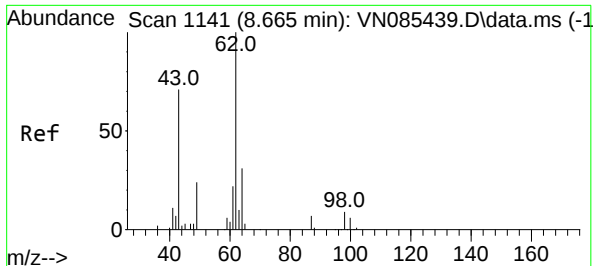

#42

1,2-Dichloroethane

Concen: 0.249 ug/l

RT: 8.677 min Scan# 1143

Delta R.T. 0.012 min

Lab File: VN085491.D

Acq: 17 Jan 2025 14:24

Instrument :

MSVOA\_N





ClientSampleId :

Tgt Ion: 62 Resp: 1003

Ion Ratio Lower Upper

62 100

98 0.0 0.0 17.0

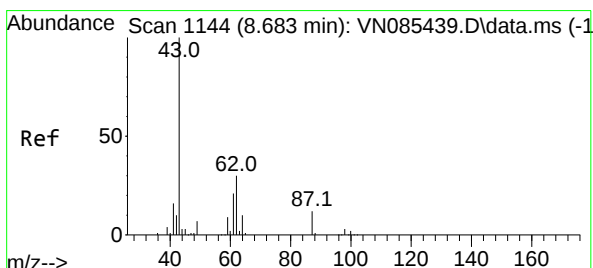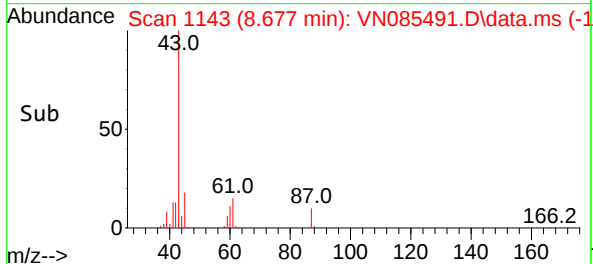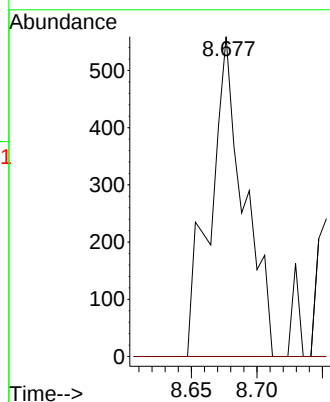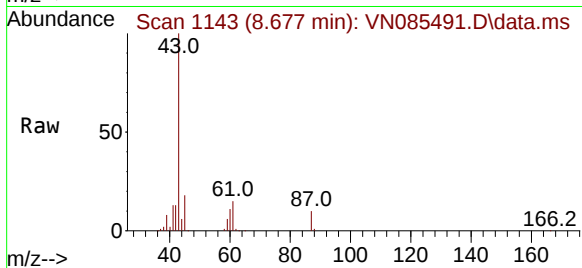

#43

Isopropyl Acetate

Concen: 38.751 ug/l

RT: 8.682 min Scan# 1144

Delta R.T. -0.000 min

Lab File: VN085491.D

Acq: 17 Jan 2025 14:24




Tgt Ion: 43 Resp: 222983


Ion Ratio Lower Upper

43 100

61 13.0 20.7 31.1#

87 8.1 9.8 14.8#

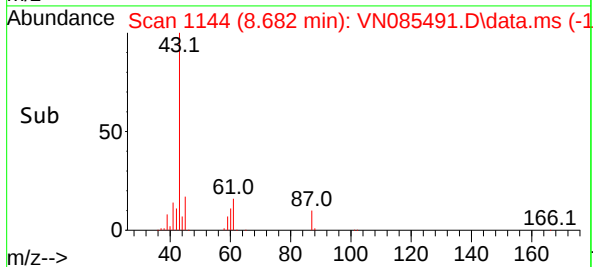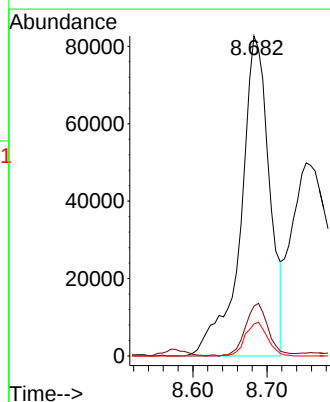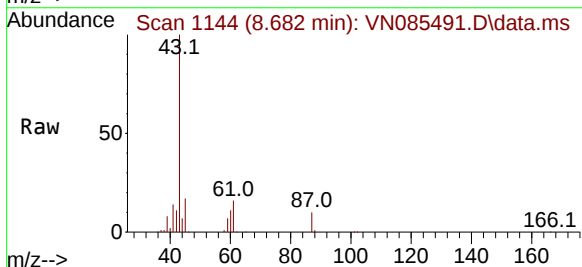

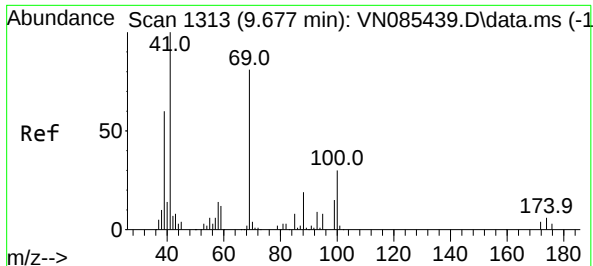

#48

Methyl methacrylate

Concen: 54.502 ug/l

RT: 9.735 min Scan# 1

Delta R.T. 0.058 min

Lab File: VN085491.D

Acq: 17 Jan 2025 14:24

Instrument :

MSVOA\_N

ClientSampleId :





Tgt Ion: 41 Resp: 141135

Ion Ratio Lower Upper

41 100

69 0.0 64.7 97.1#

39 58.1 49.0 73.6

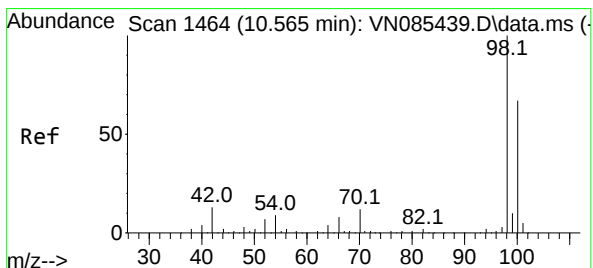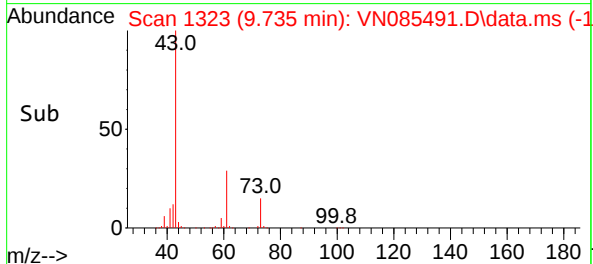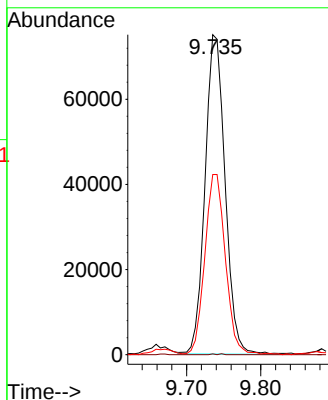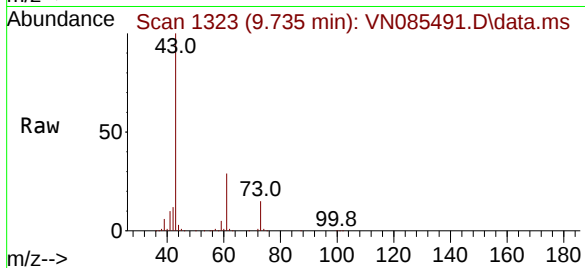

#50

Toluene-d8

Concen: 50.199 ug/l

RT: 10.565 min Scan# 1464

Delta R.T. -0.000 min

Lab File: VN085491.D




Acq: 17 Jan 2025 14:24


Tgt Ion: 98 Resp: 452140

Ion Ratio Lower Upper

98 100

100 64.9 52.2 78.4


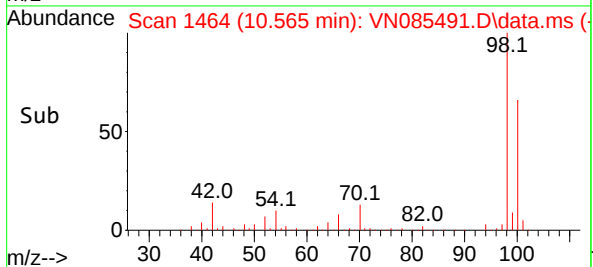
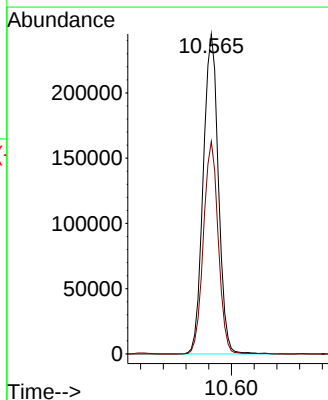
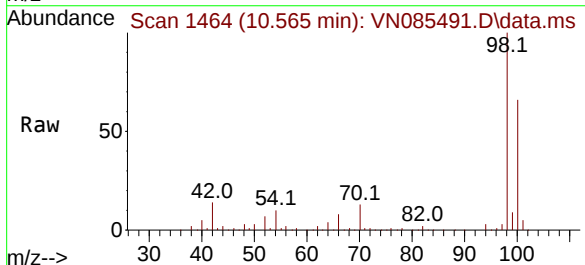




#51  
4-Methyl-2-Pentanone  
Concen: 4.513 ug/l  
RT: 10.441 min Scan# 1443  
Delta R.T. 0.000 min  
Lab File: VN085491.D  
Acq: 17 Jan 2025 14:24




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 43 Resp: 15071  
Ion Ratio Lower Upper  
43 100  
58 24.6 30.5 45.7#



#53  
t-1,3-Dichloropropene  
Concen: 0.233 ug/l  
RT: 10.718 min Scan# 1490  
Delta R.T. -0.118 min  
Lab File: VN085491.D  
Acq: 17 Jan 2025 14:24

Tgt Ion: 75 Resp: 884  
Ion Ratio Lower Upper  
75 100  
77 35.7 23.5 35.3#


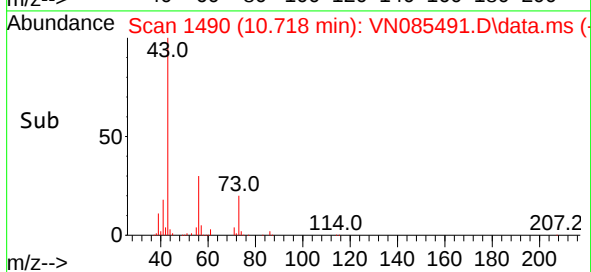

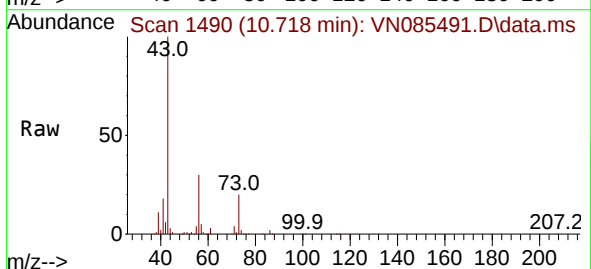




#54  
 cis-1,3-Dichloropropene  
 Concen: 11.041 ug/l  
 RT: 10.353 min Scan# 1428  
 Delta R.T. 0.047 min  
 Lab File: VN085491.D  
 Acq: 17 Jan 2025 14:24




Instrument :  
 MSVOA\_N  
 ClientSampleId :


Tgt Ion: 75 Resp: 44737  
 Ion Ratio Lower Upper  
 75 100  
 77 0.0 25.0 37.4#  
 39 41.0 43.1 64.7#

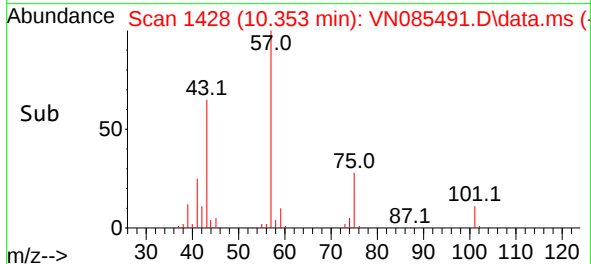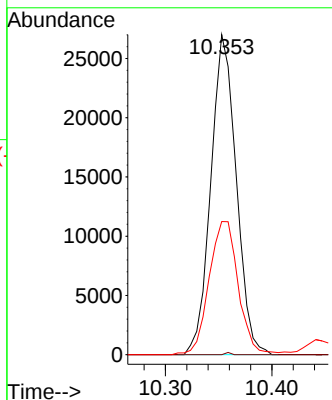

#56  
 Ethyl methacrylate  
 Concen: 1.949 ug/l  
 RT: 10.823 min Scan# 1508  
 Delta R.T. -0.048 min  
 Lab File: VN085491.D  
 Acq: 17 Jan 2025 14:24

Tgt Ion: 69 Resp: 75  
 Ion Ratio Lower Upper  
 69 100  
 41 0.0 54.6 82.0#  
 39 0.0 32.4 48.6#

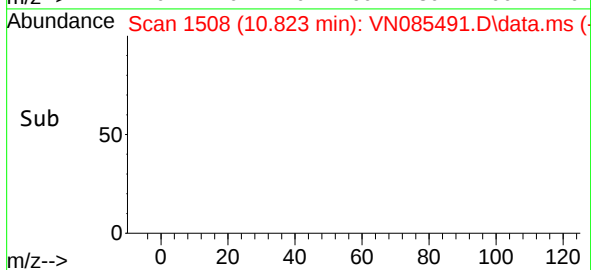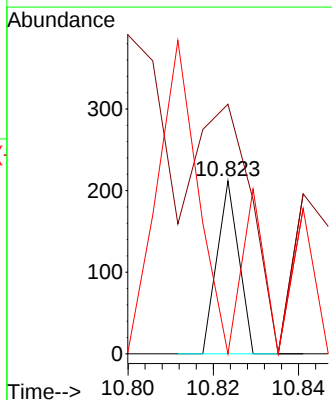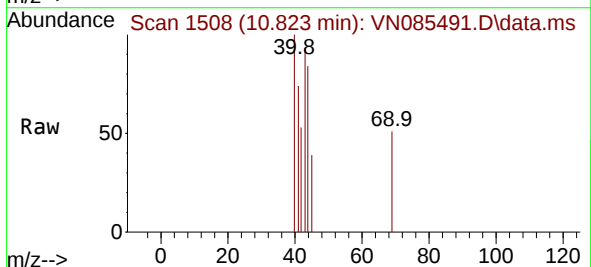



#57

1,3-Dichloropropane

Concen: 1.561 ug/l

RT: 11.200 min Scan# 1572

Delta R.T. 0.041 min


Lab File: VN085491.D

Acq: 17 Jan 2025 14:24

Instrument :

MSVOA\_N

ClientSampleId :



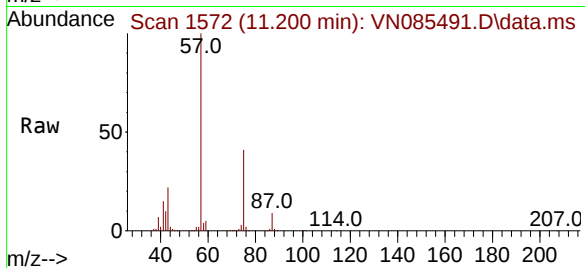


Tgt Ion: 76 Resp: 6655

Ion Ratio Lower Upper

76 100

78 0.0 25.6 38.4#

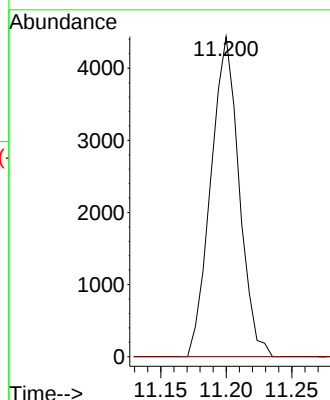

#59

2-Hexanone

Concen: 35.829 ug/l

RT: 11.200 min Scan# 1572

Delta R.T. 0.012 min

Lab File: VN085491.D




Acq: 17 Jan 2025 14:24


Tgt Ion: 43 Resp: 84180

Ion Ratio Lower Upper

43 100

58 23.8 26.2 78.6#


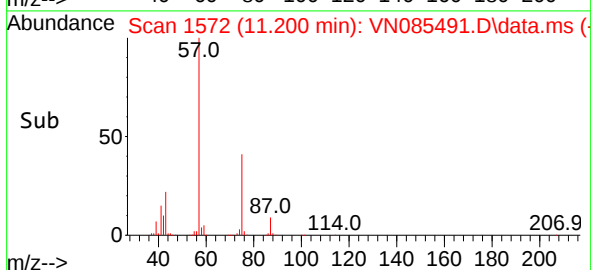
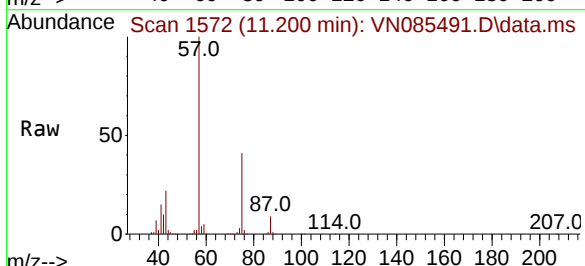
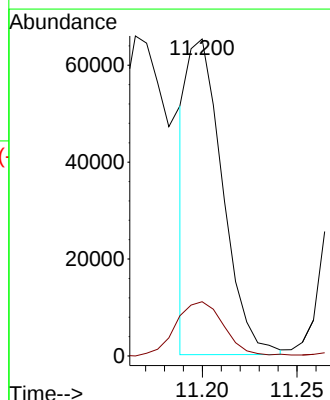




#62  
4-Bromofluorobenzene  
Concen: 45.506 ug/l  
RT: 12.847 min Scan# 1852  
Delta R.T. -0.000 min  
Lab File: VN085491.D  
Acq: 17 Jan 2025 14:24




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 95 Resp: 140205  
Ion Ratio Lower Upper  
95 100  
174 75.4 0.0 145.0  
176 70.3 0.0 142.4

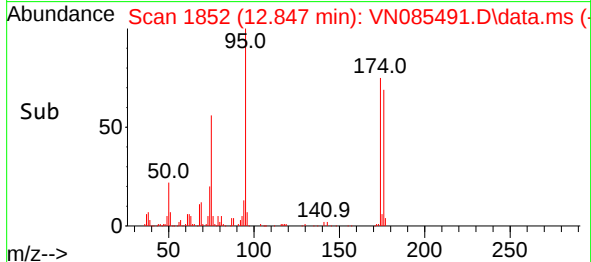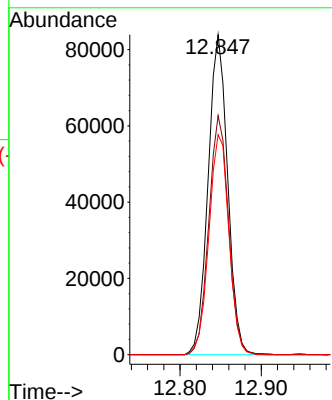

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.865 min Scan# 1685  
Delta R.T. -0.000 min  
Lab File: VN085491.D  
Acq: 17 Jan 2025 14:24

Tgt Ion: 117 Resp: 324540  
Ion Ratio Lower Upper  
117 100  
82 59.8 48.6 72.8  
119 32.6 26.6 39.8

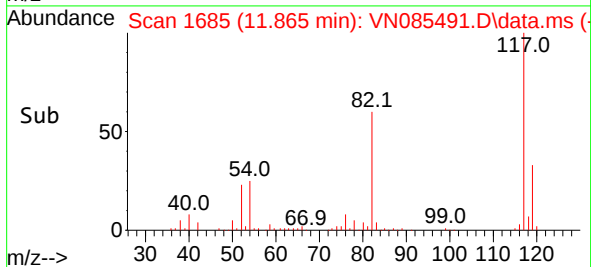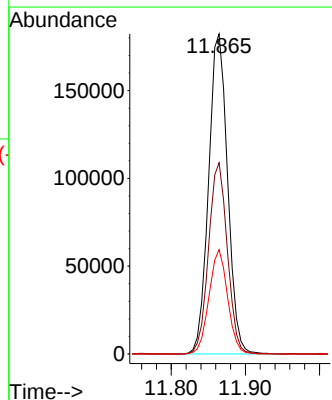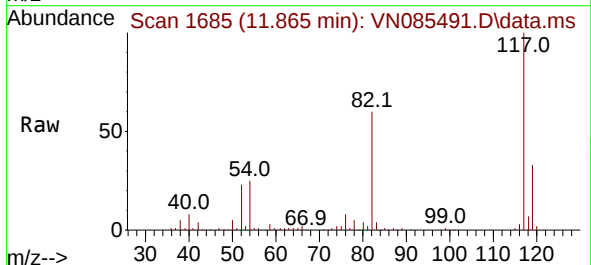



#71

Bromoform

Concen: 0.438 ug/l

RT: 12.841 min Scan# 1851

Delta R.T. 0.265 min


Lab File: VN085491.D

Acq: 17 Jan 2025 14:24




Instrument :

MSVOA\_N

ClientSampleId :

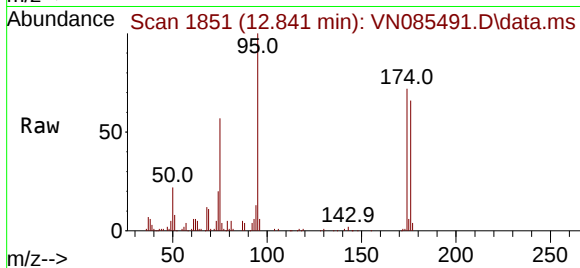

|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 173   | Resp: | 817   |
| Ion Ratio | Lower | Upper |       |
| 173       | 100   |       |       |
| 175       | 787.0 | 24.4  | 73.2# |
| 254       | 0.0   | 0.0   | 0.0   |



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l




RT: 13.788 min Scan# 2012


Delta R.T. -0.000 min

Lab File: VN085491.D

Acq: 17 Jan 2025 14:24


|           |       |       |        |
|-----------|-------|-------|--------|
| Tgt Ion:  | 152   | Resp: | 121820 |
| Ion Ratio | Lower | Upper |        |
| 152       | 100   |       |        |
| 115       | 62.6  | 31.1  | 93.3   |
| 150       | 159.3 | 0.0   | 343.6  |

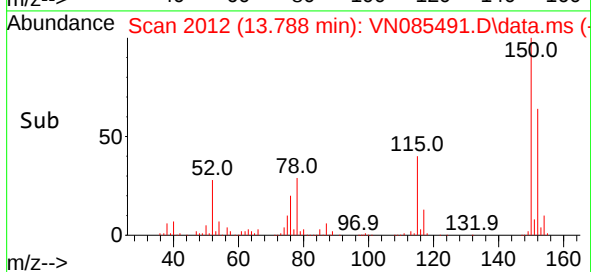






#74  
N-amy1 acetate  
Concen: 0.516 ug/l  
RT: 12.465 min Scan# 11  
Delta R.T. -0.024 min  
Lab File: VN085491.D  
Acq: 17 Jan 2025 14:24

Instrument :  
MSVOA\_N  
ClientSampleId :







Tgt Ion: 43 Resp: 1908  
Ion Ratio Lower Upper  
43 100  
70 0.0 34.0 51.0#  
55 10.8 21.4 32.2#  
61 0.0 19.0 28.4#

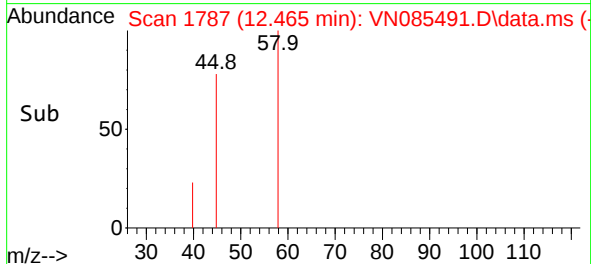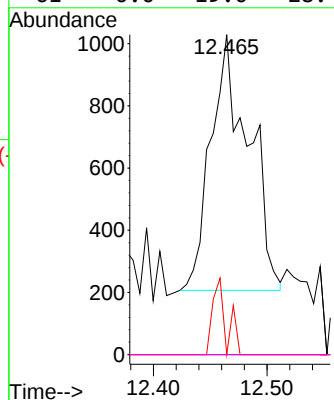

#76  
1,2,3-Trichloropropane  
Concen: 31.437 ug/l  
RT: 12.847 min Scan# 1852  
Delta R.T. -0.141 min  
Lab File: VN085491.D  
Acq: 17 Jan 2025 14:24


Tgt Ion: 75 Resp: 77838  
Ion Ratio Lower Upper  
75 100  
77 1.2 109.7 329.2#

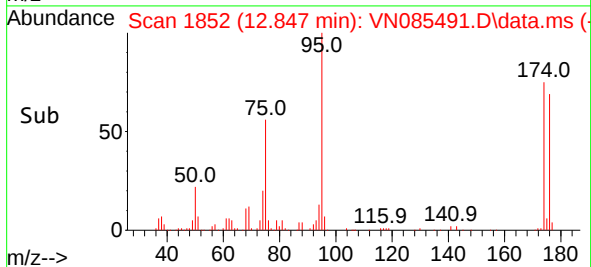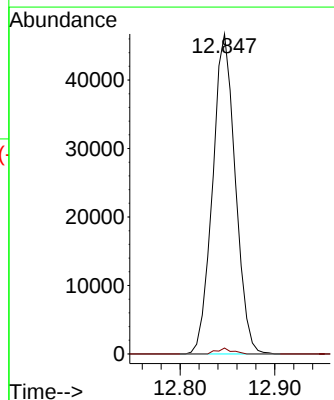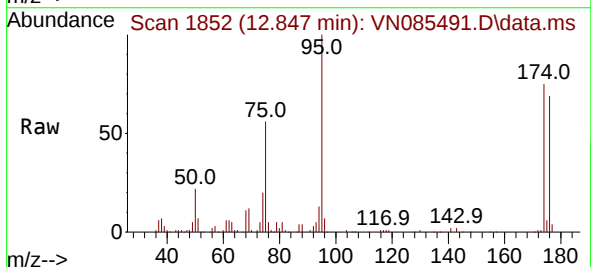



#81  
 trans-1,4-Dichloro-2-butene  
 Concen: 85.054 ug/l  
 RT: 12.847 min Scan# 11  
 Delta R.T. 0.112 min  
 Lab File: VN085491.D  
 Acq: 17 Jan 2025 14:24

Instrument :  
 MSVOA\_N  
 ClientSampleId :

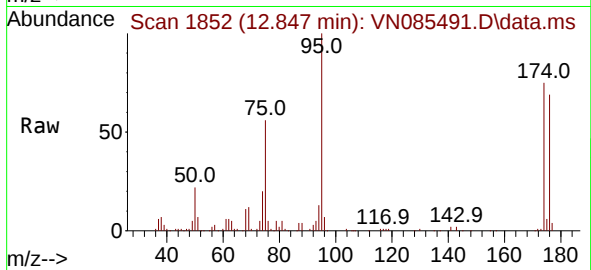

Tgt Ion: 75 Resp: 77838  
 Ion Ratio Lower Upper  
 75 100  
 53 0.3 95.6 143.4#  
 89 0.0 37.0 55.6#

