


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN011819\
Data File : VN053467.D
Acq On : 18 Jan 2019 12:43
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 10 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011519W.M
Title : SW846 8260
Last Update : Wed Jan 16 03:10:53 2019

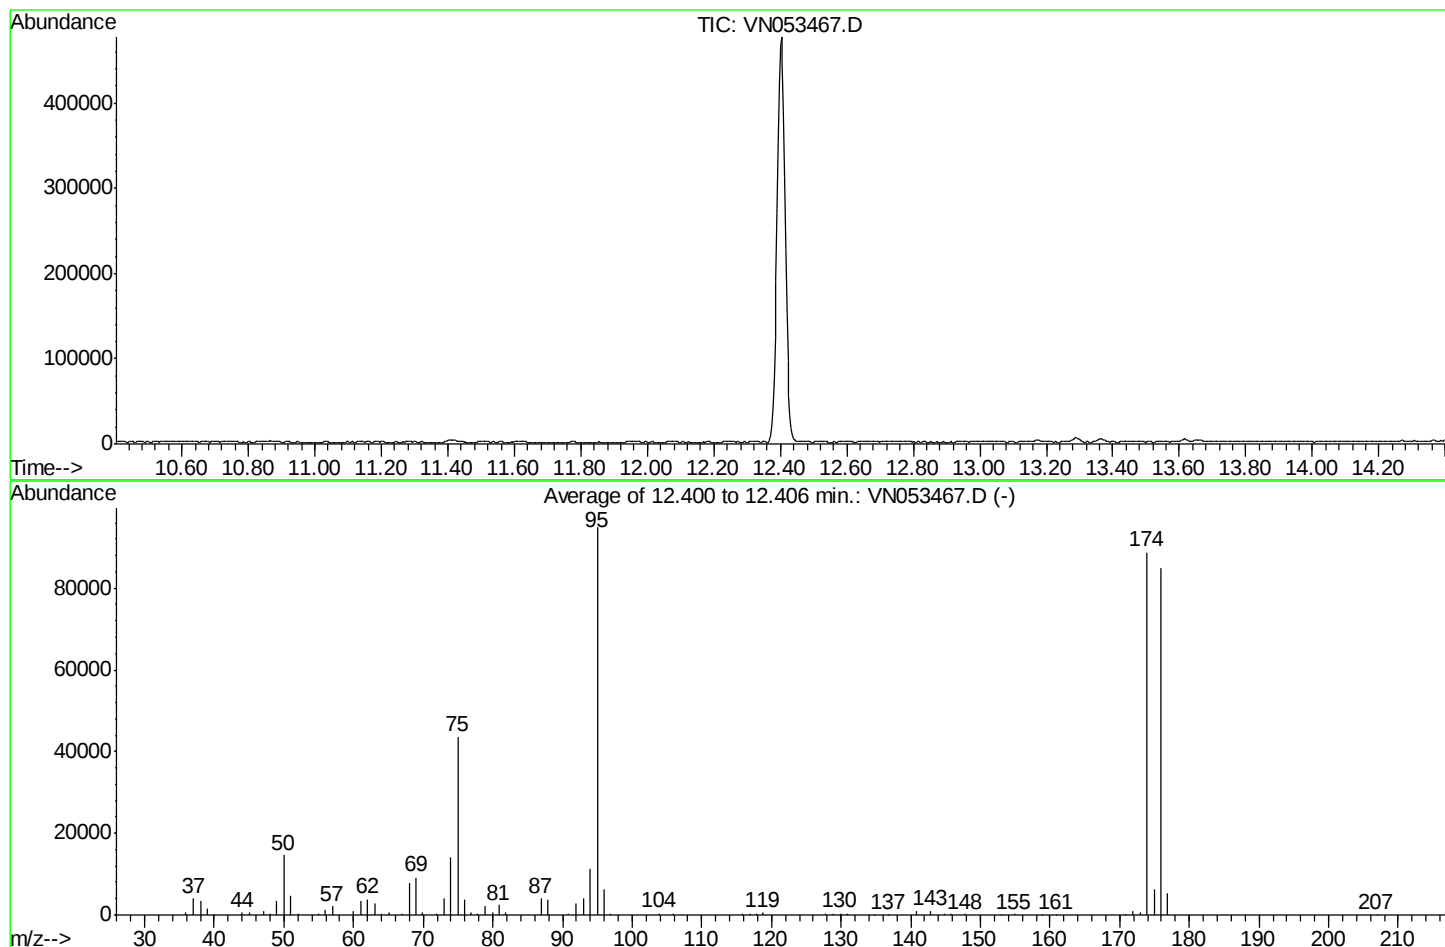

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	14688	PASS
75	95	30	60	46.0	43621	PASS
95	95	100	100	100.0	94888	PASS
96	95	5	9	6.7	6374	PASS
173	174	0.00	2	0.9	777	PASS
174	95	50	100	93.5	88685	PASS
175	174	5	9	7.0	6239	PASS
176	174	95	101	95.9	85005	PASS
177	176	5	9	6.5	5484	PASS