
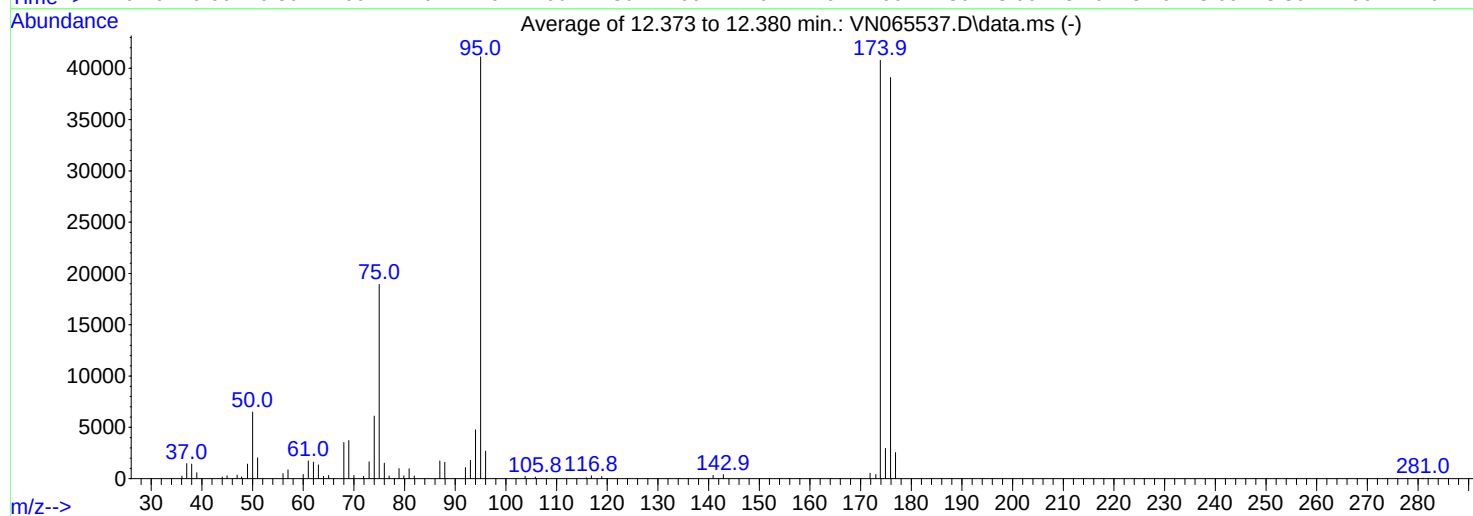


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011821\
 Data File : VN065537.D
 Acq On : 18 Jan 2021 9:33
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011821W.M
 Title : SW846 8260
 Last Update : Mon Jan 18 18:11:15 2021

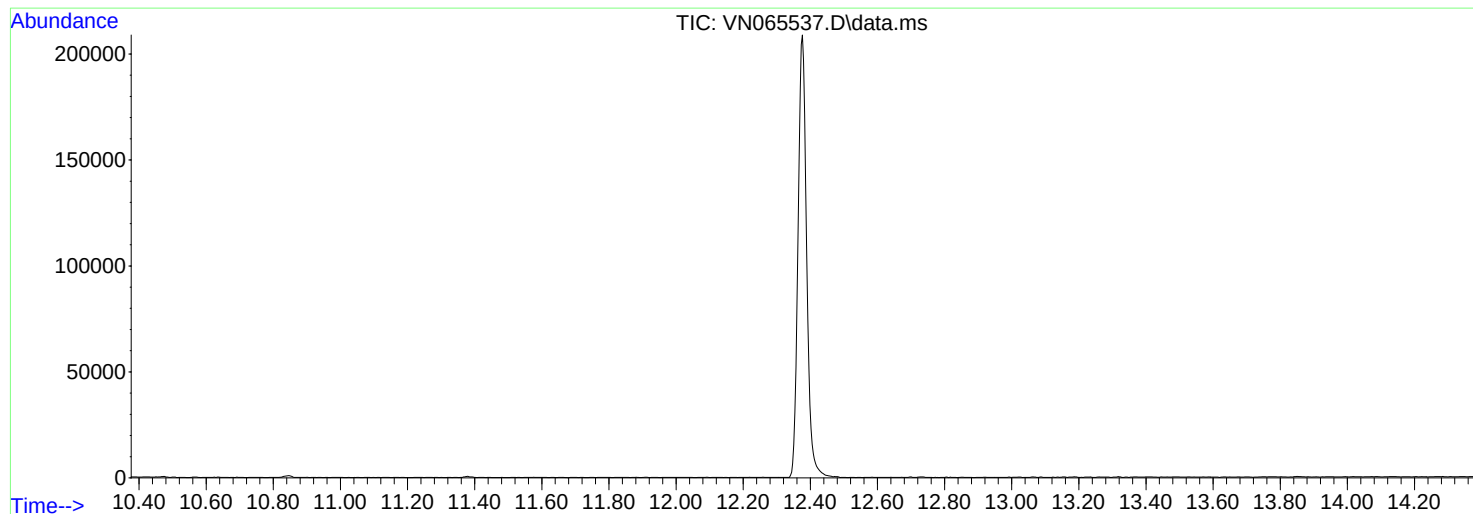

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	6497	PASS
75	95	30	60	46.1	18936	PASS
95	95	100	100	100.0	41117	PASS
96	95	5	9	6.5	2688	PASS
173	174	0.00	2	1.0	409	PASS
174	95	50	100	99.2	40784	PASS
175	174	5	9	7.2	2944	PASS
176	174	95	101	95.9	39104	PASS
177	176	5	9	6.5	2544	PASS