

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011822\
 Data File : VN070672.D
 Acq On : 18 Jan 2022 18:02
 Operator : JC/MD
 Sample : VN0118WBL01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0118WBL01

Quant Time: Jan 19 01:11:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 18 13:32:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.086	168	1112742	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	1778905	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	1550020	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	556763	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	726094	45.531	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	91.060%
35) Dibromofluoromethane	8.021	113	519611	47.089	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	94.180%
50) Toluene-d8	10.440	98	2163469	46.540	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	93.080%
62) 4-Bromofluorobenzene	12.731	95	685344	41.373	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	82.740%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011822\
Data File : VN070672.D
Acq On : 18 Jan 2022 18:02
Operator : JC/MD
Sample : VN0118WBL01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0118WBL01

Quant Time: Jan 19 01:11:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 18 13:32:07 2022
Response via : Initial Calibration




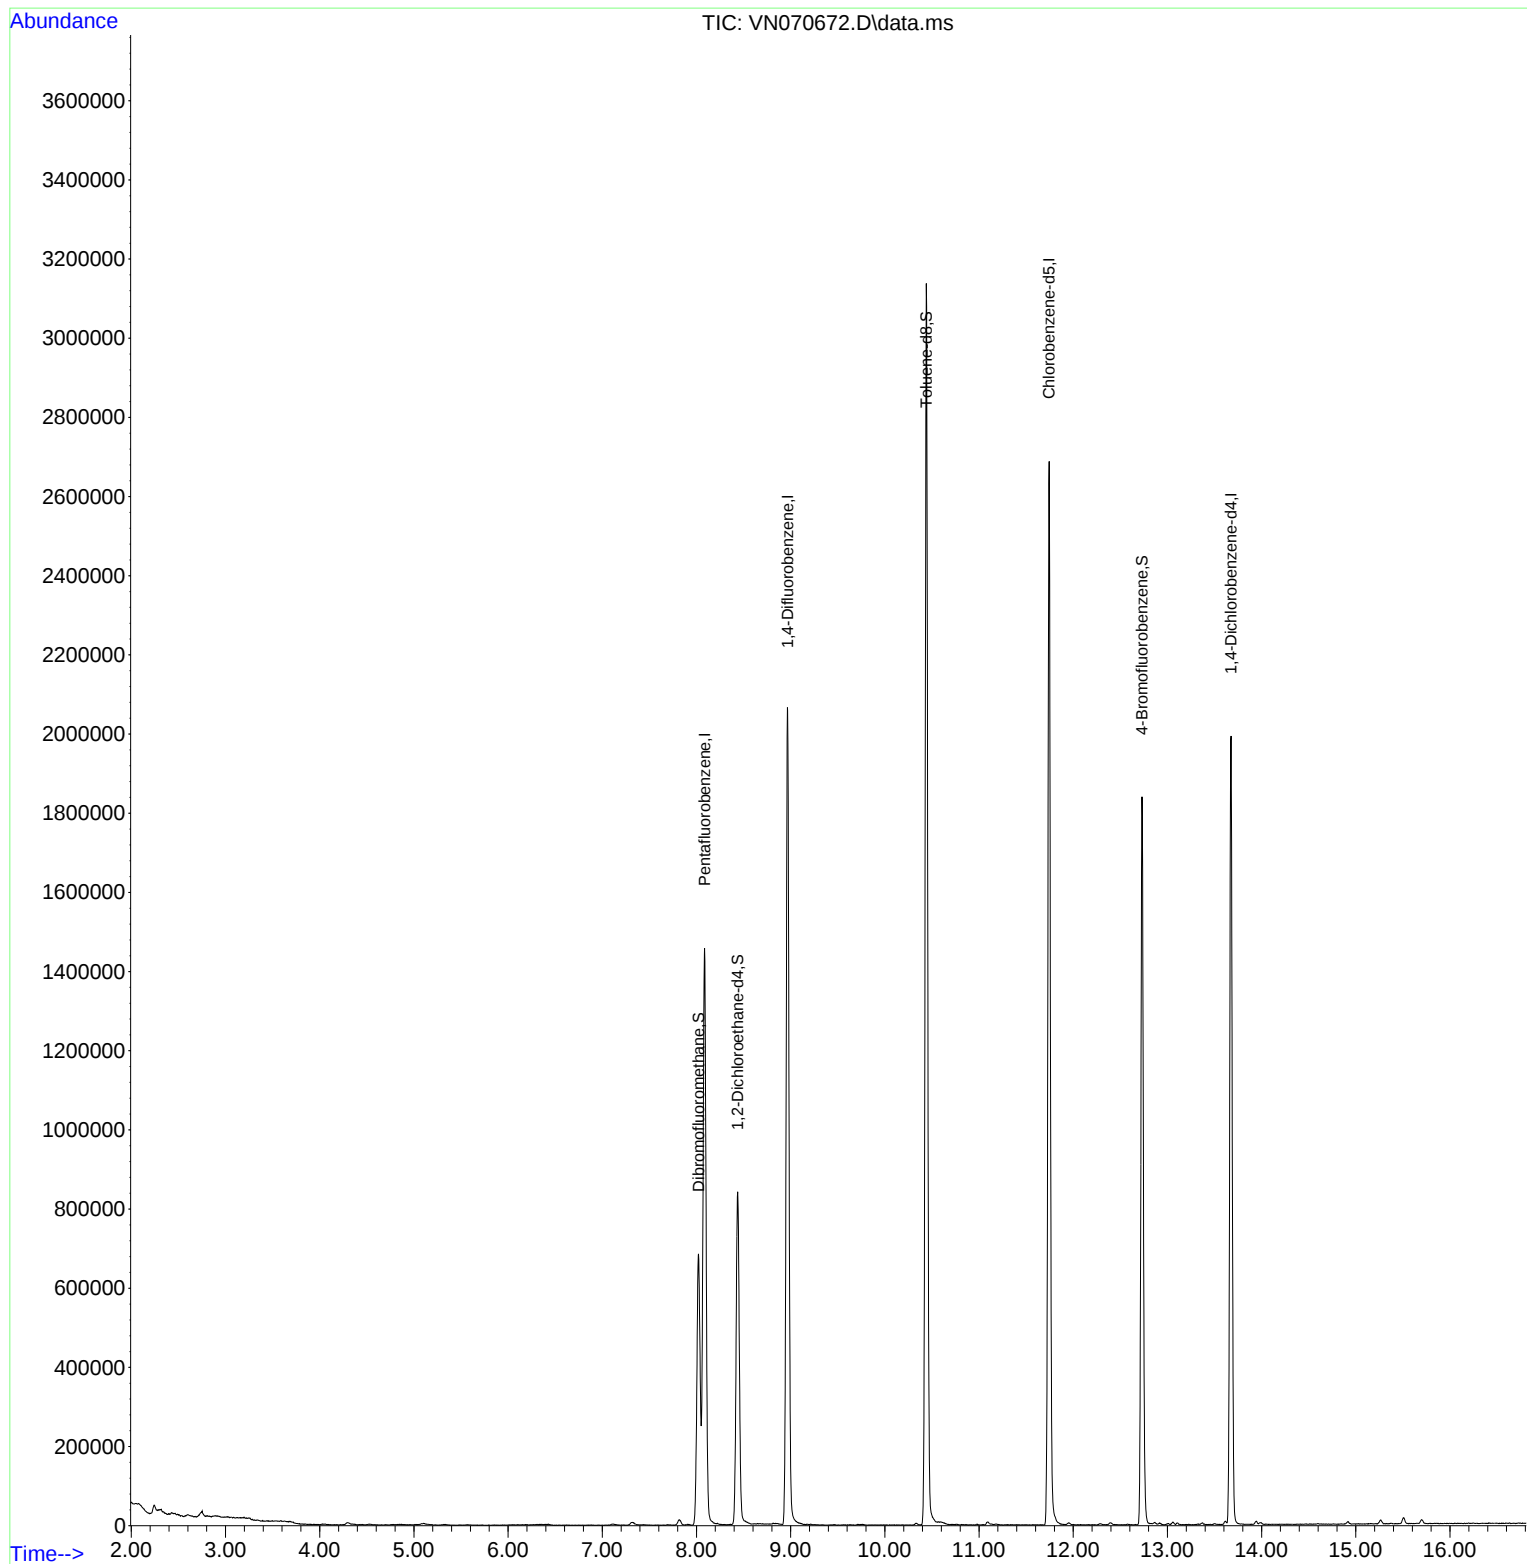


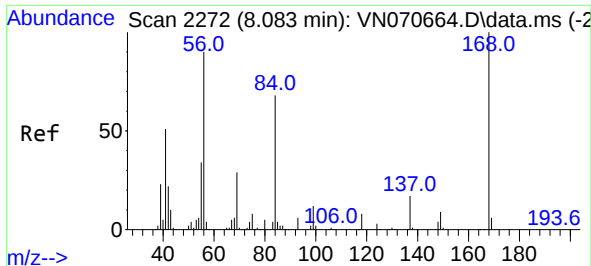

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 21
Delta R.T. 0.003 min
Lab File: VN070672.D
Acq: 18 Jan 2022 18:02




Instrument :
MSVOA_N
ClientSampleId :
VN0118WBL01


Tgt Ion:168 Resp: 1112742
Ion Ratio Lower Upper
168 100
99 59.2 41.3 61.9

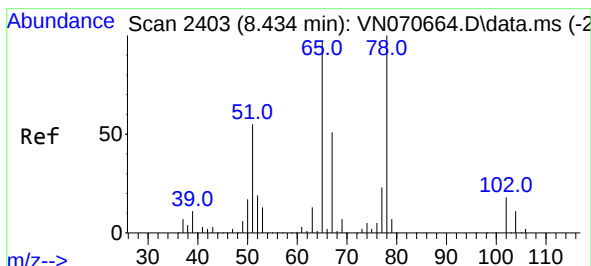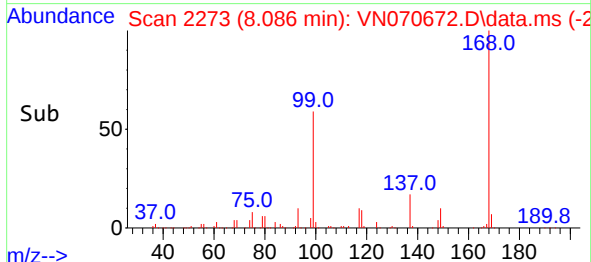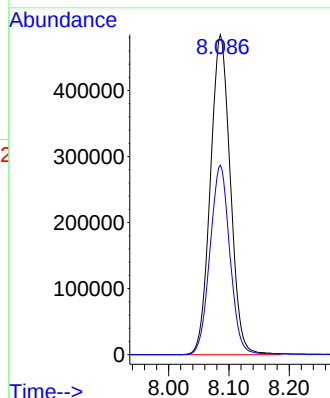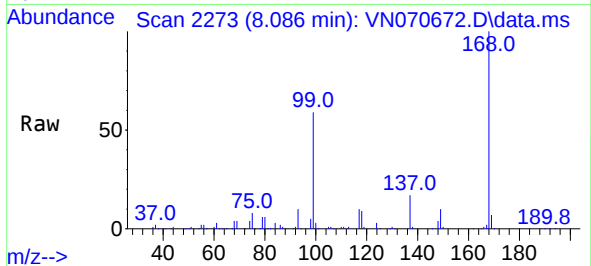

#33
1,2-Dichloroethane-d4
Concen: 45.531 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. 0.003 min
Lab File: VN070672.D
Acq: 18 Jan 2022 18:02

Tgt Ion: 65 Resp: 726094
Ion Ratio Lower Upper
65 100
67 53.1 0.0 103.0

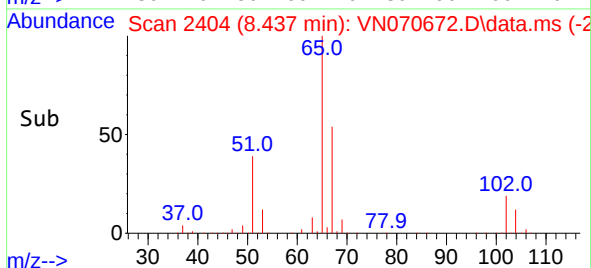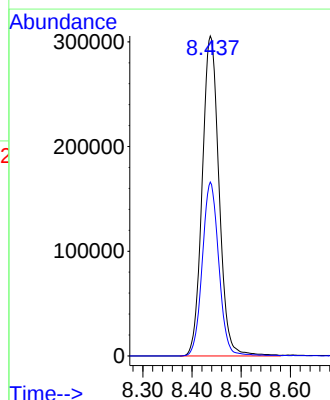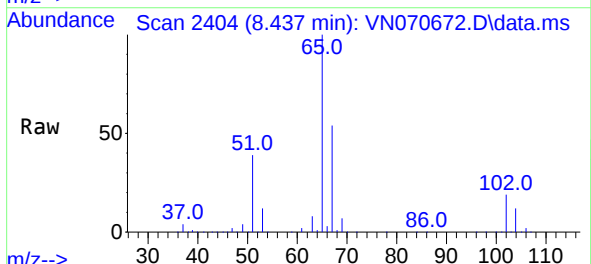

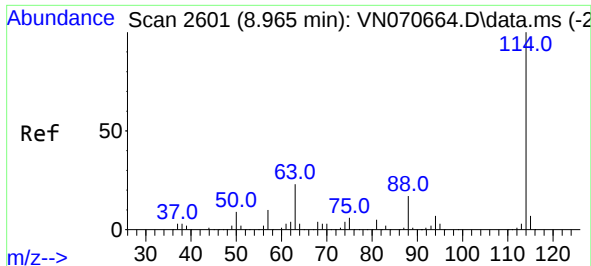

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.968 min Scan# 2

Delta R.T. 0.003 min

Lab File: VN070672.D

Acq: 18 Jan 2022 18:02

Instrument :

MSVOA_N

ClientSampleId :

VN0118WBL01





Tgt Ion:114 Resp: 1778905

Ion Ratio Lower Upper

114 100

63 23.6 0.0 37.8

88 16.7 0.0 27.4

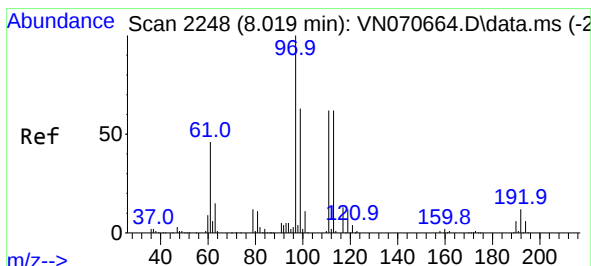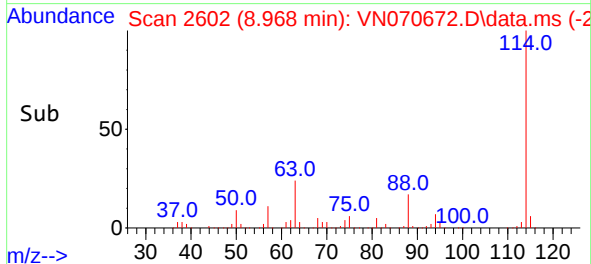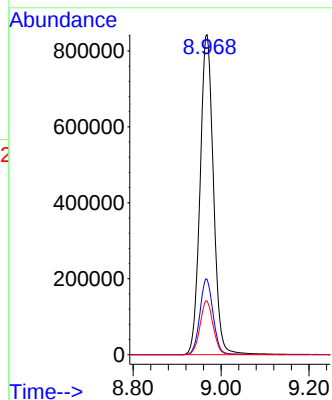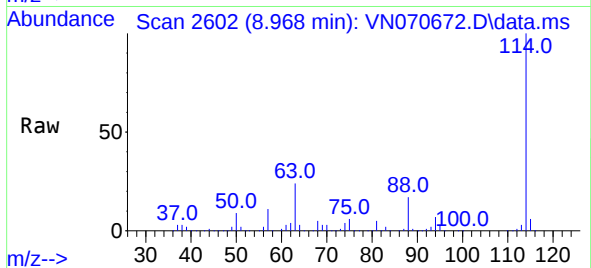

#35

Dibromofluoromethane

Concen: 47.089 ug/l

RT: 8.021 min Scan# 2249

Delta R.T. 0.002 min

Lab File: VN070672.D

Acq: 18 Jan 2022 18:02




Tgt Ion:113 Resp: 519611


Ion Ratio Lower Upper

113 100

111 101.4 82.2 123.2

192 19.3 16.9 25.3


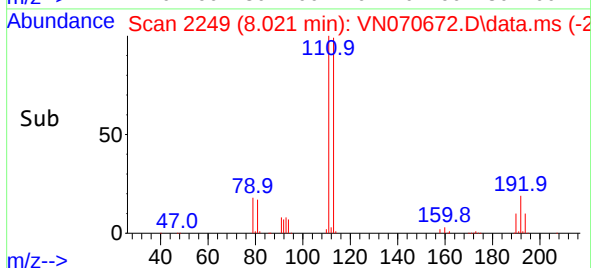
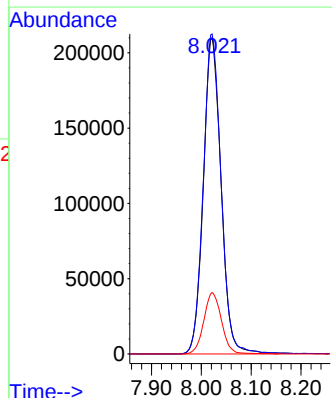
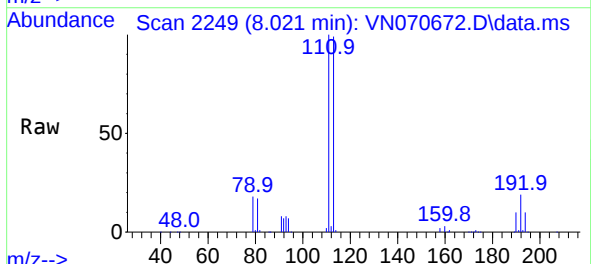


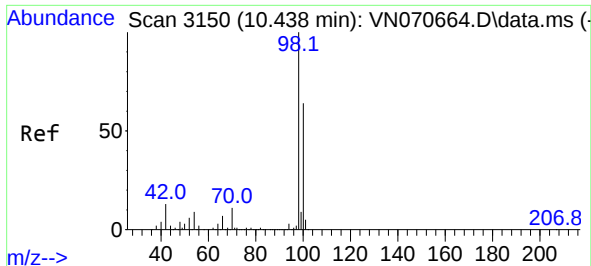

#50
Toluene-d8
Concen: 46.540 ug/l
RT: 10.440 min Scan# 3151
Delta R.T. 0.002 min
Lab File: VN070672.D
Acq: 18 Jan 2022 18:02




Instrument :
MSVOA_N
ClientSampleId :
VN0118WBL01


Tgt Ion: 98 Resp: 2163469
Ion Ratio Lower Upper
98 100
100 64.4 50.4 75.6

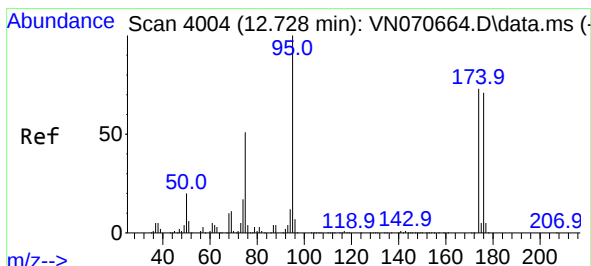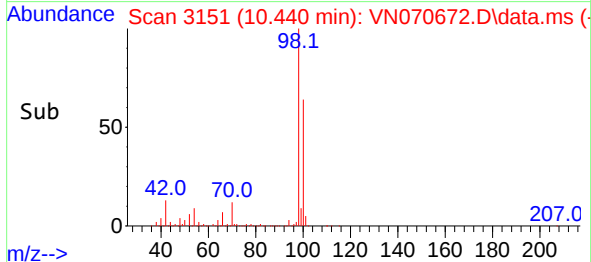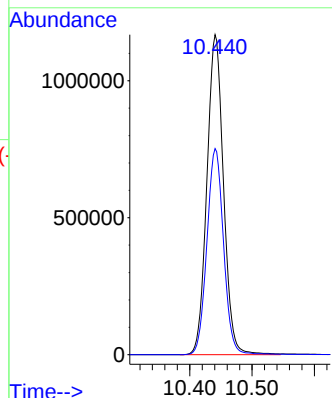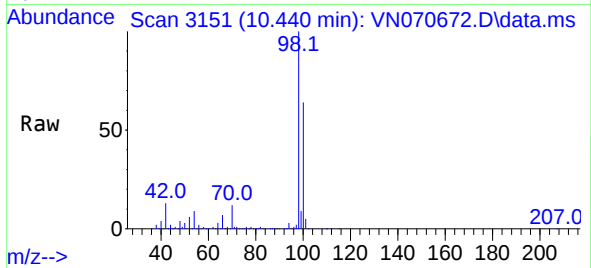

#62
4-Bromofluorobenzene
Concen: 41.373 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.003 min
Lab File: VN070672.D
Acq: 18 Jan 2022 18:02

Tgt Ion: 95 Resp: 685344
Ion Ratio Lower Upper
95 100
174 74.2 0.0 187.2
176 72.1 0.0 181.4


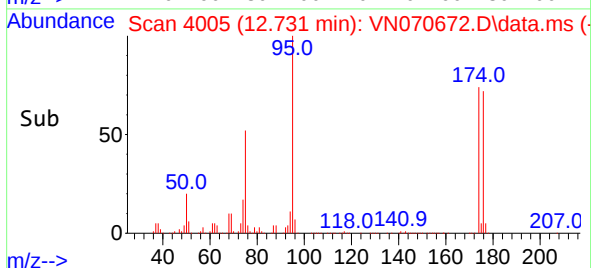
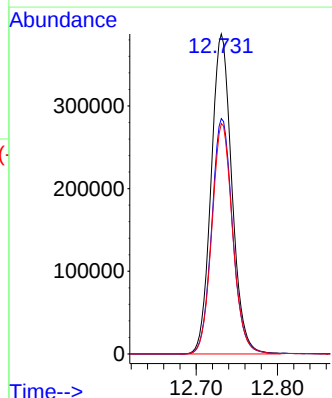
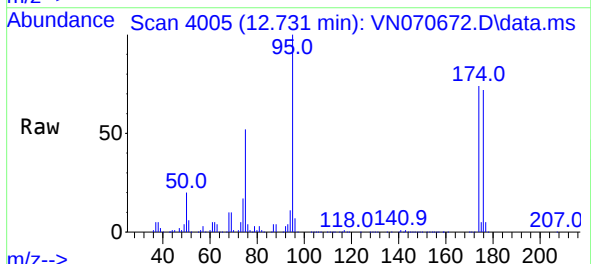


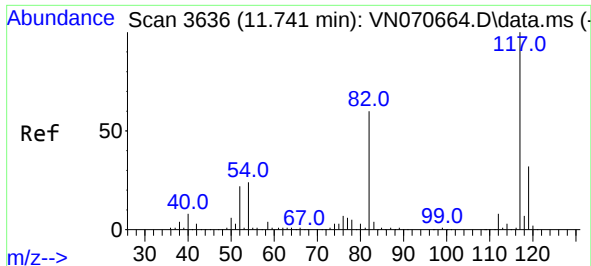

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 30
Delta R.T. 0.003 min
Lab File: VN070672.D
Acq: 18 Jan 2022 18:02

Instrument :
MSVOA_N
ClientSampleId :
VN0118WBL01

Tgt Ion:117 Resp: 1550020
Ion Ratio Lower Upper
117 100
82 59.7 42.4 63.6
119 32.1 25.4 38.2

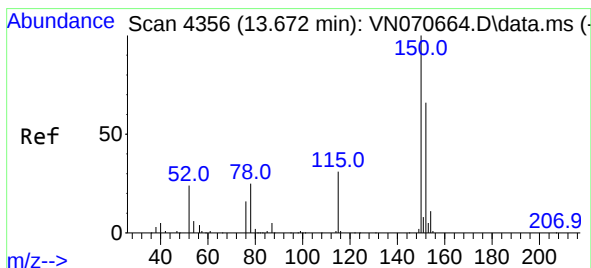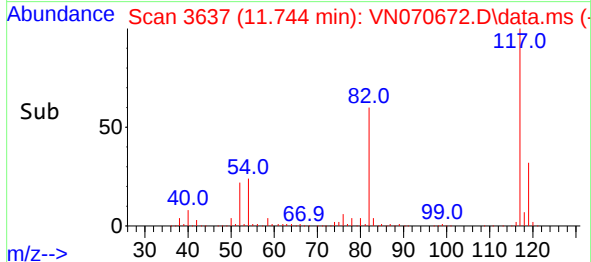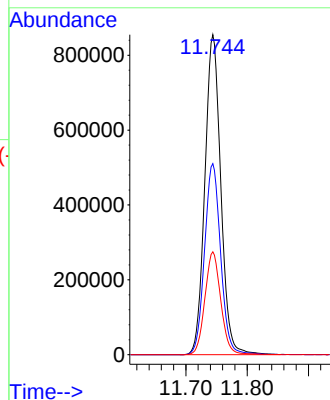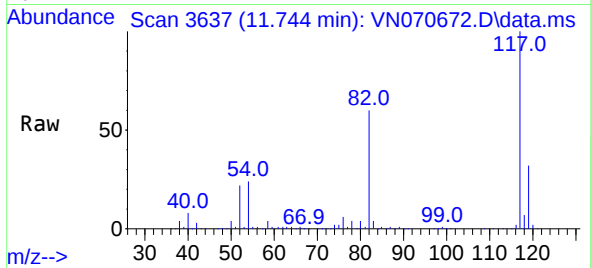

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. 0.003 min
Lab File: VN070672.D
Acq: 18 Jan 2022 18:02

Tgt Ion:152 Resp: 556763
Ion Ratio Lower Upper
152 100
115 62.2 27.5 82.5
150 158.6 0.0 344.4

