


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011822\
 Data File : VN070660.D
 Acq On : 18 Jan 2022 9:48
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
 Title : SW846 8260
 Last Update : Tue Jan 18 13:32:07 2022

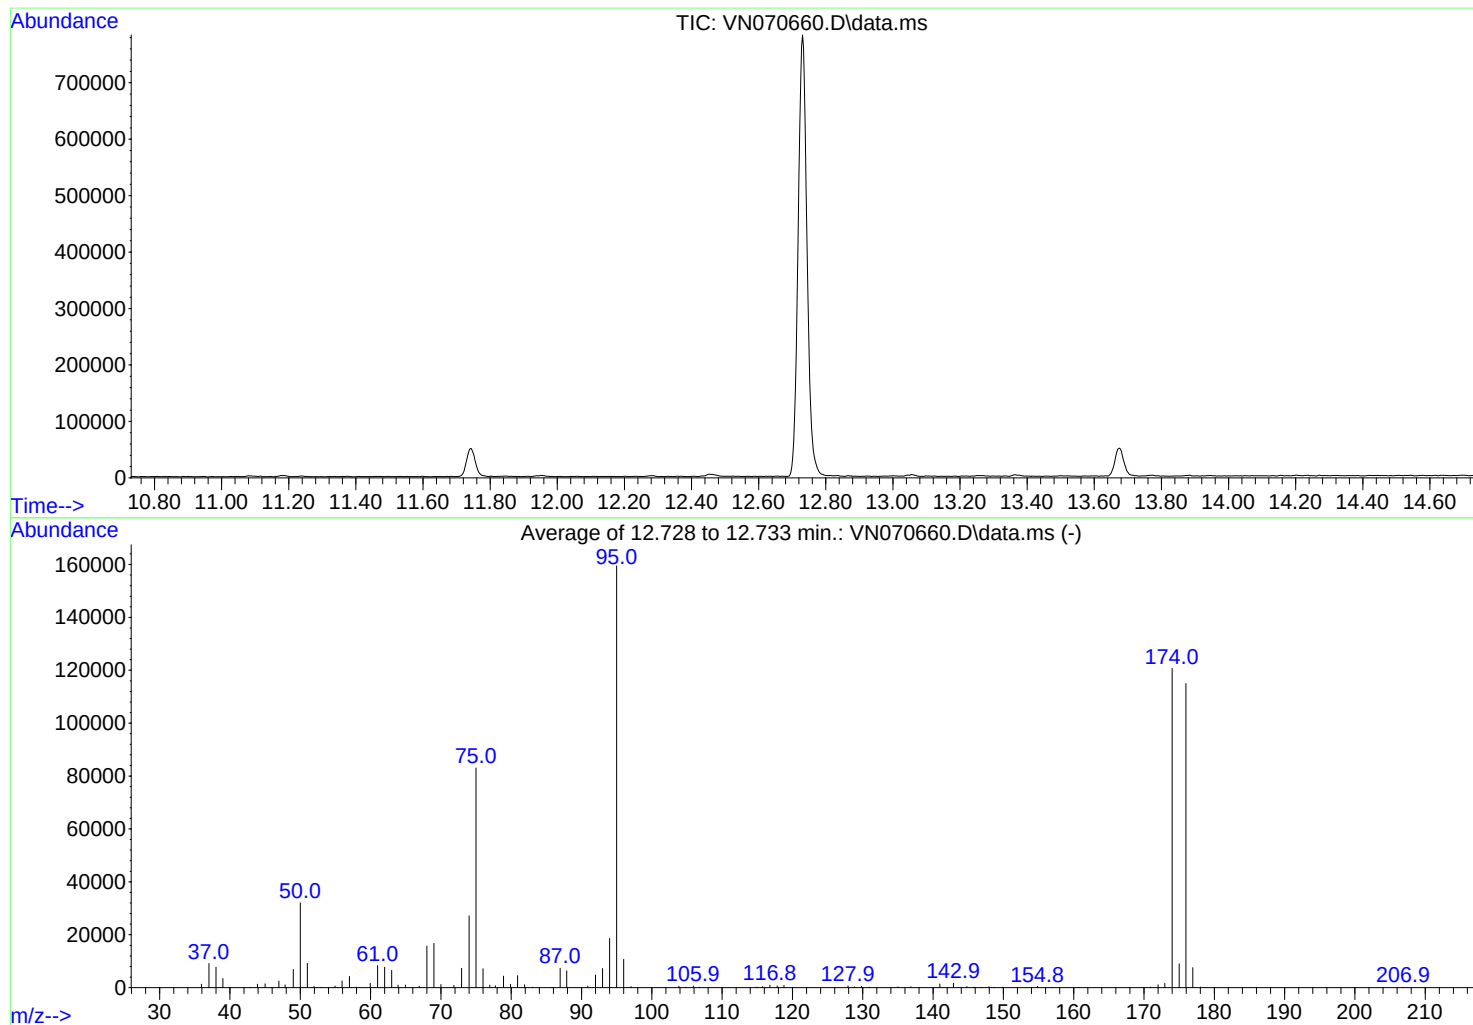

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3986

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	32056	PASS
75	95	30	60	52.1	83077	PASS
95	95	100	100	100.0	159488	PASS
96	95	5	9	6.7	10736	PASS
173	174	0.00	2	1.3	1611	PASS
174	95	50	100	75.7	120675	PASS
175	174	5	9	7.5	9027	PASS
176	174	95	101	95.3	114997	PASS
177	176	5	9	6.6	7575	PASS