

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011823\
 Data File : VN076293.D
 Acq On : 18 Jan 2023 12:59
 Operator : JC\MD
 Sample : 01190-14DL 10X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 WS-2DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
 Title : SW846 8260

Signal : TIC: VN076293.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	8.177	1030	1041	1045	rBV	237977	570426	19.49%	1.501%
2	8.230	1045	1050	1063	rVB	468959	1040639	35.55%	2.738%
3	8.588	1101	1111	1124	rBV2	236697	578417	19.76%	1.522%
4	9.106	1189	1199	1214	rBV	617249	1250319	42.72%	3.289%
5	9.606	1273	1284	1291	rBV3	26719	61795	2.11%	0.163%
6	10.571	1439	1448	1454	rBV	910553	1688260	57.68%	4.441%
7	10.635	1454	1459	1466	rVB	218663	407590	13.93%	1.072%
8	10.747	1472	1478	1486	rVB4	18255	36810	1.26%	0.097%
9	11.423	1583	1593	1598	rBV3	20487	44097	1.51%	0.116%
10	11.871	1660	1669	1679	rBV	775945	1427335	48.77%	3.755%
11	11.965	1679	1685	1695	rVV	267839	475240	16.24%	1.250%
12	12.071	1695	1703	1713	rVV	1020684	1948251	66.56%	5.125%
13	12.400	1748	1759	1767	rBV	616933	1090490	37.26%	2.869%
14	12.488	1767	1774	1779	rVB3	17101	34680	1.18%	0.091%
15	12.582	1779	1790	1793	rBV6	25709	72123	2.46%	0.190%
16	12.700	1805	1810	1815	rBV	74798	120083	4.10%	0.316%
17	12.853	1830	1836	1845	rVB	640709	1104297	37.73%	2.905%
18	13.035	1861	1867	1872	rBV	214149	348187	11.90%	0.916%
19	13.100	1872	1878	1882	rBV	893136	1535612	52.46%	4.040%
20	13.129	1882	1883	1887	rVB	154830	137932	4.71%	0.363%
21	13.176	1887	1891	1897	rVB	522501	891610	30.46%	2.346%
22	13.229	1897	1900	1905	rVB2	22198	34805	1.19%	0.092%
23	13.341	1905	1919	1925	rBV	430430	770989	26.34%	2.028%
24	13.400	1925	1929	1936	rBV4	27059	52902	1.81%	0.139%
25	13.482	1936	1943	1955	rVB	1783116	2926929	100.00%	7.700%
26	13.617	1955	1966	1971	rBV3	88494	168386	5.75%	0.443%
27	13.676	1971	1976	1981	rBV	155480	260417	8.90%	0.685%
28	13.729	1981	1985	1990	rBV2	64876	111044	3.79%	0.292%
29	13.794	1990	1996	1999	rBV	822311	1518221	51.87%	3.994%
30	13.959	2017	2024	2025	rBV2	134923	218632	7.47%	0.575%
31	13.994	2025	2030	2034	rBV2	541073	1109105	37.89%	2.918%
32	14.112	2045	2050	2057	rBV2	262366	461236	15.76%	1.213%
33	14.188	2058	2063	2068	rVV	171170	246517	8.42%	0.649%
34	14.247	2068	2073	2075	rVV	277485	417333	14.26%	1.098%
35	14.276	2075	2078	2083	rVV	265631	396185	13.54%	1.042%
36	14.335	2083	2088	2093	rVB	389552	603208	20.61%	1.587%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011823\
 Data File : VN076293.D
 Acq On : 18 Jan 2023 12:59
 Operator : JC\MD
 Sample : 01190-14DL 10X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 WS-2DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
 Title : SW846 8260

37	14.400	2093	2099	2102	rBV	95791	159119	5.44%	0.419%
38	14.447	2102	2107	2112	rVB2	414870	696008	23.78%	1.831%
39	14.517	2116	2119	2123	rVB3	32672	44924	1.53%	0.118%
40	14.582	2123	2130	2134	rBV2	177420	309709	10.58%	0.815%
41	14.659	2134	2143	2146	rBV	241029	525431	17.95%	1.382%
42	14.694	2146	2149	2153	rVV	336577	455189	15.55%	1.197%
43	14.735	2153	2156	2160	rVB	131673	170433	5.82%	0.448%
44	14.776	2160	2163	2171	rVB4	79022	175972	6.01%	0.463%
45	14.882	2171	2181	2184	rBV2	118298	255169	8.72%	0.671%
46	14.929	2184	2189	2192	rBV	390099	663458	22.67%	1.745%
47	14.964	2192	2195	2201	rVB2	318828	510721	17.45%	1.344%
48	15.053	2201	2210	2217	rBV3	751981	1908080	65.19%	5.020%
49	15.211	2231	2237	2244	rBV	651253	1157223	39.54%	3.044%
50	15.323	2244	2256	2260	rBV2	239880	611147	20.88%	1.608%
51	15.441	2269	2276	2284	rVB2	232021	592888	20.26%	1.560%
52	15.511	2284	2288	2297	rVB9	43817	108861	3.72%	0.286%
53	15.594	2297	2302	2306	rBV6	90554	190140	6.50%	0.500%
54	15.641	2306	2310	2315	rVV	166344	305162	10.43%	0.803%
55	15.700	2315	2320	2325	rVV	215450	400693	13.69%	1.054%
56	15.753	2325	2329	2330	rVV3	112144	157064	5.37%	0.413%
57	15.788	2331	2335	2338	rVV	165924	347468	11.87%	0.914%
58	15.835	2339	2343	2354	rVB2	257033	528902	18.07%	1.391%
59	15.947	2354	2362	2370	rBV	187192	448500	15.32%	1.180%
60	16.023	2372	2375	2380	rBV5	26600	38703	1.32%	0.102%
61	16.129	2385	2393	2394	rBV4	117455	203678	6.96%	0.536%
62	16.170	2394	2400	2411	rVB2	509973	1106592	37.81%	2.911%
63	16.258	2411	2415	2420	rBV4	49546	89444	3.06%	0.235%
64	16.347	2421	2430	2436	rBV3	97045	255783	8.74%	0.673%
65	16.506	2446	2457	2471	rBV2	317407	871625	29.78%	2.293%
66	16.623	2473	2477	2482	rVB3	33908	53544	1.83%	0.141%
67	16.717	2483	2493	2499	rBV2	213571	510674	17.45%	1.343%




Sum of corrected areas: 38012406

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011823\
Data File : VN076293.D
Acq On : 18 Jan 2023 12:59
Operator : JC\MD
Sample : 01190-14DL 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WS-2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

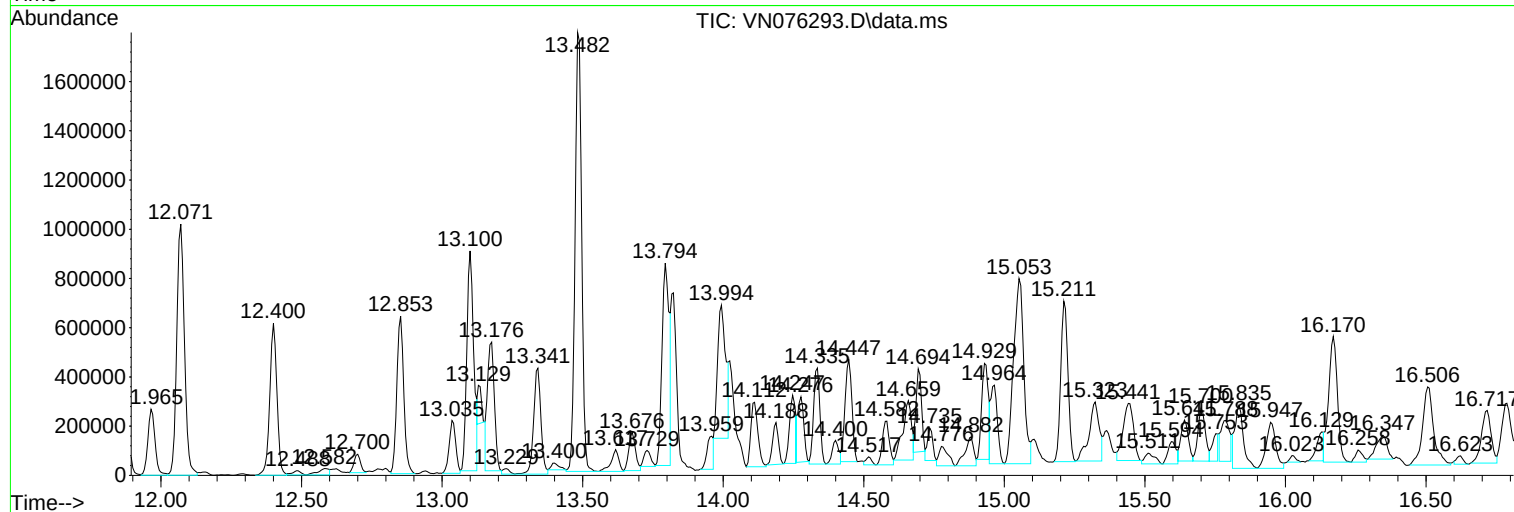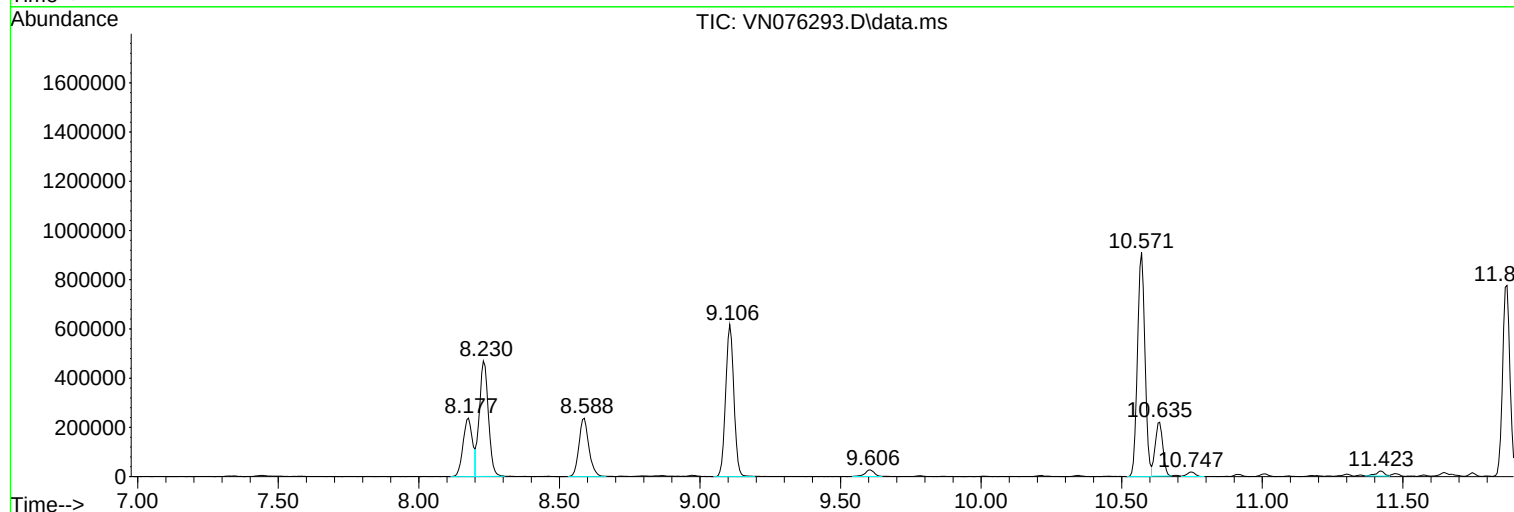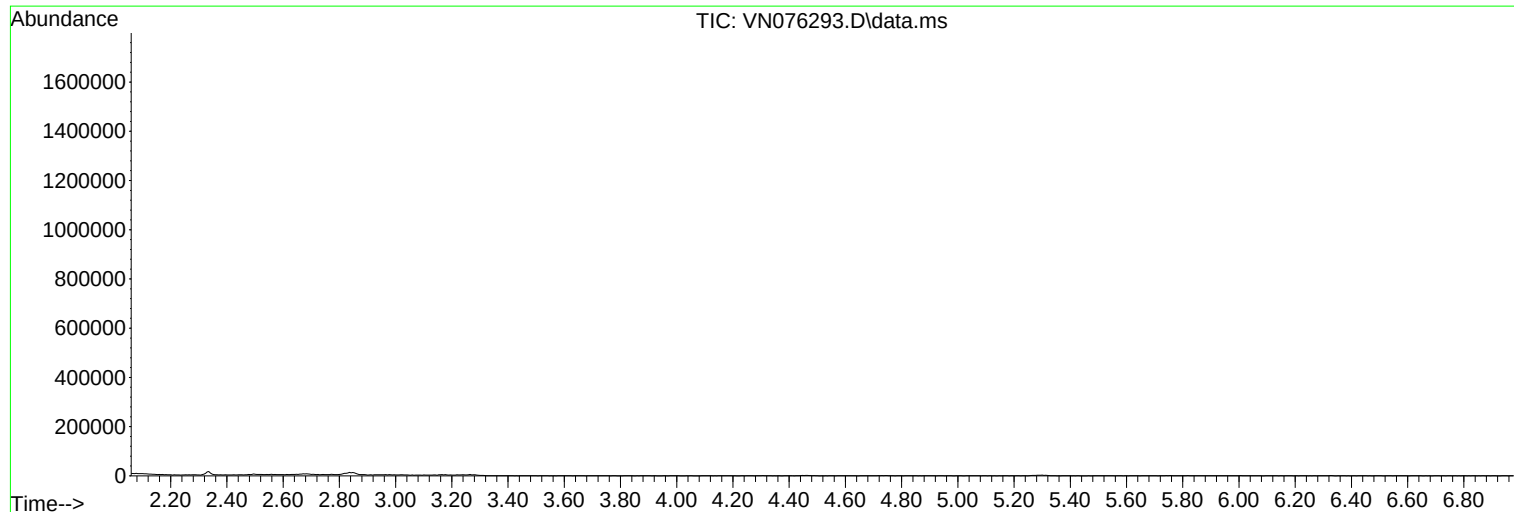

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011823\
Data File : VN076293.D
Acq On : 18 Jan 2023 12:59
Operator : JC\MD
Sample : 01190-14DL 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WS-2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011823\
Data File : VN076293.D
Acq On : 18 Jan 2023 12:59
Operator : JC\MD
Sample : 01190-14DL 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WS-2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc