
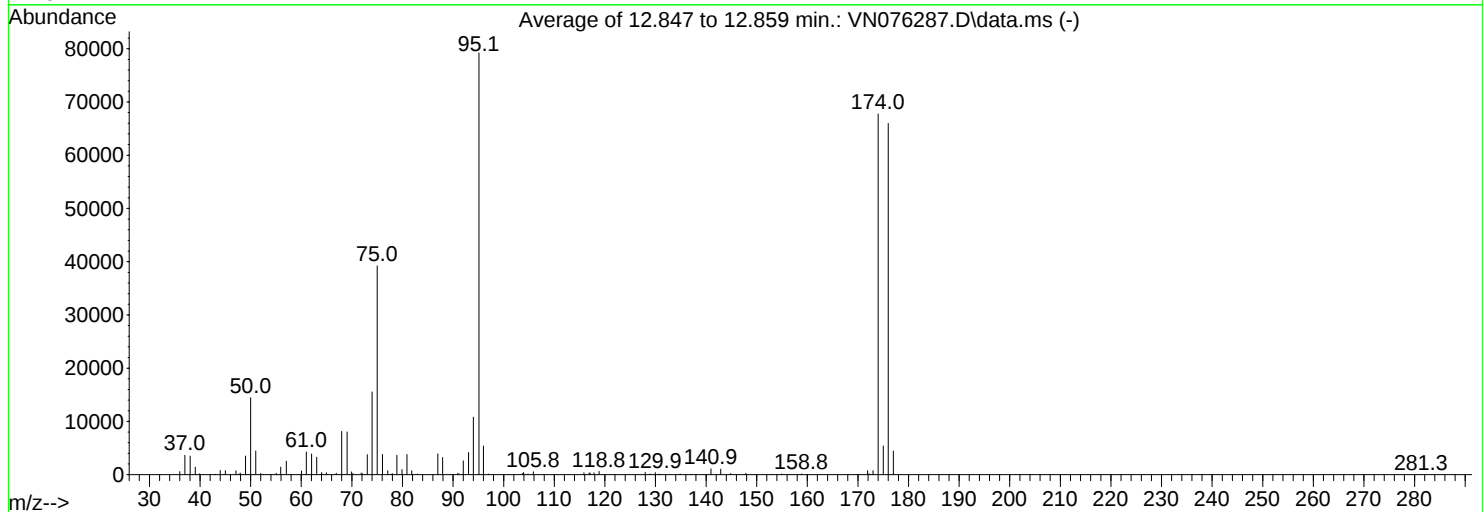


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN011823\  
Data File : VN076287.D  
Acq On : 18 Jan 2023 08:40  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N011623W.M  
Title : SW846 8260  
Last Update : Tue Jan 17 03:59:22 2023

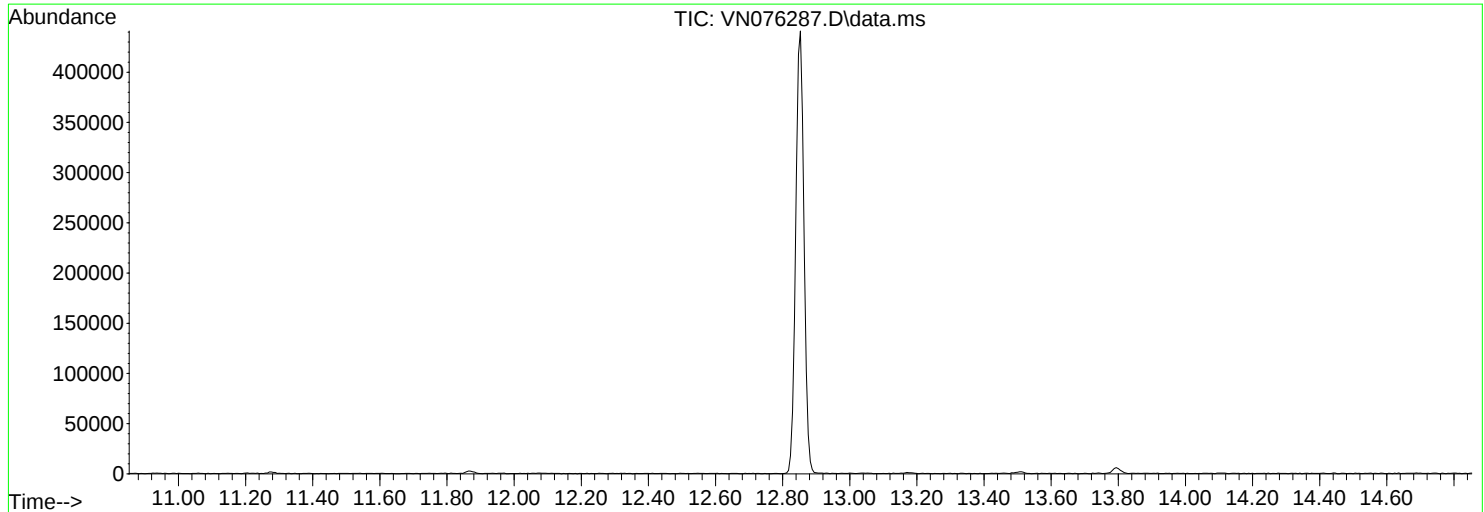

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 18.2         | 14449      | PASS                |
| 75             | 95              | 30              | 60              | 49.5         | 39219      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 79229      | PASS                |
| 96             | 95              | 5               | 9               | 6.8          | 5381       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.1          | 757        | PASS                |
| 174            | 95              | 50              | 100             | 85.5         | 67741      | PASS                |
| 175            | 174             | 5               | 9               | 7.9          | 5371       | PASS                |
| 176            | 174             | 95              | 101             | 97.4         | 65976      | PASS                |
| 177            | 176             | 5               | 9               | 6.7          | 4441       | PASS                |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 36.00 | 582    | 49.00 | 3494   | 63.05 | 3283   | 74.00 | 1552   |
| 37.00 | 3644   | 50.00 | 14449  | 64.05 | 385    | 75.00 | 3921   |
| 38.05 | 3496   | 51.00 | 4456   | 64.95 | 379    | 76.05 | 377    |
| 39.05 | 1425   | 52.00 | 231    | 66.90 | 286    | 77.10 | 71     |
| 39.95 | 175    | 55.05 | 253    | 68.00 | 8122   | 77.80 | 92     |
| 43.00 | 58     | 55.95 | 1425   | 69.05 | 8034   | 78.00 | 187    |
| 44.00 | 799    | 57.05 | 2539   | 69.95 | 527    | 78.90 | 3626   |
| 45.00 | 747    | 58.00 | 51     | 70.20 | 223    | 79.90 | 963    |
| 47.10 | 736    | 60.05 | 707    | 71.85 | 296    | 80.90 | 3798   |
| 47.70 | 121    | 61.00 | 4271   | 72.10 | 172    | 81.85 | 716    |
| 47.95 | 315    | 62.05 | 3878   | 73.05 | 3756   | 83.00 | 128    |

Average of 12.847 to 12.859 min.: VN076287.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z    | abund. | m/z    | abund. | m/z    | abund. |
|--------|--------|--------|--------|--------|--------|--------|--------|
| 87.00  | 3908   | 103.95 | 403    | 129.95 | 392    | 158.85 | 134    |
| 87.95  | 3207   | 104.80 | 126    | 130.70 | 132    | 171.90 | 764    |
| 90.95  | 279    | 105.85 | 530    | 134.85 | 134    | 172.20 | 198    |
| 91.20  | 141    | 109.90 | 61     | 136.90 | 64     | 173.00 | 757    |
| 92.00  | 2603   | 115.85 | 358    | 140.95 | 1070   | 174.00 | 67741  |
| 93.05  | 4152   | 116.90 | 366    | 142.90 | 1029   | 175.00 | 5371   |
| 94.00  | 10780  | 117.10 | 228    | 144.85 | 226    | 176.00 | 65976  |
| 95.10  | 79229  | 117.85 | 371    | 147.85 | 253    | 177.00 | 4441   |
| 96.00  | 5381   | 118.85 | 596    | 149.70 | 52     | 178.00 | 72     |
| 97.05  | 127    | 127.95 | 409    | 152.90 | 52     | 281.30 | 54     |
| 103.70 | 200    | 128.90 | 128    | 154.95 | 115    |        |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB