


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011921\
 Data File : VN065547.D
 Acq On : 19 Jan 2021 9:21
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011821W.M
 Title : SW846 8260
 Last Update : Mon Jan 18 18:11:15 2021

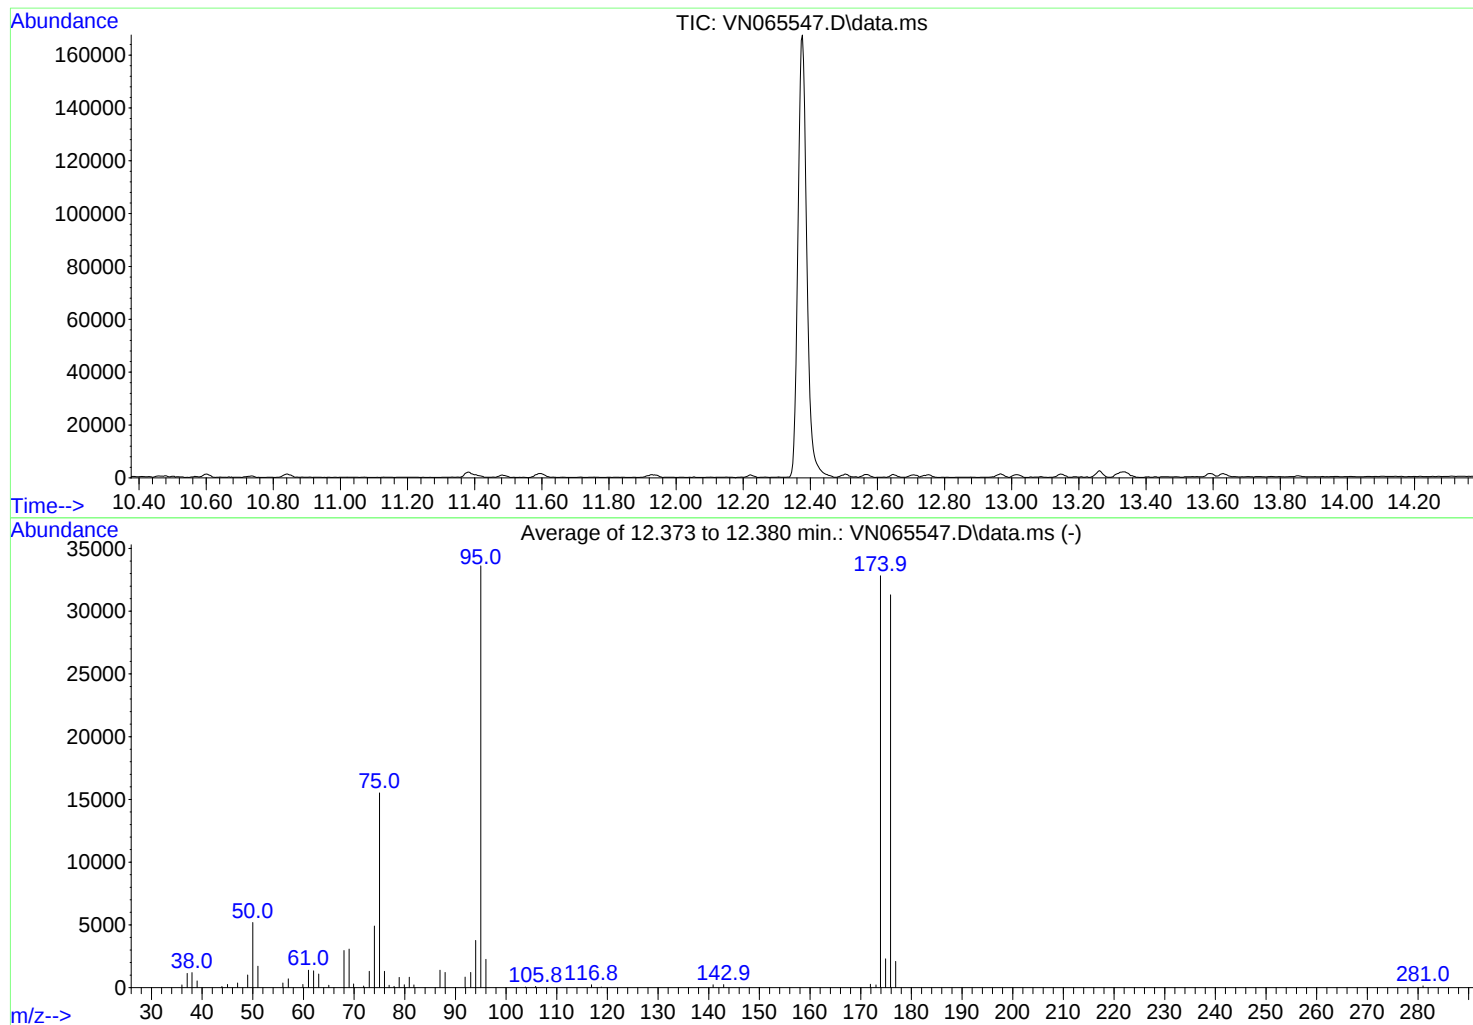

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	5195	PASS
75	95	30	60	46.2	15520	PASS
95	95	100	100	100.0	33616	PASS
96	95	5	9	6.7	2256	PASS
173	174	0.00	2	0.7	220	PASS
174	95	50	100	97.6	32824	PASS
175	174	5	9	7.0	2301	PASS
176	174	95	101	95.4	31309	PASS
177	176	5	9	6.7	2091	PASS