


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011922\
Data File : VN070689.D
Acq On : 19 Jan 2022 9:46
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
Title : SW846 8260
Last Update : Tue Jan 18 13:32:07 2022

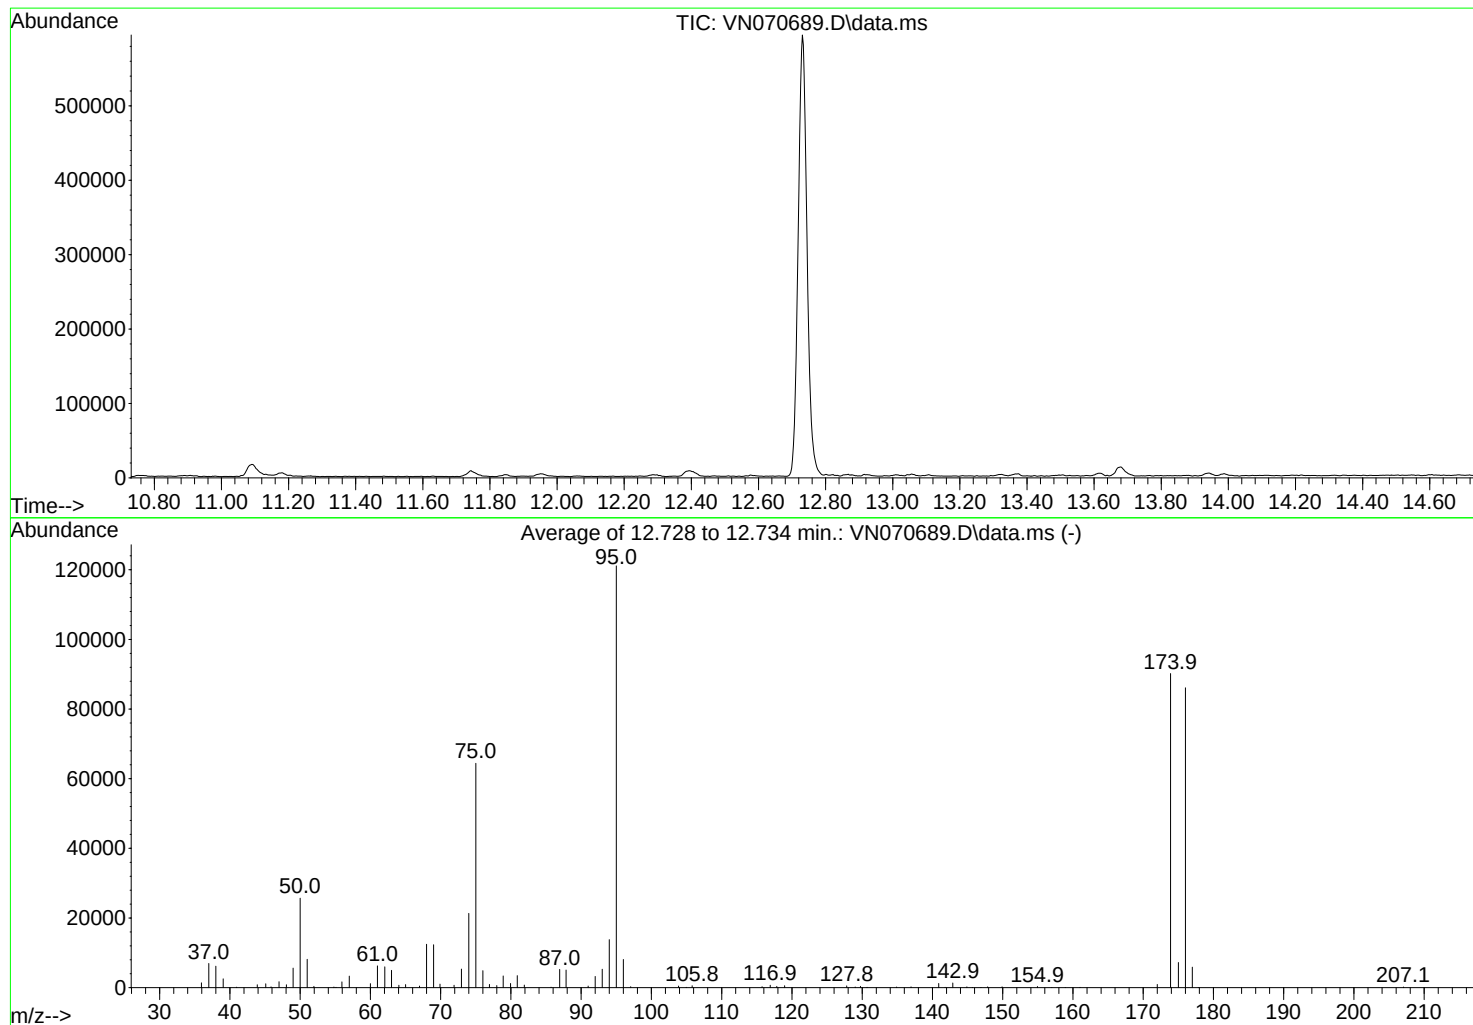

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3987

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.2	25688	PASS
75	95	30	60	53.2	64443	PASS
95	95	100	100	100.0	121125	PASS
96	95	5	9	6.7	8107	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.5	90184	PASS
175	174	5	9	8.0	7223	PASS
176	174	95	101	95.5	86104	PASS
177	176	5	9	6.8	5874	PASS