

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011923\
 Data File : VN076327.D
 Acq On : 19 Jan 2023 16:55
 Operator : JC\MD
 Sample : 01221-01DL 25X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-10-0118DL

Quant Time: Jan 20 00:59:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 17 03:59:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	399186	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	619169	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	537045	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	229642	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	203339	45.494	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	90.980%		
35) Dibromofluoromethane	8.177	113	185333	47.851	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	95.700%		
50) Toluene-d8	10.571	98	703054	49.151	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	98.300%		
62) 4-Bromofluorobenzene	12.853	95	227897	48.804	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	97.600%		
Target Compounds						Qvalue
11) Tert butyl alcohol	5.542	59	1502	2.512	ug/l #	72
16) Acetone	4.453	43	14009	9.707	ug/l #	84
19) Methyl tert-butyl Ether	5.806	73	38903	3.125	ug/l #	91
20) Methylene Chloride	5.277	84	635	Below Cal	#	57
25) 2-Butanone	7.500	43	2196	1.003	ug/l	97
31) Cyclohexane	8.236	56	11260	1.640	ug/l #	38
36) 1,1-Dichloropropene	8.230	75	28475	5.174	ug/l #	49
37) Ethyl Acetate	7.500	43	2196	0.534	ug/l #	67
38) Carbon Tetrachloride	8.230	117	37979	6.188	ug/l #	16
39) Methylcyclohexane	9.606	83	3059	0.455	ug/l #	70
48) Methyl methacrylate	9.606	41	1323	0.389	ug/l #	70
51) 4-Methyl-2-Pentanone	10.441	43	1108	0.263	ug/l #	78
52) Toluene	10.630	92	3457	0.314	ug/l	92
59) 2-Hexanone	11.171	43	1009	0.330	ug/l #	21
67) Ethyl Benzene	11.965	91	384467	19.788	ug/l	100
68) m/p-Xylenes	12.076	106	102536	13.161	ug/l	99
69) o-Xylene	12.400	106	13130	1.716	ug/l	96
71) Bromoform	12.853	173	1577	0.517	ug/l #	1
73) Isopropylbenzene	12.694	105	20718	1.166	ug/l	97
76) 1,2,3-Trichloropropane	12.853	75	117116	27.570	ug/l #	1
78) n-propylbenzene	13.035	91	45662	2.278	ug/l	97
79) 2-Chlorotoluene	13.135	91	8351	0.679	ug/l #	40
80) 1,3,5-Trimethylbenzene	13.135	105	70650	4.747	ug/l	64
81) trans-1,4-Dichloro-2-b...	12.853	75	117116	84.854	ug/l #	11
82) 4-Chlorotoluene	13.135	91	8351	0.679	ug/l #	40
83) tert-Butylbenzene	13.676	119	3503	0.265	ug/l	74
84) 1,2,4-Trimethylbenzene	13.488	105	394882	26.460	ug/l	98
85) sec-Butylbenzene	13.488	105	394882	21.499	ug/l #	56
89) n-Butylbenzene	14.059	91	3820	0.319	ug/l #	55
90) Hexachloroethane	14.329	117	3085	1.183	ug/l #	12
95) Naphthalene	15.641	128	54750	6.259	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011923\
Data File : VN076327.D
Acq On : 19 Jan 2023 16:55
Operator : JC\MD
Sample : 01221-01DL 25X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-10-0118DL

Quant Time: Jan 20 00:59:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 17 03:59:22 2023
Response via : Initial Calibration

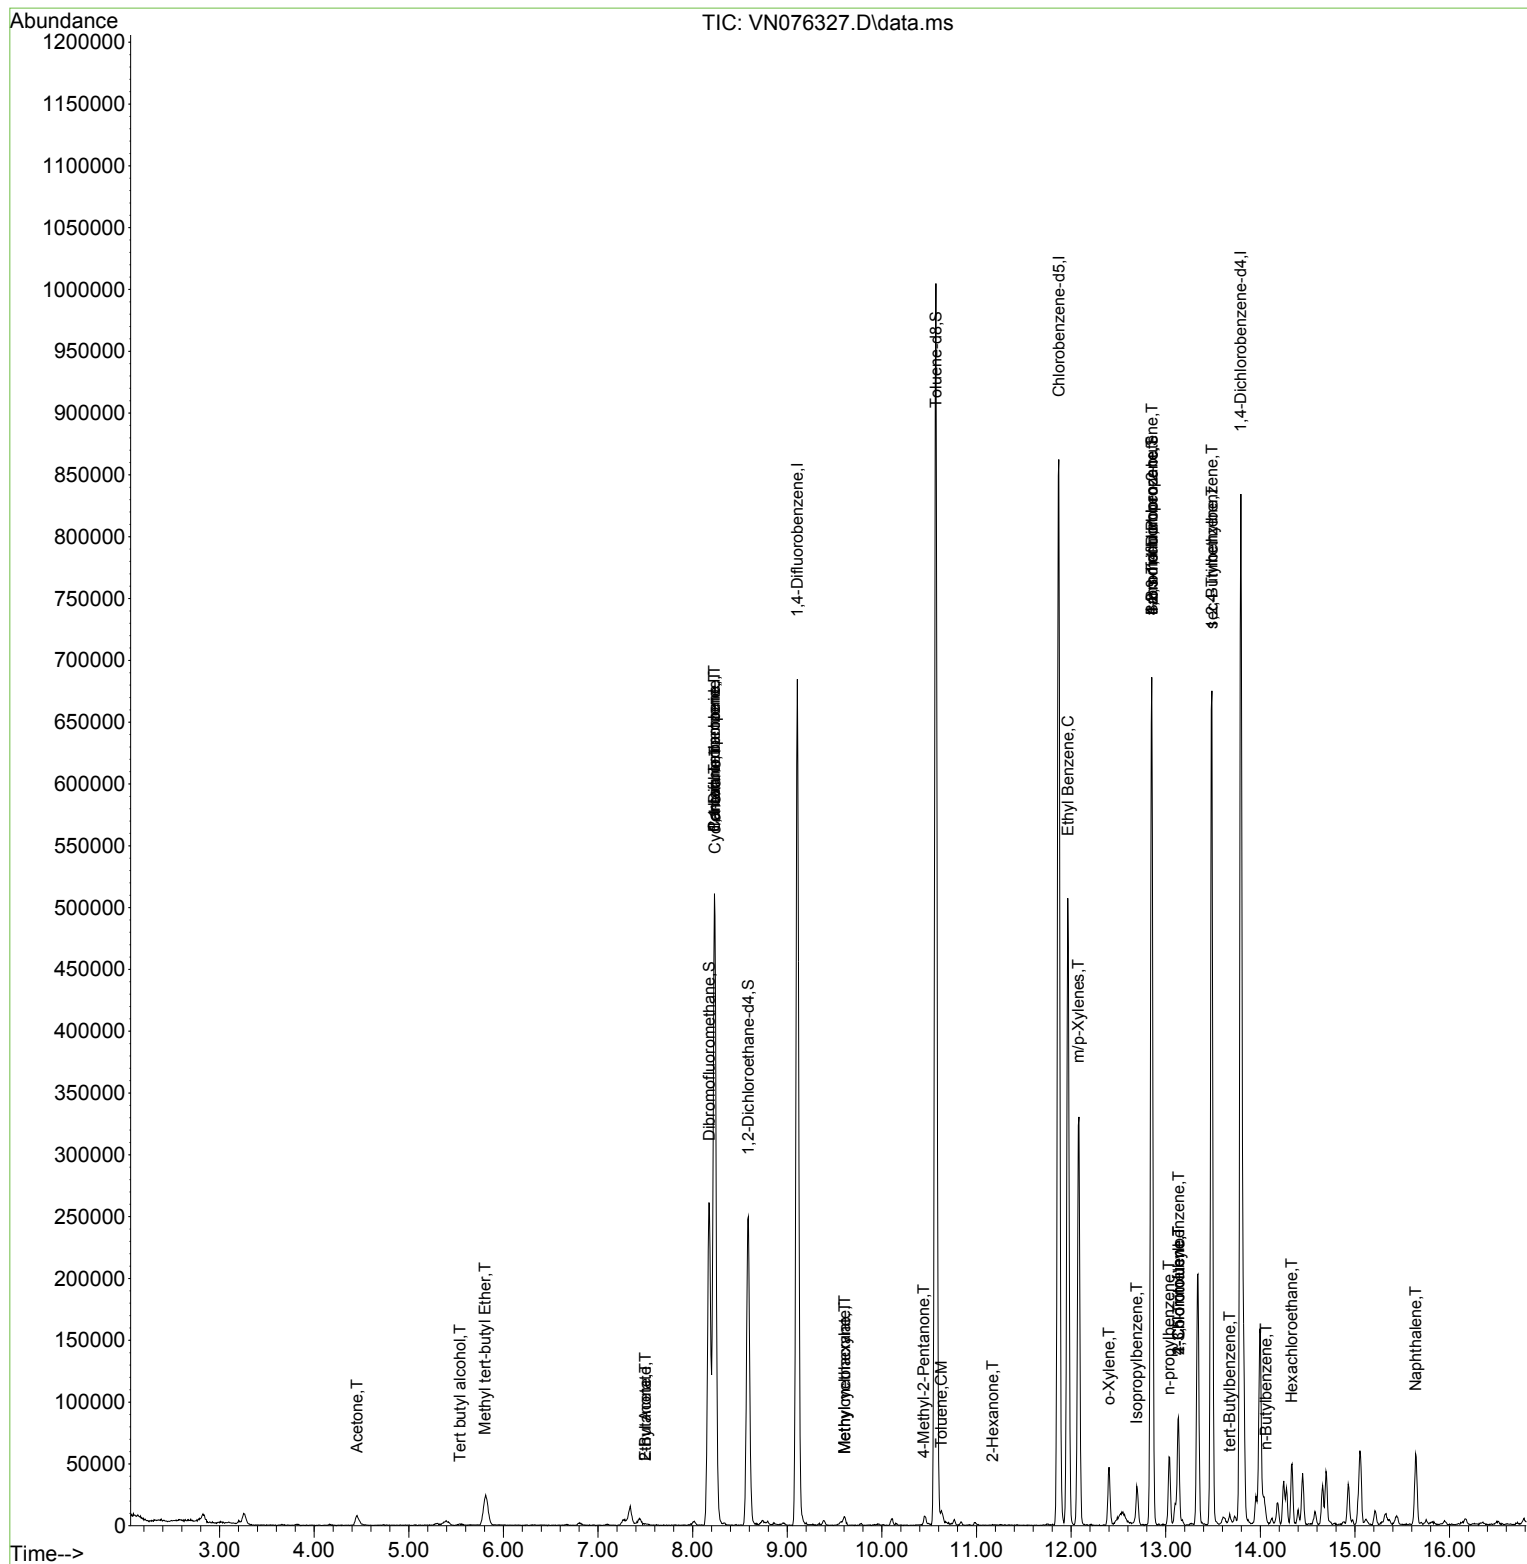



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.230 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN076327.D

Acq: 19 Jan 2023 16:55

Instrument :

MSVOA_N

ClientSampleId :





MW-10-0118DL

Tgt Ion:168 Resp: 399186

Ion Ratio Lower Upper

168 100

99 54.5 41.6 62.4

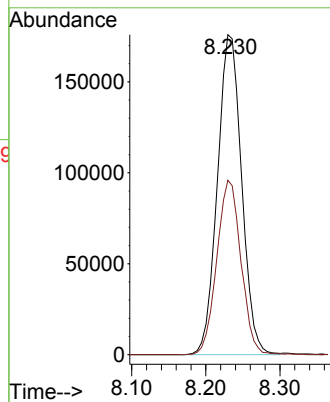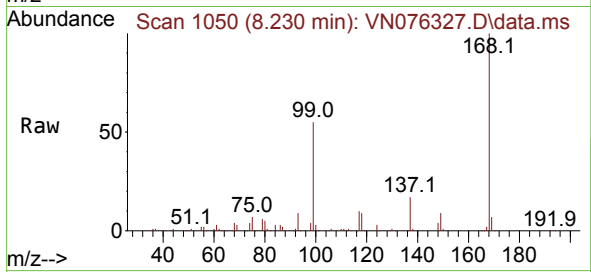

#11

Tert butyl alcohol

Concen: 2.512 ug/l

RT: 5.542 min Scan# 593

Delta R.T. 0.012 min

Lab File: VN076327.D




Acq: 19 Jan 2023 16:55


Tgt Ion: 59 Resp: 1502

Ion Ratio Lower Upper

59 100

57 0.0 8.5 12.7#


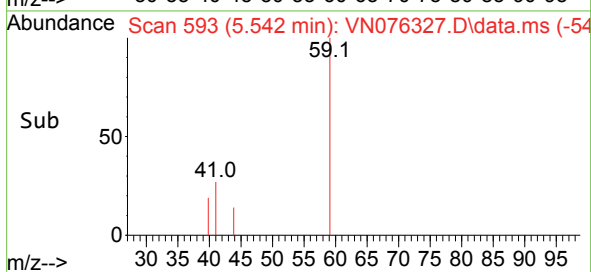
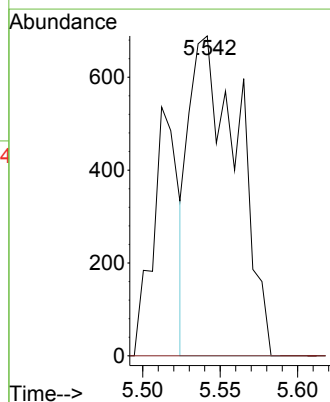
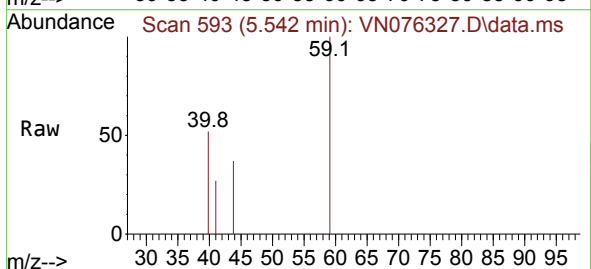




#16
Acetone
Concen: 9.707 ug/l
RT: 4.453 min Scan# 406
Delta R.T. 0.011 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0118DL

Tgt Ion: 43 Resp: 14009
Ion Ratio Lower Upper
43 100
58 42.6 26.7 40.1#

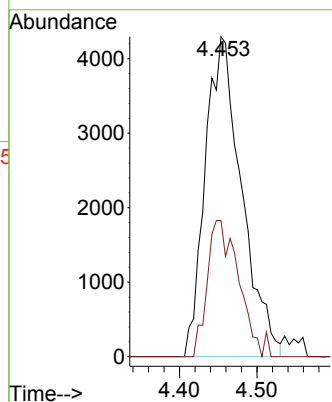

#19
Methyl tert-butyl Ether
Concen: 3.125 ug/l
RT: 5.806 min Scan# 638
Delta R.T. 0.000 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55

Tgt Ion: 73 Resp: 38903
Ion Ratio Lower Upper
73 100
57 23.9 15.9 23.9#


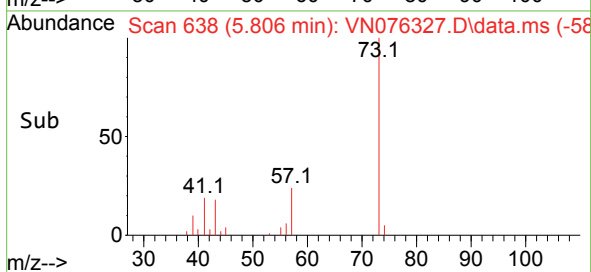
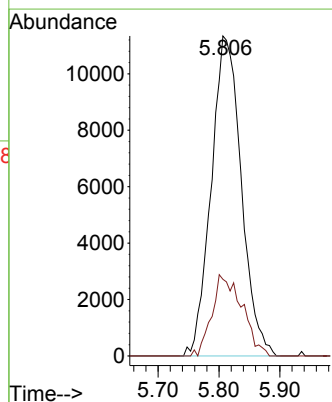





#20
Methylene Chloride
Concen: Below Cal
RT: 5.277 min Scan# 54
Delta R.T. -0.012 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0118DL


Tgt Ion: 84	Resp: 635
Ion Ratio	Lower Upper
84 100	
49 91.5	84.5 126.7
51 0.0	26.0 39.0#
86 0.0	52.0 78.0#

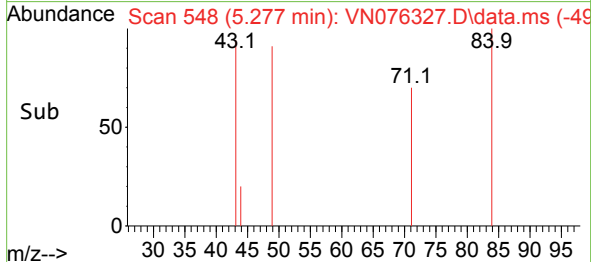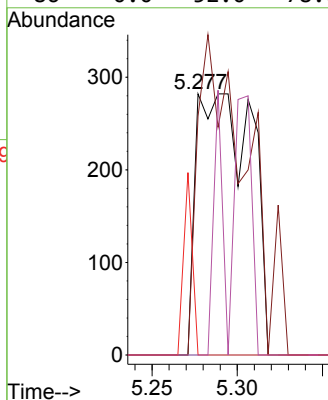

#25
2-Butanone
Concen: 1.003 ug/l
RT: 7.500 min Scan# 926
Delta R.T. 0.012 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55


Tgt Ion: 43	Resp: 2196
Ion Ratio	Lower Upper
43 100	
72 35.9	27.4 41.2

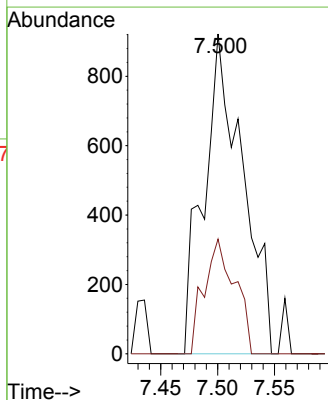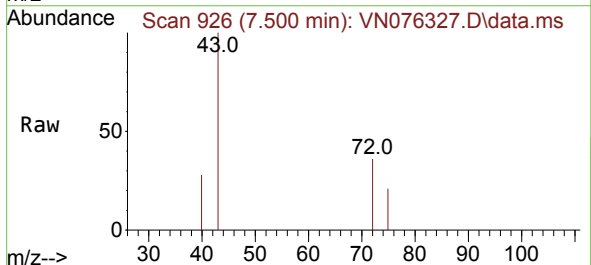






#31
Cyclohexane
Concen: 1.640 ug/l
RT: 8.236 min Scan# 1051
Delta R.T. -0.023 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55

Instrument :
MSVOA_N
ClientSampleId :
MW-10-0118DL







Tgt Ion: 56 Resp: 11260
Ion Ratio Lower Upper
56 100
69 139.6 25.8 38.8#
84 117.8 79.0 118.4

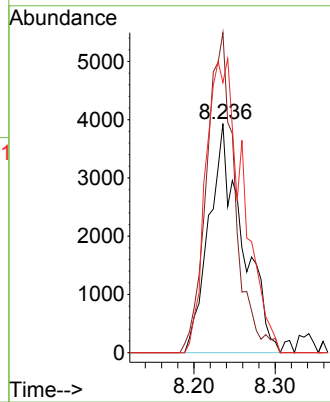

#33
1,2-Dichloroethane-d4
Concen: 45.494 ug/l
RT: 8.588 min Scan# 1111
Delta R.T. 0.006 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55

Tgt Ion: 65 Resp: 203339
Ion Ratio Lower Upper
65 100
67 51.8 0.0 104.6

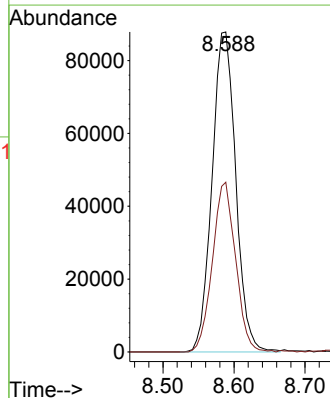



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN076327.D

Acq: 19 Jan 2023 16:55

Instrument :

MSVOA_N

ClientSampleId :

MW-10-0118DL





Tgt Ion:114 Resp: 619169

Ion Ratio Lower Upper

114 100

63 17.4 0.0 35.8

88 14.8 0.0 28.0

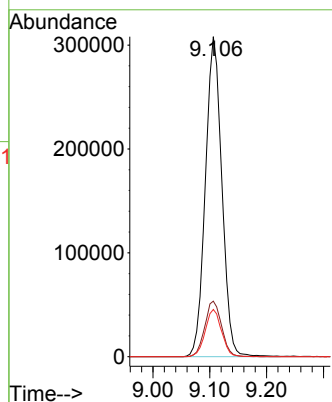

#35

Dibromofluoromethane

Concen: 47.851 ug/l

RT: 8.177 min Scan# 1041

Delta R.T. 0.006 min

Lab File: VN076327.D

Acq: 19 Jan 2023 16:55




Tgt Ion:113 Resp: 185333


Ion Ratio Lower Upper

113 100

111 102.6 82.7 124.1

192 20.2 15.6 23.4

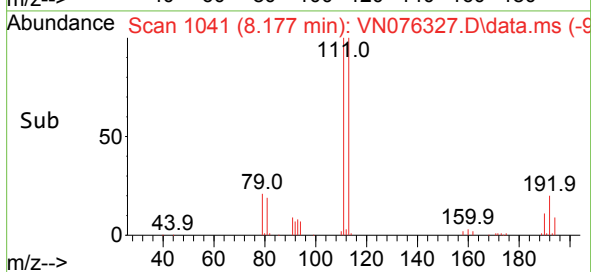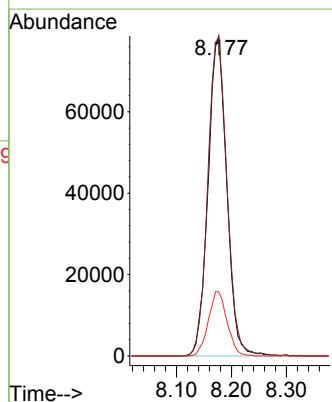



#36

1,1-Dichloropropene

Concen: 5.174 ug/l

RT: 8.230 min Scan# 1075

Delta R.T. -0.147 min

Lab File: VN076327.D

Acq: 19 Jan 2023 16:55

Instrument :

MSVOA_N

ClientSampleId :

MW-10-0118DL





Tgt Ion: 75 Resp: 28475

Ion Ratio Lower Upper

75 100

110 10.0 18.8 56.3#

77 0.0 25.0 37.4#

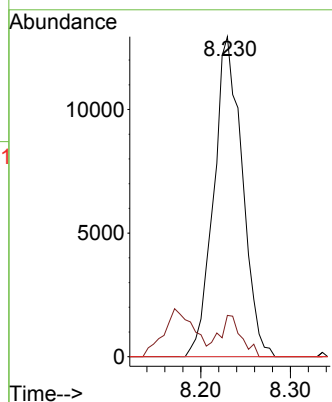

#37

Ethyl Acetate

Concen: 0.534 ug/l

RT: 7.500 min Scan# 926

Delta R.T. -0.065 min

Lab File: VN076327.D

Acq: 19 Jan 2023 16:55




Tgt Ion: 43 Resp: 2196


Ion Ratio Lower Upper

43 100

61 0.0 11.1 16.7#

70 0.0 10.0 15.0#









#38
Carbon Tetrachloride
Concen: 6.188 ug/l
RT: 8.230 min Scan# 1073
Delta R.T. -0.135 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0118DL


Tgt Ion:117 Resp: 37979
Ion Ratio Lower Upper
117 100
119 3.9 75.4 113.0#
121 0.0 24.2 36.2#



#39
Methylcyclohexane
Concen: 0.455 ug/l
RT: 9.606 min Scan# 1284
Delta R.T. 0.006 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55

Tgt Ion: 83 Resp: 3059
Ion Ratio Lower Upper
83 100
55 89.9 51.7 77.5#
98 31.7 40.0 60.0#









#48
Methyl methacrylate
Concen: 0.389 ug/l
RT: 9.606 min Scan# 11
Delta R.T. -0.076 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0118DL


Tgt Ion: 41 Resp: 1323
Ion Ratio Lower Upper
41 100
69 55.0 80.8 121.2#
39 62.8 54.4 81.6



#50
Toluene-d8
Concen: 49.151 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55

Tgt Ion: 98 Resp: 703054
Ion Ratio Lower Upper
98 100
100 66.0 52.2 78.4





#51

4-Methyl-2-Pentanone

Concen: 0.263 ug/l

RT: 10.441 min Scan# 1426

Delta R.T. -0.006 min

Lab File: VN076327.D

Acq: 19 Jan 2023 16:55

Instrument :

MSVOA_N

ClientSampleId :





MW-10-0118DL

Tgt Ion: 43 Resp: 1108

Ion Ratio Lower Upper

43 100

58 29.6 35.1 52.7#

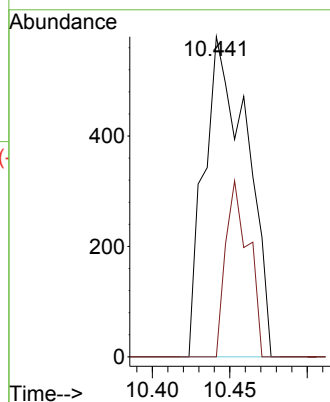

#52

Toluene

Concen: 0.314 ug/l

RT: 10.630 min Scan# 1458

Delta R.T. 0.001 min

Lab File: VN076327.D




Acq: 19 Jan 2023 16:55


Tgt Ion: 92 Resp: 3457

Ion Ratio Lower Upper

92 100

91 181.7 136.6 205.0









#59
2-Hexanone
Concen: 0.330 ug/l
RT: 11.171 min Scan# 11550
Delta R.T. -0.023 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0118DL


Tgt Ion: 43 Resp: 1009
Ion Ratio Lower Upper
43 100
58 0.0 30.1 90.3#

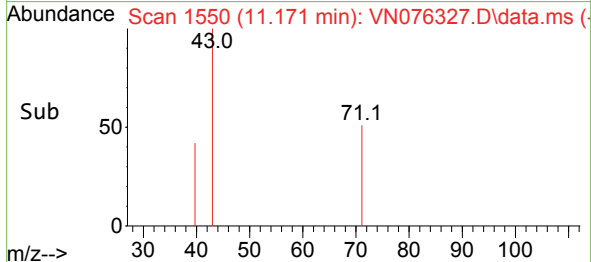

#62
4-Bromofluorobenzene
Concen: 48.804 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55

Tgt Ion: 95 Resp: 227897
Ion Ratio Lower Upper
95 100
174 87.6 0.0 174.6
176 83.2 0.0 167.8




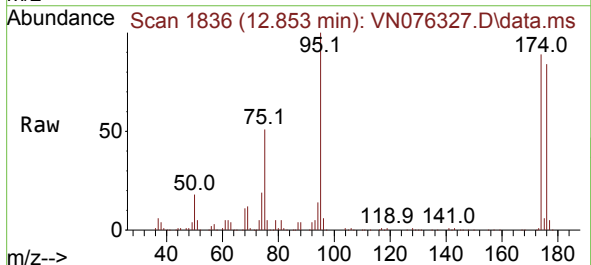




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0118DL


Tgt Ion:117 Resp: 537045
Ion Ratio Lower Upper
117 100
82 51.2 42.2 63.2
119 32.0 26.9 40.3

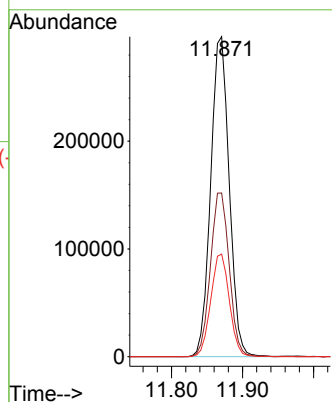

#67
Ethyl Benzene
Concen: 19.788 ug/l
RT: 11.965 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55

Tgt Ion: 91 Resp: 384467
Ion Ratio Lower Upper
91 100
106 32.2 25.5 38.3



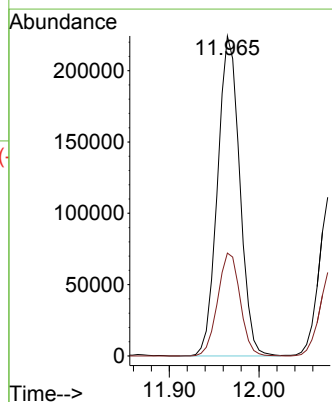





#68
m/p-Xylenes
Concen: 13.161 ug/l
RT: 12.076 min Scan# 1703
Delta R.T. 0.006 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0118DL


Tgt Ion:106 Resp: 102536
Ion Ratio Lower Upper
106 100
91 195.1 157.5 236.3

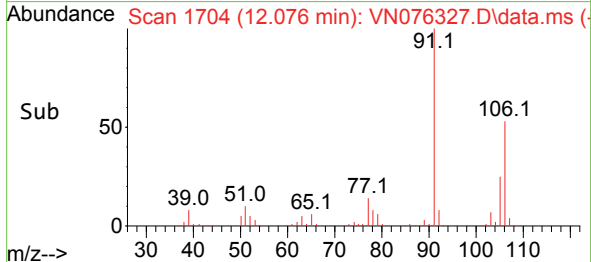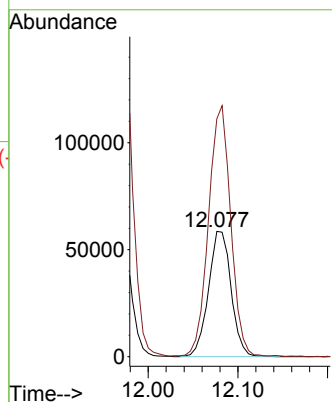

#69
o-Xylene
Concen: 1.716 ug/l
RT: 12.400 min Scan# 1759
Delta R.T. 0.000 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55

Tgt Ion:106 Resp: 13130
Ion Ratio Lower Upper
106 100
91 213.0 103.2 309.4

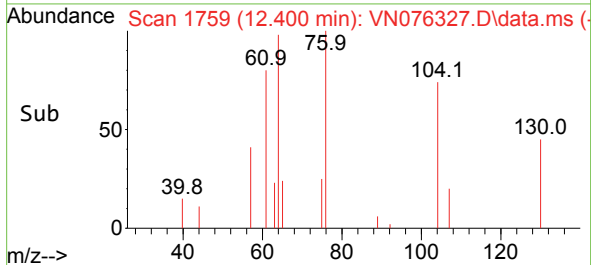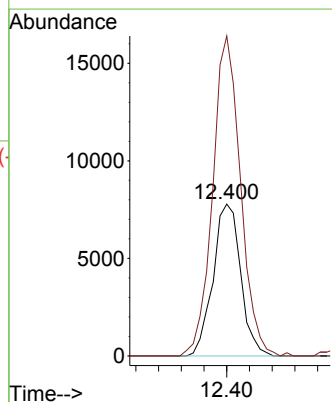



#71

Bromoform

Concen: 0.517 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. 0.271 min

Lab File: VN076327.D

Acq: 19 Jan 2023 16:55

Instrument :

MSVOA_N

ClientSampleId :

MW-10-0118DL





Tgt Ion:173 Resp: 1577

Ion Ratio Lower Upper

173 100

175 775.1 24.1 72.4#

254 0.0 0.0 0.0



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 1996

Delta R.T. 0.000 min

Lab File: VN076327.D

Acq: 19 Jan 2023 16:55




Tgt Ion:152 Resp: 229642


Ion Ratio Lower Upper

152 100

115 60.2 29.6 88.9

150 159.0 0.0 351.4

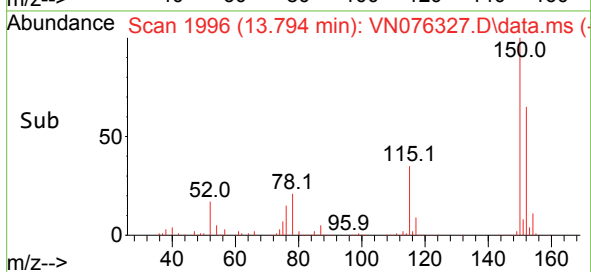



#73

Isopropylbenzene

Concen: 1.166 ug/l

RT: 12.694 min Scan# 1809

Delta R.T. 0.000 min

Lab File: VN076327.D

Acq: 19 Jan 2023 16:55

Instrument :

MSVOA_N

ClientSampleId :





MW-10-0118DL

Tgt Ion:105 Resp: 20718

Ion Ratio Lower Upper

105 100

120 25.3 13.4 40.1



#76

1,2,3-Trichloropropane

Concen: 27.570 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. -0.141 min

Lab File: VN076327.D




Acq: 19 Jan 2023 16:55


Tgt Ion: 75 Resp: 117116

Ion Ratio Lower Upper

75 100

77 1.3 75.2 225.6#


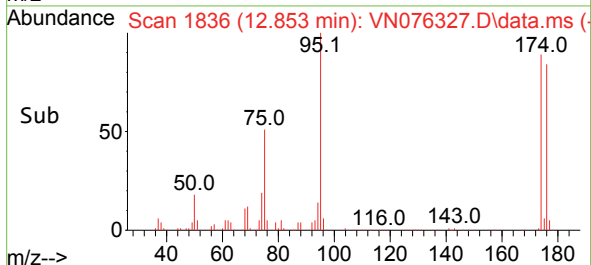






#78
n-propylbenzene
Concen: 2.278 ug/l
RT: 13.035 min Scan# 1867
Delta R.T. 0.000 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0118DL


Tgt Ion: 91 Resp: 45662
Ion Ratio Lower Upper
91 100
120 24.9 11.9 35.5



#79
2-Chlorotoluene
Concen: 0.679 ug/l
RT: 13.135 min Scan# 1884
Delta R.T. 0.006 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55

Tgt Ion: 91 Resp: 8351
Ion Ratio Lower Upper
91 100
126 0.0 17.4 52.2#







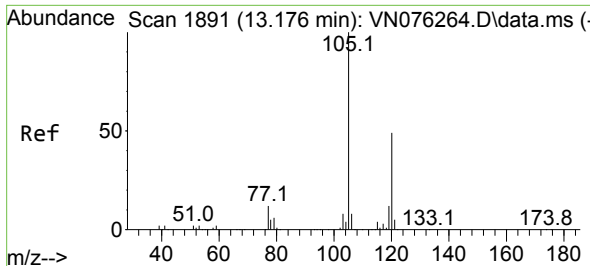

#80
 1,3,5-Trimethylbenzene
 Concen: 4.747 ug/l
 RT: 13.135 min Scan# 1884
 Delta R.T. -0.041 min
 Lab File: VN076327.D
 Acq: 19 Jan 2023 16:55




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-10-0118DL


Tgt Ion:105 Resp: 70650
 Ion Ratio Lower Upper
 105 100
 120 25.1 25.0 75.0

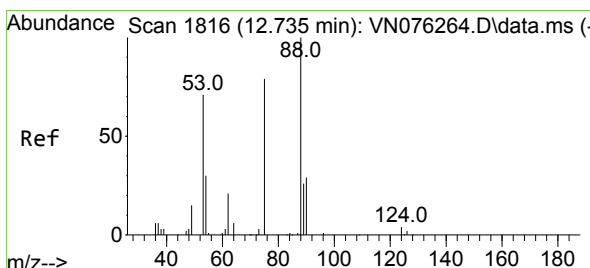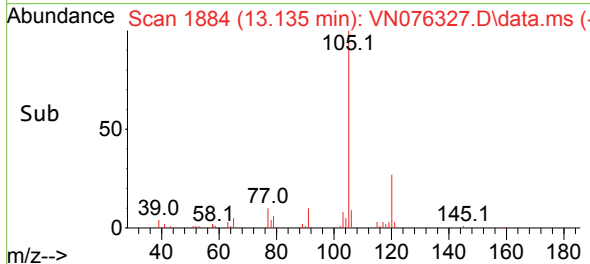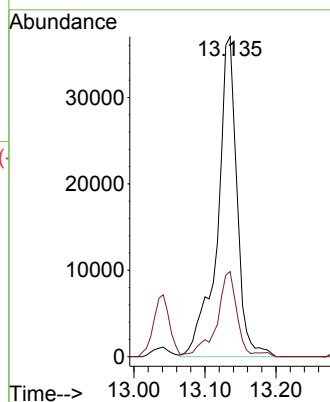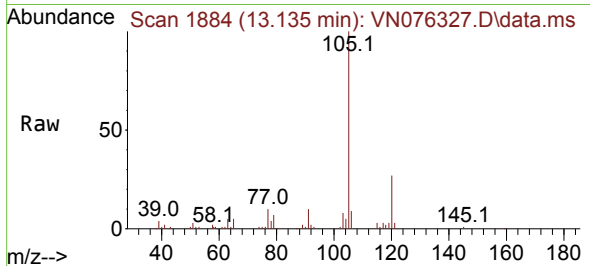

#81
 trans-1,4-Dichloro-2-butene
 Concen: 84.854 ug/l
 RT: 12.853 min Scan# 1836
 Delta R.T. 0.118 min
 Lab File: VN076327.D
 Acq: 19 Jan 2023 16:55

Tgt Ion: 75 Resp: 117116
 Ion Ratio Lower Upper
 75 100
 53 0.0 75.8 113.8#
 89 0.0 37.0 55.6#


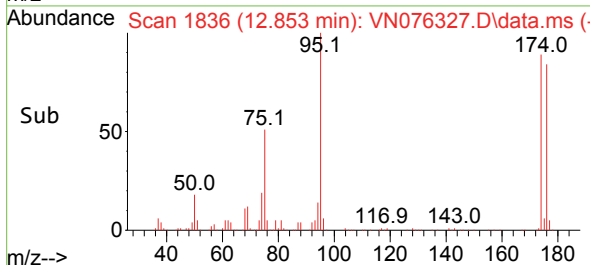

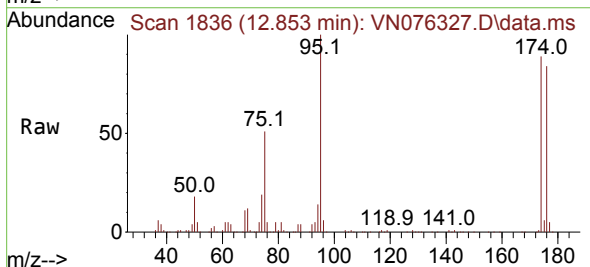




#82
4-Chlorotoluene
Concen: 0.679 ug/l
RT: 13.135 min Scan# 1884
Delta R.T. 0.006 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0118DL


Tgt Ion: 91 Resp: 8351
Ion Ratio Lower Upper
91 100
126 0.0 17.4 52.2#



#83
tert-Butylbenzene
Concen: 0.265 ug/l
RT: 13.676 min Scan# 1976
Delta R.T. 0.235 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55

Tgt Ion: 119 Resp: 3503
Ion Ratio Lower Upper
119 100
91 37.3 32.2 96.6
134 24.0 13.6 40.8









#84
1,2,4-Trimethylbenzene
Concen: 26.460 ug/l
RT: 13.488 min Scan# 1943
Delta R.T. 0.006 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0118DL


Tgt Ion:105 Resp: 394882
Ion Ratio Lower Upper
105 100
120 47.0 22.9 68.5

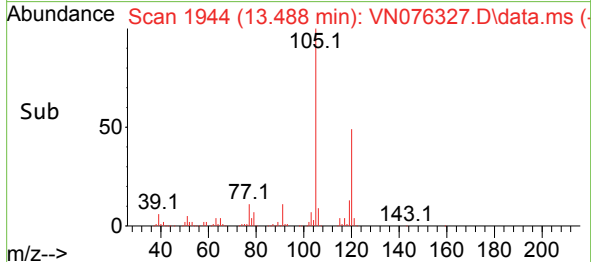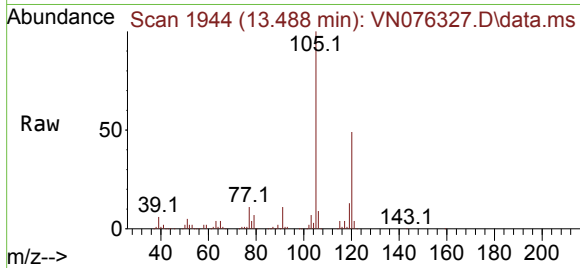

#85
sec-Butylbenzene
Concen: 21.499 ug/l
RT: 13.488 min Scan# 1944
Delta R.T. -0.129 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55

Tgt Ion:105 Resp: 394882
Ion Ratio Lower Upper
105 100
134 0.0 10.3 30.8#




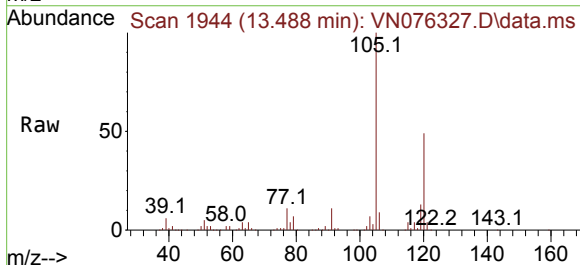


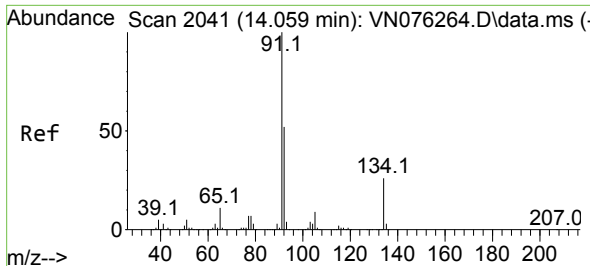

#89
n-Butylbenzene
Concen: 0.319 ug/l
RT: 14.059 min Scan# 2041
Delta R.T. -0.000 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0118DL


Tgt Ion: 91 Resp: 3820
Ion Ratio Lower Upper
91 100
92 49.5 26.3 78.9
134 91.5 13.2 39.5#

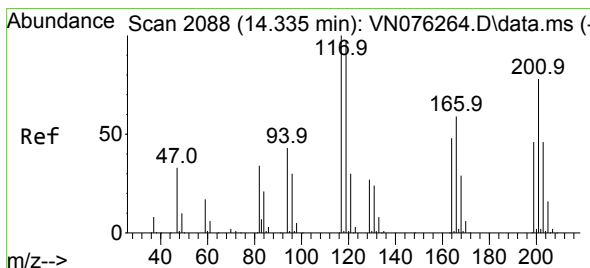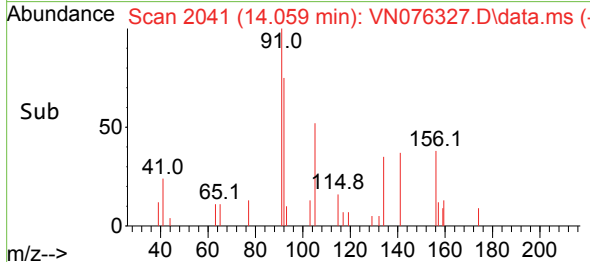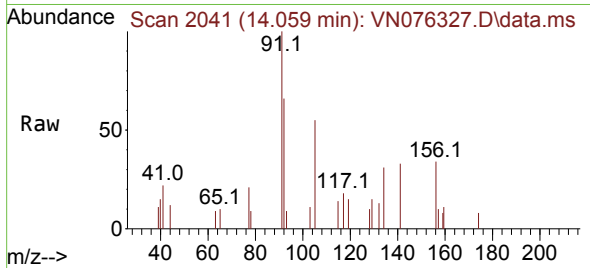

#90
Hexachloroethane
Concen: 1.183 ug/l
RT: 14.329 min Scan# 2087
Delta R.T. -0.006 min
Lab File: VN076327.D
Acq: 19 Jan 2023 16:55


Tgt Ion: 117 Resp: 3085
Ion Ratio Lower Upper
117 100
201 0.0 37.3 111.9#

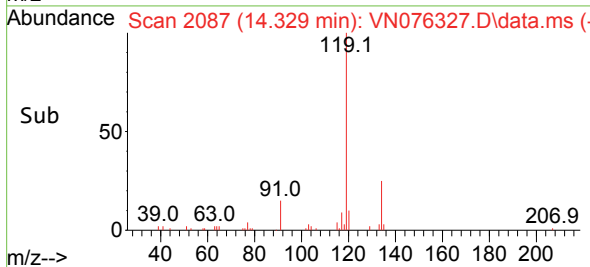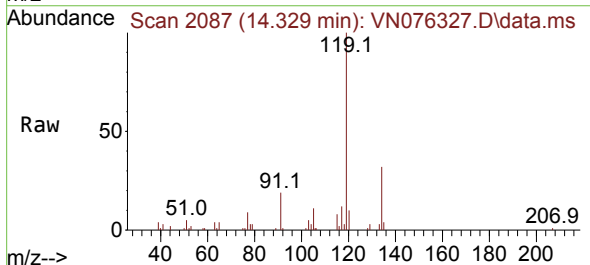

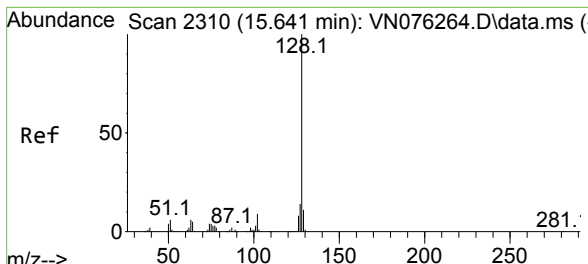

#95
 Naphthalene
 Concen: 6.259 ug/l
 RT: 15.641 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN076327.D
 Acq: 19 Jan 2023 16:55

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-10-0118DL

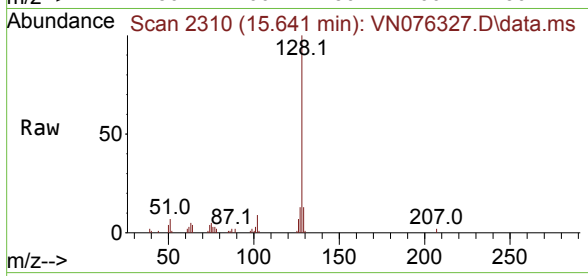

Tgt Ion:128 Resp: 54750

Ion	Ratio	Lower	Upper
128	100		
127	12.1	10.3	15.5
129	11.0	8.6	13.0

