

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011923\
 Data File : VN076326.D
 Acq On : 19 Jan 2023 16:31
 Operator : JC\MD
 Sample : 01208-01DL 5X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 33894DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
 Title : SW846 8260

Signal : TIC: VN076326.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.677	100	106	113	rBV	63995	116118	5.72%	0.436%
2	3.806	289	298	314	rBV	315476	843954	41.59%	3.170%
3	3.983	321	328	336	rVB2	11279	30204	1.49%	0.113%
4	7.441	906	916	924	rBV2	8200	23598	1.16%	0.089%
5	8.177	1029	1041	1045	rBV	249405	603337	29.73%	2.267%
6	8.230	1045	1050	1066	rVB	489794	1100133	54.21%	4.133%
7	8.588	1099	1111	1127	rBV2	259279	690469	34.03%	2.594%
8	9.106	1190	1199	1208	rBV	651985	1319430	65.02%	4.957%
9	9.600	1275	1283	1290	rVB2	9647	20463	1.01%	0.077%
10	10.571	1439	1448	1453	rBV	962541	1762618	86.86%	6.621%
11	10.635	1453	1459	1472	rVB	791429	1486823	73.27%	5.585%
12	11.865	1657	1668	1678	rBV	842661	1524632	75.13%	5.727%
13	11.965	1678	1685	1695	rVV	293159	504061	24.84%	1.894%
14	12.071	1695	1703	1715	rVV	912481	1706919	84.12%	6.412%
15	12.400	1749	1759	1769	rBV	693657	1203255	59.30%	4.520%
16	12.694	1803	1809	1817	rVB	53246	91171	4.49%	0.342%
17	12.853	1828	1836	1845	rVB	675826	1144633	56.41%	4.300%
18	13.035	1860	1867	1872	rBV	112319	182970	9.02%	0.687%
19	13.100	1872	1878	1882	rVV	485263	838163	41.30%	3.149%
20	13.135	1882	1884	1887	rVV	200116	252926	12.46%	0.950%
21	13.176	1887	1891	1899	rVB	227425	363731	17.92%	1.366%
22	13.335	1910	1918	1926	rBV	281352	471627	23.24%	1.772%
23	13.482	1937	1943	1950	rBV	860602	1395429	68.77%	5.242%
24	13.617	1958	1966	1971	rBV3	28588	52562	2.59%	0.197%
25	13.676	1971	1976	1981	rVB	53999	81709	4.03%	0.307%
26	13.729	1981	1985	1989	rBV	22962	30985	1.53%	0.116%
27	13.794	1989	1996	2008	rVV2	867268	2029247	100.00%	7.623%
28	13.953	2016	2023	2024	rBV	52340	65047	3.21%	0.244%
29	13.994	2024	2030	2046	rVB4	384171	1029408	50.73%	3.867%
30	14.117	2046	2051	2056	rVB4	32652	54458	2.68%	0.205%
31	14.188	2056	2063	2068	rBV	71373	118012	5.82%	0.443%
32	14.247	2068	2073	2075	rBV	103775	155206	7.65%	0.583%
33	14.276	2075	2078	2082	rVV	95211	142052	7.00%	0.534%
34	14.335	2082	2088	2094	rVB	142469	226575	11.17%	0.851%
35	14.400	2094	2099	2102	rBV	48867	83127	4.10%	0.312%
36	14.447	2102	2107	2116	rVB2	167346	292980	14.44%	1.101%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011923\
 Data File : VN076326.D
 Acq On : 19 Jan 2023 16:31
 Operator : JC\MD
 Sample : 01208-01DL 5X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 33894DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
 Title : SW846 8260

37	14.576	2124	2129	2134	rVB2	60138	97076	4.78%	0.365%
38	14.659	2134	2143	2146	rBV	93307	168093	8.28%	0.631%
39	14.694	2146	2149	2154	rVV	143611	216330	10.66%	0.813%
40	14.735	2154	2156	2160	rVB	32747	38998	1.92%	0.147%
41	14.876	2172	2180	2184	rBV3	33241	64170	3.16%	0.241%
42	14.929	2184	2189	2194	rBV	178860	310177	15.29%	1.165%
43	15.053	2201	2210	2217	rBV4	362299	818009	40.31%	3.073%
44	15.211	2230	2237	2244	rBV	313645	565788	27.88%	2.125%
45	15.323	2244	2256	2260	rBV5	83877	228845	11.28%	0.860%
46	15.447	2268	2277	2285	rVB4	91643	244360	12.04%	0.918%
47	15.600	2297	2303	2304	rVV3	13102	21384	1.05%	0.080%
48	15.641	2304	2310	2316	rVV	82514	162815	8.02%	0.612%
49	15.700	2316	2320	2325	rVV2	73174	133424	6.58%	0.501%
50	15.782	2325	2334	2354	rVB6	65151	296003	14.59%	1.112%
51	15.947	2354	2362	2371	rBV2	65399	142640	7.03%	0.536%
52	16.170	2383	2400	2409	rVB	180877	477785	23.54%	1.795%
53	16.264	2409	2416	2421	rBV6	14043	32630	1.61%	0.123%
54	16.341	2421	2429	2437	rVV3	36121	89273	4.40%	0.335%
55	16.506	2446	2457	2469	rBV2	111974	278412	13.72%	1.046%
56	16.717	2482	2493	2499	rBV5	51865	130250	6.42%	0.489%
57	16.782	2499	2504	2505	rBV2	49209	65164	3.21%	0.245%


Sum of corrected areas: 26619658

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011923\
Data File : VN076326.D
Acq On : 19 Jan 2023 16:31
Operator : JC\MD
Sample : 01208-01DL 5X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
33894DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

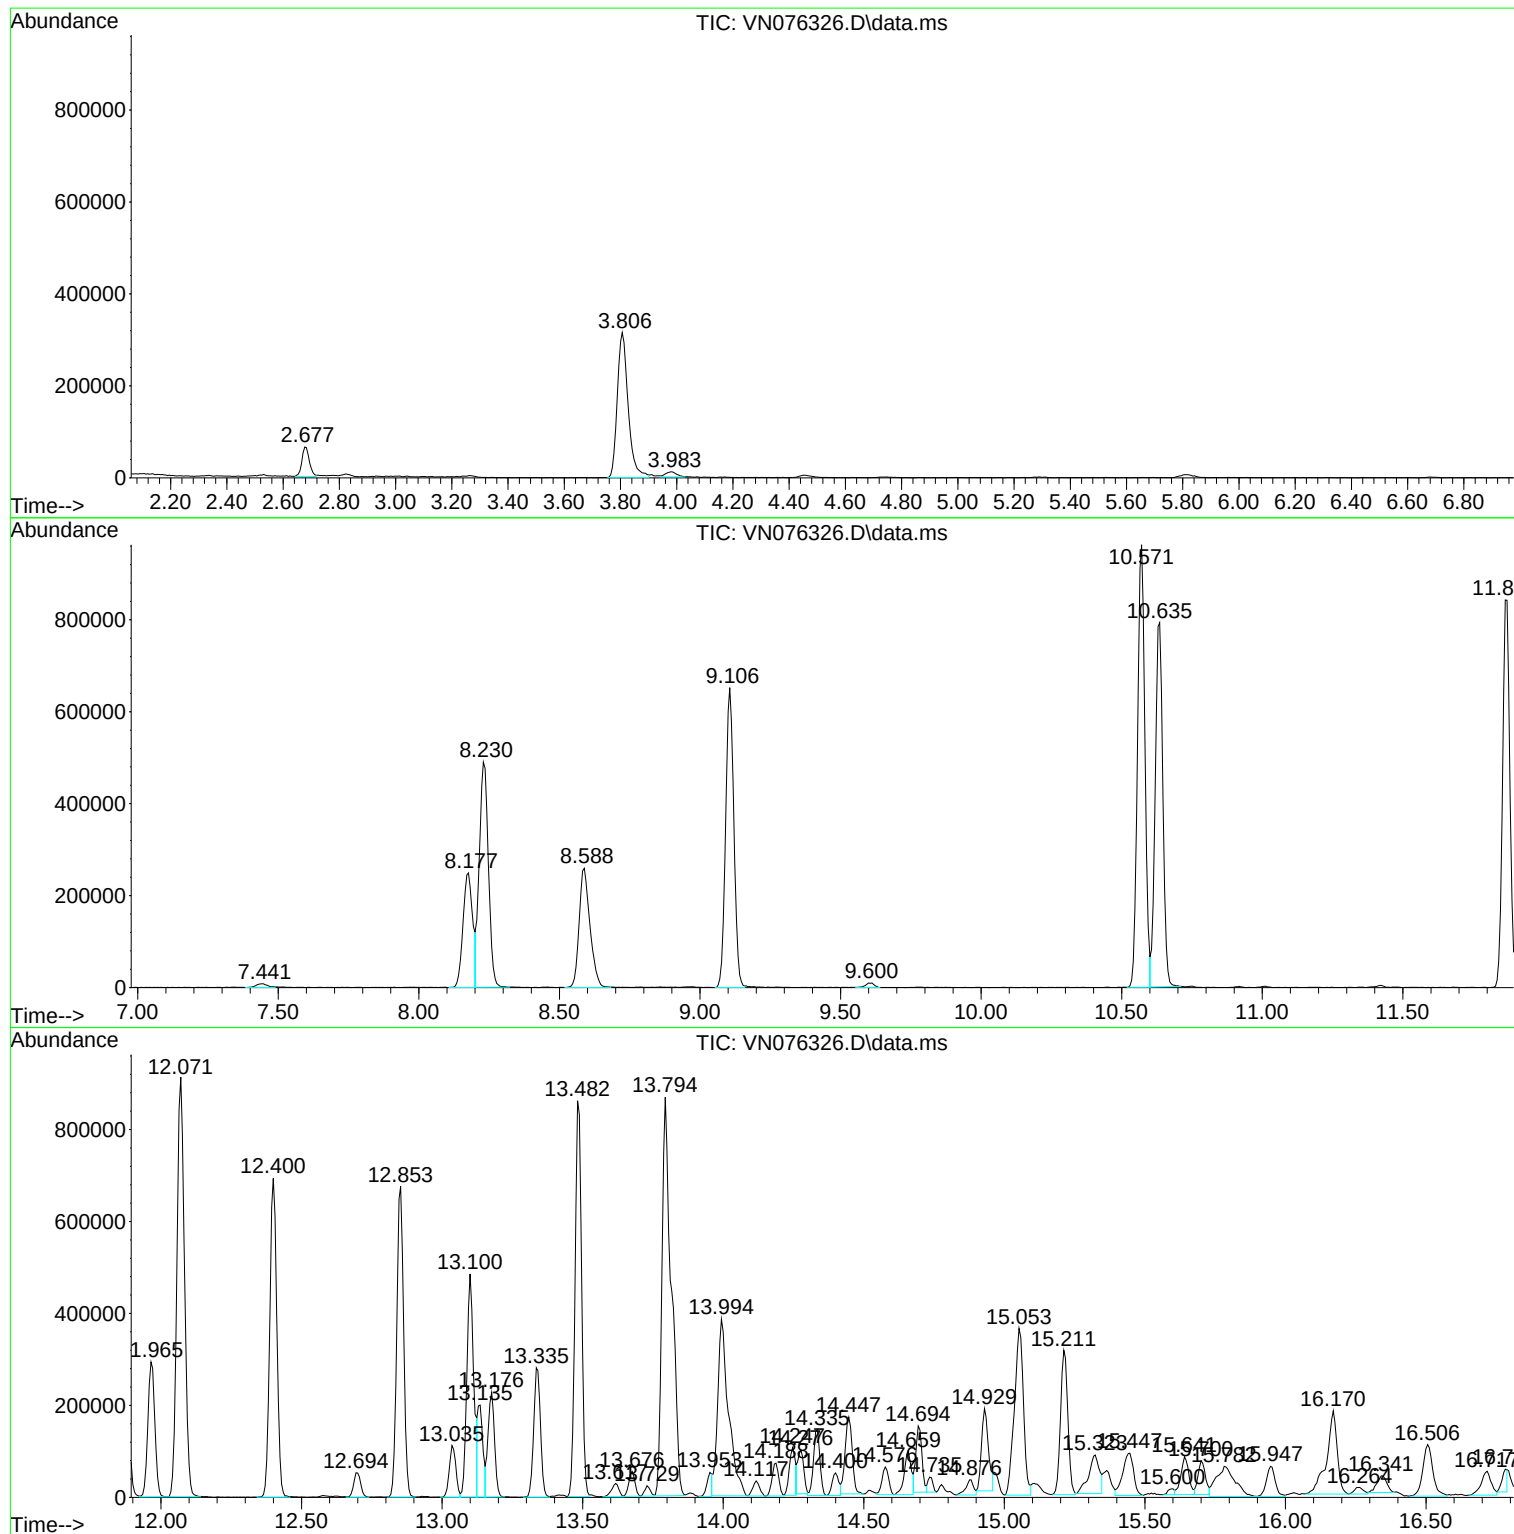

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011923\
Data File : VN076326.D
Acq On : 19 Jan 2023 16:31
Operator : JC\MD
Sample : 01208-01DL 5X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
33894DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011923\
Data File : VN076326.D
Acq On : 19 Jan 2023 16:31
Operator : JC\MD
Sample : 01208-01DL 5X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
33894DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc