


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011923\
Data File : VN076309.D
Acq On : 19 Jan 2023 09:13
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Title : SW846 8260
Last Update : Tue Jan 17 03:59:22 2023

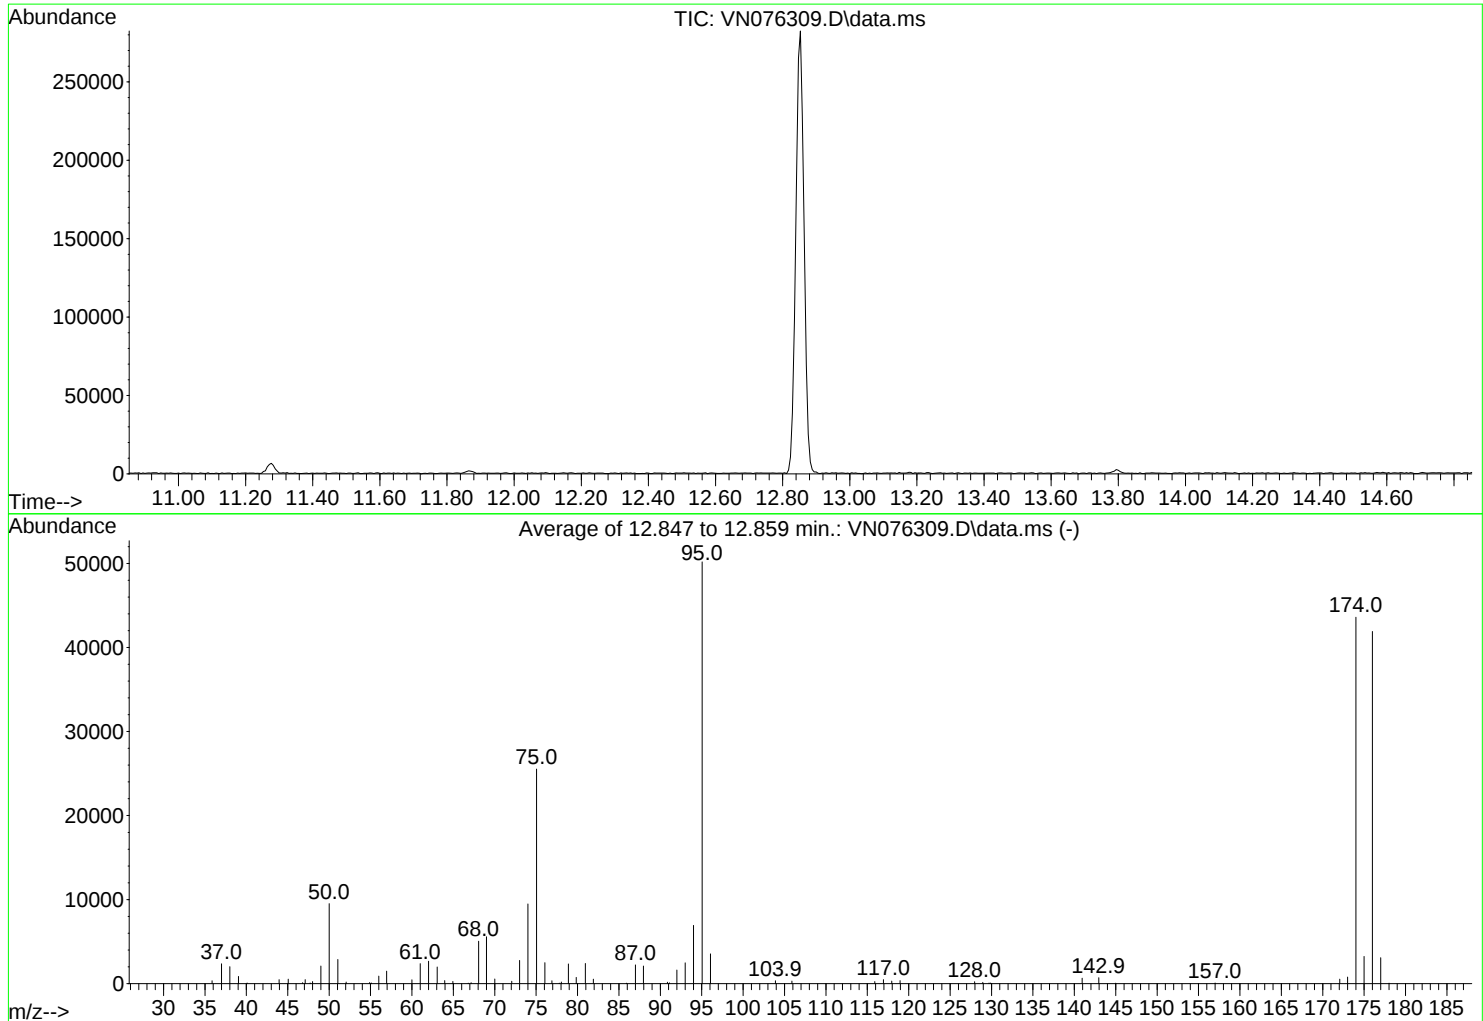

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	9524	PASS
75	95	30	60	50.9	25528	PASS
95	95	100	100	100.0	50187	PASS
96	95	5	9	7.1	3550	PASS
173	174	0.00	2	1.8	784	PASS
174	95	50	100	86.9	43589	PASS
175	174	5	9	7.4	3243	PASS
176	174	95	101	96.1	41901	PASS
177	176	5	9	7.4	3087	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	334	49.00	2093	63.05	1981	75.05	2552
37.00	2358	50.00	9524	63.95	368	76.05	2501
38.00	2024	51.05	2870	64.95	277	76.90	341
39.05	864	52.05	187	66.80	51	77.80	61
40.10	71	54.90	132	67.15	108	78.05	201
43.95	480	55.10	83	68.05	5050	78.90	2341
45.05	528	56.00	902	69.00	5588	79.85	736
46.80	122	56.95	1488	70.00	555	80.95	2397
47.10	468	60.00	457	72.05	289	81.90	528
47.70	73	61.00	2386	73.00	2770	85.90	54
48.00	252	62.00	2667	74.00	9479	87.00	2227

Average of 12.847 to 12.859 min.: VN076309.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.95	2105	116.95	476	172.05	530		
90.85	174	117.95	307	173.00	784		
91.10	97	118.95	371	174.00	43589		
92.00	1612	127.95	231	175.00	3243		
93.00	2470	128.95	153	176.00	41901		
94.00	6935	129.70	70	177.00	3087		
95.05	50187	129.90	71	178.00	51		
96.05	3550	140.95	652				
103.90	346	142.95	700				
105.90	299	145.00	58				
115.90	252	157.00	69				

Instrument :

MSVOA_N

ClientSampleId :

BFB