


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012021\
 Data File : VN065559.D
 Acq On : 20 Jan 2021 9:30
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N011321W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Jan 14 04:12:08 2021

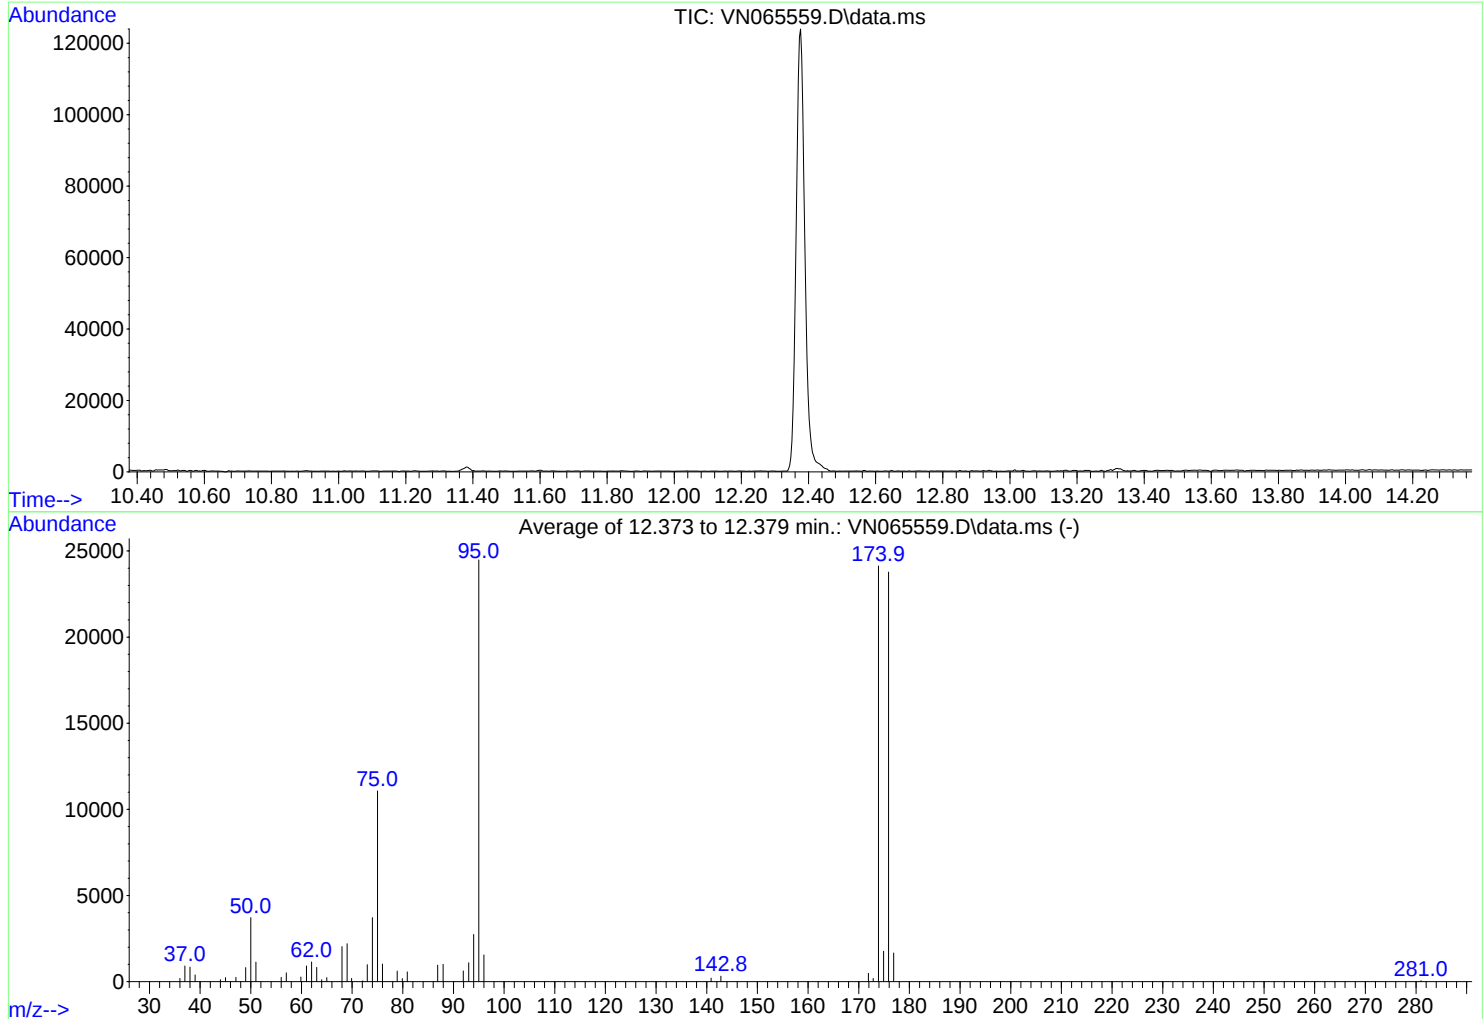

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3295

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	3719	PASS
75	95	30	60	45.2	11068	PASS
95	95	100	100	100.0	24483	PASS
96	95	5	9	6.3	1551	PASS
173	174	0.00	2	0.8	186	PASS
174	95	50	100	98.5	24125	PASS
175	174	5	9	7.3	1766	PASS
176	174	95	101	98.6	23776	PASS
177	176	5	9	7.0	1666	PASS