
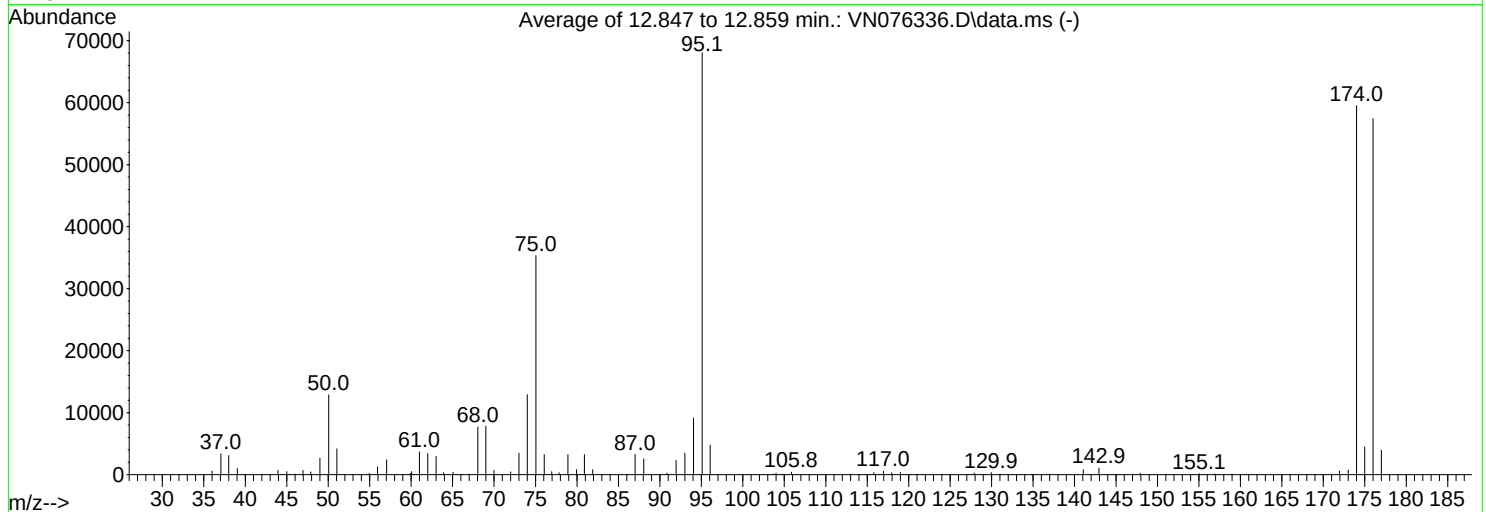


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012023\
Data File : VN076336.D
Acq On : 20 Jan 2023 09:54
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Title : SW846 8260
Last Update : Tue Jan 17 03:59:22 2023

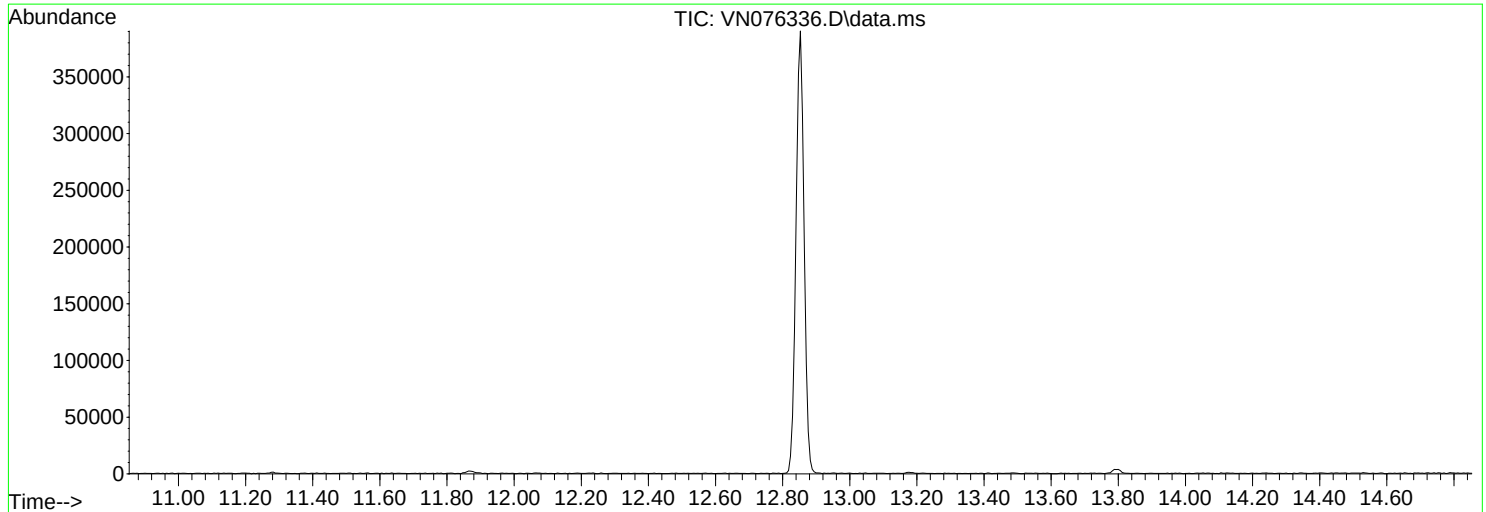

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	12889	PASS
75	95	30	60	51.9	35331	PASS
95	95	100	100	100.0	68035	PASS
96	95	5	9	7.0	4788	PASS
173	174	0.00	2	1.3	746	PASS
174	95	50	100	87.5	59504	PASS
175	174	5	9	7.5	4460	PASS
176	174	95	101	96.5	57435	PASS
177	176	5	9	6.8	3920	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	596	50.05	12889	63.90	320	76.95	491
37.05	3352	51.05	4171	65.05	395	77.85	309
38.00	3084	52.00	52	67.00	74	78.90	325
39.05	972	54.95	214	68.05	7672	79.95	79
39.90	7	55.95	1261	69.00	7808	80.90	3220
43.95	692	57.05	2401	70.00	711	81.90	799
45.00	505	59.90	213	72.00	437	86.10	52
46.00	104	60.05	501	73.00	3464	87.00	3262
46.95	702	61.00	3672	74.00	12908	88.05	2552
47.90	437	62.00	3396	75.05	35331	90.85	261
49.00	2634	63.00	2936	76.05	3239	91.95	2301

Average of 12.847 to 12.859 min.: VN076336.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.00	3457	117.95	321	145.00	62	174.00	59504
94.05	9147	119.00	372	145.20	56	175.00	4460
95.10	68035	127.90	262	147.00	69	176.00	57435
96.05	4788	128.80	73	147.90	239	177.00	3920
103.70	105	129.95	337	155.05	148	177.90	52
104.00	255	131.00	77	156.90	123		
104.80	76	134.80	63	159.00	69		
105.85	400	136.80	65	160.70	56		
112.90	86	137.00	95	171.00	71		
115.80	310	141.05	789	171.95	557		
116.95	533	142.95	1051	173.00	746		