


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012122\
 Data File : VN070724.D
 Acq On : 21 Jan 2022 9:39
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
 Title : SW846 8260
 Last Update : Tue Jan 18 13:32:07 2022

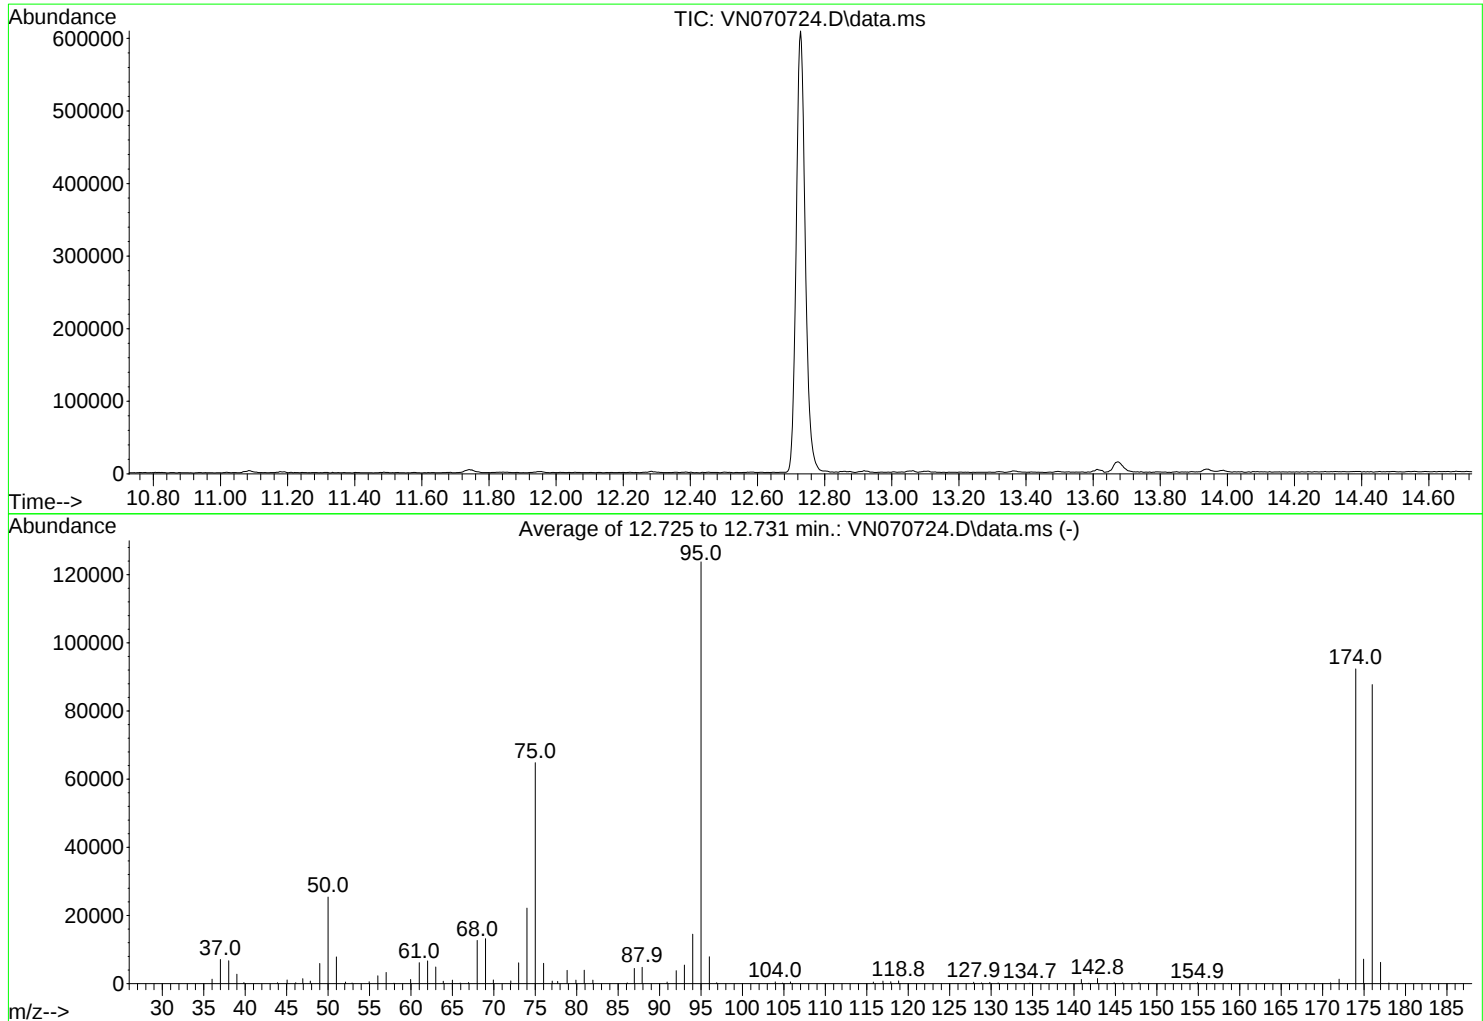

AutoFind: Scans 4003, 4004, 4005; Background Corrected with Scan 3985

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	25408	PASS
75	95	30	60	52.4	64829	PASS
95	95	100	100	100.0	123760	PASS
96	95	5	9	6.4	7900	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.6	92333	PASS
175	174	5	9	7.8	7205	PASS
176	174	95	101	95.1	87768	PASS
177	176	5	9	7.1	6237	PASS